

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP010003.D
 Acq On : 21 Apr 2022 06:44
 Operator : CG/JU
 Sample : N2473-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	44	48	60	rVB2	24774	43654	0.74%	0.095%
2	3.793	116	120	131	rBV	130927	247174	4.17%	0.535%
3	4.122	172	176	179	rBV3	5233	7972	0.13%	0.017%
4	5.052	330	334	341	rBV4	6784	13875	0.23%	0.030%
5	5.252	363	368	373	rVB5	6616	9536	0.16%	0.021%
6	6.952	651	657	662	rBV9	5712	12060	0.20%	0.026%
7	7.099	676	682	693	rBV	136938	235823	3.98%	0.511%
8	7.269	704	711	722	rBV	473580	798623	13.48%	1.729%
9	7.469	738	745	758	rBV	476725	802567	13.55%	1.738%
10	7.828	800	806	813	rVB5	9385	17119	0.29%	0.037%
11	7.940	817	825	840	rBV	439593	804237	13.57%	1.741%
12	8.299	878	886	892	rVB	32971	56111	0.95%	0.122%
13	8.646	933	945	958	rBV	439169	735484	12.41%	1.593%
14	9.099	1015	1022	1036	rBV	670799	1130121	19.07%	2.447%
15	9.552	1093	1099	1104	rVB	18636	27981	0.47%	0.061%
16	9.822	1136	1145	1160	rBV	525696	913457	15.42%	1.978%
17	10.363	1229	1237	1254	rBV	803127	1370442	23.13%	2.968%
18	10.610	1273	1279	1286	rBV	109683	188198	3.18%	0.408%
19	10.746	1295	1302	1317	rVB	699948	1182961	19.97%	2.562%
20	10.875	1317	1324	1342	rBV	653853	1202614	20.30%	2.604%
21	11.134	1362	1368	1374	rBV3	22136	38658	0.65%	0.084%
22	11.399	1409	1413	1423	rVB5	8793	20473	0.35%	0.044%
23	11.599	1444	1447	1452	rVB7	4170	6245	0.11%	0.014%
24	12.181	1541	1546	1550	rBV7	4534	7668	0.13%	0.017%
25	12.334	1566	1572	1577	rBV2	14769	23737	0.40%	0.051%
26	12.940	1671	1675	1681	rBV7	8328	15359	0.26%	0.033%
27	13.410	1751	1755	1758	rVB4	9677	11600	0.20%	0.025%
28	13.898	1834	1838	1840	rBV5	7294	9849	0.17%	0.021%
29	13.981	1845	1852	1858	rBV	1830107			

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
 Data File : BP010003.D
 Acq On : 21 Apr 2022 06:44
 Operator : CG/JU
 Sample : N2473-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	15.563	2115	2121	2133	rBV	2640530	3817189	64.43%	8.266%
38	15.675	2134	2140	2154	rVV	957726	1326320	22.39%	2.872%
39	15.804	2154	2162	2169	rVB	31505	53373	0.90%	0.116%
40	16.245	2233	2237	2240	rBV5	6631	12081	0.20%	0.026%
41	16.351	2251	2255	2261	rVB4	14455	23586	0.40%	0.051%
42	17.004	2360	2366	2372	rVB4	6155	11244	0.19%	0.024%
43	17.110	2376	2384	2394	rVV8	11009	30475	0.51%	0.066%
44	17.192	2394	2398	2402	rBV7	4438	7547	0.13%	0.016%
45	17.322	2413	2420	2428	rBV	1596350	2261976	38.18%	4.898%
46	17.422	2430	2437	2457	rVB2	3285687	4682452	79.03%	10.139%
47	17.581	2460	2464	2466	rBV5	4989	7338	0.12%	0.016%
48	17.986	2531	2533	2536	rVB4	6500	7541	0.13%	0.016%
49	18.204	2565	2570	2578	rBV3	76533	115716	1.95%	0.251%
50	18.275	2580	2582	2586	rVB3	11232	12470	0.21%	0.027%
51	18.528	2621	2625	2631	rVB9	8938	17048	0.29%	0.037%
52	19.228	2740	2744	2751	rVB2	47608	60959	1.03%	0.132%
53	19.298	2751	2756	2762	rBV	46071	70771	1.19%	0.153%
54	19.375	2765	2769	2773	rVB3	16214	20799	0.35%	0.045%
55	19.580	2802	2804	2809	rVB5	14540	12640	0.21%	0.027%
56	19.651	2810	2816	2829	rBV	4436996	5924632	100.00%	12.829%
57	20.139	2897	2899	2903	rBV5	10836	16562	0.28%	0.036%
58	21.110	3059	3064	3072	rBV	424800	595197	10.05%	1.289%
59	21.404	3108	3114	3125	rBV	1757674	2475443	41.78%	5.360%
60	23.698	3496	3504	3511	rBV	2539681	4944255	83.45%	10.706%
61	23.851	3523	3530	3545	rVB2	1071336	2269171	38.30%	4.914%




Sum of corrected areas: 46181495

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP010003.D
Acq On : 21 Apr 2022 06:44
Operator : CG/JU
Sample : N2473-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J25

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

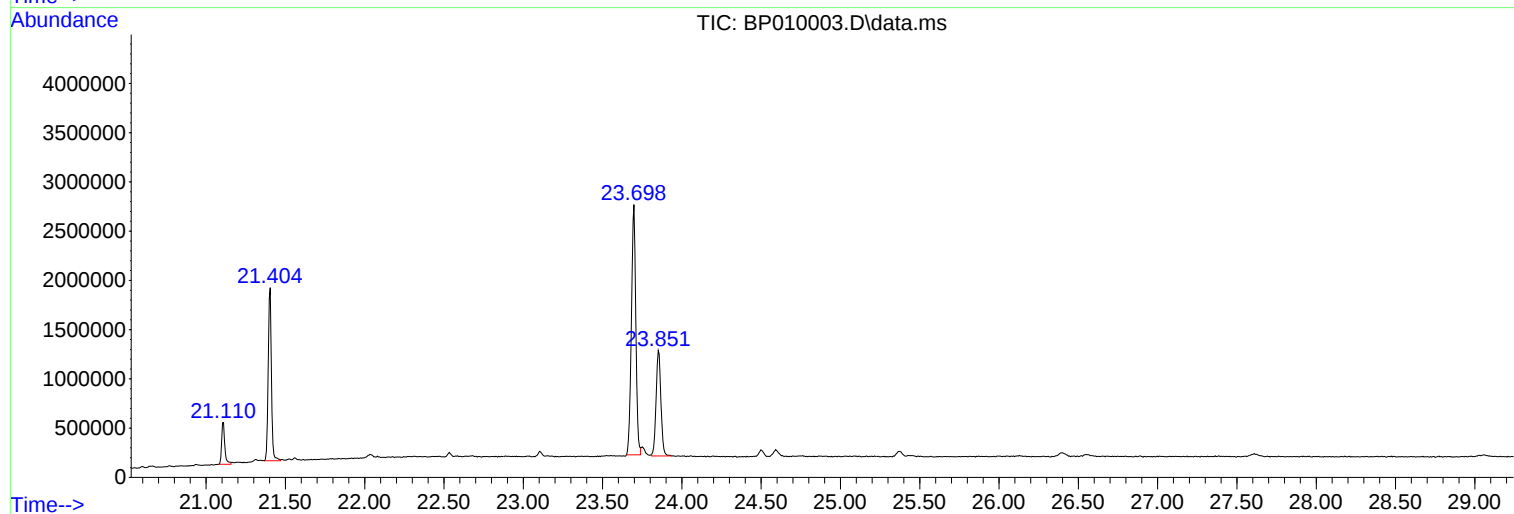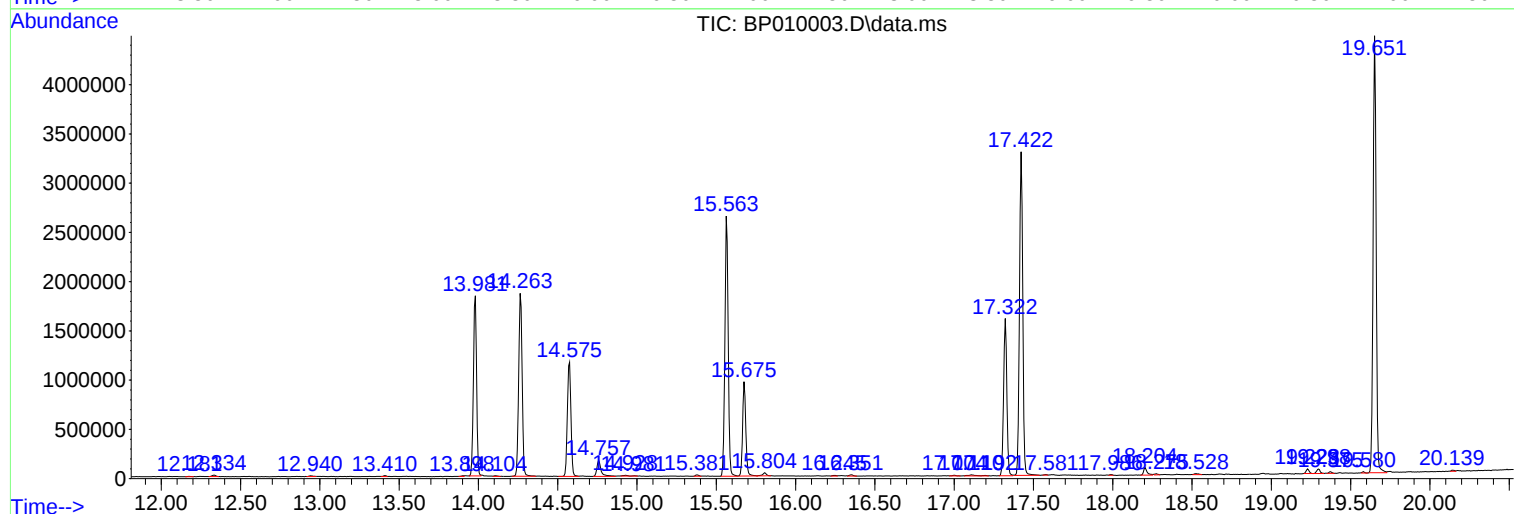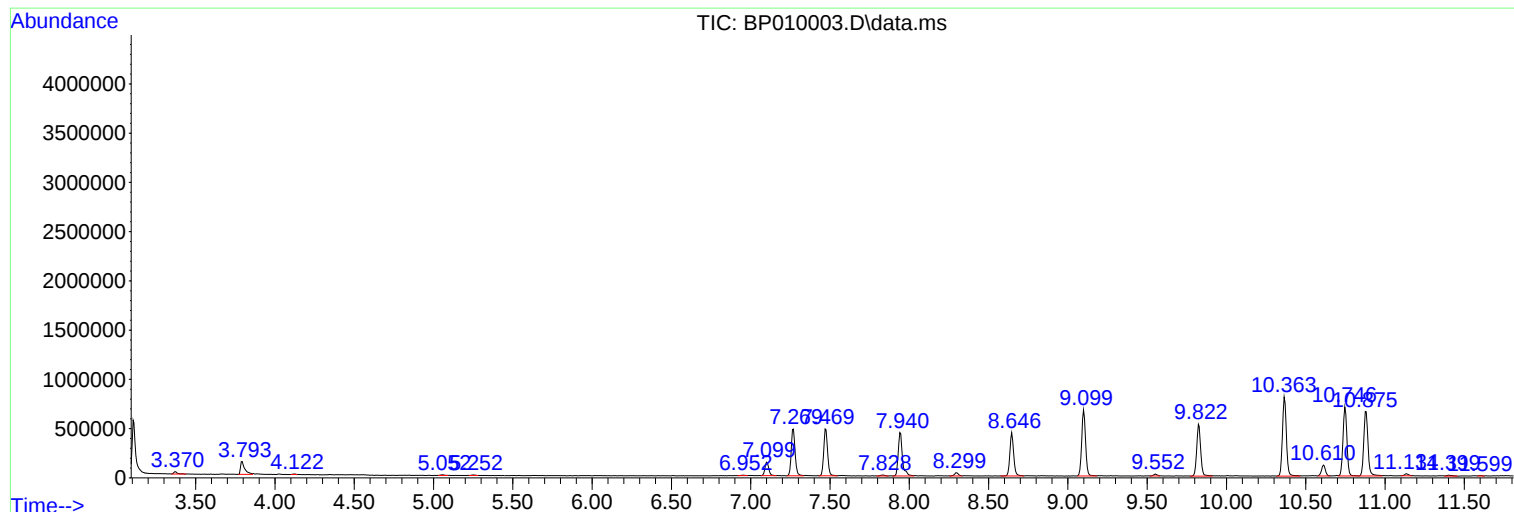

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP010003.D
Acq On : 21 Apr 2022 06:44
Operator : CG/JU
Sample : N2473-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J25










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,2,4-trichloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.610	3.18 ng/ul	188198	Naphthalene-d8	10.746

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	98
2			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
3			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
4			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
5			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98

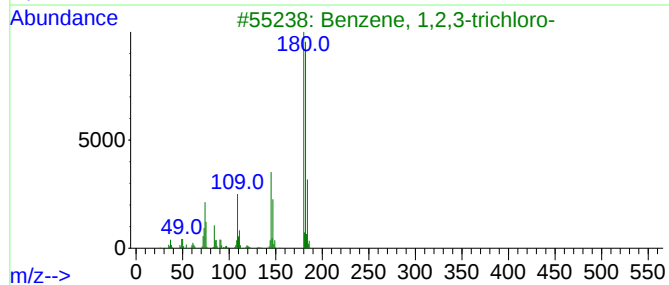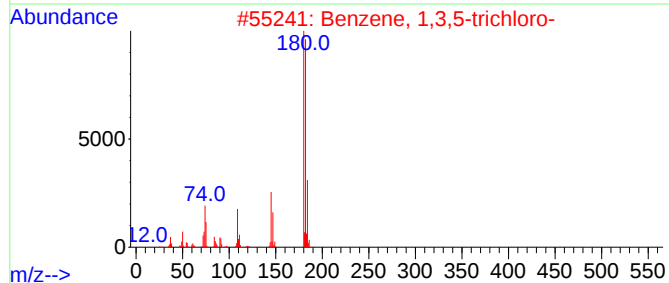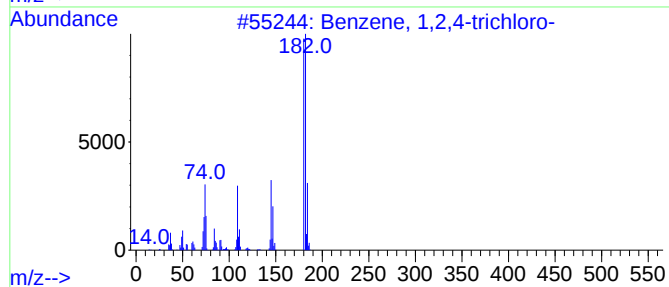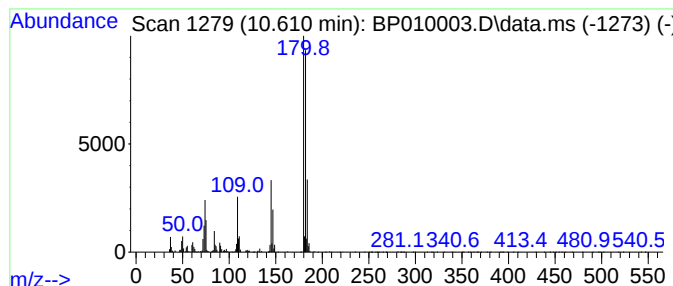










Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP010003.D
Acq On : 21 Apr 2022 06:44
Operator : CG/JU
Sample : N2473-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J25

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 1

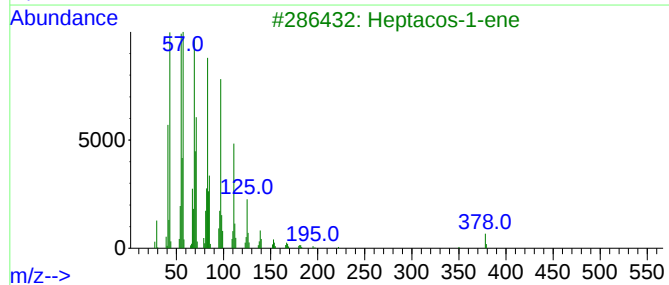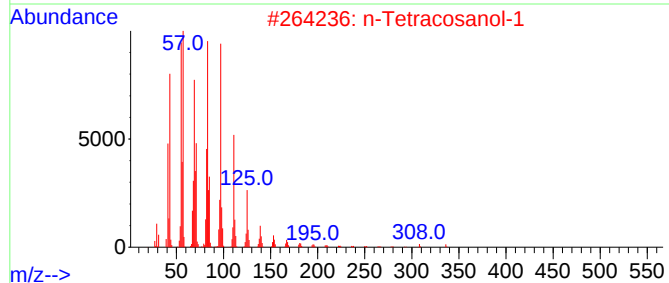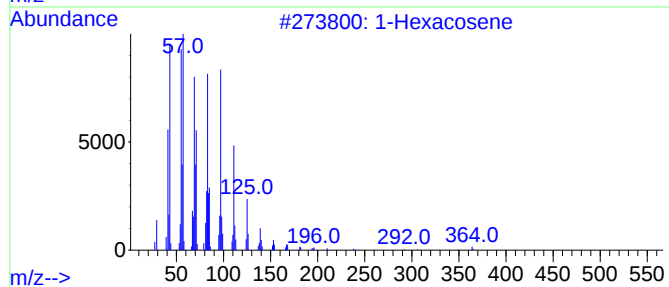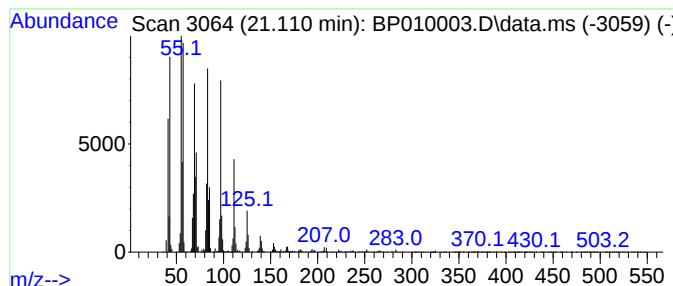

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041922\
Data File : BP010003.D
Acq On : 21 Apr 2022 06:44
Operator : CG/JU
Sample : N2473-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J25

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,2,4-...	10.610	3.2	ng/ul	188198	2	10.746	1182960	20.0
(DEL) Alkane: S...	21.110	4.8	ng/ul	595197	5	21.404	2475440	20.0