

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
 Data File : BP014729.D
 Acq On : 19 Apr 2023 14:28
 Operator : CG/JU
 Sample : 02378-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMJ9

Quant Time: Apr 20 01:46:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 19 01:37:13 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	179681	20.000	ng/ul	0.00
20) Naphthalene-d8	10.981	136	755169	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.786	164	486082	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.533	188	1114312	20.000	ng/ul	0.00
79) Chrysene-d12	21.610	240	1052830	20.000	ng/ul	0.00
88) Perylene-d12	24.186	264	1160123	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	20777	4.596	ng/uL	0.00
4) Pyridine-d5	3.922	84	108070	8.780	ng/ul	0.00
7) Phenol-d5	7.287	99	95465	6.145	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.469	67	337305	35.194	ng/ul	0.00
11) 2-Chlorophenol-d4	7.675	132	299531	25.961	ng/ul	0.00
15) 4-Methylphenol-d8	8.846	113	156352	12.910	ng/ul	0.00
21) Nitrobenzene-d5	9.322	128	182420	38.550	ng/ul	0.00
24) 2-Nitrophenol-d4	10.051	143	162025	37.910	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	354004	30.505	ng/ul	0.00
31) 4-Chloroaniline-d4	11.110	131	296183	16.722	ng/ul	0.00
46) Dimethylphthalate-d6	14.186	166	1535181	39.887	ng/ul	0.00
49) Acenaphthylene-d8	14.481	160	1684662	37.769	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	30197	4.933	ng/ul	0.00
60) Fluorene-d10	15.775	176	1342024	40.636	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	122411	27.145	ng/ul	0.00
73) Anthracene-d10	17.633	188	2157259	40.074	ng/ul	0.00
81) Pyrene-d10	19.851	212	2630947	43.623	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.021	264	2585566	43.001	ng/ul	0.00
Target Compounds						
59) Diethylphthalate	15.586	149	45783	1.217	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014729.D
Acq On : 19 Apr 2023 14:28
Operator : CG/JU
Sample : 02378-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMJ9

Quant Time: Apr 20 01:46:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 19 01:37:13 2023
Response via : Initial Calibration

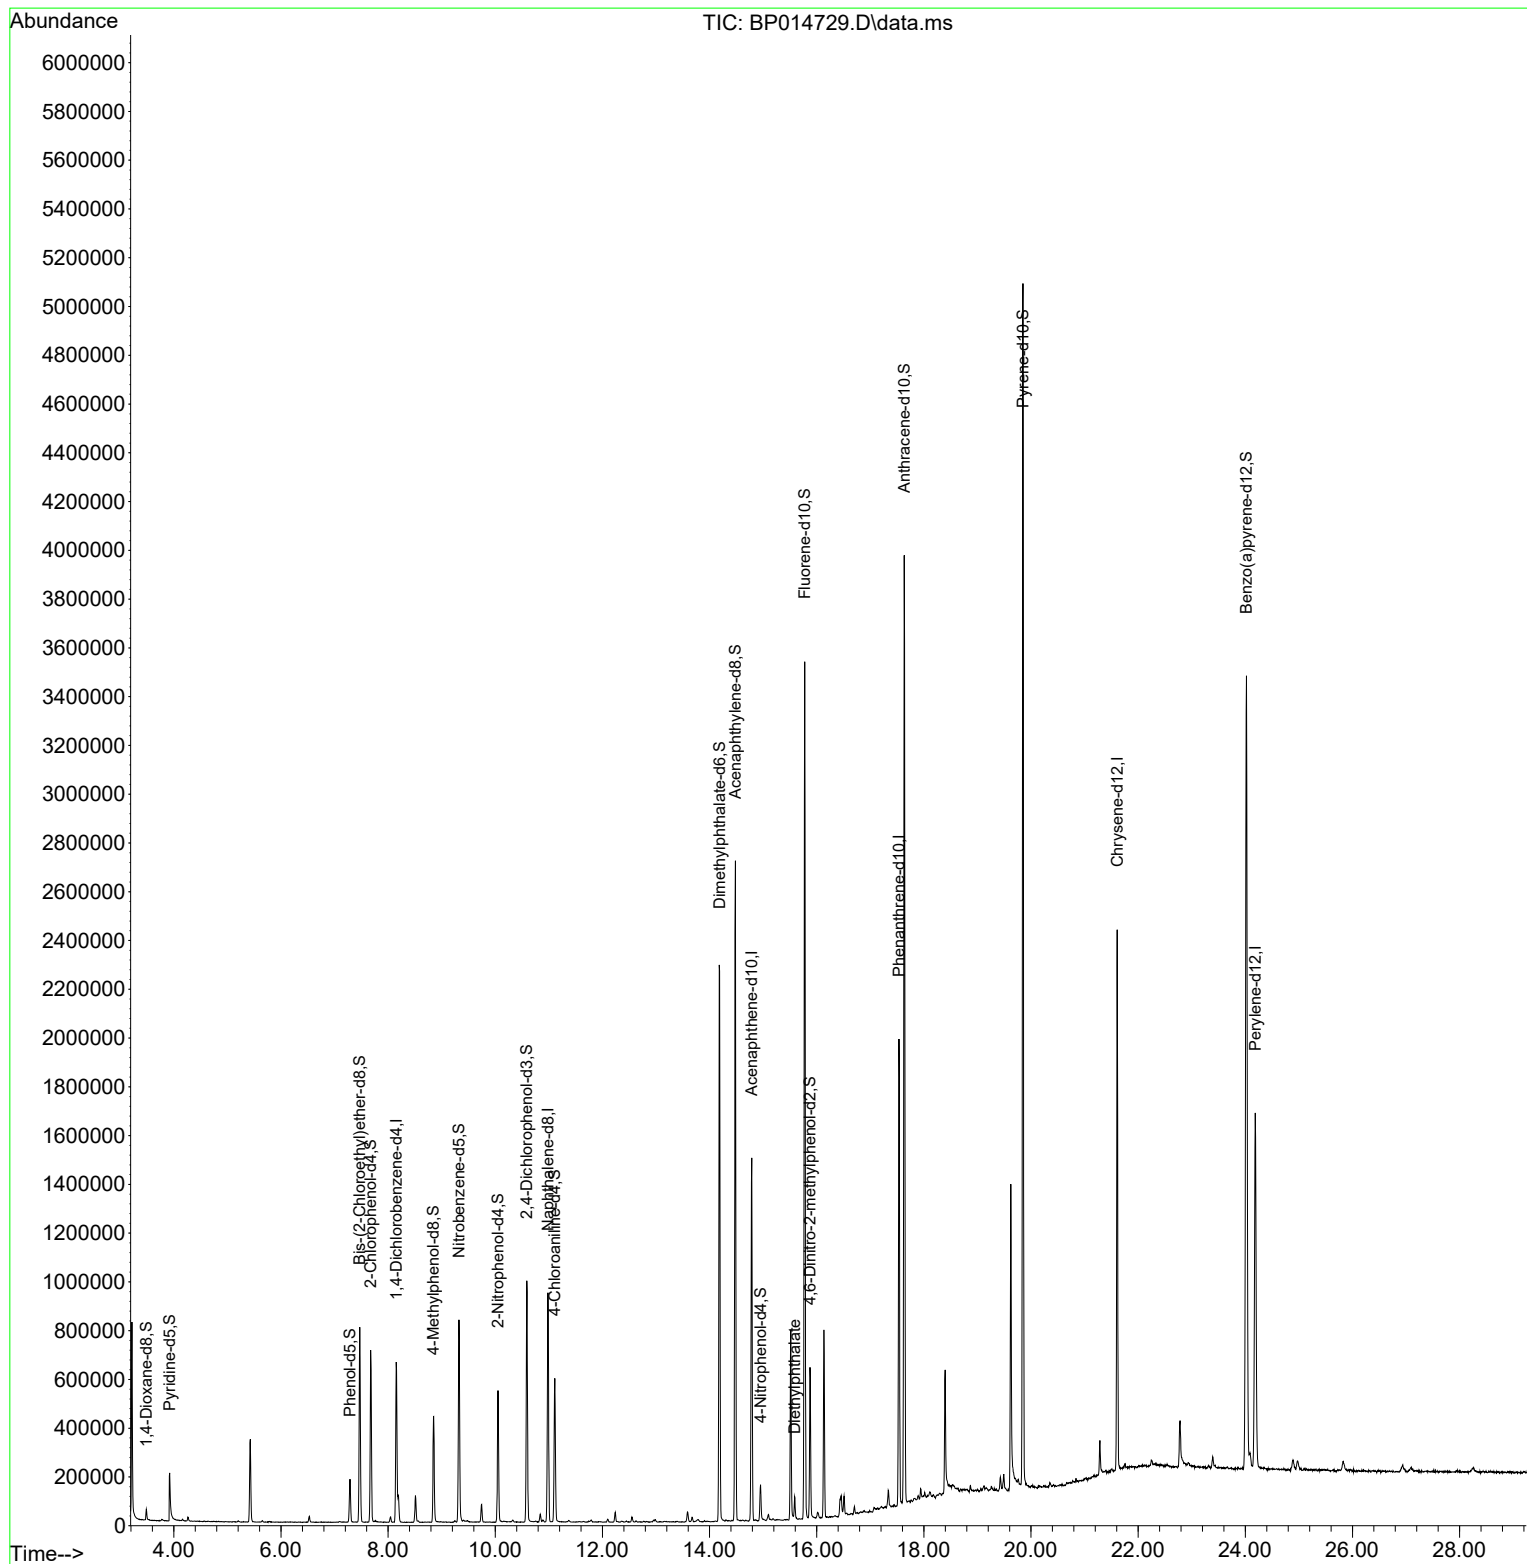

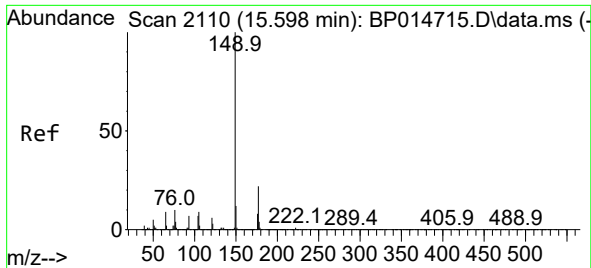

#59

Diethylphthalate

Concen: 1.217 ng/ul

RT: 15.586 min Scan# 2110

Delta R.T. -0.012 min

Lab File: BP014729.D


Acq: 19 Apr 2023 14:28

Instrument :

BNA_P

ClientSampleId :

COMJ9

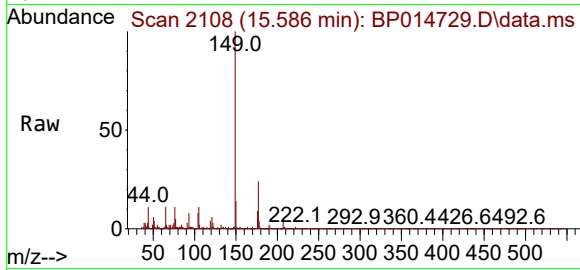

Tgt Ion:149 Resp: 45783

Ion Ratio Lower Upper

149 100

177 23.9 17.8 26.8

150 14.0 9.4 14.2

