

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
 Data File : BP014730.D
 Acq On : 19 Apr 2023 15:01
 Operator : CG/JU
 Sample : 02340-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE05

Quant Time: Apr 20 01:46:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 19 01:37:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.158	152	179171	20.000	ng/u1	0.00
20) Naphthalene-d8	10.981	136	750860	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	479496	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.534	188	1089000	20.000	ng/u1	0.00
79) Chrysene-d12	21.610	240	1044174	20.000	ng/u1	0.00
88) Perylene-d12	24.186	264	1154986	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	25101	5.568	ng/uL	0.00
4) Pyridine-d5	3.922	84	51450	4.192	ng/u1	0.00
7) Phenol-d5	7.287	99	101810	6.572	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.469	67	281634	29.469	ng/u1	0.00
11) 2-Chlorophenol-d4	7.675	132	269245	23.403	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	186605	15.452	ng/u1	0.00
21) Nitrobenzene-d5	9.322	128	148664	31.597	ng/u1	0.00
24) 2-Nitrophenol-d4	10.052	143	133286	31.365	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	311223	26.972	ng/u1	0.00
31) 4-Chloroaniline-d4	11.110	131	254495	14.451	ng/u1	0.00
46) Dimethylphthalate-d6	14.187	166	1278873	33.684	ng/u1	0.00
49) Acenaphthylene-d8	14.481	160	1383688	31.448	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	27874	4.616	ng/u1	0.00
60) Fluorene-d10	15.775	176	1092989	33.550	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	95624	21.698	ng/u1	0.00
73) Anthracene-d10	17.634	188	1828309	34.753	ng/u1	0.00
81) Pyrene-d10	19.845	212	2177845	36.410	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.021	264	2147172	35.869	ng/u1	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.523	88	32660	6.708	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014730.D
Acq On : 19 Apr 2023 15:01
Operator : CG/JU
Sample : 02340-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE05

Quant Time: Apr 20 01:46:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 19 01:37:13 2023
Response via : Initial Calibration

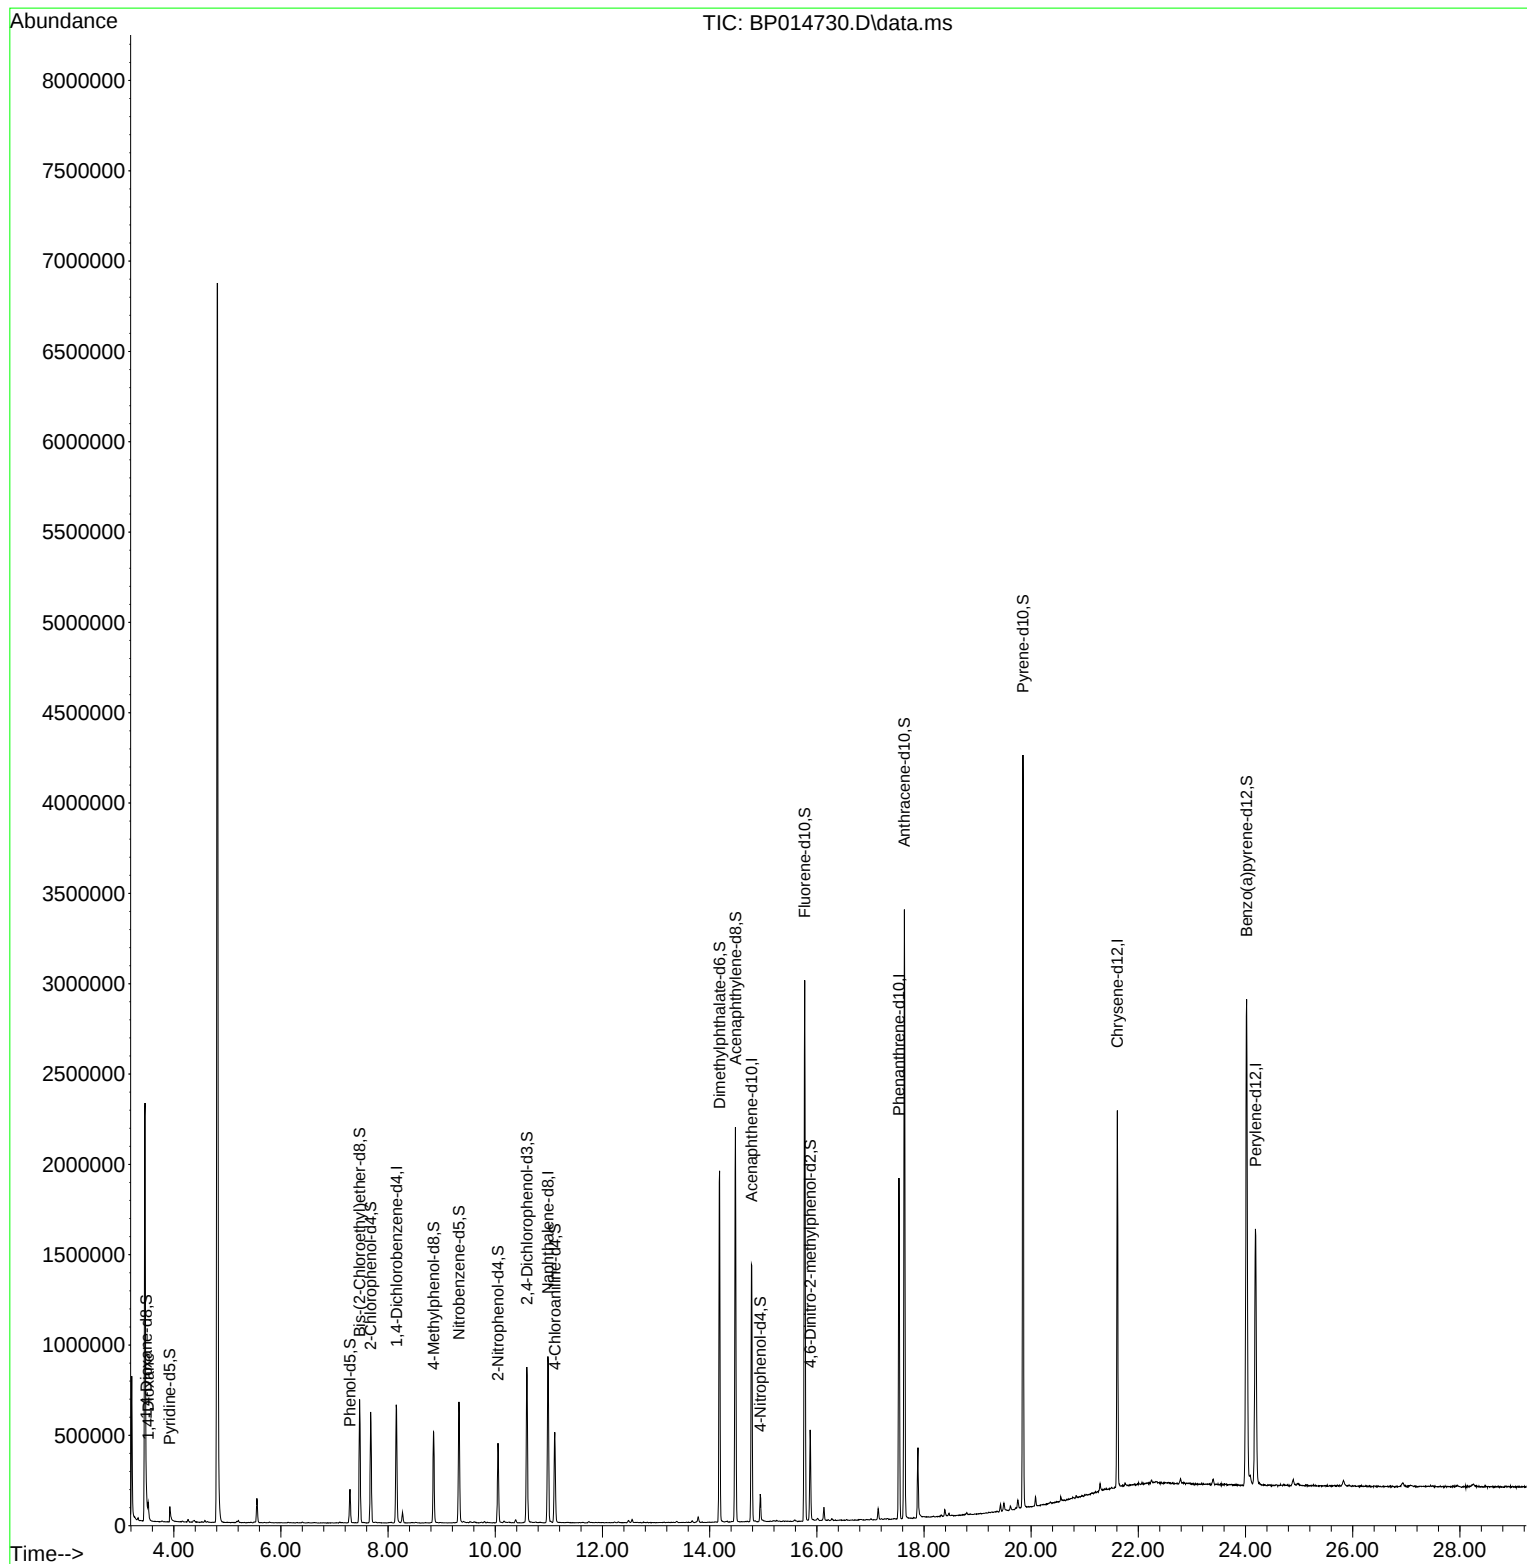

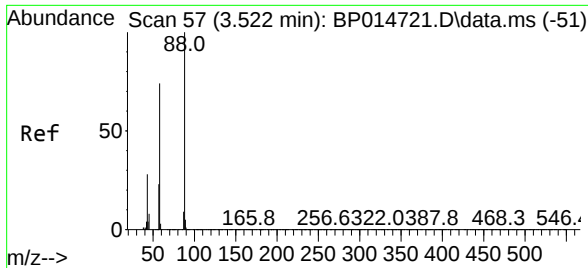

#2
 1,4-Dioxane
 Concen: 6.708 ng/uL
 RT: 3.523 min Scan# 51
 Delta R.T. -0.001 min
 Lab File: BP014730.D
 Acq: 19 Apr 2023 15:01

Instrument :
 BNA_P
 ClientSampleId :
 BHE05

Tgt Ion: 88 Resp: 32660
 Ion Ratio Lower Upper
 88 100
 43 30.9 25.0 37.6
 58 73.0 54.9 82.3

