

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
 Data File : BP014732.D
 Acq On : 19 Apr 2023 16:09
 Operator : CG/JU
 Sample : 02340-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE08

Quant Time: Apr 20 01:47:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 19 01:37:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	172829	20.000	ng/u1	0.00
20) Naphthalene-d8	10.981	136	700511	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.787	164	442604	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.534	188	978046	20.000	ng/u1	0.00
79) Chrysene-d12	21.610	240	901064	20.000	ng/u1	0.00
88) Perylene-d12	24.186	264	998085	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	19692	4.528	ng/uL	0.00
4) Pyridine-d5	3.922	84	52816	4.461	ng/u1	0.00
7) Phenol-d5	7.287	99	79023	5.288	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.469	67	249356	27.049	ng/u1	0.00
11) 2-Chlorophenol-d4	7.675	132	228729	20.611	ng/u1	0.00
15) 4-Methylphenol-d8	8.852	113	145741	12.511	ng/u1	0.00
21) Nitrobenzene-d5	9.322	128	131265	29.904	ng/u1	0.00
24) 2-Nitrophenol-d4	10.052	143	110447	27.858	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	259448	24.101	ng/u1	0.00
31) 4-Chloroaniline-d4	11.110	131	265574	16.164	ng/u1	0.00
46) Dimethylphthalate-d6	14.187	166	1105808	31.553	ng/u1	0.00
49) Acenaphthylene-d8	14.481	160	1172710	28.874	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	20750	3.722	ng/u1	0.00
60) Fluorene-d10	15.775	176	970105	32.260	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.881	200	82822	20.925	ng/u1	0.00
73) Anthracene-d10	17.633	188	1659748	35.128	ng/u1	0.00
81) Pyrene-d10	19.851	212	1953202	37.840	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.021	264	1886472	36.468	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.522	88	13293	2.830	ng/uL	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014732.D
Acq On : 19 Apr 2023 16:09
Operator : CG/JU
Sample : 02340-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE08

Quant Time: Apr 20 01:47:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 19 01:37:13 2023
Response via : Initial Calibration

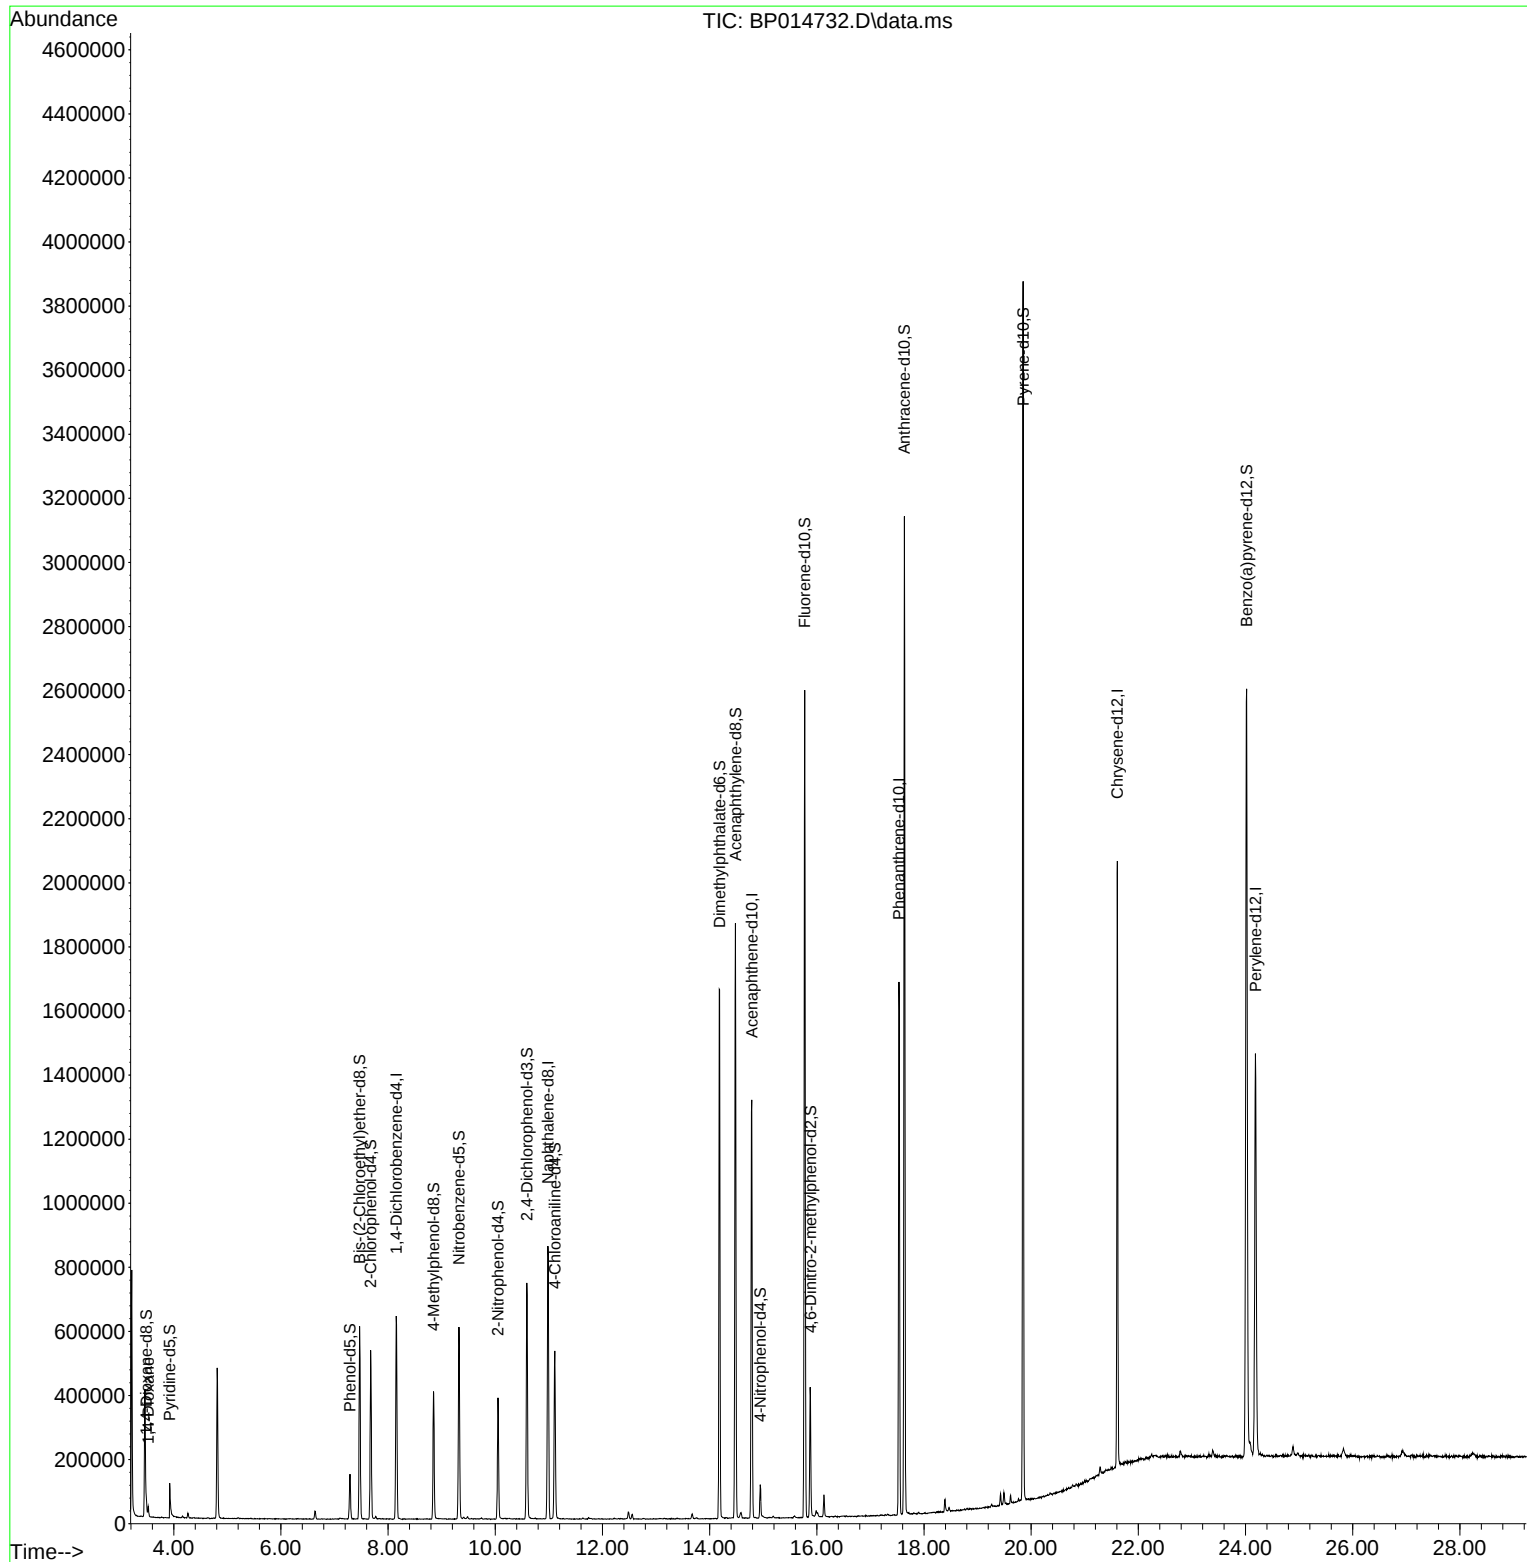

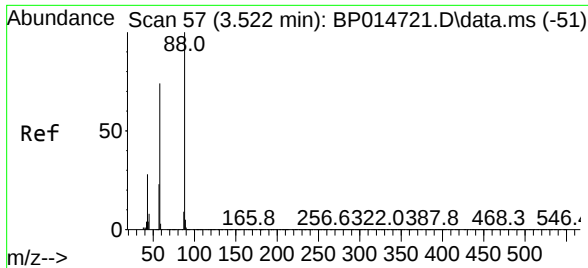

#2
 1,4-Dioxane
 Concen: 2.830 ng/uL
 RT: 3.522 min Scan# 51
 Delta R.T. -0.001 min
 Lab File: BP014732.D
 Acq: 19 Apr 2023 16:09

Instrument :
 BNA_P
 ClientSampleId :
 BHE08

Tgt Ion: 88	Resp:	13293
Ion	Ratio	Lower Upper
88	100	
43	34.6	25.0 37.6
58	73.2	54.9 82.3

