

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
 Data File : BP014733.D
 Acq On : 19 Apr 2023 16:42
 Operator : CG/JU
 Sample : 02340-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE06

Quant Time: Apr 20 01:47:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 19 01:37:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	146328	20.000	ng/u1	0.00
20) Naphthalene-d8	10.981	136	608387	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.787	164	388690	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.533	188	870489	20.000	ng/u1	0.00
79) Chrysene-d12	21.610	240	820244	20.000	ng/u1	0.00
88) Perylene-d12	24.186	264	908547	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	23759	6.453	ng/uL	0.00
4) Pyridine-d5	3.922	84	91320	9.110	ng/u1	0.00
7) Phenol-d5	7.287	99	102749	8.121	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.469	67	290393	37.205	ng/u1	0.00
11) 2-Chlorophenol-d4	7.675	132	281599	29.970	ng/u1	0.00
15) 4-Methylphenol-d8	8.852	113	183779	18.633	ng/u1	0.00
21) Nitrobenzene-d5	9.322	128	153043	40.145	ng/u1	0.00
24) 2-Nitrophenol-d4	10.051	143	135364	39.313	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	308635	33.012	ng/u1	0.00
31) 4-Chloroaniline-d4	11.110	131	260009	18.221	ng/u1	0.00
46) Dimethylphthalate-d6	14.187	166	1204498	39.137	ng/u1	0.00
49) Acenaphthylene-d8	14.481	160	1360558	38.146	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	25515	5.212	ng/u1	0.00
60) Fluorene-d10	15.775	176	1049912	39.757	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.881	200	84575	24.008	ng/u1	0.00
73) Anthracene-d10	17.633	188	1738094	41.331	ng/u1	0.00
81) Pyrene-d10	19.851	212	2102605	44.748	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.021	264	2128933	45.210	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.522	88	29866	7.511	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014733.D
Acq On : 19 Apr 2023 16:42
Operator : CG/JU
Sample : 02340-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE06

Quant Time: Apr 20 01:47:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 19 01:37:13 2023
Response via : Initial Calibration

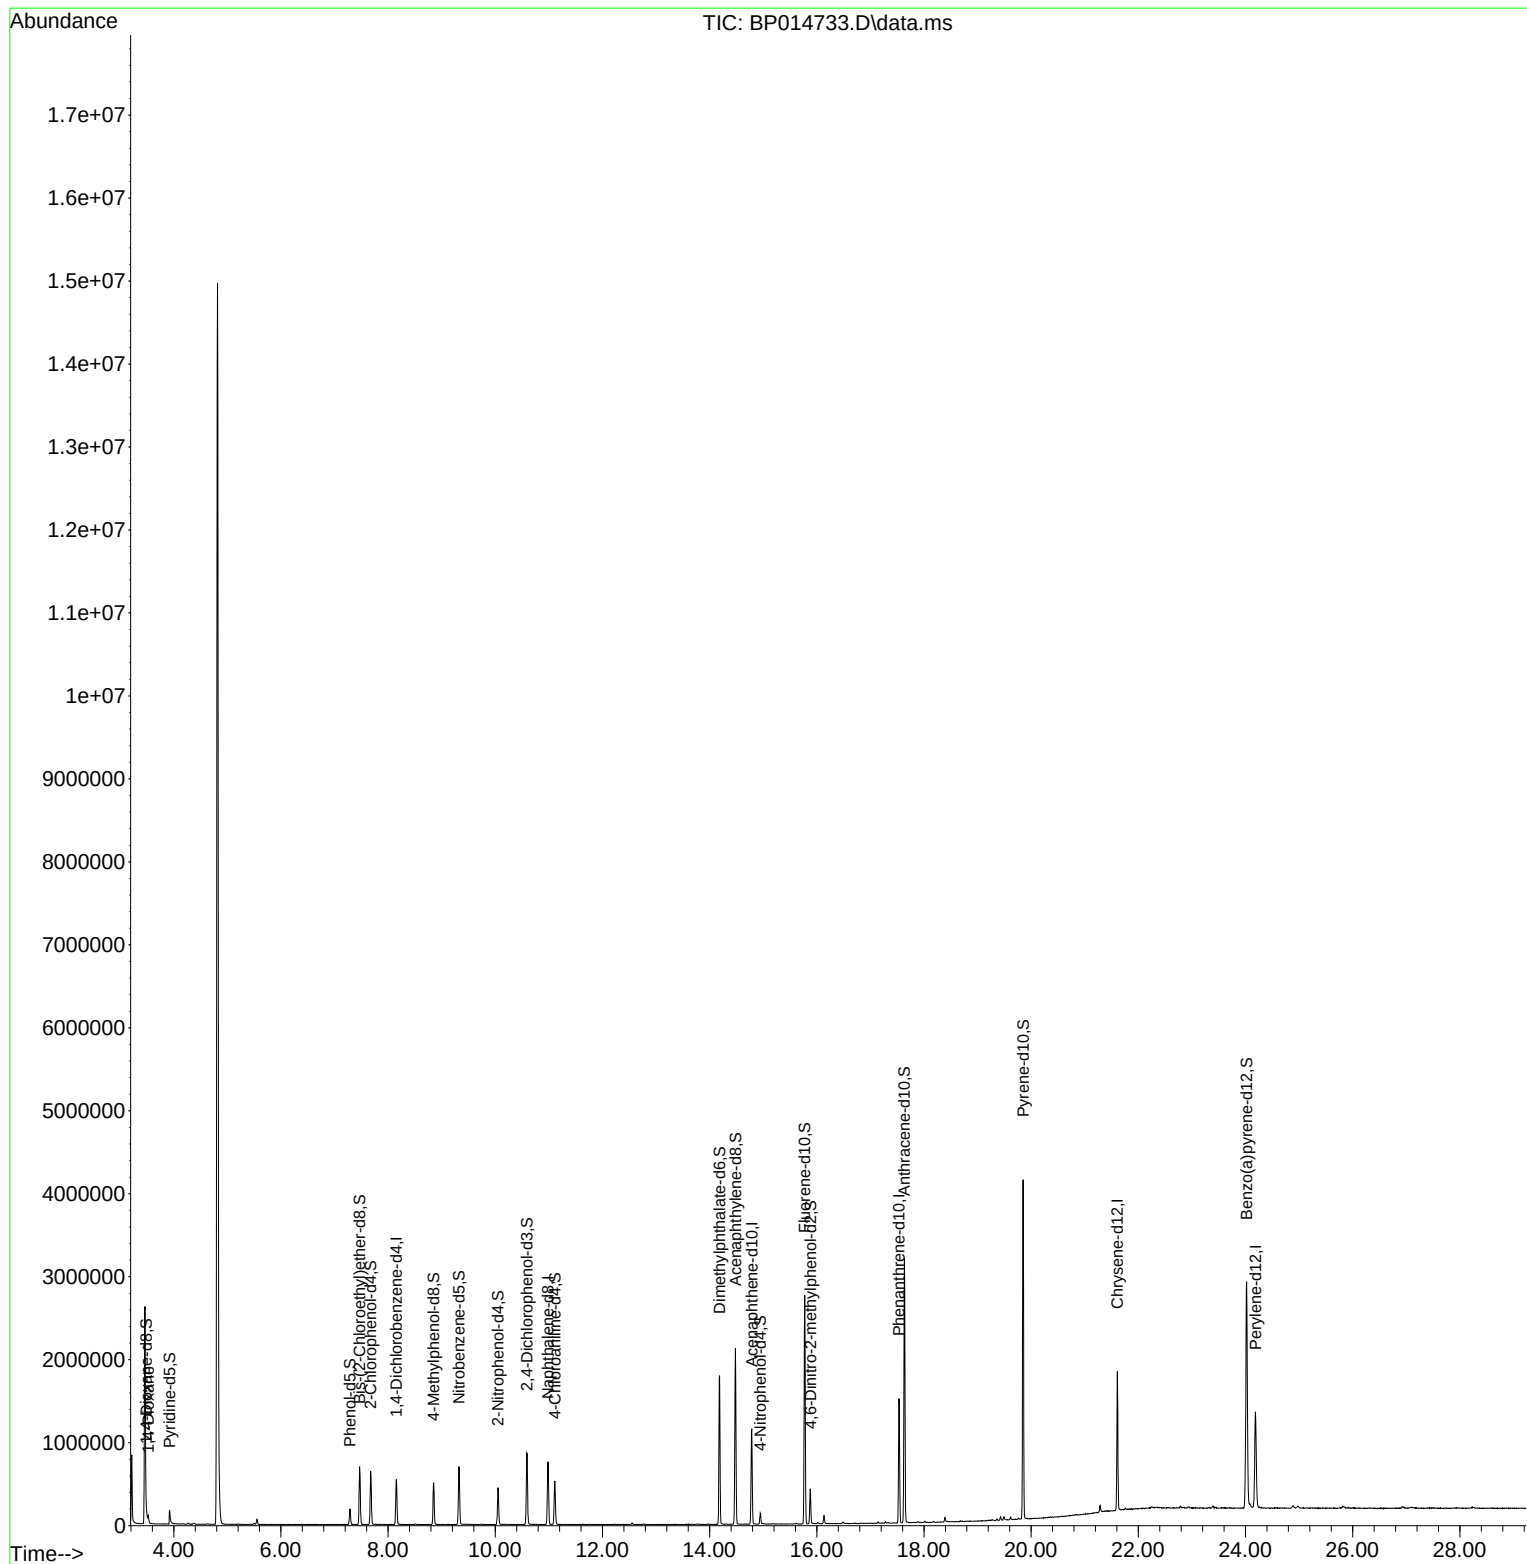

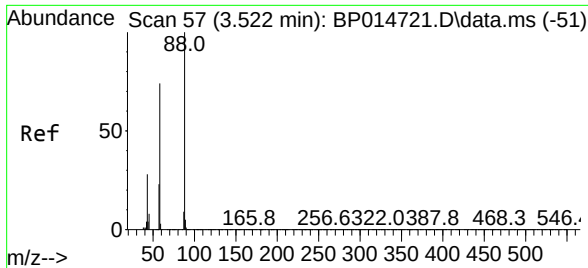

#2
 1,4-Dioxane
 Concen: 7.511 ng/uL
 RT: 3.522 min Scan# 51
 Delta R.T. -0.001 min
 Lab File: BP014733.D
 Acq: 19 Apr 2023 16:42

Instrument :
 BNA_P
 ClientSampleId :
 BHE06

Tgt Ion: 88	Resp:	29866
Ion	Ratio	Lower Upper
88	100	
43	28.6	25.0 37.6
58	68.5	54.9 82.3

