

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
 Data File : BP014723.D
 Acq On : 19 Apr 2023 11:07
 Operator : CG/JU
 Sample : PB152181BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK181

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	3	5	11	rVB	78307	79778	1.60%	0.174%
2	3.487	47	51	58	rBV	56978	72087	1.45%	0.157%
3	4.264	178	183	188	rBV	13935	20680	0.42%	0.045%
4	5.375	369	372	379	rVB8	4243	6856	0.14%	0.015%
5	7.287	690	697	711	rBV	779517	1192509	23.95%	2.599%
6	7.469	720	728	740	rVB	669510	1032654	20.74%	2.251%
7	7.675	754	763	773	rBV	778929	1206490	24.23%	2.629%
8	8.152	837	844	854	rVB	666202	1063557	21.36%	2.318%
9	8.852	955	963	977	rBV	898991	1467697	29.48%	3.199%
10	9.322	1034	1043	1053	rBV	655747	1057065	21.23%	2.304%
11	10.052	1159	1167	1177	rBV	424363	664995	13.36%	1.449%
12	10.587	1249	1258	1273	rBV	882011	1425603	28.63%	3.107%
13	10.981	1317	1325	1333	rBV	907675	1522052	30.57%	3.317%
14	11.110	1345	1347	1356	rVB9	3555	7419	0.15%	0.016%
15	12.551	1587	1592	1598	rVB2	18923	29355	0.59%	0.064%
16	13.675	1778	1783	1789	rVB2	13790	20316	0.41%	0.044%
17	14.187	1861	1870	1882	rBV	1809300	2519621	50.61%	5.491%
18	14.481	1912	1920	1929	rBV	1963155	2830022	56.84%	6.168%
19	14.787	1965	1972	1979	rBV	1443959	2087131	41.92%	4.549%
20	14.945	1992	1999	2013	rBV	670185	962486	19.33%	2.098%
21	15.192	2037	2041	2046	rVB7	4166	6641	0.13%	0.014%
22	15.775	2133	2140	2147	rBV	2772791	3681934	73.95%	8.025%
23	15.875	2151	2157	2172	rVV	402655	562805	11.30%	1.227%
24	16.016	2177	2181	2188	rVB4	11886	19130	0.38%	0.042%
25	16.281	2221	2226	2232	rVB2	13504	21749	0.44%	0.047%
26	17.210	2381	2384	2387	rBV5	3627	4986	0.10%	0.011%
27	17.534	2433	2439	2447	rBV	1760296	2543588	51.09%	5.544%
28	17.634	2449	2456	2465	rBV	2988313	4088627	82.12%	8.911%
29	18.181	2546	2549	2554	rVB6	5480	7589	0.15%	0.017%
30	19.428	2757	2761	2768	rBV2	35164	49470	0.99%	0.108%
31	19.492	2768	2772	2777	rBV2	32659	42593	0.86%	0.093%
32	19.851	2827	2833	2842	rBV	3699637	4838858	97.19%	10.546%
33	21.610	3126	3132	3142	rBV	2166713	2784575	55.93%	6.069%
34	24.021	3534	3542	3559	rVB2	2442162	4978716	100.00%	10.851%
35	24.192	3563	3571	3582	rVB2	1403368	2983281	59.92%	6.502%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014723.D
Acq On : 19 Apr 2023 11:07
Operator : CG/JU
Sample : PB152181BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK181

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Title : SVOA CALIBRATION




Sum of corrected areas: 45882915

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014723.D
Acq On : 19 Apr 2023 11:07
Operator : CG/JU
Sample : PB152181BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK181

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

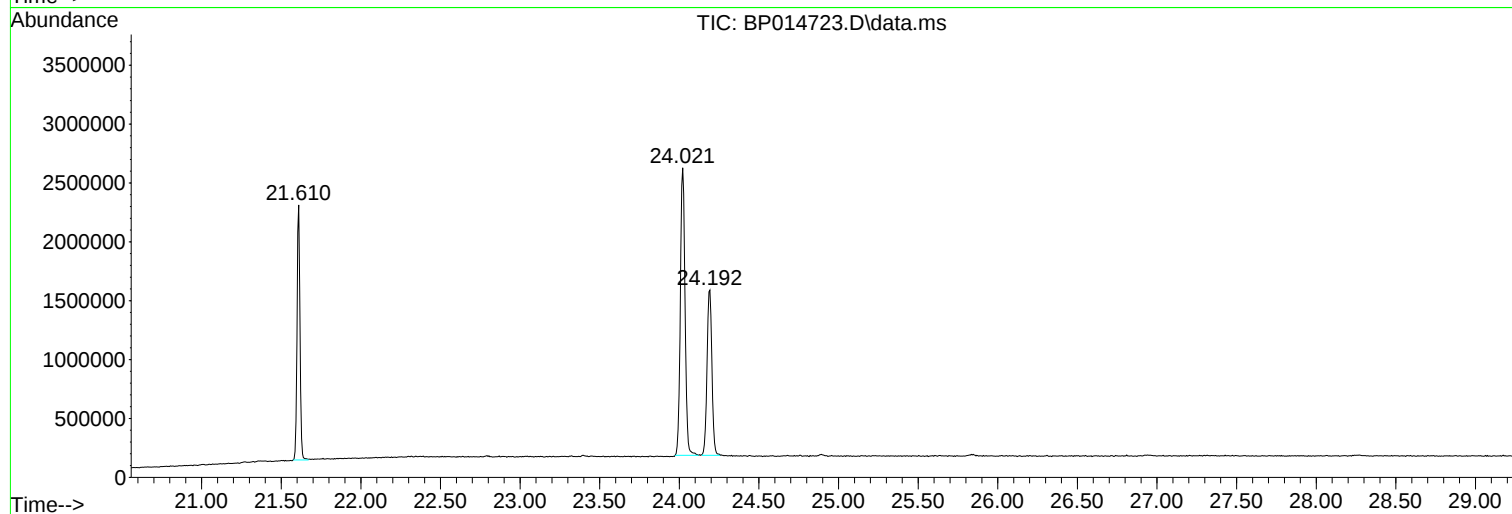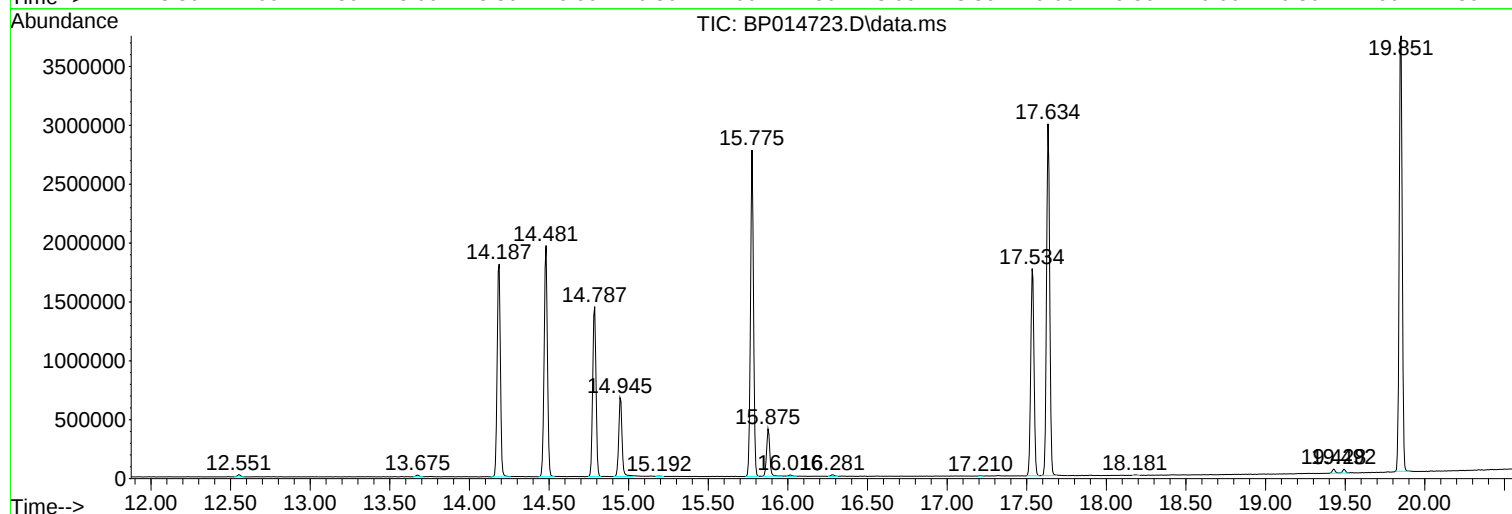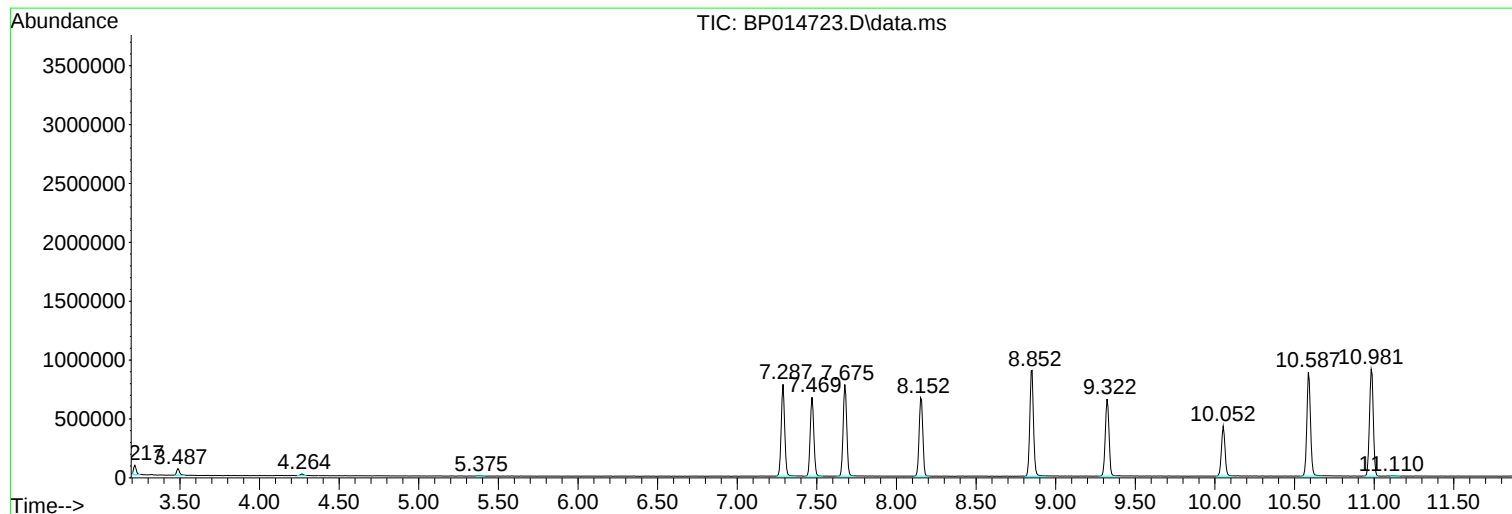

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014723.D
Acq On : 19 Apr 2023 11:07
Operator : CG/JU
Sample : PB152181BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK181

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014723.D
Acq On : 19 Apr 2023 11:07
Operator : CG/JU
Sample : PB152181BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK181

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------