

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
 Data File : BP014734.D
 Acq On : 19 Apr 2023 17:16
 Operator : CG/JU
 Sample : 02340-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	3	5	18	rVB	658443	687803	14.51%	1.700%
2	3.487	46	51	58	rVB	41595	52070	1.10%	0.129%
3	3.934	125	127	138	rBV	38974	71284	1.50%	0.176%
4	4.164	161	166	171	rBV4	4059	7188	0.15%	0.018%
5	4.264	179	183	190	rVB	24512	33938	0.72%	0.084%
6	4.634	242	246	252	rBV8	3996	8012	0.17%	0.020%
7	6.040	481	485	488	rBV4	4610	6541	0.14%	0.016%
8	7.287	691	697	706	rVB	140108	217553	4.59%	0.538%
9	7.469	721	728	735	rBV	569475	864866	18.24%	2.138%
10	7.675	755	763	772	rBV	507255	792310	16.71%	1.958%
11	8.152	837	844	851	rBV	620694	982824	20.73%	2.429%
12	8.205	851	853	858	rVB4	9128	12787	0.27%	0.032%
13	8.846	955	962	973	rBV	383506	630377	13.30%	1.558%
14	8.981	980	985	992	rVB	11148	17459	0.37%	0.043%
15	9.258	1027	1032	1036	rBV6	3231	5267	0.11%	0.013%
16	9.322	1036	1043	1053	rVV	561636	897191	18.93%	2.218%
17	9.481	1065	1070	1077	rVB7	10158	15711	0.33%	0.039%
18	10.052	1158	1167	1181	rBV	351975	572585	12.08%	1.415%
19	10.587	1250	1258	1269	rBV	686898	1129020	23.82%	2.791%
20	10.875	1303	1307	1313	rBV8	3543	6817	0.14%	0.017%
21	10.981	1317	1325	1333	rBV	844842	1397042	29.47%	3.453%
22	11.110	1339	1347	1356	rBV	311802	514109	10.84%	1.271%
23	11.640	1434	1437	1442	rVB5	5375	7334	0.15%	0.018%
24	11.746	1447	1455	1459	rBV10	5102	9756	0.21%	0.024%
25	12.234	1533	1538	1545	rVB4	8439	14028	0.30%	0.035%
26	12.551	1584	1592	1600	rBV3	16607	25923	0.55%	0.064%
27	13.069	1675	1680	1683	rVB7	4021	5865	0.12%	0.014%
28	13.675	1778	1783	1792	rVB5	13013	27205	0.57%	0.067%
29	13.757	1792	1797	1801	rBV8	3091	5525	0.12%	0.014%
30	14.181	1862	1869	1876	rBV	1505954	2090916	44.11%	5.168%
31	14.434	1906	1912	1913	rBV5	4188	6501	0.14%	0.016%
32	14.481	1913	1920	1929	rVB	1743883	2474591	52.20%	6.117%
33	14.781	1964	1971	1979	rBV	1281983	1947231	41.07%	4.813%
34	14.857	1979	1984	1990	rVB3	17178	25366	0.54%	0.063%
35	14.945	1993	1999	2004	rBV	104507	153940	3.25%	0.381%
36	15.192	2035	2041	2045	rVB9	4309	7239	0.15%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
 Data File : BP014734.D
 Acq On : 19 Apr 2023 17:16
 Operator : CG/JU
 Sample : 02340-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

37	15.451	2080	2085	2092	rVB4	6843	13748	0.29%	0.034%
38	15.775	2133	2140	2147	rBV	2297749	3229395	68.12%	7.982%
39	15.875	2151	2157	2169	rVV	397768	546434	11.53%	1.351%
40	16.016	2177	2181	2187	rVB5	9793	14875	0.31%	0.037%
41	16.134	2196	2201	2206	rBV2	16902	22737	0.48%	0.056%
42	16.563	2270	2274	2279	rVB8	3074	5115	0.11%	0.013%
43	17.122	2364	2369	2372	rBV3	6848	9252	0.20%	0.023%
44	17.534	2432	2439	2449	rBV	1622666	2229564	47.03%	5.511%
45	17.634	2449	2456	2467	rBV	3040033	4043901	85.30%	9.995%
46	18.186	2544	2550	2556	rBV	158754	201694	4.25%	0.499%
47	18.386	2581	2584	2590	rBV3	24177	35952	0.76%	0.089%
48	19.428	2757	2761	2765	rVB3	33955	44217	0.93%	0.109%
49	19.492	2768	2772	2777	rBV2	37862	48865	1.03%	0.121%
50	19.616	2789	2793	2798	rBV4	25288	37799	0.80%	0.093%
51	19.845	2826	2832	2844	rBV	3510933	4740702	100.00%	11.718%
52	21.610	3126	3132	3139	rBV	1677581	2342338	49.41%	5.790%
53	24.021	3534	3542	3551	rBV2	2234719	4693907	99.01%	11.602%
54	24.186	3563	3570	3587	rVB2	1169928	2472599	52.16%	6.112%




Sum of corrected areas: 40457268

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014734.D
Acq On : 19 Apr 2023 17:16
Operator : CG/JU
Sample : 02340-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

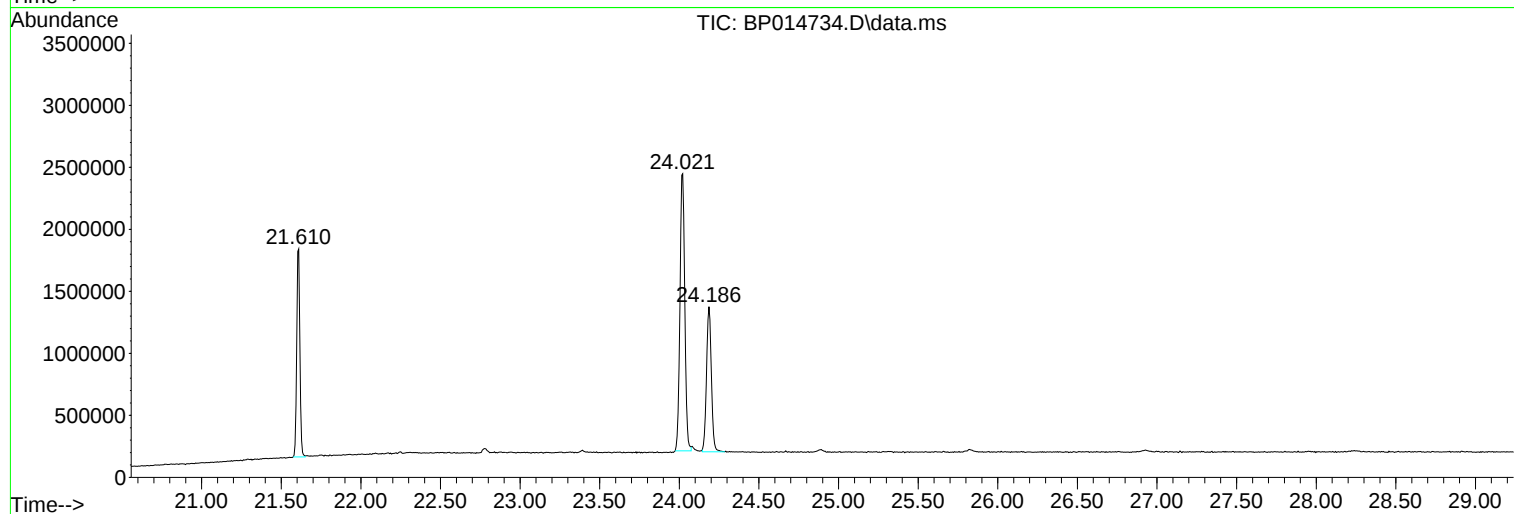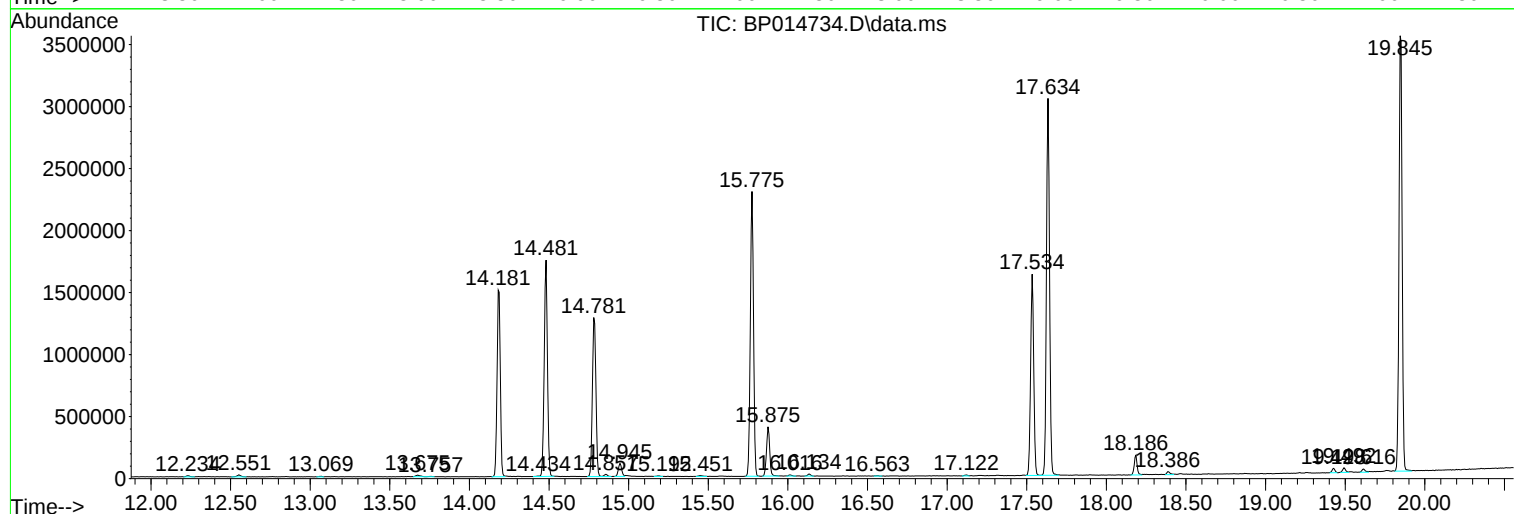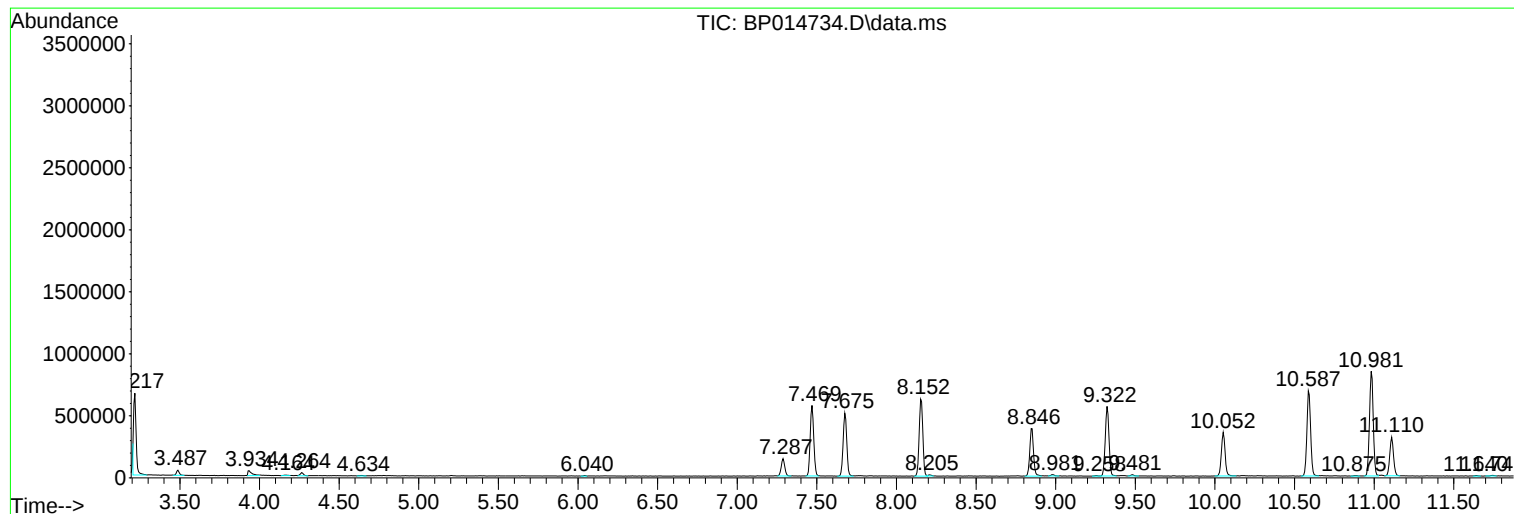

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014734.D
Acq On : 19 Apr 2023 17:16
Operator : CG/JU
Sample : 02340-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE09










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.217	14.00 ng/ul	687803	1,4-Dichlorobenzene-d4	8.158

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	74		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23		
5	Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9		

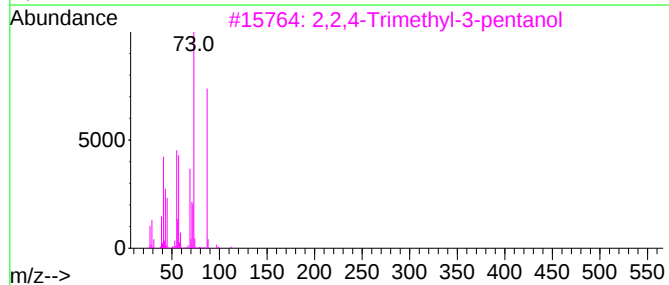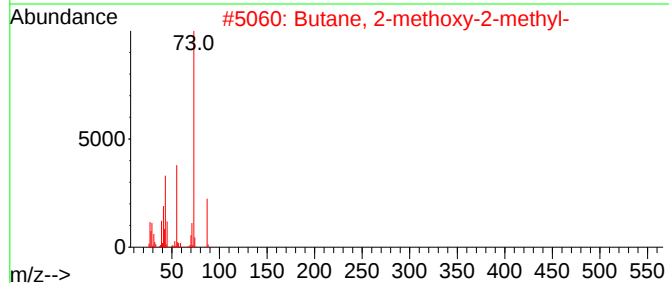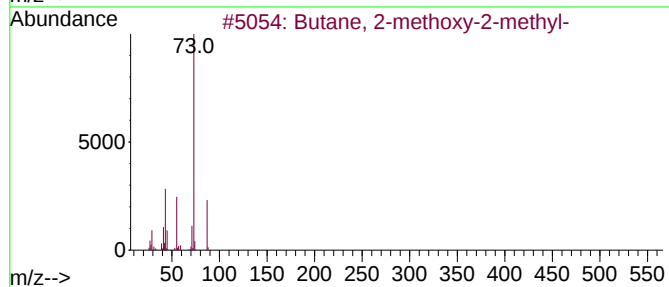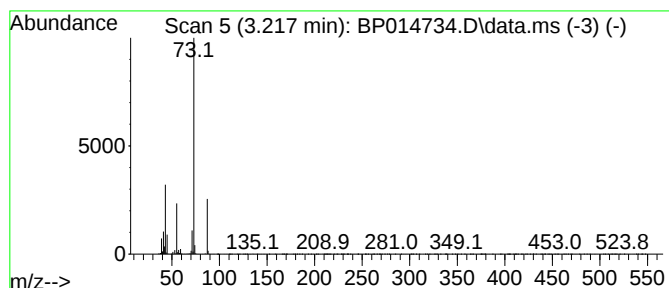

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014734.D
Acq On : 19 Apr 2023 17:16
Operator : CG/JU
Sample : 02340-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.217	14.0	ng/u1	687803	1	8.158	982824	20.0