

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
 Data File : BP014738.D
 Acq On : 19 Apr 2023 20:04
 Operator : CG/JU
 Sample : PB152205BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK205

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	3	5	15	rVB	70723	89313	1.16%	0.121%
2	3.487	47	51	60	rVB	83123	109962	1.43%	0.149%
3	3.922	123	125	139	rBV	120720	174247	2.26%	0.237%
4	4.264	179	183	192	rVB	20610	29811	0.39%	0.040%
5	4.487	216	221	225	rVB8	4384	7774	0.10%	0.011%
6	5.369	367	371	376	rBV6	4668	8604	0.11%	0.012%
7	7.287	688	697	706	rBV	1218337	1864633	24.18%	2.533%
8	7.469	721	728	738	rVB	1045591	1611202	20.89%	2.188%
9	7.675	755	763	771	rBV	1225075	1915298	24.84%	2.601%
10	8.152	837	844	852	rBV	1111547	1736469	22.52%	2.359%
11	8.852	953	963	972	rBV	1488327	2411262	31.27%	3.275%
12	9.322	1035	1043	1057	rBV	1122324	1792144	23.24%	2.434%
13	10.052	1159	1167	1179	rBV	819028	1299240	16.85%	1.765%
14	10.587	1249	1258	1265	rBV	1475649	2363566	30.65%	3.210%
15	10.640	1265	1267	1273	rVB6	14069	21720	0.28%	0.030%
16	10.981	1317	1325	1335	rVB	1577216	2567121	33.29%	3.487%
17	11.110	1342	1347	1350	rBV6	5356	8725	0.11%	0.012%
18	12.481	1573	1580	1586	rBV	11394	19209	0.25%	0.026%
19	12.551	1586	1592	1598	rVV2	30054	46689	0.61%	0.063%
20	14.181	1862	1869	1881	rBV	2859962	4095447	53.11%	5.563%
21	14.481	1912	1920	1932	rBV	3120771	4693027	60.86%	6.374%
22	14.781	1964	1971	1979	rBV	2479036	3614381	46.87%	4.909%
23	14.951	1992	2000	2013	rBV	1249879	1825252	23.67%	2.479%
24	15.775	2132	2140	2147	rBV	4217523	6064263	78.64%	8.237%
25	15.875	2149	2157	2170	rBV	952956	1266713	16.43%	1.721%
26	16.010	2176	2180	2189	rVB4	18411	32372	0.42%	0.044%
27	16.281	2221	2226	2232	rBV	16072	25120	0.33%	0.034%
28	17.316	2398	2402	2406	rBV4	6046	8755	0.11%	0.012%
29	17.533	2432	2439	2447	rBV	3221597	4409499	57.18%	5.989%
30	17.633	2449	2456	2470	rVV	4787854	6593805	85.51%	8.956%
31	18.180	2546	2549	2552	rVB5	6291	8152	0.11%	0.011%
32	18.828	2656	2659	2664	rVB4	11278	14873	0.19%	0.020%
33	19.422	2756	2760	2765	rBV	51771	74727	0.97%	0.101%
34	19.492	2767	2772	2775	rBV	51354	68936	0.89%	0.094%
35	19.845	2826	2832	2842	rBV	5947346	7711570	100.00%	10.474%
36	21.604	3126	3131	3142	rVB	3509843	4526027	58.69%	6.147%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014738.D
Acq On : 19 Apr 2023 20:04
Operator : CG/JU
Sample : PB152205BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK205

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Title : SVOA CALIBRATION

37	24.015	3533	3541	3559	rVB	3131637	6437214	83.47%	8.743%
38	24.186	3561	3570	3586	rVB2	1869660	4077286	52.87%	5.538%




Sum of corrected areas: 73624408

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014738.D
Acq On : 19 Apr 2023 20:04
Operator : CG/JU
Sample : PB152205BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

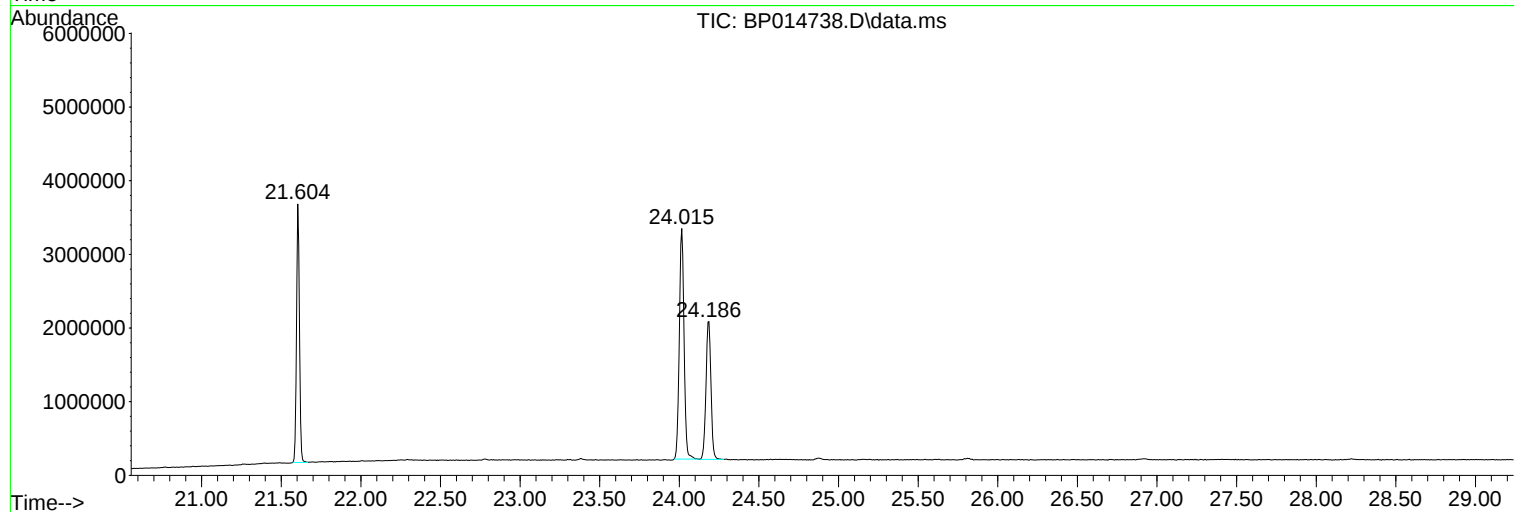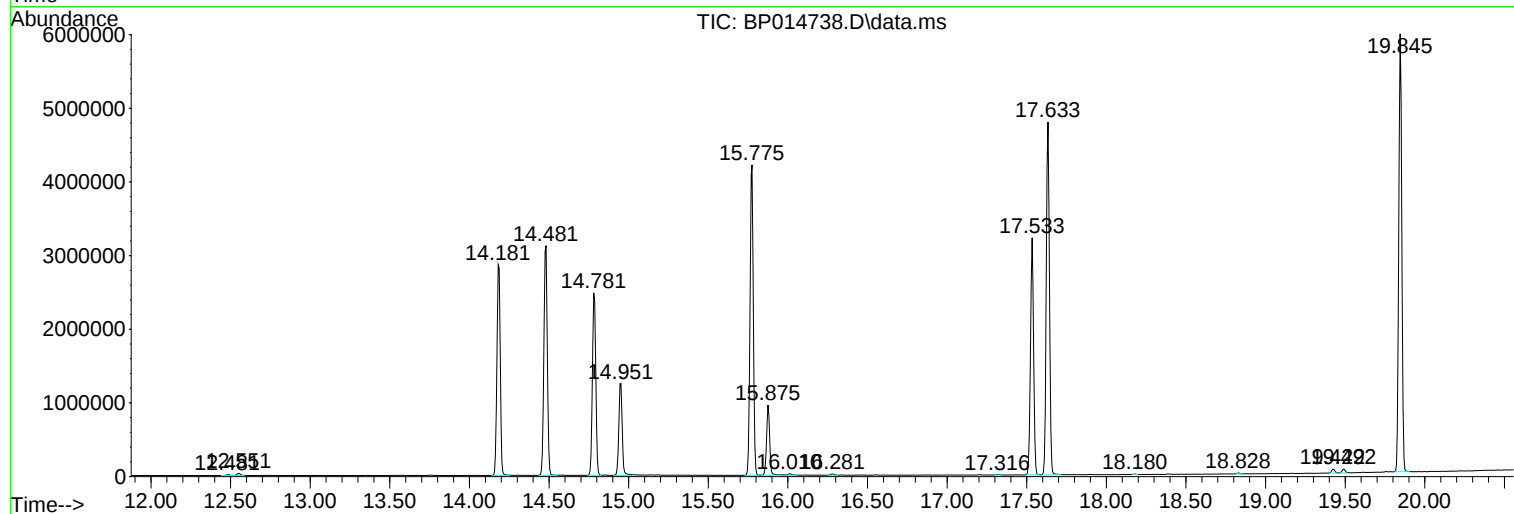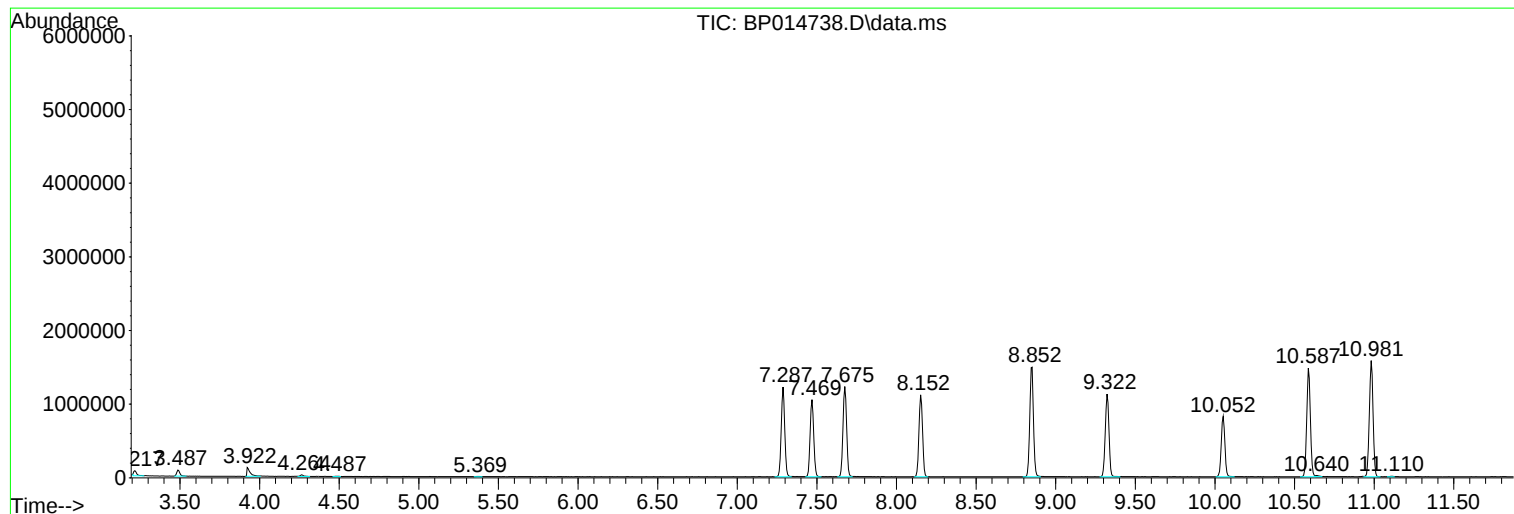

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014738.D
Acq On : 19 Apr 2023 20:04
Operator : CG/JU
Sample : PB152205BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041923\
Data File : BP014738.D
Acq On : 19 Apr 2023 20:04
Operator : CG/JU
Sample : PB152205BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc