

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014752.D
 Acq On : 20 Apr 2023 12:55
 Operator : CG/JU
 Sample : 02122-02DL 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9A2DL

Quant Time: Apr 20 22:38:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 20 02:32:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	222781	20.000	ng/u1	0.00
20) Naphthalene-d8	10.981	136	891062	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	525498	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.533	188	1084661	20.000	ng/u1	0.00
79) Chrysene-d12	21.604	240	984814	20.000	ng/u1	0.00
88) Perylene-d12	24.180	264	1112452	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	1627	0.290	ng/uL	0.00
4) Pyridine-d5	3.934	84	15066	0.987	ng/u1	0.02
7) Phenol-d5	7.287	99	16641	0.864	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.463	67	26587	2.237	ng/u1	0.00
11) 2-Chlorophenol-d4	7.675	132	23946	1.674	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	27164	1.809	ng/u1	0.00
21) Nitrobenzene-d5	9.316	128	11655	2.087	ng/u1	0.00
24) 2-Nitrophenol-d4	10.046	143	8900	1.765	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	26240	1.916	ng/u1	0.00
31) 4-Chloroaniline-d4	11.104	131	42107	2.015	ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	114482	2.751	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	118959	2.467	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	1879	0.284	ng/u1	0.00
60) Fluorene-d10	15.769	176	99005	2.773	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	3472	0.791	ng/u1	-0.01
73) Anthracene-d10	17.628	188	145265	2.772	ng/u1	0.00
81) Pyrene-d10	19.845	212	164499	2.916	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	149966	2.601	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.522	88	135284	22.347	ng/uL 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014752.D
Acq On : 20 Apr 2023 12:55
Operator : CG/JU
Sample : 02122-02DL 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A2DL

Quant Time: Apr 20 22:38:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 20 02:32:50 2023
Response via : Initial Calibration

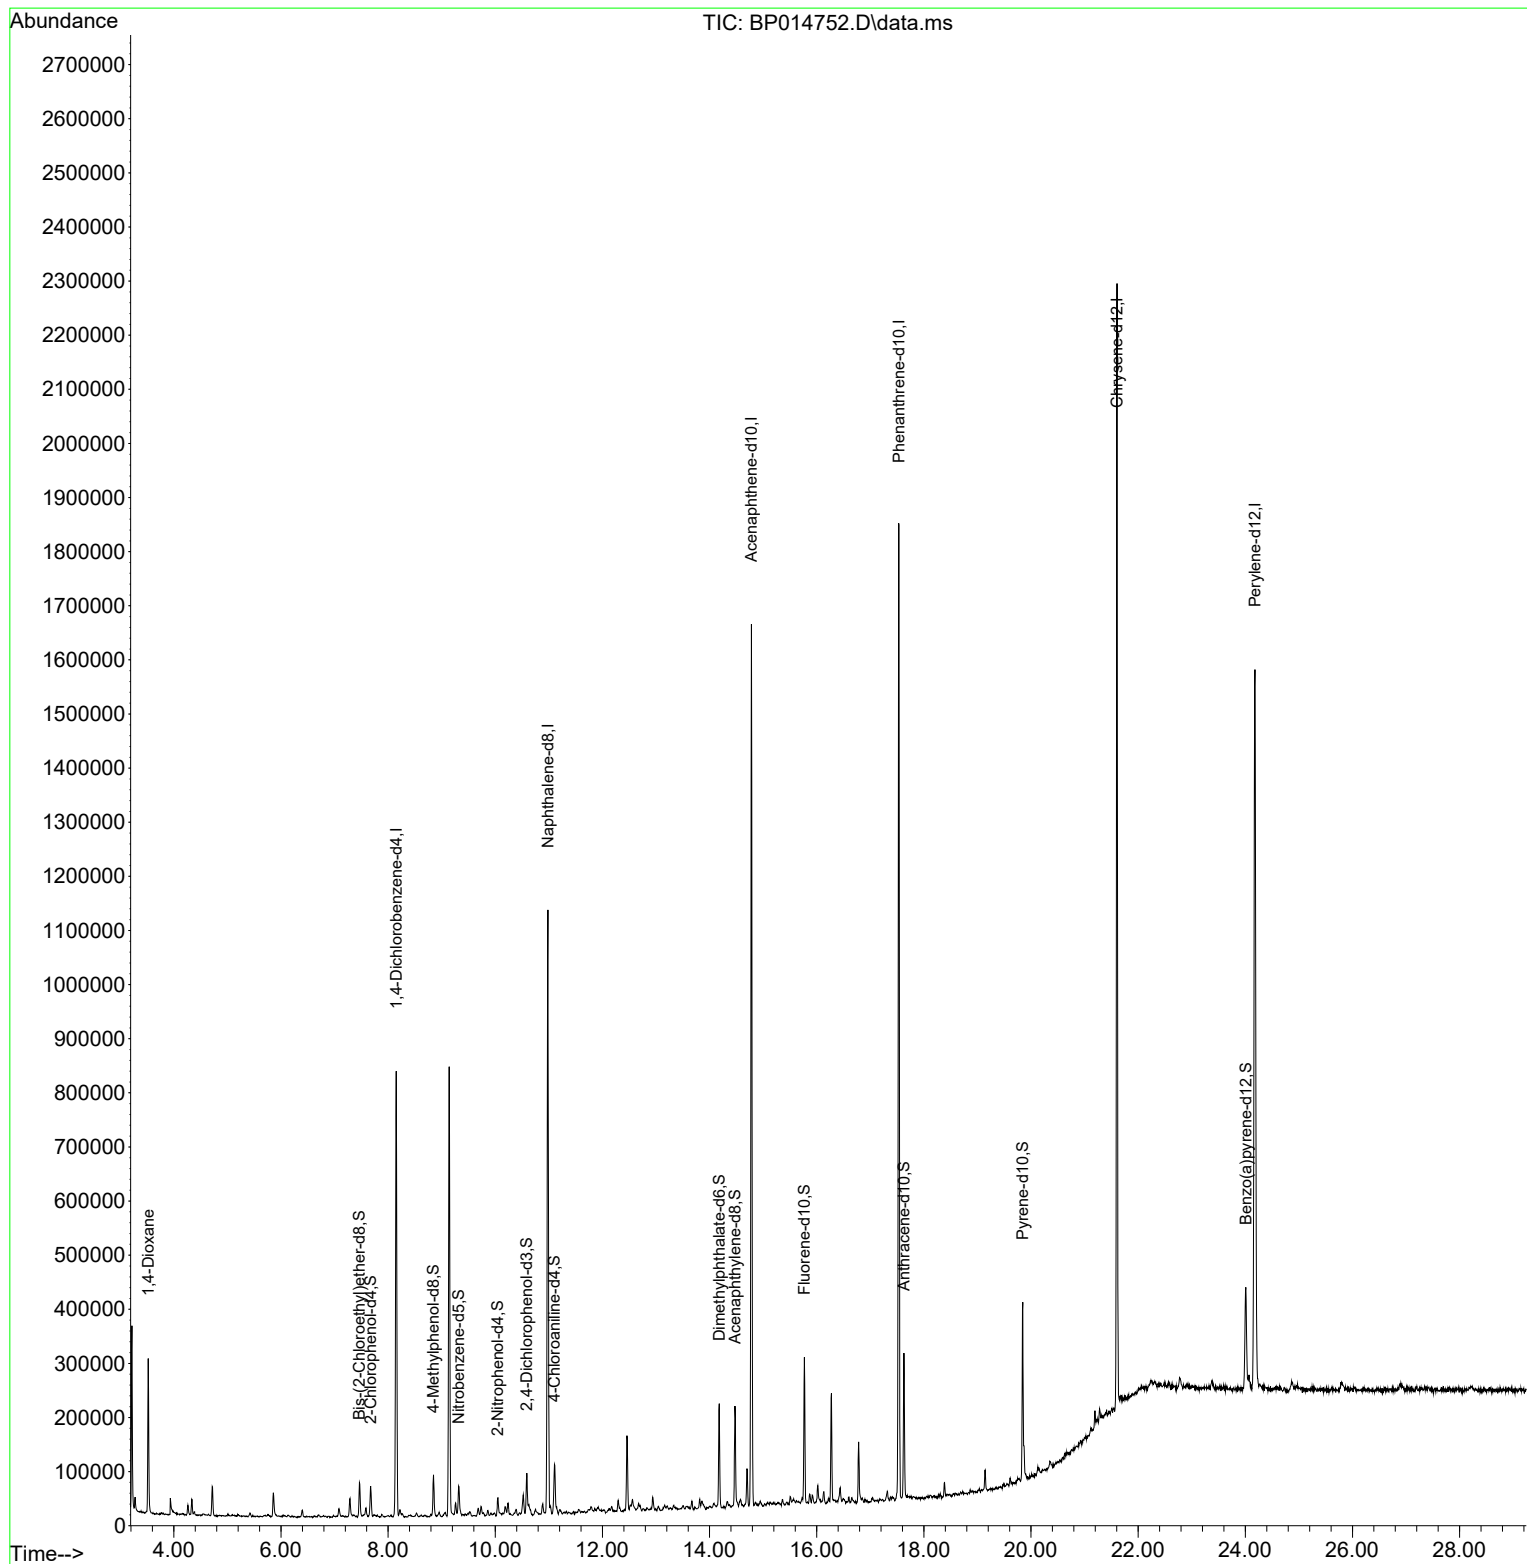

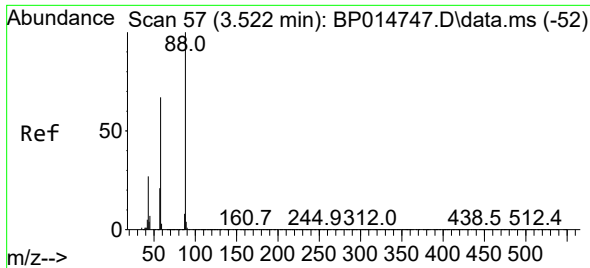

#2
 1,4-Dioxane
 Concen: 22.347 ng/uL
 RT: 3.522 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BP014752.D
 Acq: 20 Apr 2023 12:55

Instrument :
 BNA_P
 ClientSampleId :
 CB9A2DL

Tgt Ion: 88 Resp: 135284
 Ion Ratio Lower Upper
 88 100
 43 27.2 25.0 37.6
 58 73.7 54.9 82.3

