

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014753.D
 Acq On : 20 Apr 2023 13:29
 Operator : CG/JU
 Sample : 02122-04DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9A6DL

Quant Time: Apr 20 22:38:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 20 02:32:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	227264	20.000	ng/u1	0.00
20) Naphthalene-d8	10.981	136	913828	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	548183	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.534	188	1134125	20.000	ng/u1	0.00
79) Chrysene-d12	21.604	240	1032627	20.000	ng/u1	0.00
88) Perylene-d12	24.180	264	1174926	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	1209	0.211	ng/uL	0.00
4) Pyridine-d5	3.934	84	13927	0.895	ng/u1	0.02
7) Phenol-d5	7.287	99	12260	0.624	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.463	67	23088	1.905	ng/u1	0.00
11) 2-Chlorophenol-d4	7.675	132	20118	1.379	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	20442	1.334	ng/u1	0.00
21) Nitrobenzene-d5	9.322	128	10161	1.774	ng/u1	0.00
24) 2-Nitrophenol-d4	10.052	143	7687	1.486	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	22051	1.570	ng/u1	0.00
31) 4-Chloroaniline-d4	11.110	131	35001	1.633	ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	93872	2.163	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	94646	1.882	ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	1565	0.227	ng/u1	0.00
60) Fluorene-d10	15.769	176	77874	2.091	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	2806	0.611	ng/u1	0.00
73) Anthracene-d10	17.628	188	116968	2.135	ng/u1	0.00
81) Pyrene-d10	19.845	212	130892	2.213	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	118452	1.945	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.523	88	109038	17.656	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014753.D
Acq On : 20 Apr 2023 13:29
Operator : CG/JU
Sample : 02122-04DL 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A6DL

Quant Time: Apr 20 22:38:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 20 02:32:50 2023
Response via : Initial Calibration

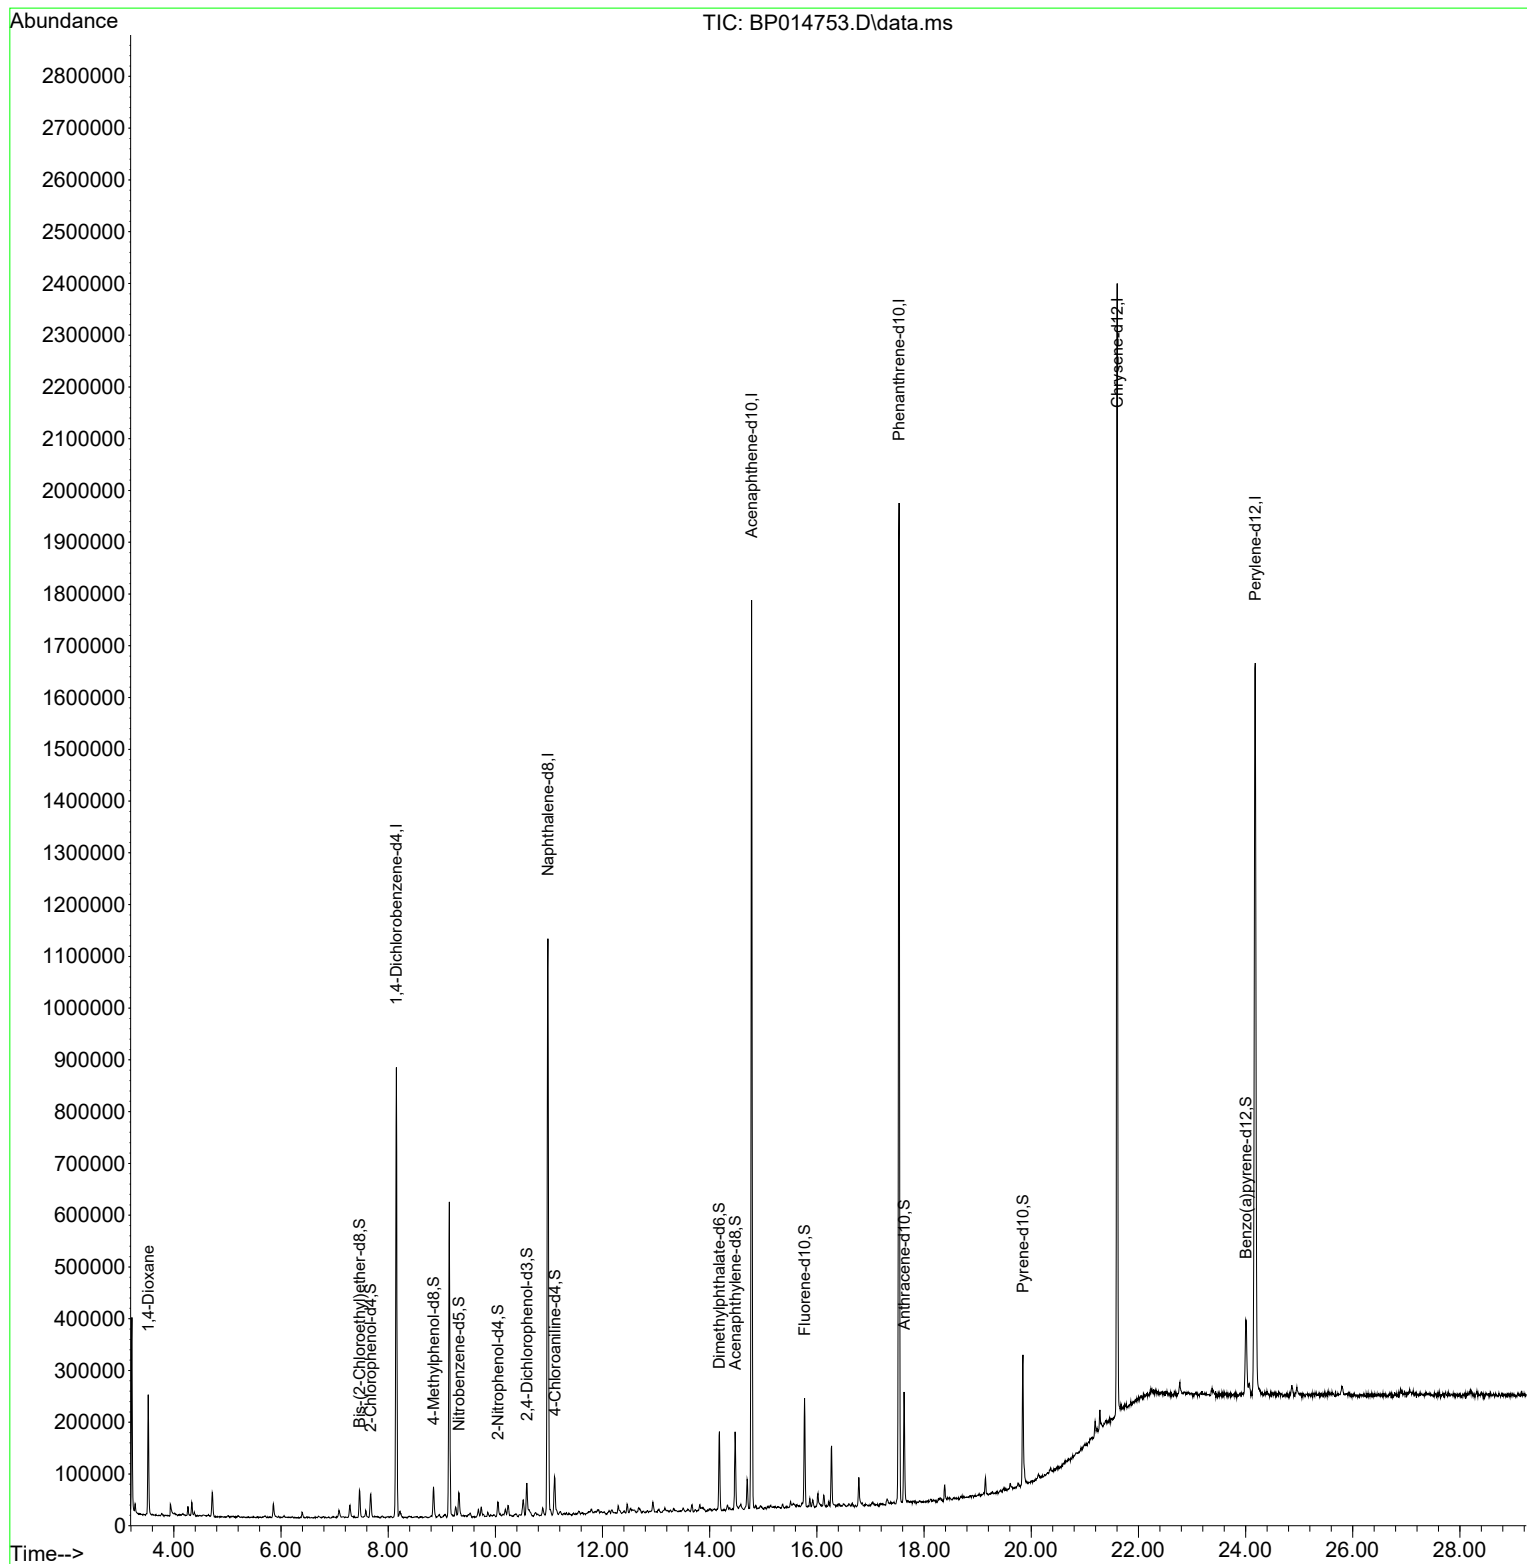

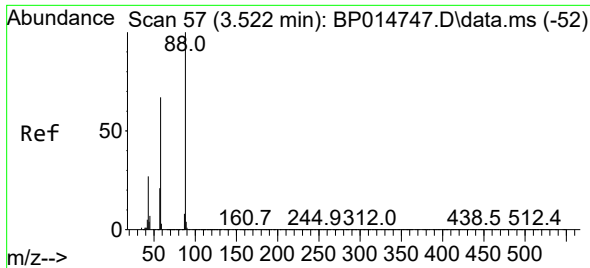

#2
 1,4-Dioxane
 Concen: 17.656 ng/uL
 RT: 3.523 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BP014753.D
 Acq: 20 Apr 2023 13:29

Instrument :
 BNA_P
 ClientSampleId :
 CB9A6DL

Tgt Ion: 88 Resp: 109038
 Ion Ratio Lower Upper
 88 100
 43 28.2 25.0 37.6
 58 66.7 54.9 82.3

