

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014765.D
 Acq On : 20 Apr 2023 20:12
 Operator : CG/JU
 Sample : 02378-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMK3

Quant Time: Apr 20 23:37:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 20 02:32:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	275504	20.000	ng/u1	0.00
20) Naphthalene-d8	10.975	136	1149460	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	694266	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.528	188	1339671	20.000	ng/u1	0.00
79) Chrysene-d12	21.598	240	1048662	20.000	ng/u1	0.00
88) Perylene-d12	24.174	264	1161268	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	28279	4.080	ng/uL	0.00
4) Pyridine-d5	3.922	84	72054	3.818	ng/u1	0.00
7) Phenol-d5	7.287	99	165131	6.932	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.463	67	452454	30.789	ng/u1	0.00
11) 2-Chlorophenol-d4	7.675	132	460140	26.011	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	271587	14.625	ng/u1	0.00
21) Nitrobenzene-d5	9.322	128	272347	37.812	ng/u1	0.00
24) 2-Nitrophenol-d4	10.046	143	271948	41.803	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	525535	29.752	ng/u1	0.00
31) 4-Chloroaniline-d4	11.104	131	172979	6.416	ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	1845773	33.576	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	2105340	33.047	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	43539	4.979	ng/u1	0.00
60) Fluorene-d10	15.769	176	1580406	33.504	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	169419	31.250	ng/u1	0.00
73) Anthracene-d10	17.628	188	2252305	34.802	ng/u1	0.00
81) Pyrene-d10	19.845	212	2448376	40.757	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.004	264	2200038	36.553	ng/u1	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.523	88	9311	1.244	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014765.D
Acq On : 20 Apr 2023 20:12
Operator : CG/JU
Sample : 02378-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMK3


Quant Time: Apr 20 23:37:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 20 02:32:50 2023
Response via : Initial Calibration

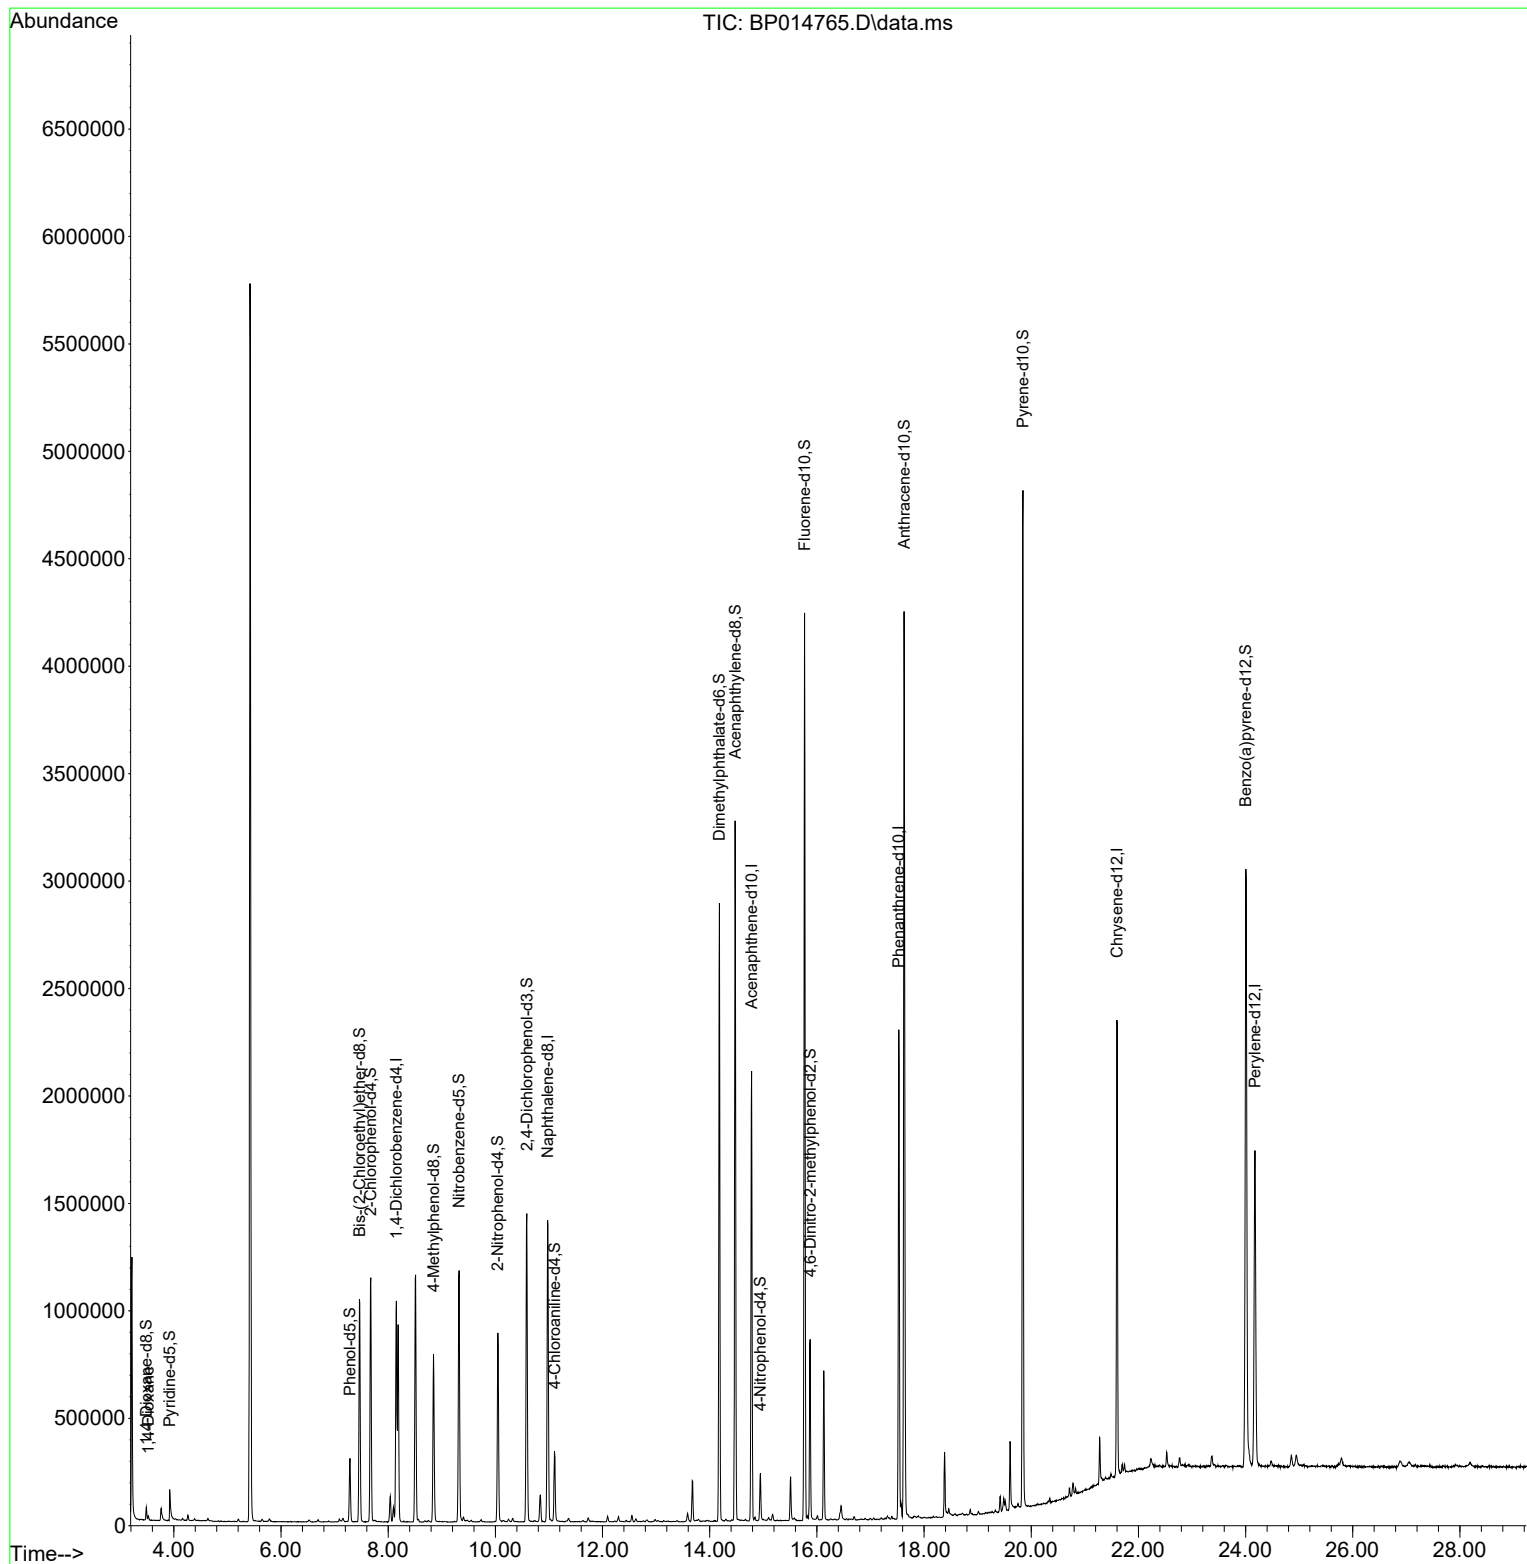

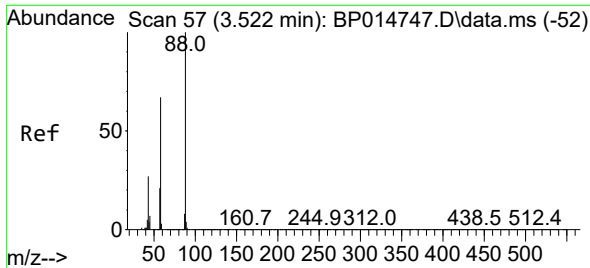

#2
 1,4-Dioxane
 Concen: 1.244 ng/uL
 RT: 3.523 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BP014765.D
 Acq: 20 Apr 2023 20:12

Instrument :
 BNA_P
 ClientSampleId :
 COMK3

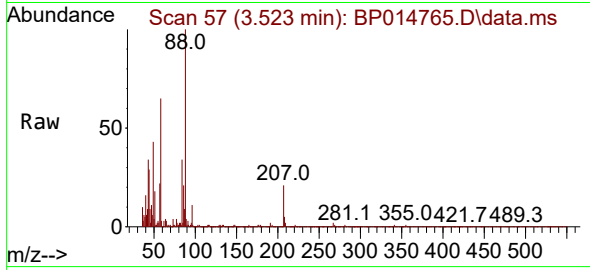

Tgt Ion:	88	Resp:	9311
Ion	Ratio	Lower	Upper
88	100		
43	34.2	25.0	37.6
58	65.5	54.9	82.3

