

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014786.D
 Acq On : 21 Apr 2023 12:23
 Operator : CG/JU
 Sample : 02340-20DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE21DL

Quant Time: Apr 21 22:34:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 20 02:32:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	263781	20.000	ng/u1	0.00
20) Naphthalene-d8	10.981	136	1070761	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	640873	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.528	188	1294059	20.000	ng/u1	0.00
79) Chrysene-d12	21.598	240	1026835	20.000	ng/u1	0.00
88) Perylene-d12	24.169	264	1117392	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	9371	1.412	ng/uL	0.00
4) Pyridine-d5	3.934	84	16746	0.927	ng/u1	0.02
7) Phenol-d5	7.287	99	36931	1.619	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.464	67	109974	7.816	ng/u1	0.00
11) 2-Chlorophenol-d4	7.675	132	99438	5.871	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	67668	3.806	ng/u1	0.00
21) Nitrobenzene-d5	9.316	128	54681	8.150	ng/u1	0.00
24) 2-Nitrophenol-d4	10.046	143	47058	7.765	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	108223	6.577	ng/u1	0.00
31) 4-Chloroaniline-d4	11.105	131	92290	3.675	ng/u1	0.00
46) Dimethylphthalate-d6	14.175	166	424912	8.373	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	450543	7.661	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	7459	0.924	ng/u1	0.00
60) Fluorene-d10	15.769	176	364754	8.377	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	24110	4.604	ng/u1	-0.01
73) Anthracene-d10	17.628	188	548926	8.781	ng/u1	0.00
81) Pyrene-d10	19.839	212	599898	10.199	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.004	264	530975	9.168	ng/u1	-0.01


Target Compounds					Qvalue
2) 1,4-Dioxane	3.523	88	109793	15.317 ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014786.D
Acq On : 21 Apr 2023 12:23
Operator : CG/JU
Sample : 02340-20DL 5X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE21DL


Quant Time: Apr 21 22:34:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 20 02:32:50 2023
Response via : Initial Calibration

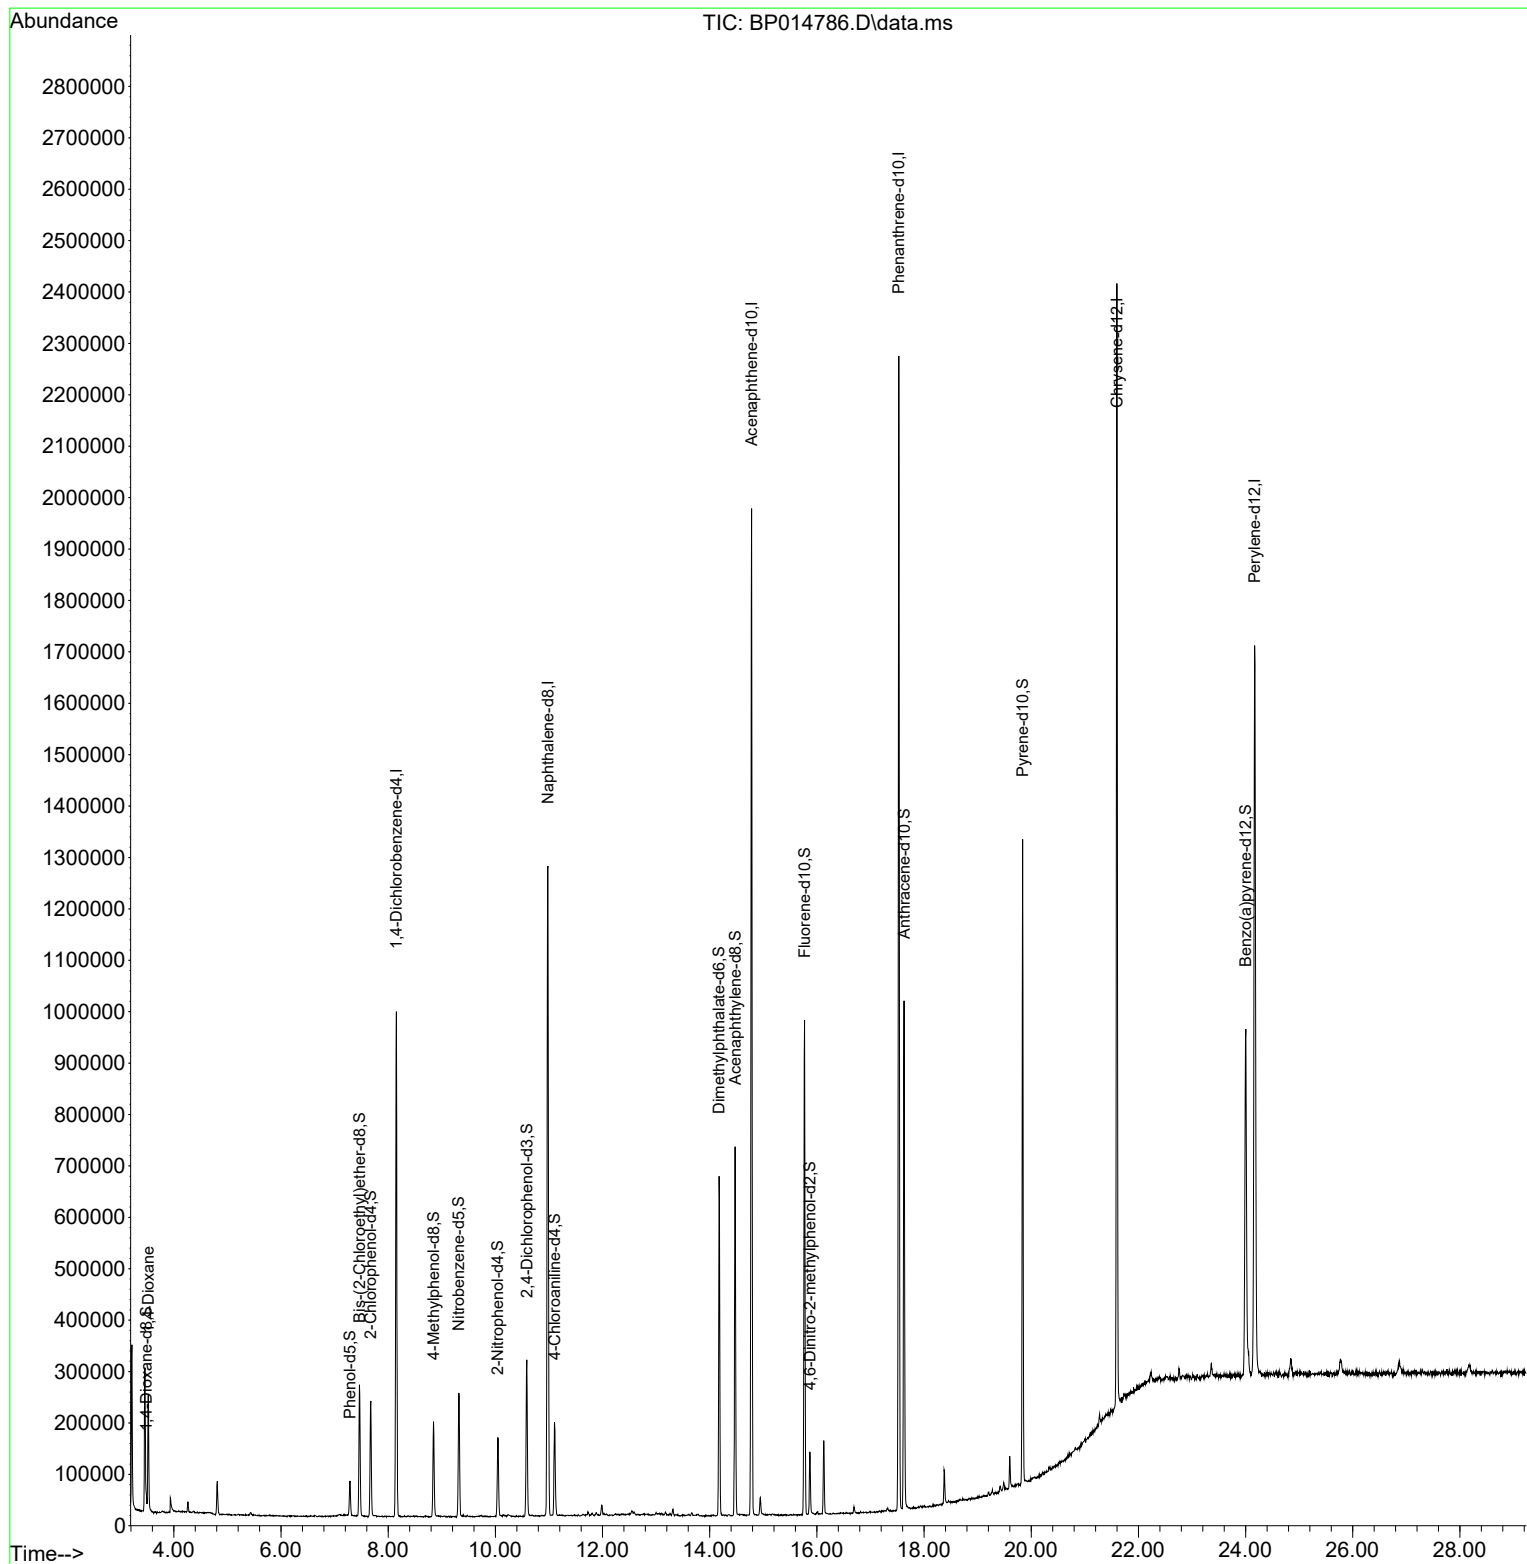

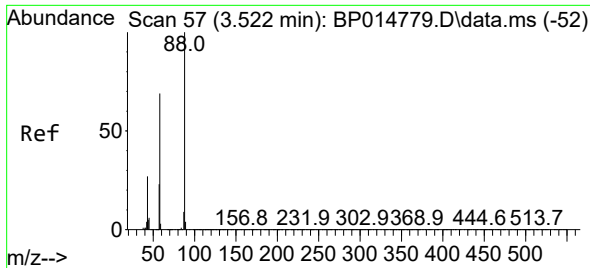

#2
 1,4-Dioxane
 Concen: 15.317 ng/uL
 RT: 3.523 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BP014786.D
 Acq: 21 Apr 2023 12:23

Instrument :
 BNA_P
 ClientSampleId :
 BHE21DL

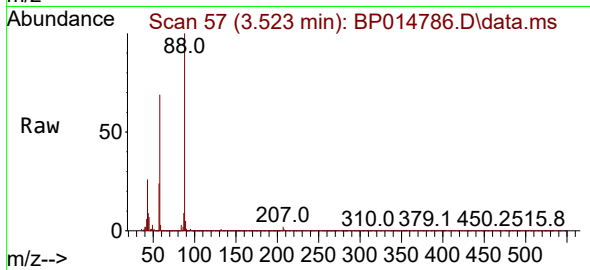

Tgt Ion: 88 Resp: 109793

Ion	Ratio	Lower	Upper
88	100		
43	26.2	25.0	37.6
58	69.2	54.9	82.3

