

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014774.D
 Acq On : 21 Apr 2023 01:12
 Operator : CG/JU
 Sample : 02340-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE20

Quant Time: Apr 21 02:54:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 20 02:32:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	274685	20.000	ng/u1	0.00
20) Naphthalene-d8	10.975	136	1157355	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	712043	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.528	188	1426557	20.000	ng/u1	0.00
79) Chrysene-d12	21.598	240	1037530	20.000	ng/u1	0.00
88) Perylene-d12	24.168	264	1128928	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	17415	2.520	ng/uL	0.00
4) Pyridine-d5	3.917	84	160640	8.537	ng/u1	0.00
7) Phenol-d5	7.287	99	175802	7.402	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.463	67	518258	35.372	ng/u1	0.00
11) 2-Chlorophenol-d4	7.675	132	504658	28.612	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	332079	17.936	ng/u1	0.00
21) Nitrobenzene-d5	9.322	128	298844	41.207	ng/u1	0.00
24) 2-Nitrophenol-d4	10.046	143	288728	44.080	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	560983	31.542	ng/u1	0.00
31) 4-Chloroaniline-d4	11.104	131	549120	20.229	ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	2030880	36.021	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	2307305	35.313	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	42658	4.757	ng/u1	0.00
60) Fluorene-d10	15.769	176	1721429	35.583	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	176423	30.560	ng/u1	0.00
73) Anthracene-d10	17.628	188	2589714	37.578	ng/u1	0.00
81) Pyrene-d10	19.839	212	2706953	45.545	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.004	264	2348212	40.132	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.522	88	11249	1.507	ng/uL	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014774.D
Acq On : 21 Apr 2023 01:12
Operator : CG/JU
Sample : 02340-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE20

Quant Time: Apr 21 02:54:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 20 02:32:50 2023
Response via : Initial Calibration

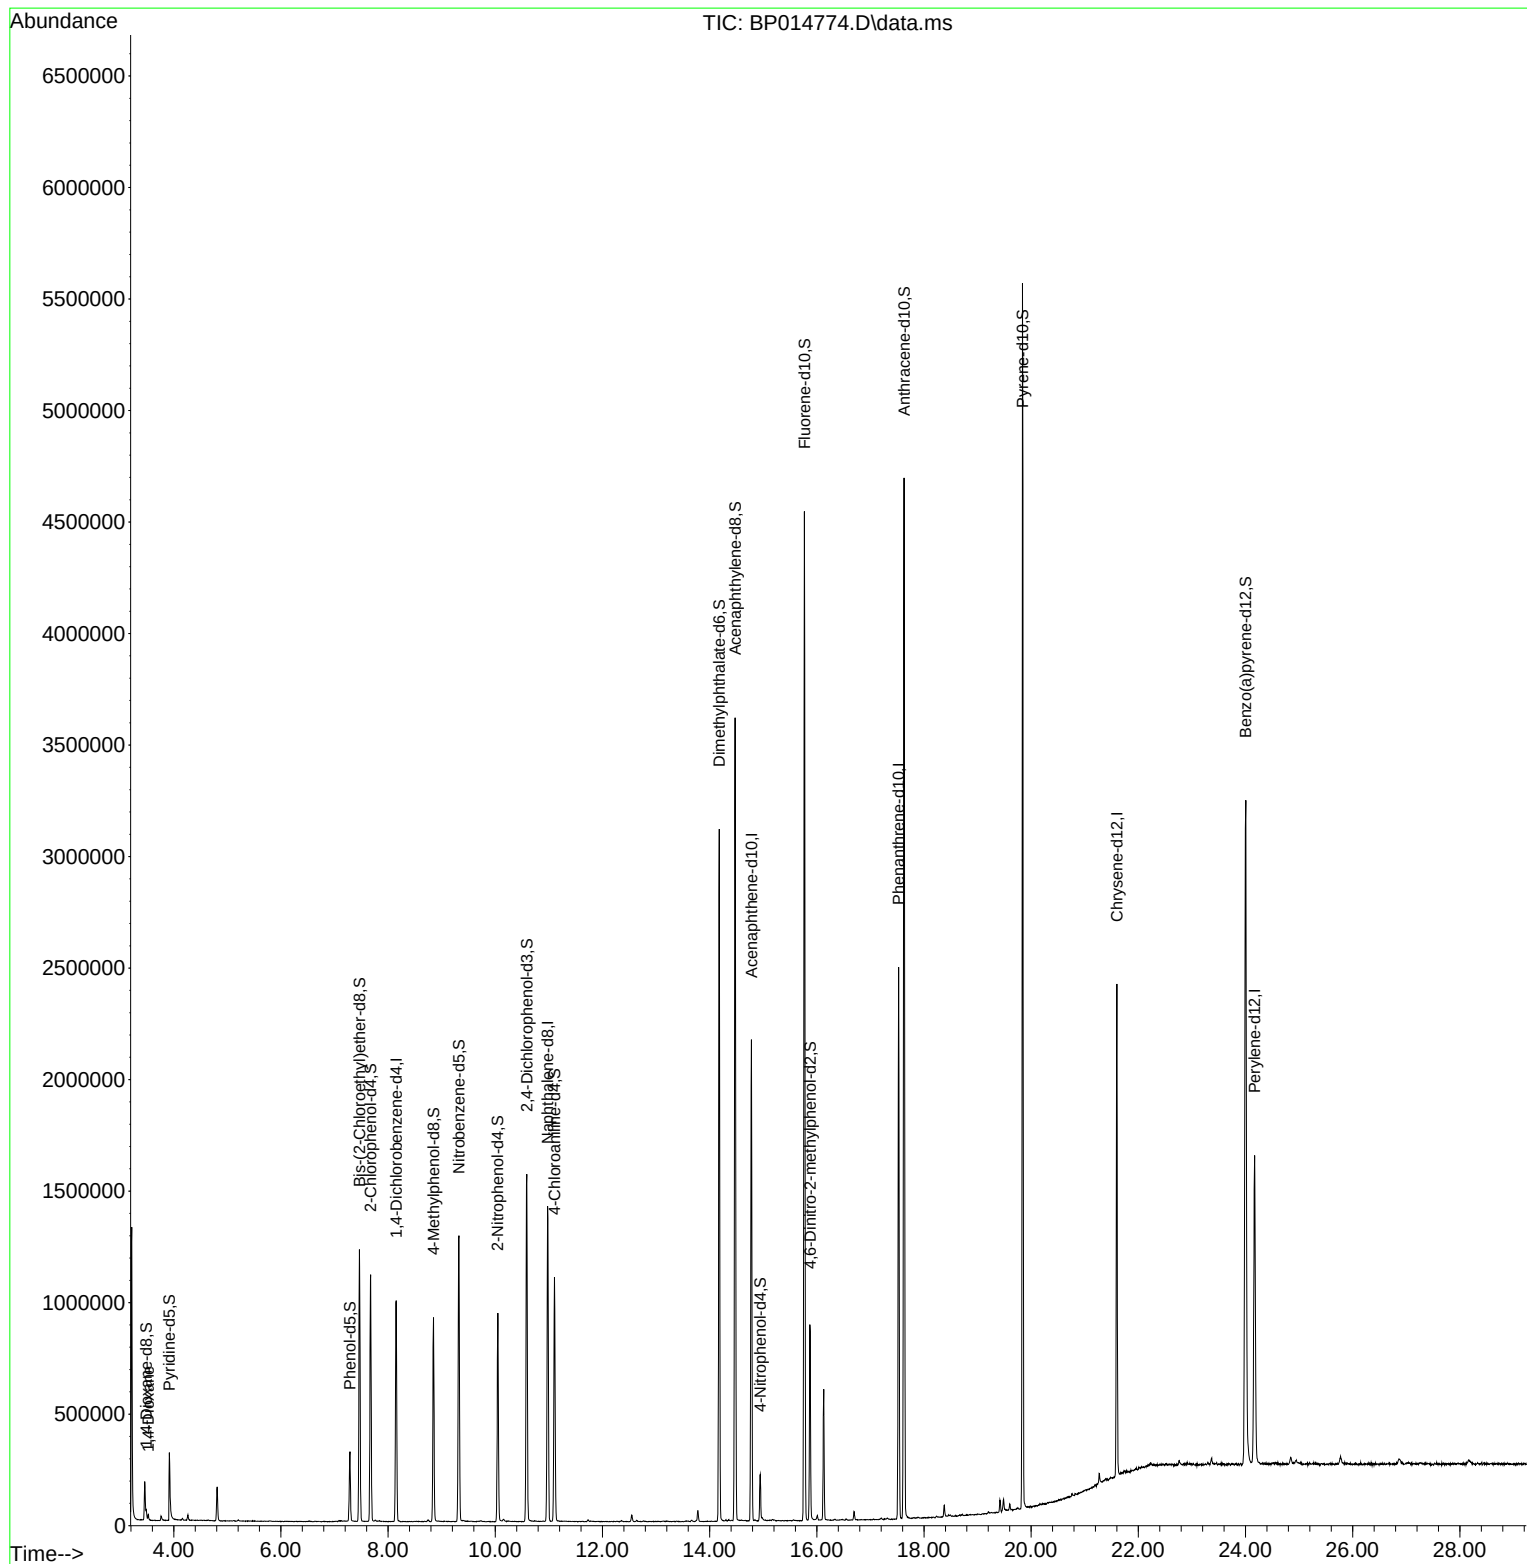

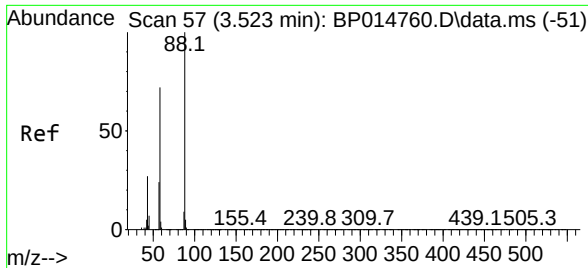

#2
 1,4-Dioxane
 Concen: 1.507 ng/uL
 RT: 3.522 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BP014774.D
 Acq: 21 Apr 2023 01:12

Instrument :
 BNA_P
 ClientSampleId :
 BHE20

Tgt Ion: 88 Resp: 11249
 Ion Ratio Lower Upper
 88 100
 43 29.6 25.0 37.6
 58 76.8 54.9 82.3

