

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014775.D
 Acq On : 21 Apr 2023 01:45
 Operator : CG/JU
 Sample : 02340-20
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE21

Quant Time: Apr 21 02:54:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 20 02:32:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Dichlorobenzene-d4	8.152	152	301779	20.000 ng/u1	0.00
20) Naphthalene-d8	10.975	136	1279005	20.000 ng/u1	0.00
38) Acenaphthene-d10	14.781	164	812574	20.000 ng/u1	0.00
64) Phenanthrene-d10	17.528	188	1700251	20.000 ng/u1	0.00
79) Chrysene-d12	21.598	240	1196466	20.000 ng/u1	0.00
88) Perylene-d12	24.168	264	1184307	20.000 ng/u1	-0.01
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.487	96	41586	5.477 ng/uL	0.00
4) Pyridine-d5	3.916	84	103238	4.994 ng/u1	0.00
7) Phenol-d5	7.287	99	196775	7.542 ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.463	67	528759	32.848 ng/u1	0.00
11) 2-Chlorophenol-d4	7.669	132	535020	27.610 ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	373271	18.351 ng/u1	0.00
21) Nitrobenzene-d5	9.322	128	318402	39.728 ng/u1	0.00
24) 2-Nitrophenol-d4	10.046	143	314028	43.382 ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	627748	31.939 ng/u1	0.00
31) 4-Chloroaniline-d4	11.104	131	493718	16.458 ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	2354789	36.599 ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	2621798	35.162 ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	60343	5.896 ng/u1	0.00
60) Fluorene-d10	15.769	176	2003578	36.291 ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	231985	33.716 ng/u1	0.00
73) Anthracene-d10	17.628	188	3179378	38.708 ng/u1	0.00
81) Pyrene-d10	19.839	212	3333872	48.642 ng/u1	0.00
92) Benzo(a)pyrene-d12	24.004	264	2564465	41.779 ng/u1	-0.01
Target Compounds					
2) 1,4-Dioxane	3.522	88	511061	62.320 ng/uL	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014775.D
Acq On : 21 Apr 2023 01:45
Operator : CG/JU
Sample : 02340-20
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE21


Quant Time: Apr 21 02:54:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 20 02:32:50 2023
Response via : Initial Calibration

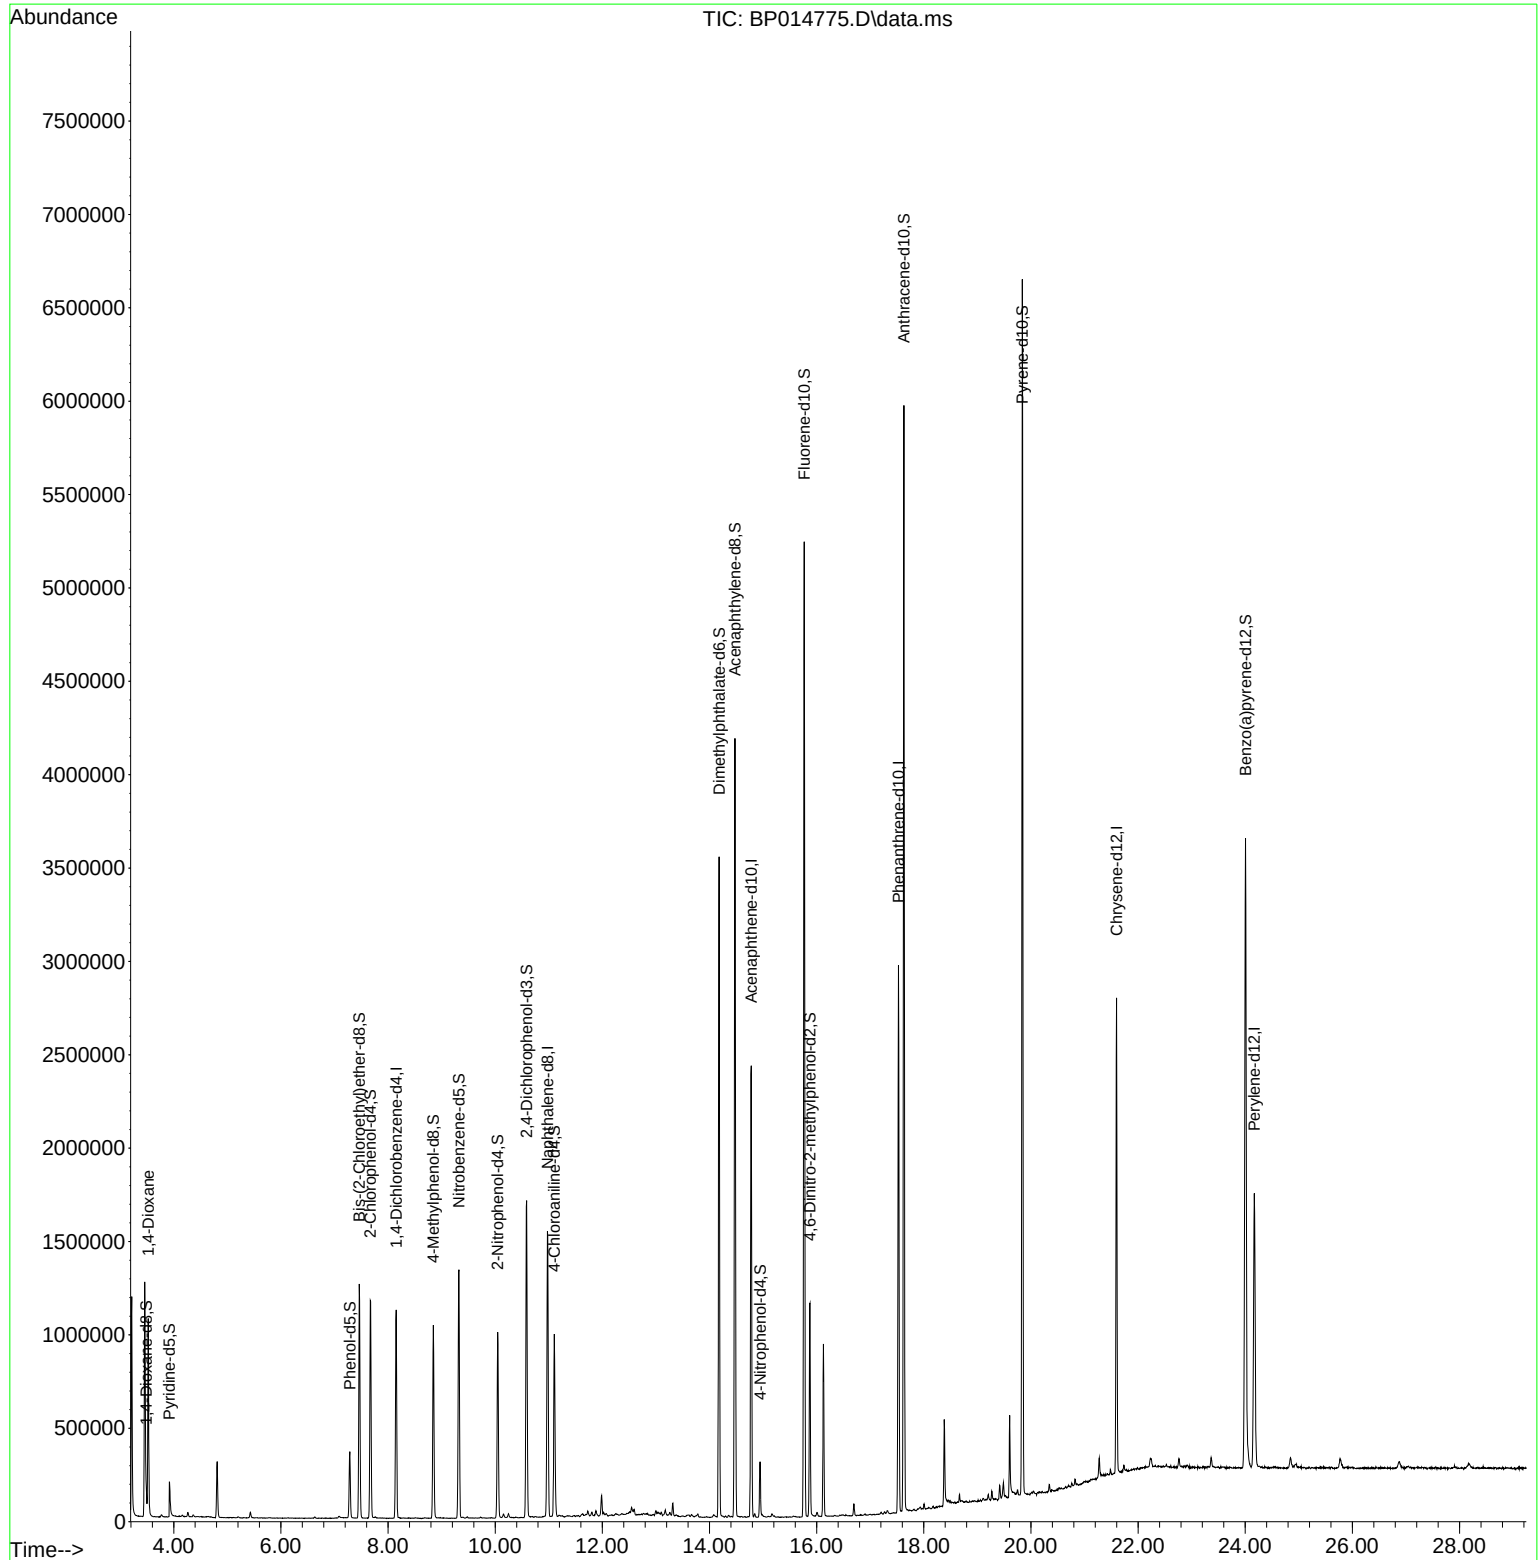

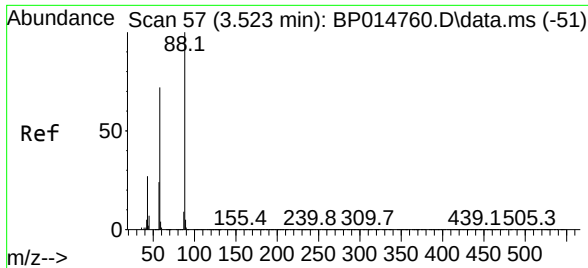

#2
 1,4-Dioxane
 Concen: 62.320 ng/uL
 RT: 3.522 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BP014775.D
 Acq: 21 Apr 2023 01:45

Instrument :
 BNA_P
 ClientSampleId :
 BHE21

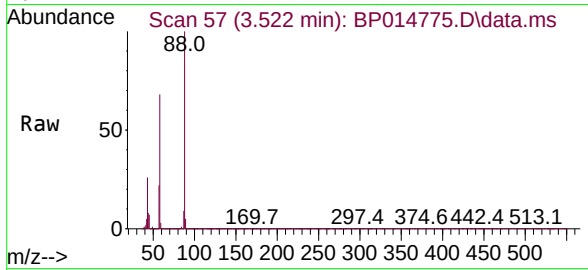

Tgt Ion: 88 Resp: 511061

Ion	Ratio	Lower	Upper
88	100		
43	25.5	25.0	37.6
58	67.7	54.9	82.3

