

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014776.D
 Acq On : 21 Apr 2023 02:19
 Operator : CG/JU
 Sample : 02340-21
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE22

Quant Time: Apr 21 03:30:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 20 02:32:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	255607	20.000	ng/u1	0.00
20) Naphthalene-d8	10.975	136	1032746	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	622078	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.528	188	1365616	20.000	ng/u1	0.00
79) Chrysene-d12	21.598	240	1368468	20.000	ng/u1	0.00
88) Perylene-d12	24.168	264	1540241	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	29168	4.535	ng/uL	0.00
4) Pyridine-d5	3.917	84	143475	8.194	ng/u1	0.00
7) Phenol-d5	7.287	99	156872	7.098	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.463	67	429626	31.511	ng/u1	0.00
11) 2-Chlorophenol-d4	7.669	132	432268	26.337	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	279353	16.214	ng/u1	0.00
21) Nitrobenzene-d5	9.322	128	246313	38.062	ng/u1	0.00
24) 2-Nitrophenol-d4	10.046	143	235341	40.264	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	467093	29.432	ng/u1	0.00
31) 4-Chloroaniline-d4	11.104	131	600703	24.799	ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	1635218	33.198	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	1869488	32.750	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	43976	5.613	ng/u1	0.00
60) Fluorene-d10	15.769	176	1425512	33.728	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	155892	28.208	ng/u1	0.00
73) Anthracene-d10	17.628	188	2390070	36.229	ng/u1	0.00
81) Pyrene-d10	19.839	212	2843005	36.266	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.004	264	3030615	37.964	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.522	88	60666	8.734	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014776.D
Acq On : 21 Apr 2023 02:19
Operator : CG/JU
Sample : 02340-21
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE22

Quant Time: Apr 21 03:30:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 20 02:32:50 2023
Response via : Initial Calibration

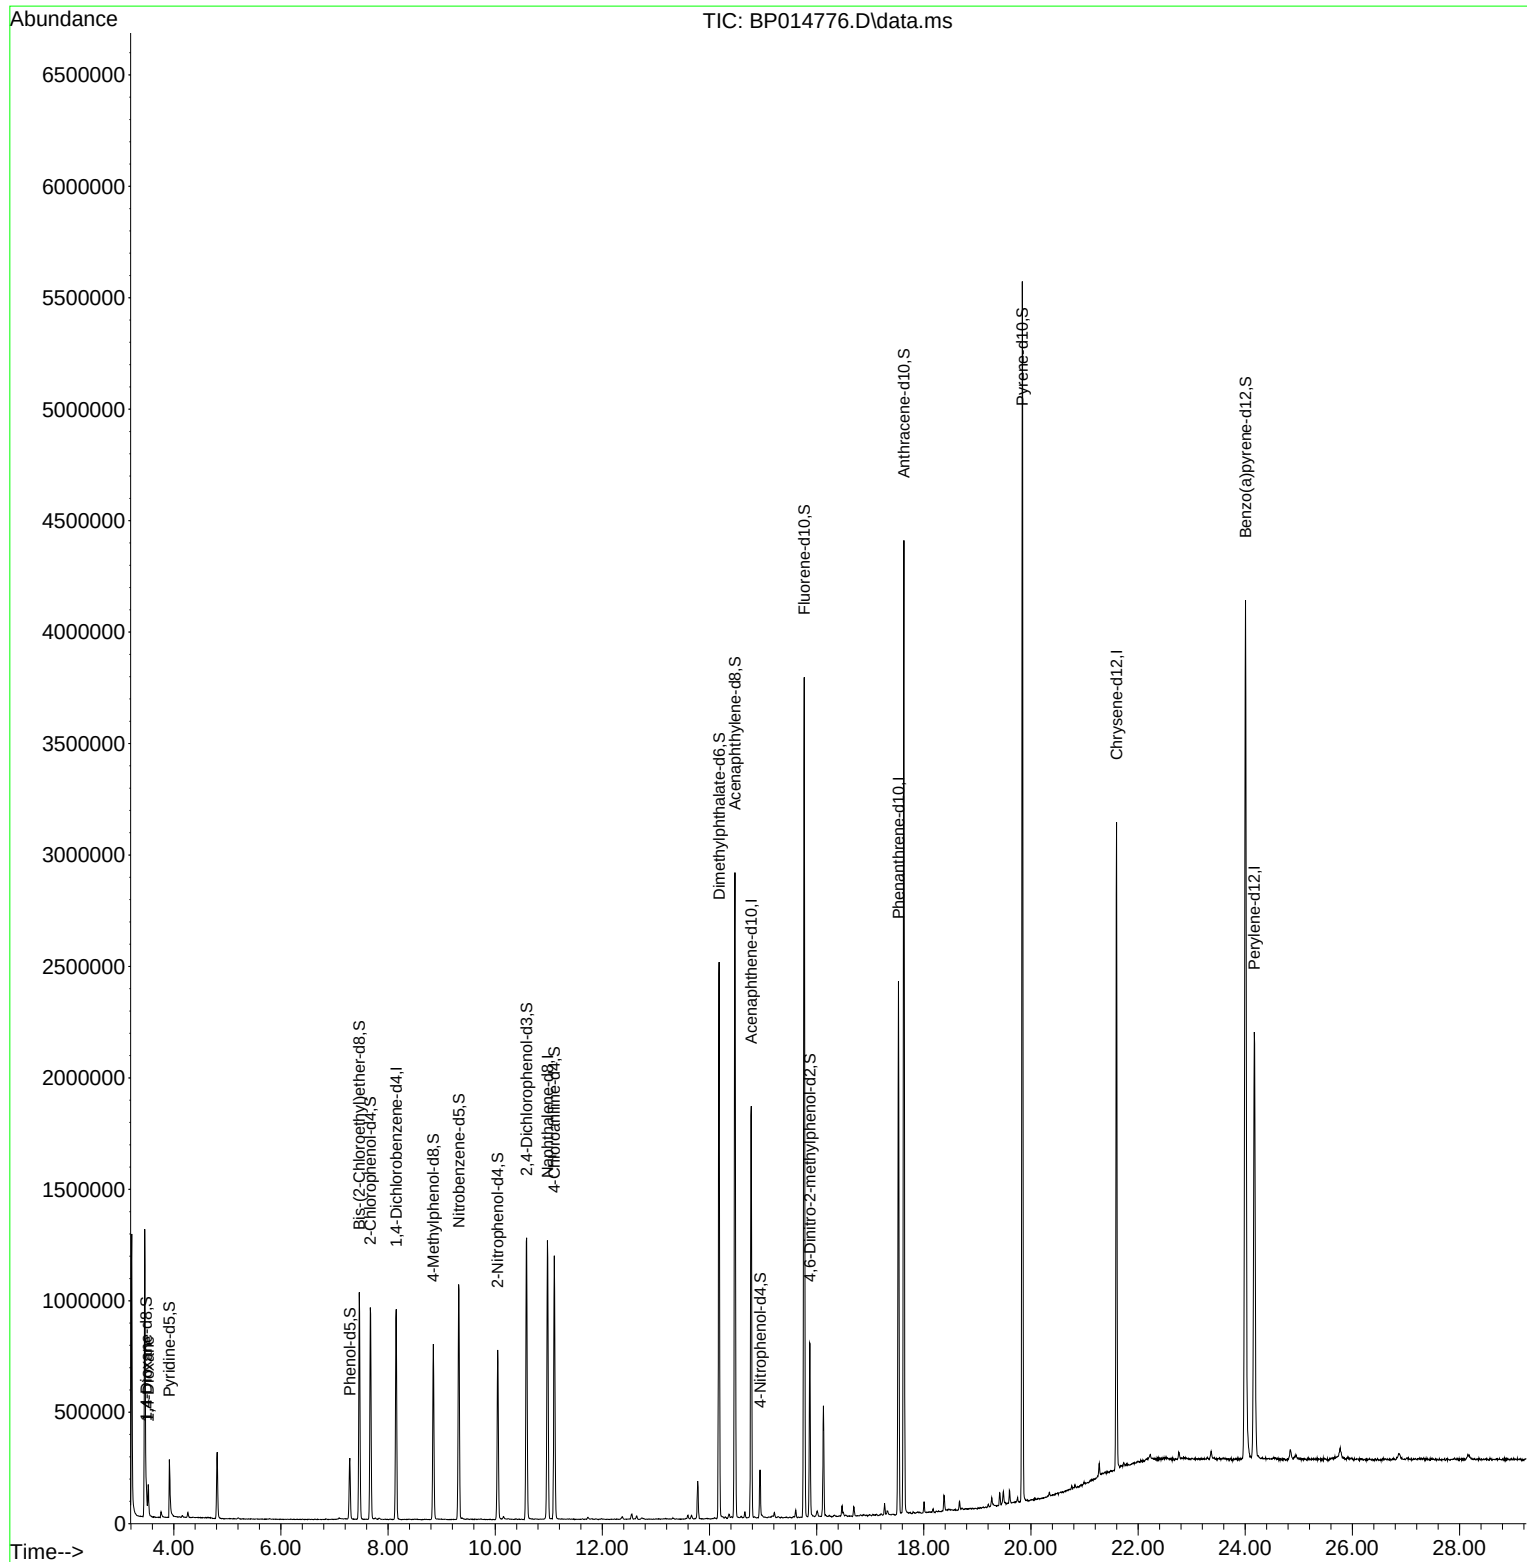

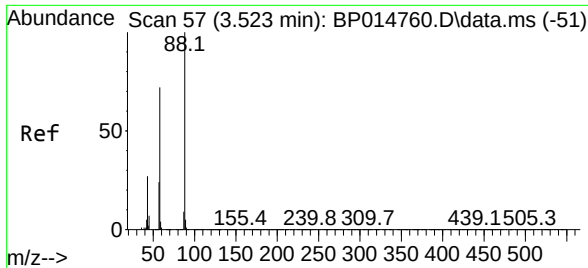

#2
 1,4-Dioxane
 Concen: 8.734 ng/uL
 RT: 3.522 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BP014776.D
 Acq: 21 Apr 2023 02:19

Instrument :
 BNA_P
 ClientSampleId :
 BHE22

Tgt Ion: 88	Resp: 60666
Ion Ratio	Lower Upper
88	100
43	29.6 25.0 37.6
58	72.3 54.9 82.3

