

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014785.D
 Acq On : 21 Apr 2023 11:50
 Operator : CG/JU
 Sample : 02392-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE12

Quant Time: Apr 21 22:33:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 20 02:32:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	278771	20.000	ng/u1	0.00
20) Naphthalene-d8	10.981	136	1173448	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	747050	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.528	188	1620486	20.000	ng/u1	0.00
79) Chrysene-d12	21.598	240	1177076	20.000	ng/u1	0.00
88) Perylene-d12	24.168	264	1041383	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	30651	4.370	ng/uL	0.00
4) Pyridine-d5	3.922	84	123826	6.484	ng/u1	0.00
7) Phenol-d5	7.287	99	160228	6.648	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.463	67	436614	29.363	ng/u1	0.00
11) 2-Chlorophenol-d4	7.675	132	430776	24.065	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	297861	15.852	ng/u1	0.00
21) Nitrobenzene-d5	9.322	128	258870	35.206	ng/u1	0.00
24) 2-Nitrophenol-d4	10.046	143	255219	38.430	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	492064	27.288	ng/u1	0.00
31) 4-Chloroaniline-d4	11.104	131	693102	25.183	ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	1971529	33.330	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	2196503	32.042	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	52260	5.554	ng/u1	0.00
60) Fluorene-d10	15.769	176	1704303	33.578	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	208976	31.867	ng/u1	0.00
73) Anthracene-d10	17.628	188	2883886	36.839	ng/u1	0.00
81) Pyrene-d10	19.839	212	3126273	46.364	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.004	264	2085633	38.641	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.523	88	23159	3.057	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014785.D
Acq On : 21 Apr 2023 11:50
Operator : CG/JU
Sample : 02392-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE12

Quant Time: Apr 21 22:33:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 20 02:32:50 2023
Response via : Initial Calibration

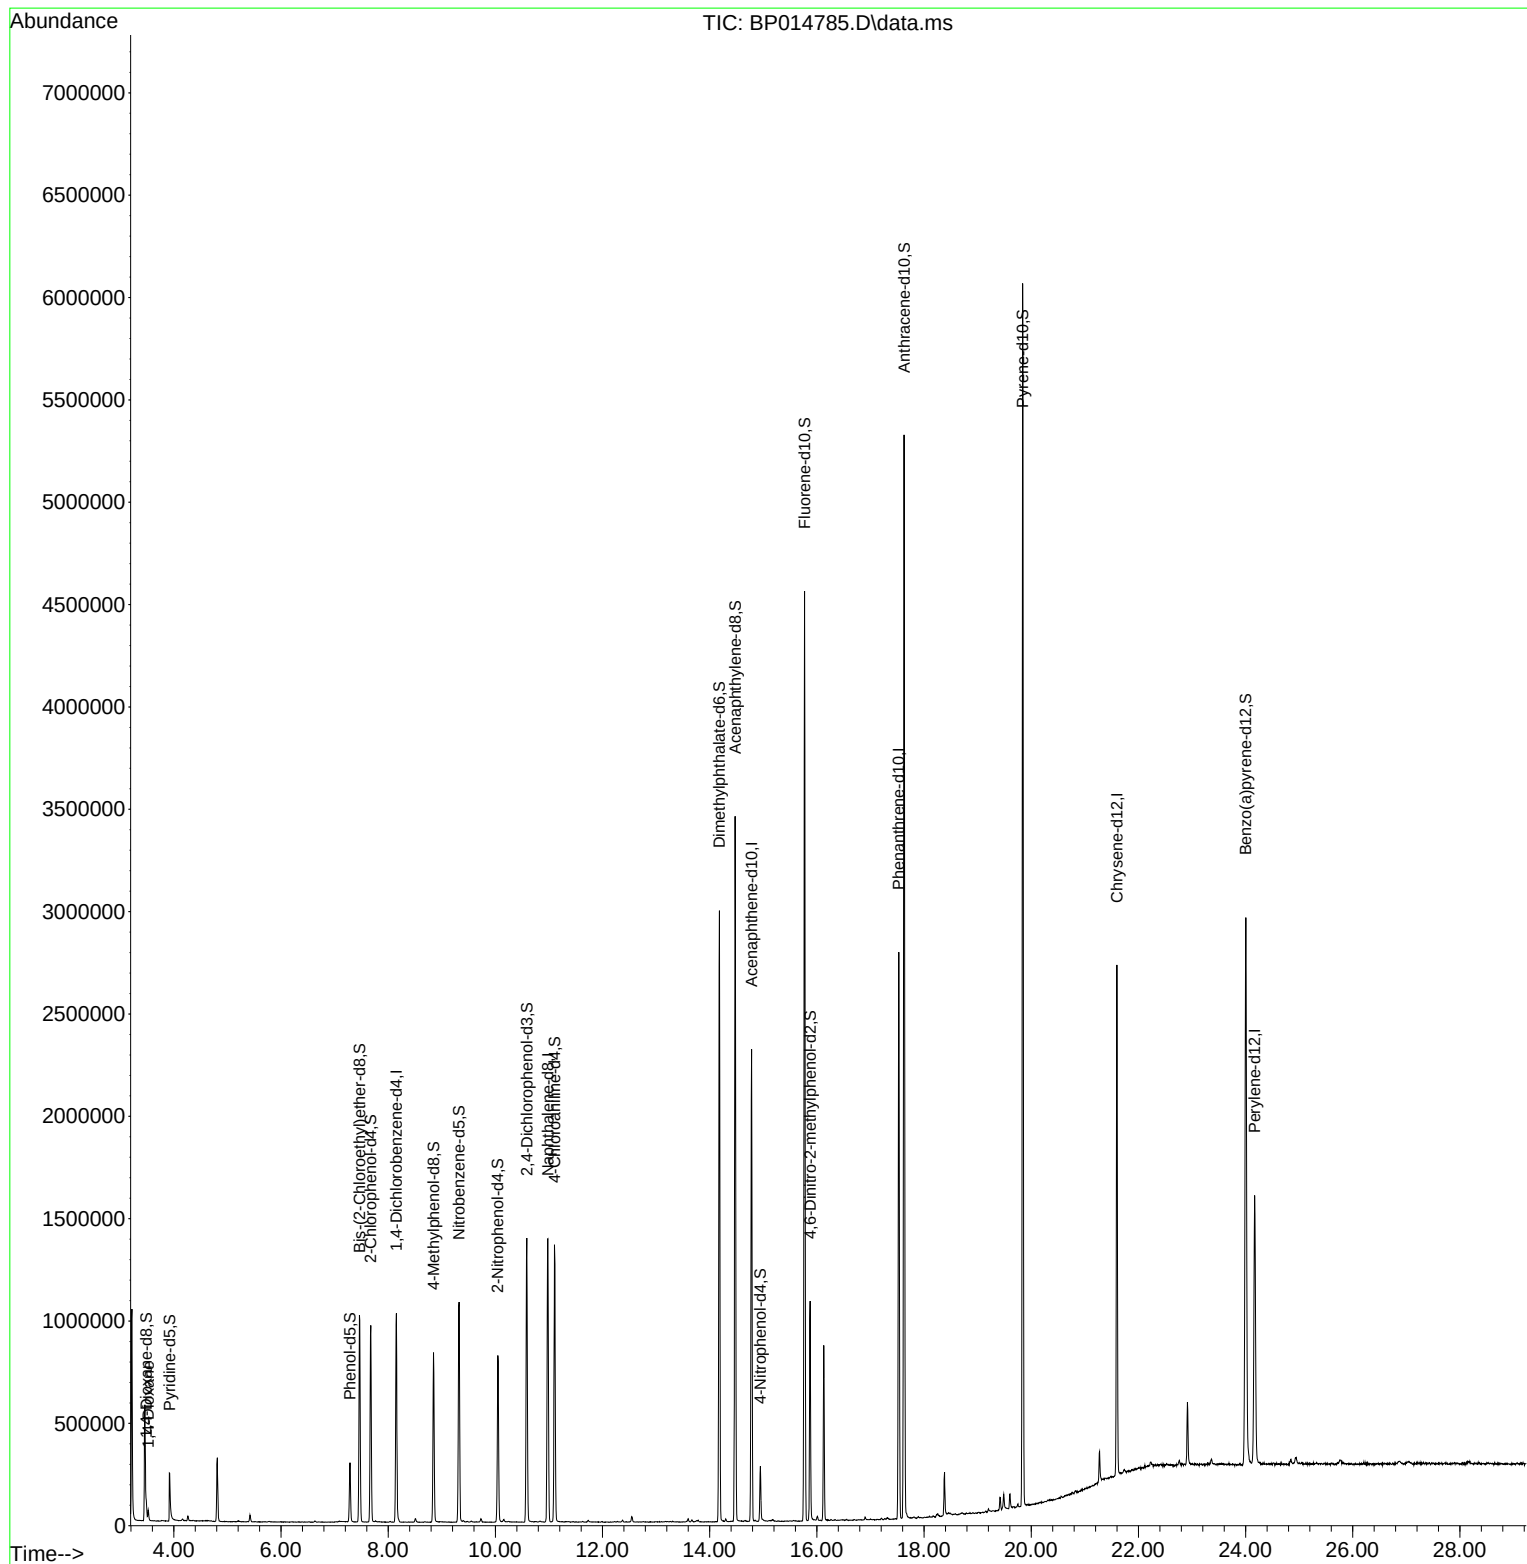

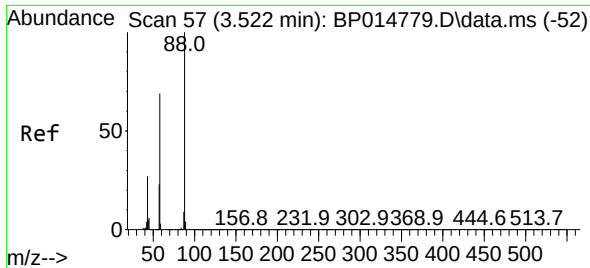

#2
 1,4-Dioxane
 Concen: 3.057 ng/uL
 RT: 3.523 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BP014785.D
 Acq: 21 Apr 2023 11:50

Instrument :
 BNA_P
 ClientSampleId :
 BHE12

Tgt Ion: 88 Resp: 23159
 Ion Ratio Lower Upper
 88 100
 43 26.0 25.0 37.6
 58 68.0 54.9 82.3

