

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014796.D
 Acq On : 21 Apr 2023 18:36
 Operator : CG/JU
 Sample : 02378-13DL 20X
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMK6DL

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 04/24/2023
 Supervised By : Jagrut Upadhyay 04/24/2023

Quant Time: Apr 21 23:23:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 20 02:32:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	315471	20.000	ng/u1	0.00
20) Naphthalene-d8	10.981	136	1305334	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	841558	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.528	188	1808374	20.000	ng/u1	0.00
79) Chrysene-d12	21.598	240	1211873	20.000	ng/u1	0.00
88) Perylene-d12	24.168	264	1151816	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	1935	0.244	ng/uL	0.00
4) Pyridine-d5	3.958	84	10439m	0.483	ng/u1	0.04
7) Phenol-d5	7.281	99	7992	0.293	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.463	67	27083	1.609	ng/u1	0.00
11) 2-Chlorophenol-d4	7.675	132	20320	1.003	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	13761	0.647	ng/u1	0.00
21) Nitrobenzene-d5	9.322	128	11483	1.404	ng/u1	0.00
24) 2-Nitrophenol-d4	10.046	143	9755	1.320	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	20395	1.017	ng/u1	0.00
31) 4-Chloroaniline-d4	11.104	131	31300	1.022	ng/u1	0.00
46) Dimethylphthalate-d6	14.175	166	102495	1.538	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	96541	1.250	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.763	176	86876	1.519	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	
73) Anthracene-d10	17.628	188	128810	1.474	ng/u1	0.00
81) Pyrene-d10	19.839	212	133160	1.918	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.998	264	80621	1.350	ng/u1	-0.02
Target Compounds						
22) Nitrobenzene	9.363	77	979922	44.090	ng/u1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014796.D
Acq On : 21 Apr 2023 18:36
Operator : CG/JU
Sample : 02378-13DL 20X
Misc :
ALS Vial : 51 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
COMK6DL

Quant Time: Apr 21 23:23:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 20 02:32:50 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Christian Giraldo 04/24/2023
Supervised By : Jagrut Upadhyay 04/24/2023

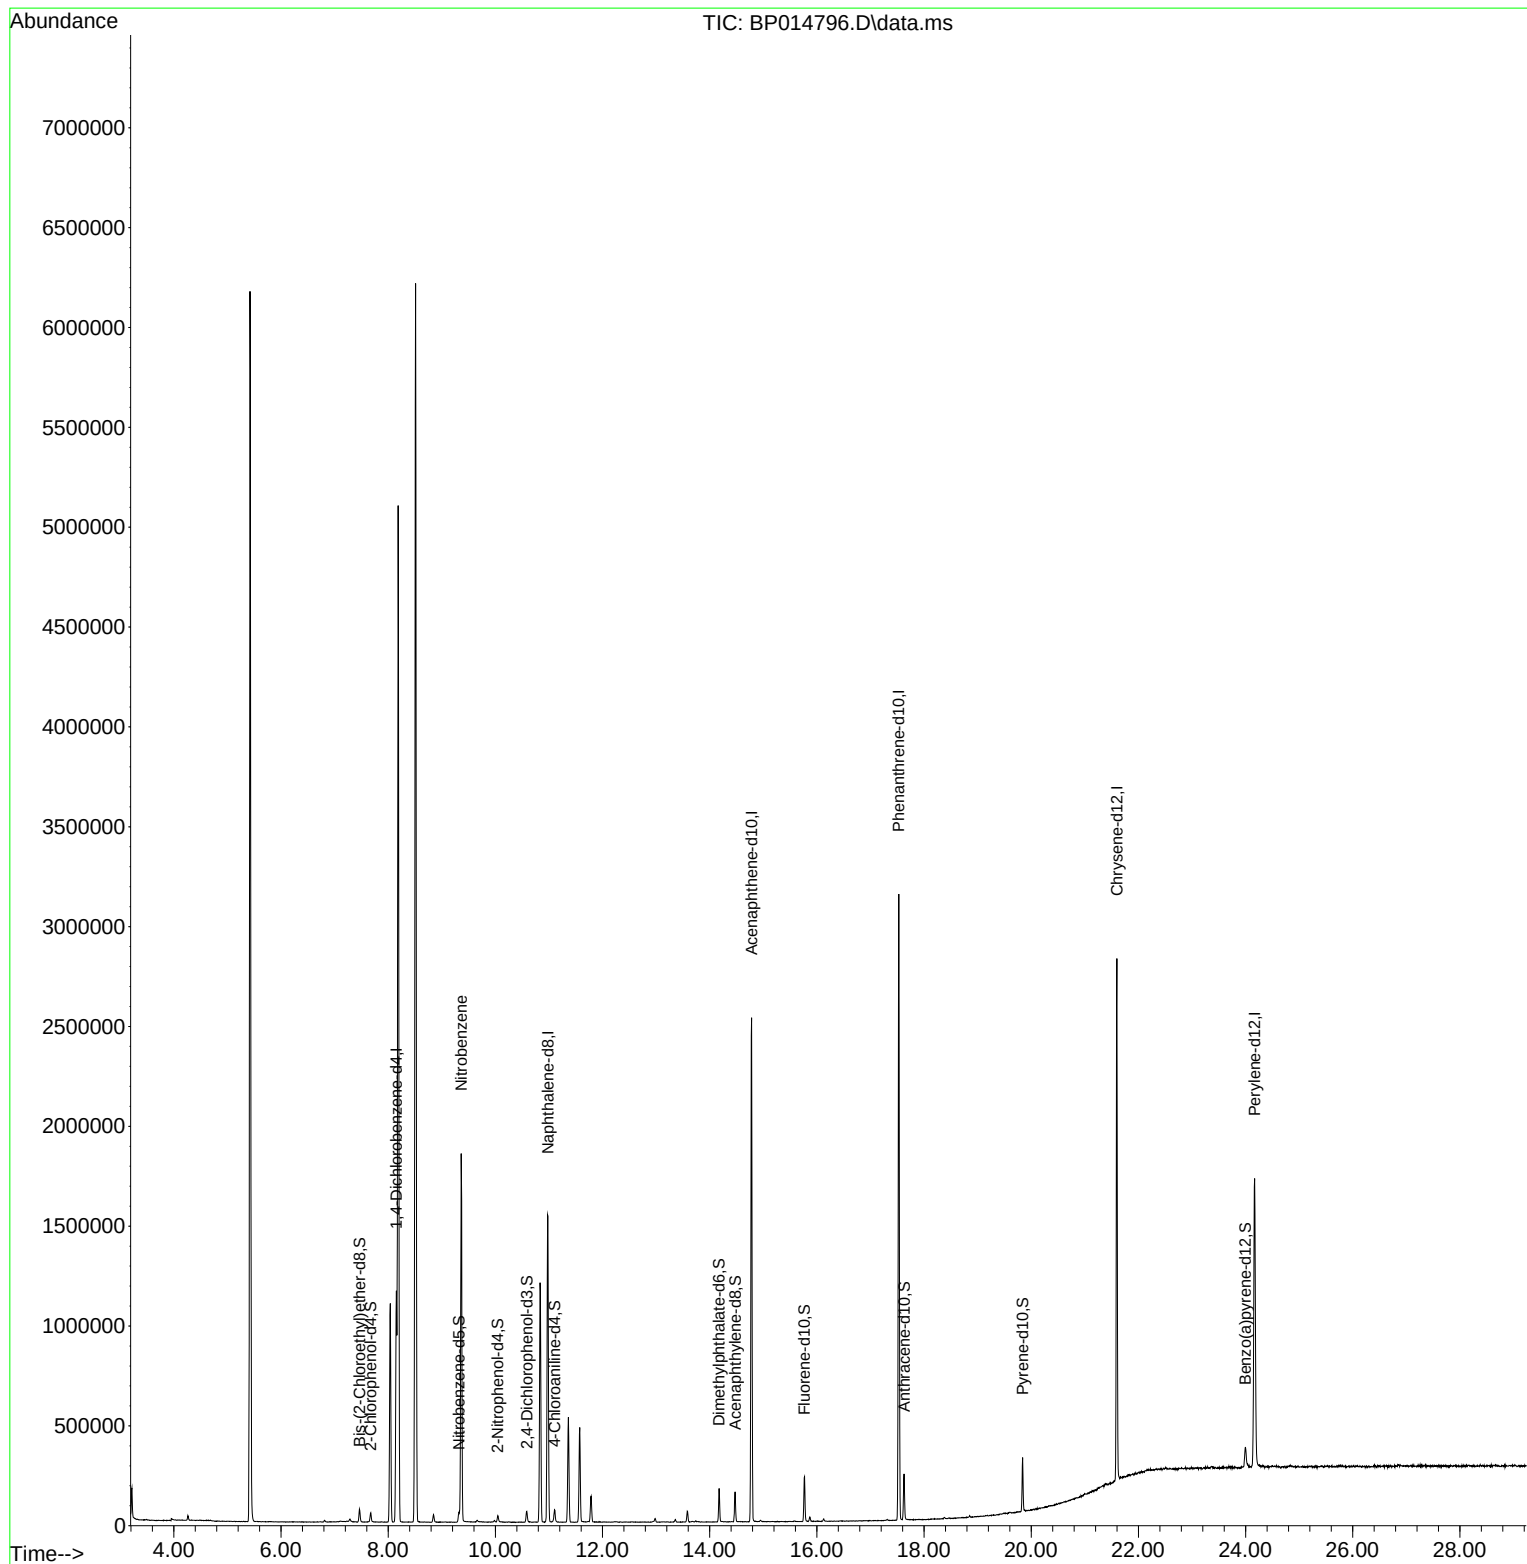

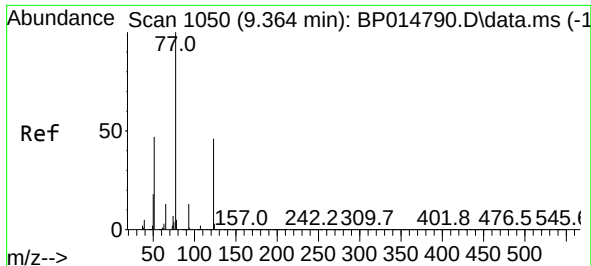

#22
 Nitrobenzene
 Concen: 44.090 ng/ul
 RT: 9.363 min Scan# 1050
 Delta R.T. -0.000 min
 Lab File: BP014796.D
 Acq: 21 Apr 2023 18:36

Instrument :
 BNA_P
 ClientSampleId :
 COMK6DL

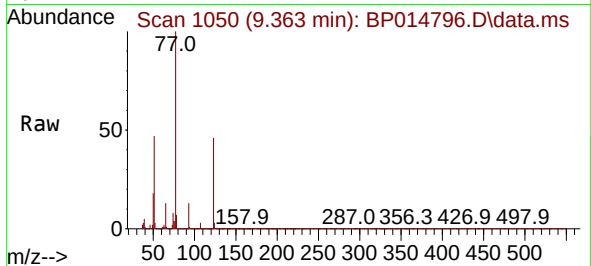

Tgt Ion: 77 Resp: 97992
 Ion Ratio Lower Upper
 77 100
 123 45.9 35.4 53.2
 65 13.0 10.8 16.2

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 04/24/2023
 Supervised By :Jagrut Upadhyay 04/24/2023

