

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014800.D
 Acq On : 21 Apr 2023 20:50
 Operator : CG/JU
 Sample : 02392-05
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE26

Quant Time: Apr 21 23:24:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 20 02:32:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	231893	20.000	ng/u1	0.00
20) Naphthalene-d8	10.981	136	949521	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	559388	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.528	188	1089240	20.000	ng/u1	0.00
79) Chrysene-d12	21.598	240	809838	20.000	ng/u1	0.00
88) Perylene-d12	24.168	264	894400	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	34834	5.970	ng/uL	0.00
4) Pyridine-d5	3.917	84	196931	12.397	ng/u1	0.00
7) Phenol-d5	7.287	99	162817	8.121	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.463	67	539909	43.649	ng/u1	0.00
11) 2-Chlorophenol-d4	7.675	132	504988	33.914	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	313624	20.065	ng/u1	0.00
21) Nitrobenzene-d5	9.322	128	308231	51.805	ng/u1	0.00
24) 2-Nitrophenol-d4	10.052	143	296149	55.109	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	569034	38.998	ng/u1	0.00
31) 4-Chloroaniline-d4	11.110	131	662194	29.734	ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	2023406	45.682	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	2332655	45.443	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	37685	5.349	ng/u1	0.00
60) Fluorene-d10	15.769	176	1717847	45.199	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	171861	38.989	ng/u1	0.00
73) Anthracene-d10	17.628	188	2477921	47.091	ng/u1	0.00
81) Pyrene-d10	19.839	212	2588178	55.790	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.004	264	2300674	49.630	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.522	88	39431	6.257	ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014800.D
Acq On : 21 Apr 2023 20:50
Operator : CG/JU
Sample : 02392-05
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE26

Quant Time: Apr 21 23:24:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 20 02:32:50 2023
Response via : Initial Calibration

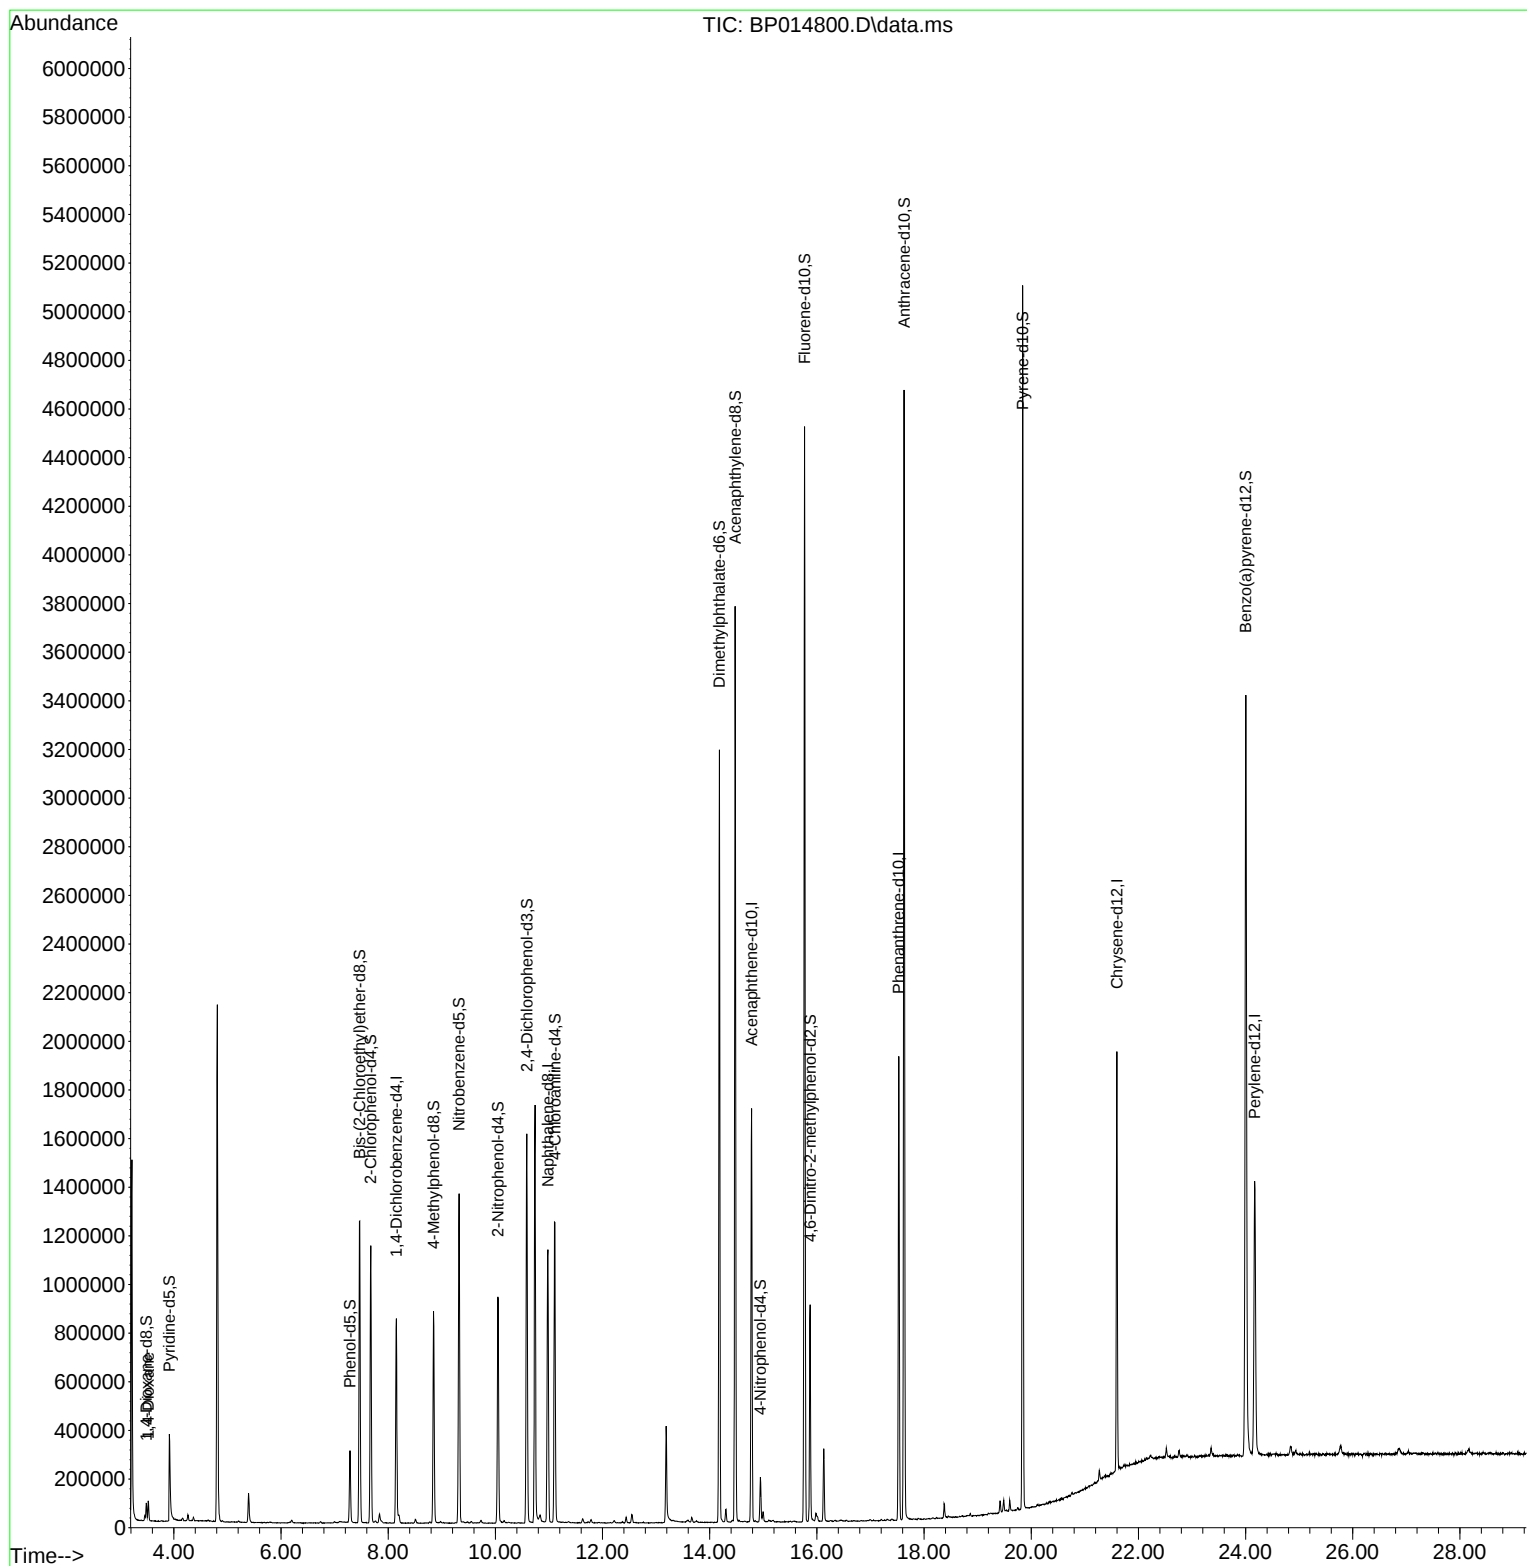

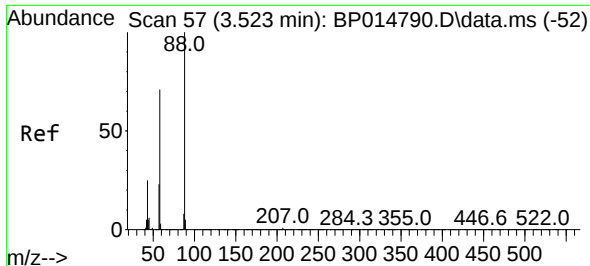

#2
 1,4-Dioxane
 Concen: 6.257 ng/uL
 RT: 3.522 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BP014800.D
 Acq: 21 Apr 2023 20:50

Instrument :
 BNA_P
 ClientSampleId :
 BHE26

Tgt Ion: 88 Resp: 39431
 Ion Ratio Lower Upper
 88 100
 43 28.8 25.0 37.6
 58 78.8 54.9 82.3

