

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014802.D
 Acq On : 21 Apr 2023 21:57
 Operator : CG/JU
 Sample : 02392-07
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE28

Quant Time: Apr 21 23:55:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 20 02:32:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.152	152	317711	20.000	ng/u1	0.00
20) Naphthalene-d8	10.981	136	1302686	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	766504	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.528	188	1504136	20.000	ng/u1	0.00
79) Chrysene-d12	21.598	240	1146035	20.000	ng/u1	0.00
88) Perylene-d12	24.169	264	1253362	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.487	96	38255	4.786	ng/uL	0.00
4) Pyridine-d5	3.923	84	147819	6.792	ng/u1	0.00
7) Phenol-d5	7.287	99	194247	7.071	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.469	67	614660	36.270	ng/u1	0.00
11) 2-Chlorophenol-d4	7.675	132	588180	28.831	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	359914	16.807	ng/u1	0.00
21) Nitrobenzene-d5	9.322	128	364071	44.601	ng/u1	0.00
24) 2-Nitrophenol-d4	10.052	143	354227	48.046	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	652004	32.570	ng/u1	0.00
31) 4-Chloroaniline-d4	11.110	131	809668	26.499	ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	2339583	38.548	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	2723639	38.723	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	45281	4.691	ng/u1	0.00
60) Fluorene-d10	15.769	176	1983452	38.086	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.875	200	205313	33.730	ng/u1	0.00
73) Anthracene-d10	17.628	188	2848482	39.201	ng/u1	0.00
81) Pyrene-d10	19.839	212	2974385	45.307	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.004	264	2725024	41.949	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.523	88	22815	2.643	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014802.D
Acq On : 21 Apr 2023 21:57
Operator : CG/JU
Sample : 02392-07
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE28

Quant Time: Apr 21 23:55:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 20 02:32:50 2023
Response via : Initial Calibration

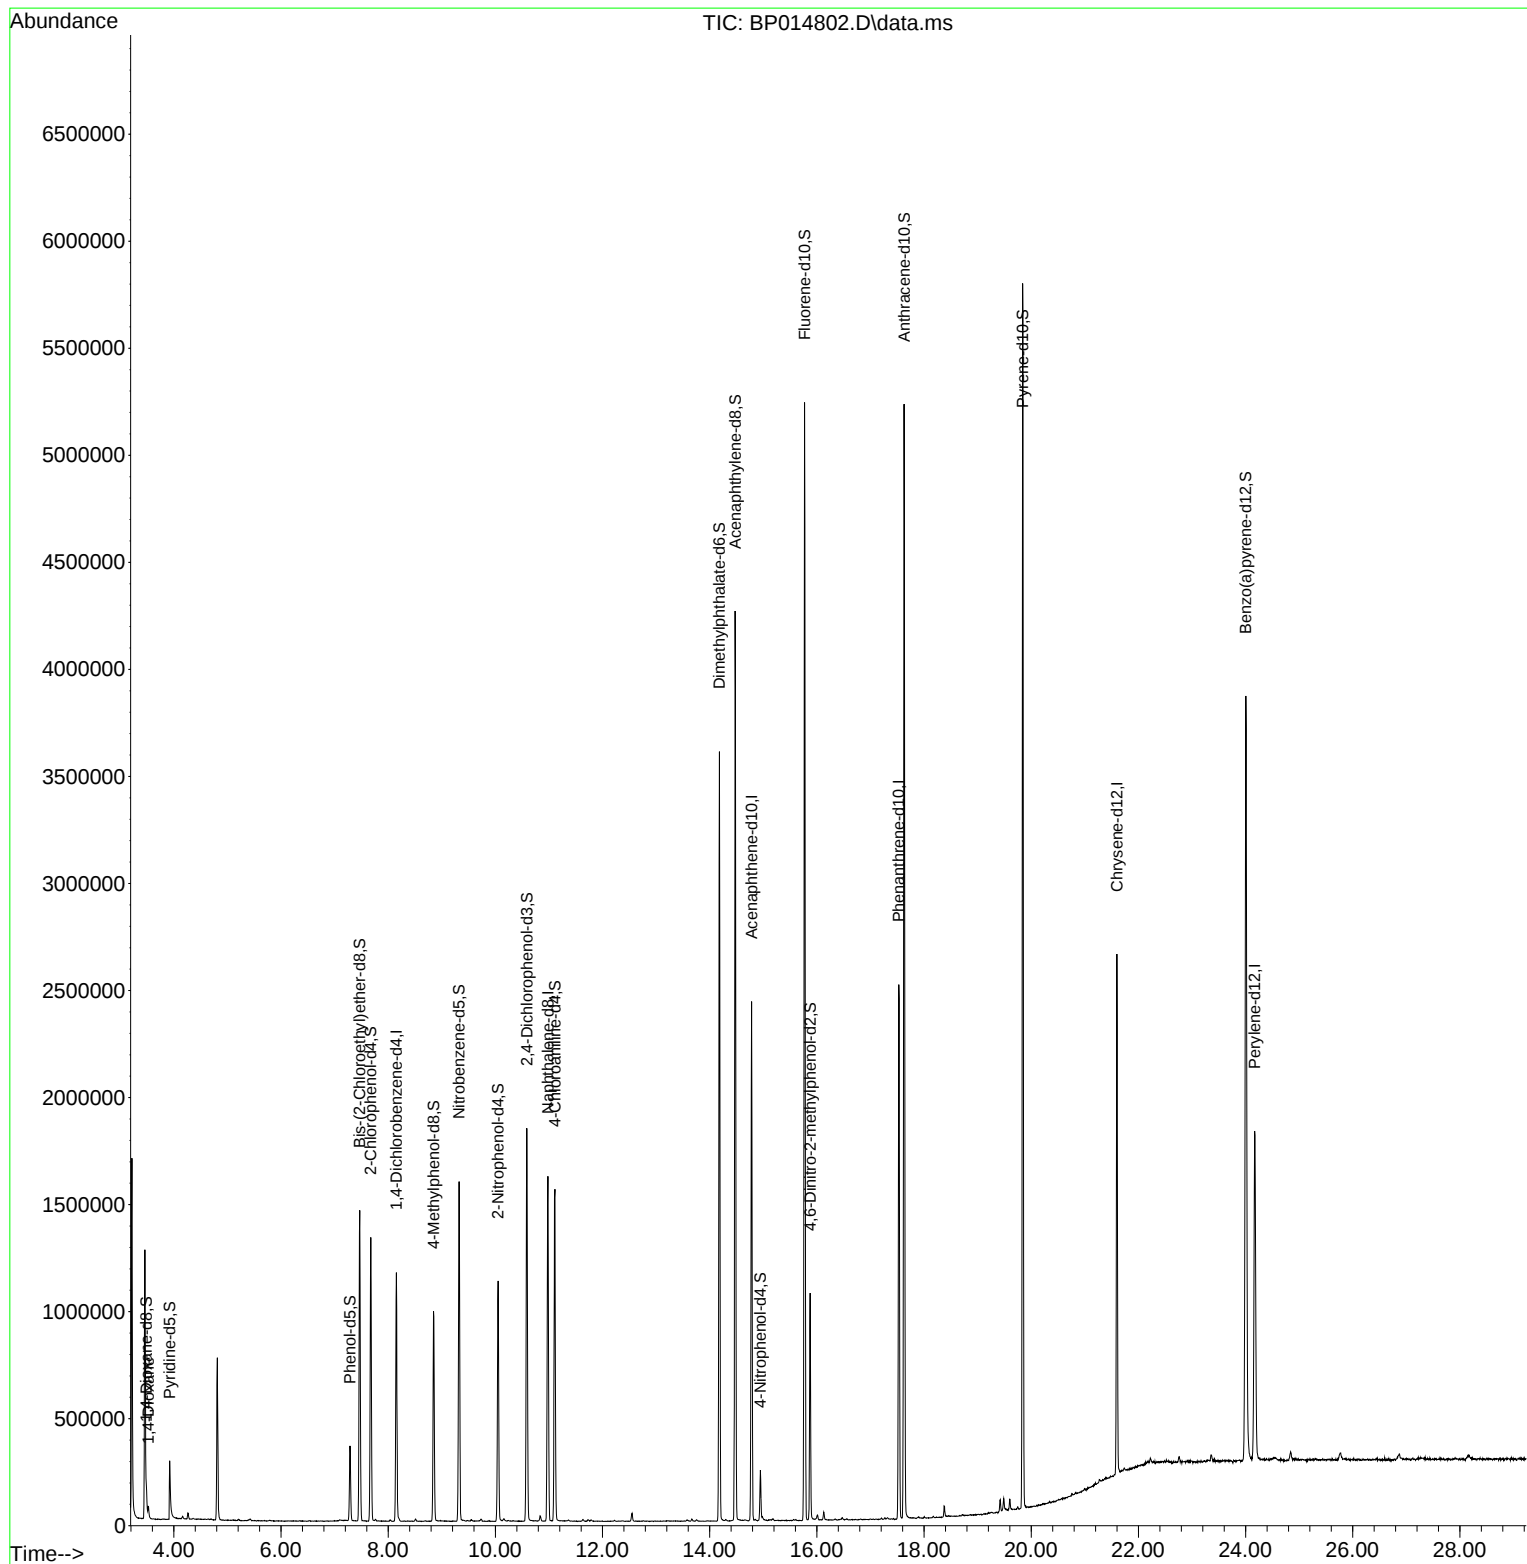

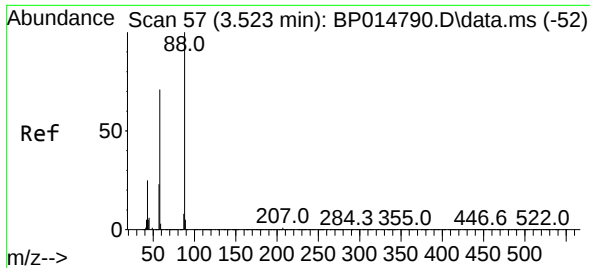

#2
 1,4-Dioxane
 Concen: 2.643 ng/uL
 RT: 3.523 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BP014802.D
 Acq: 21 Apr 2023 21:57

Instrument :
 BNA_P
 ClientSampleId :
 BHE28

Tgt Ion: 88 Resp: 22815
 Ion Ratio Lower Upper
 88 100
 43 28.0 25.0 37.6
 58 66.5 54.9 82.3

