

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014761.D
 Acq On : 20 Apr 2023 17:58
 Operator : CG/JU
 Sample : PB152246BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	11	rVB	68140	69836	1.29%	0.112%
2	3.487	46	51	59	rBV	84737	104609	1.93%	0.168%
3	3.916	120	124	142	rBV	771960	1157426	21.34%	1.862%
4	4.263	179	183	189	rVB	19906	28285	0.52%	0.045%
5	7.287	690	697	708	rBV	1147318	1751194	32.28%	2.817%
6	7.469	720	728	739	rVB	972562	1504203	27.73%	2.420%
7	7.675	755	763	774	rBV	1169057	1816030	33.48%	2.921%
8	8.152	834	844	853	rBV	968831	1527938	28.17%	2.458%
9	8.846	953	962	975	rBV	1427628	2239557	41.29%	3.602%
10	9.322	1034	1043	1052	rBV	1027262	1661762	30.64%	2.673%
11	10.051	1156	1167	1177	rBV	760707	1230582	22.69%	1.979%
12	10.587	1248	1258	1269	rBV	1357255	2222131	40.97%	3.574%
13	10.981	1316	1325	1334	rBV	1348919	2221918	40.96%	3.574%
14	11.104	1339	1346	1357	rBV	934246	1568329	28.91%	2.523%
15	12.551	1587	1592	1598	rVB2	26708	43706	0.81%	0.070%
16	13.575	1760	1766	1767	rBV6	3631	5739	0.11%	0.009%
17	13.669	1776	1782	1789	rBV2	15297	25965	0.48%	0.042%
18	14.181	1860	1869	1879	rBV	2577795	3399425	62.67%	5.468%
19	14.475	1911	1919	1928	rBV	2895415	4227184	77.93%	6.800%
20	14.781	1963	1971	1979	rBV	2064799	2979618	54.93%	4.793%
21	14.839	1979	1981	1988	rVB8	3927	6575	0.12%	0.011%
22	14.945	1990	1999	2010	rBV	993150	1378679	25.42%	2.218%
23	15.181	2035	2039	2044	rVB8	4207	6732	0.12%	0.011%
24	15.769	2132	2139	2149	rBV	3610527	5038819	92.89%	8.105%
25	15.875	2150	2157	2170	rVV	704726	969621	17.88%	1.560%
26	16.010	2175	2180	2184	rVB2	17334	25795	0.48%	0.041%
27	16.557	2269	2273	2278	rBV7	3947	6663	0.12%	0.011%
28	17.210	2379	2384	2389	rBV8	4394	7827	0.14%	0.013%
29	17.316	2398	2402	2406	rBV4	5475	9926	0.18%	0.016%
30	17.528	2432	2438	2448	rBV	2298440	3247686	59.87%	5.224%
31	17.627	2448	2455	2471	rVV	3746857	5196883	95.81%	8.359%
32	19.422	2756	2760	2765	rVB2	40385	49712	0.92%	0.080%
33	19.486	2767	2771	2776	rVV	35431	48540	0.89%	0.078%
34	19.845	2826	2832	2840	rBV	4290323	5424267	100.00%	8.725%
35	21.604	3125	3131	3142	rBV	2104587	2917461	53.79%	4.693%
36	24.010	3532	3540	3557	rBV2	2537473	5047181	93.05%	8.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014761.D
Acq On : 20 Apr 2023 17:58
Operator : CG/JU
Sample : PB152246BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK246

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Title : SVOA CALIBRATION

37	24.174	3561	3568	3582	rVB2	1396062	2999963	55.31%	4.826%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 62167767

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014761.D
Acq On : 20 Apr 2023 17:58
Operator : CG/JU
Sample : PB152246BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK246

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

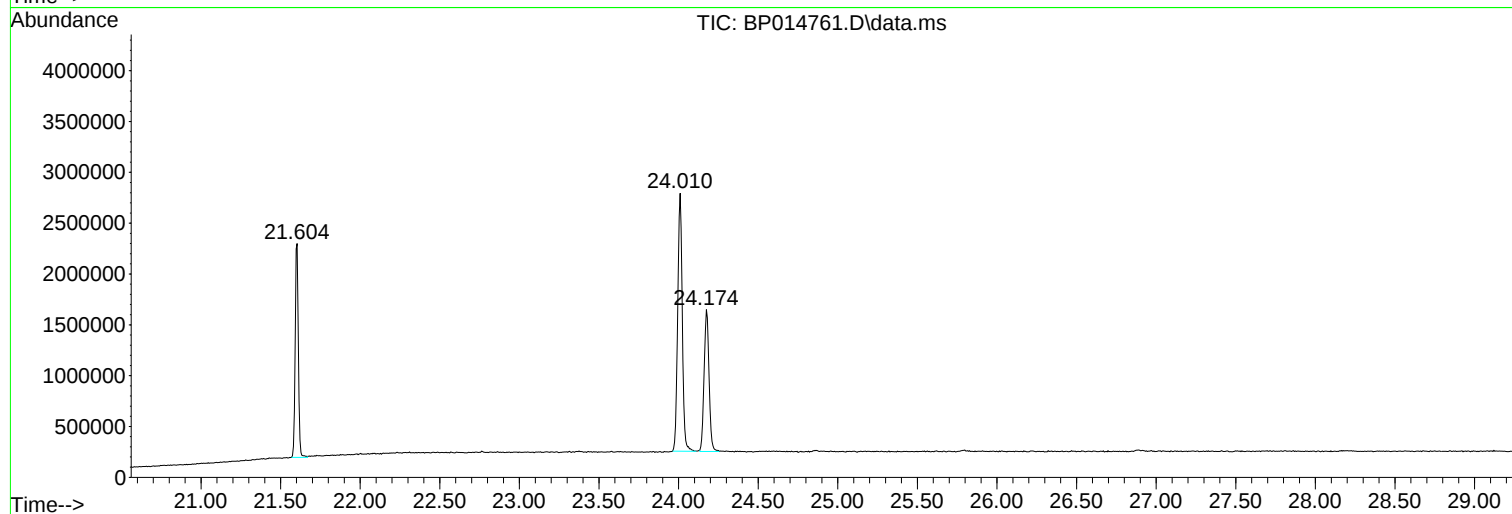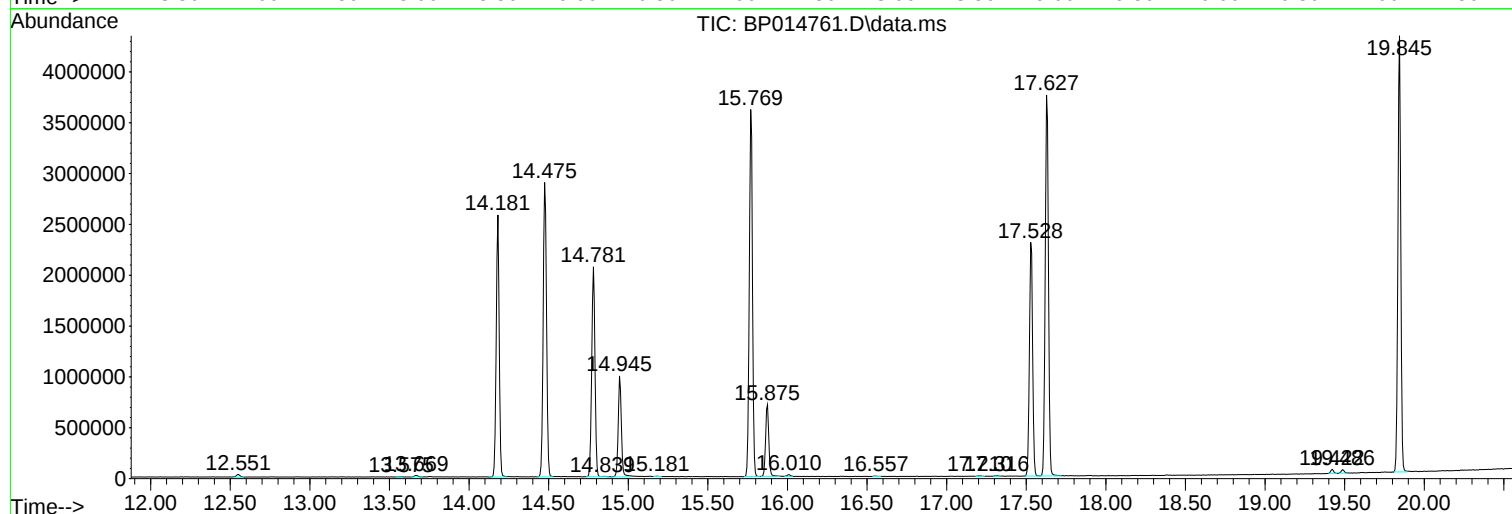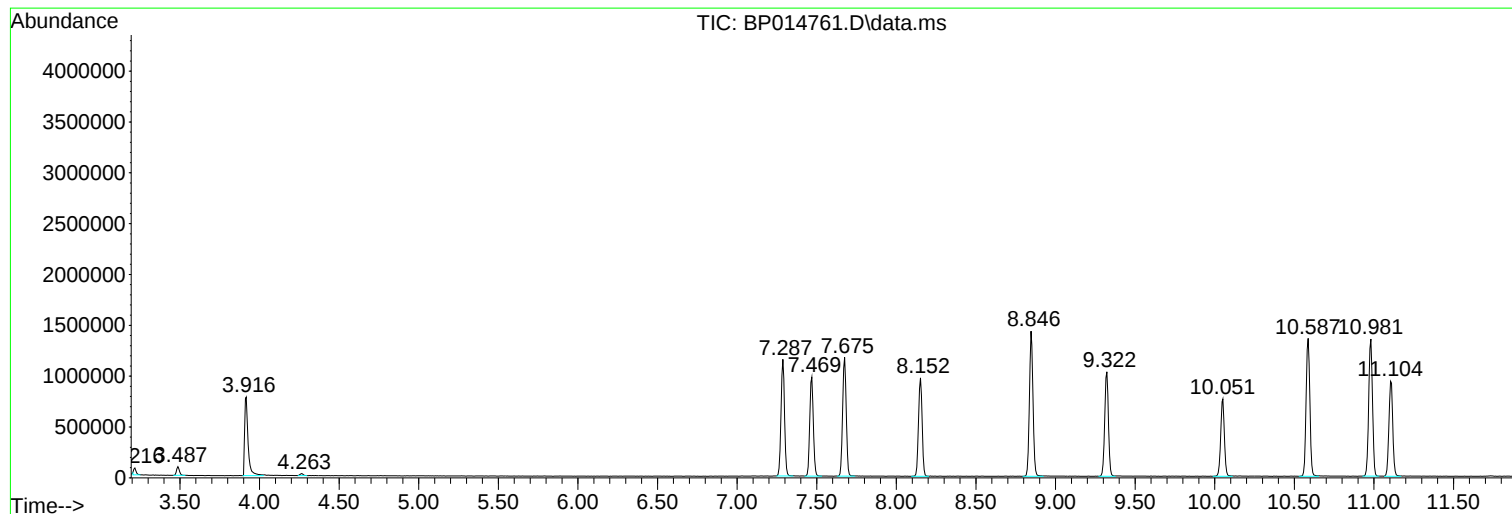

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014761.D
Acq On : 20 Apr 2023 17:58
Operator : CG/JU
Sample : PB152246BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK246

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014761.D
Acq On : 20 Apr 2023 17:58
Operator : CG/JU
Sample : PB152246BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK246

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------