

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014770.D
 Acq On : 20 Apr 2023 22:59
 Operator : CG/JU
 Sample : 02296-06DL2 25X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCBK6DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	3	5	15	rVB	124834	135958	2.22%	0.353%
2	4.264	179	183	192	rVB	21538	33153	0.54%	0.086%
3	6.652	585	589	594	rBV2	13545	25048	0.41%	0.065%
4	7.228	684	687	692	rVB3	6487	8517	0.14%	0.022%
5	7.287	692	697	702	rVV3	11348	18257	0.30%	0.047%
6	7.358	704	709	714	rVB3	6392	10174	0.17%	0.026%
7	7.463	722	727	734	rVB	47054	72081	1.18%	0.187%
8	7.675	758	763	769	rVB	31631	53355	0.87%	0.139%
9	7.793	778	783	789	rVB	16590	24658	0.40%	0.064%
10	8.152	836	844	853	rBV	1105315	1767217	28.92%	4.593%
11	8.269	858	864	869	rBV5	6435	12559	0.21%	0.033%
12	8.528	901	908	915	rBV	96276	152341	2.49%	0.396%
13	8.693	930	936	942	rBV	82745	130973	2.14%	0.340%
14	8.846	956	962	970	rVB2	24910	42423	0.69%	0.110%
15	9.316	1037	1042	1052	rVB2	38278	75818	1.24%	0.197%
16	9.522	1072	1077	1082	rVB5	10757	17477	0.29%	0.045%
17	9.646	1086	1098	1104	rBV3	21678	49864	0.82%	0.130%
18	9.704	1104	1108	1114	rVB5	5947	9698	0.16%	0.025%
19	9.793	1119	1123	1127	rVV5	4827	7973	0.13%	0.021%
20	10.046	1160	1166	1172	rBV2	19445	35151	0.58%	0.091%
21	10.216	1190	1195	1201	rVB	9265	13921	0.23%	0.036%
22	10.369	1214	1221	1232	rVB6	19152	43715	0.72%	0.114%
23	10.469	1234	1238	1245	rBV8	6060	12432	0.20%	0.032%
24	10.581	1251	1257	1266	rVB	39426	72008	1.18%	0.187%
25	10.981	1316	1325	1328	rBV	1491531	2528902	41.38%	6.573%
26	11.028	1328	1333	1341	rVV	3636756	6111469	100.00%	15.885%
27	11.104	1341	1346	1349	rVV	31758	55769	0.91%	0.145%
28	11.146	1349	1353	1362	rVB	117407	202940	3.32%	0.527%
29	11.734	1447	1453	1457	rVB6	4924	7957	0.13%	0.021%
30	12.081	1506	1512	1515	rBV8	5278	9142	0.15%	0.024%
31	12.522	1580	1587	1591	rBV	19952	33954	0.56%	0.088%
32	12.622	1594	1604	1610	rBV	321135	494097	8.08%	1.284%
33	12.740	1615	1624	1630	rBV	38949	68173	1.12%	0.177%
34	12.834	1630	1640	1648	rBV	299169	504534	8.26%	1.311%
35	13.251	1704	1711	1715	rVB6	7167	11684	0.19%	0.030%
36	13.551	1755	1762	1767	rBV4	10589	17393	0.28%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014770.D
 Acq On : 20 Apr 2023 22:59
 Operator : CG/JU
 Sample : 02296-06DL2 25X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCBK6DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

37	13.616	1767	1773	1779	rVV	229249	329386	5.39%	0.856%
38	13.669	1779	1782	1786	rVB4	9663	14131	0.23%	0.037%
39	13.810	1801	1806	1816	rVB	73814	134088	2.19%	0.349%
40	13.945	1816	1829	1830	rBV2	59696	105719	1.73%	0.275%

41	14.098	1846	1855	1860	rVV	112058	196871	3.22%	0.512%
42	14.175	1860	1868	1876	rVB2	130207	238953	3.91%	0.621%
43	14.334	1890	1895	1899	rVV2	39838	61503	1.01%	0.160%
44	14.369	1899	1901	1907	rVB2	18633	22687	0.37%	0.059%
45	14.475	1911	1919	1928	rBV	115187	221341	3.62%	0.575%

46	14.692	1950	1956	1960	rBV4	7556	12776	0.21%	0.033%
47	14.781	1960	1971	1976	rVV	2277969	3436059	56.22%	8.931%
48	14.839	1976	1981	1987	rVV	1726186	2529825	41.39%	6.575%
49	14.904	1987	1992	1998	rVV	144304	210121	3.44%	0.546%
50	14.981	2002	2005	2009	rVV4	8548	13391	0.22%	0.035%

51	15.045	2012	2016	2018	rBV4	6839	8579	0.14%	0.022%
52	15.087	2018	2023	2029	rVV	38344	57301	0.94%	0.149%
53	15.175	2031	2038	2045	rBV	1062969	1555884	25.46%	4.044%
54	15.245	2045	2050	2053	rBV4	12646	17901	0.29%	0.047%
55	15.387	2068	2074	2079	rBV6	10549	20593	0.34%	0.054%

56	15.439	2079	2083	2088	rBV5	8531	14556	0.24%	0.038%
57	15.557	2097	2103	2108	rBV7	9402	23216	0.38%	0.060%
58	15.592	2108	2109	2114	rVV5	7189	8369	0.14%	0.022%
59	15.769	2129	2139	2143	rVV	174414	267688	4.38%	0.696%
60	15.822	2143	2148	2154	rVV2	558336	780130	12.77%	2.028%

61	15.869	2154	2156	2159	rVV3	16780	20015	0.33%	0.052%
62	15.916	2159	2164	2166	rVV4	21009	33384	0.55%	0.087%
63	15.945	2166	2169	2172	rVV2	40500	58757	0.96%	0.153%
64	15.986	2172	2176	2181	rVV3	66856	102256	1.67%	0.266%
65	16.034	2181	2184	2187	rVV3	15559	25037	0.41%	0.065%

66	16.075	2187	2191	2194	rVV2	32835	49462	0.81%	0.129%
67	16.116	2194	2198	2205	rVB2	105458	168352	2.75%	0.438%
68	16.216	2212	2215	2217	rBV4	9259	10272	0.17%	0.027%
69	16.263	2218	2223	2230	rVB2	83609	169413	2.77%	0.440%
70	16.328	2230	2234	2237	rBV	24289	36280	0.59%	0.094%

71	16.498	2254	2263	2270	rBV	130322	211693	3.46%	0.550%
72	16.622	2276	2284	2288	rBV4	12359	21602	0.35%	0.056%
73	16.786	2306	2312	2316	rBV7	18855	43404	0.71%	0.113%
74	16.828	2316	2319	2324	rVB3	22014	30888	0.51%	0.080%
75	16.875	2324	2327	2331	rBV4	7464	8404	0.14%	0.022%

76	16.975	2341	2344	2352	rVB4	13156	18581	0.30%	0.048%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014770.D
 Acq On : 20 Apr 2023 22:59
 Operator : CG/JU
 Sample : 02296-06DL2 25X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCBK6DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

77	17.139	2368	2372	2374	rVV5	5919	9573	0.16%	0.025%
78	17.175	2374	2378	2384	rVB2	27046	39384	0.64%	0.102%
79	17.281	2393	2396	2399	rVV5	7467	10936	0.18%	0.028%
80	17.345	2399	2407	2412	rVB	131168	183517	3.00%	0.477%
81	17.486	2425	2431	2432	rBV5	6283	10950	0.18%	0.028%
82	17.528	2432	2438	2442	rBV	2751813	3786073	61.95%	9.841%
83	17.569	2442	2445	2451	rVB	1372487	1752350	28.67%	4.555%
84	17.628	2451	2455	2459	rBV	222499	297307	4.86%	0.773%
85	17.922	2500	2505	2510	rVV	230936	305835	5.00%	0.795%
86	18.057	2521	2528	2534	rVB5	16678	39151	0.64%	0.102%
87	18.339	2573	2576	2579	rBV5	5756	9503	0.16%	0.025%
88	18.380	2579	2583	2586	rVV	42172	57000	0.93%	0.148%
89	18.428	2586	2591	2596	rVB2	59030	88237	1.44%	0.229%
90	18.575	2609	2616	2624	rBV3	81649	147826	2.42%	0.384%
91	18.704	2635	2638	2641	rBV3	13419	13790	0.23%	0.036%
92	18.792	2650	2653	2658	rVB3	13199	17504	0.29%	0.045%
93	18.857	2660	2664	2667	rVV3	16911	21741	0.36%	0.057%
94	18.892	2667	2670	2674	rVB4	11212	13960	0.23%	0.036%
95	19.516	2771	2776	2781	rBV	191816	251216	4.11%	0.653%
96	19.598	2788	2790	2796	rVB7	10683	12935	0.21%	0.034%
97	19.839	2826	2831	2834	rBV	210943	302306	4.95%	0.786%
98	19.869	2834	2836	2843	rVB	109687	120954	1.98%	0.314%
99	21.598	3125	3130	3140	rBV	2626955	3378845	55.29%	8.782%
100	24.168	3560	3567	3578	rVB2	1664346	3443461	56.34%	8.950%




Sum of corrected areas: 38474007

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014770.D
Acq On : 20 Apr 2023 22:59
Operator : CG/JU
Sample : 02296-06DL2 25X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCBK6DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

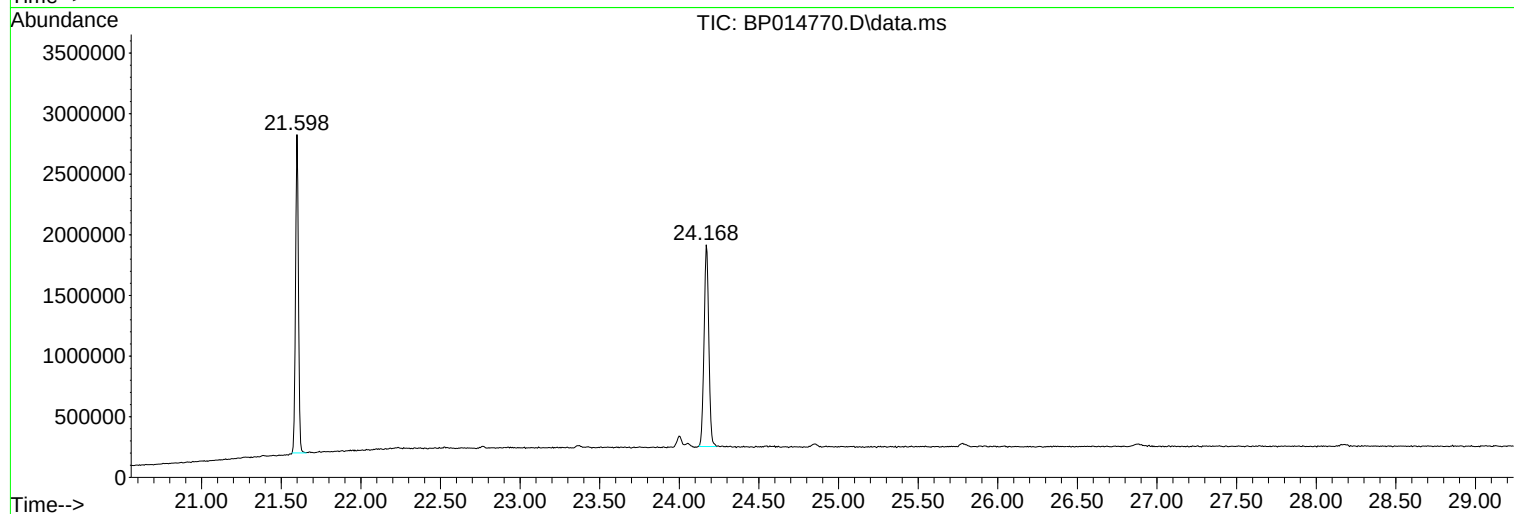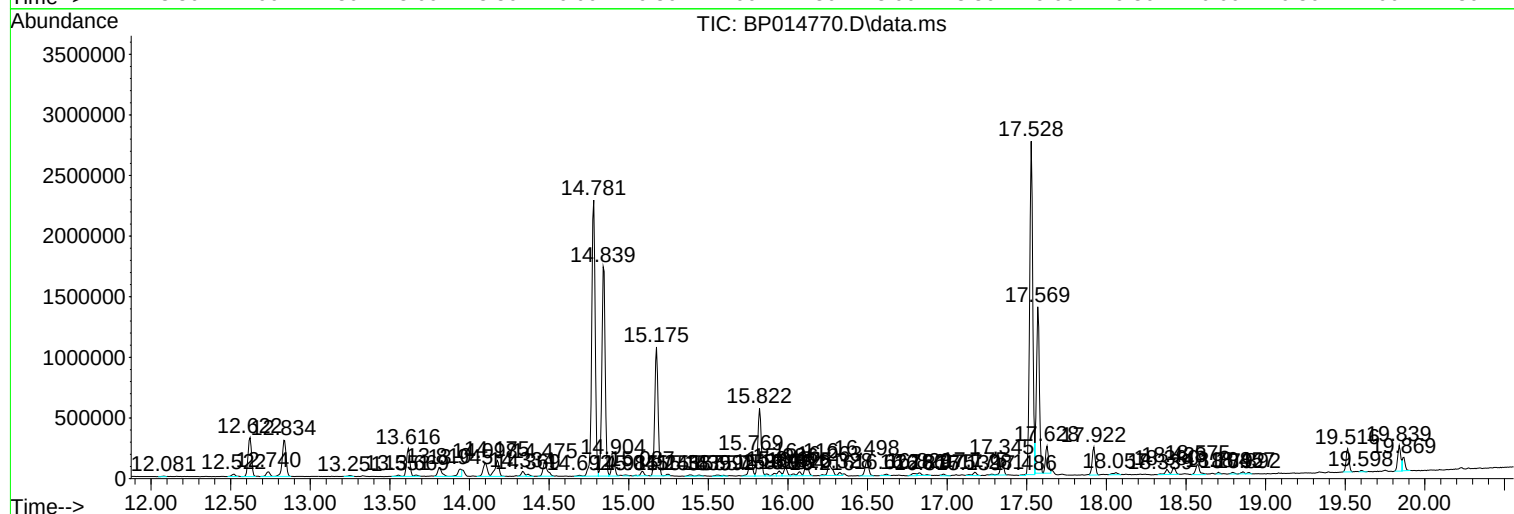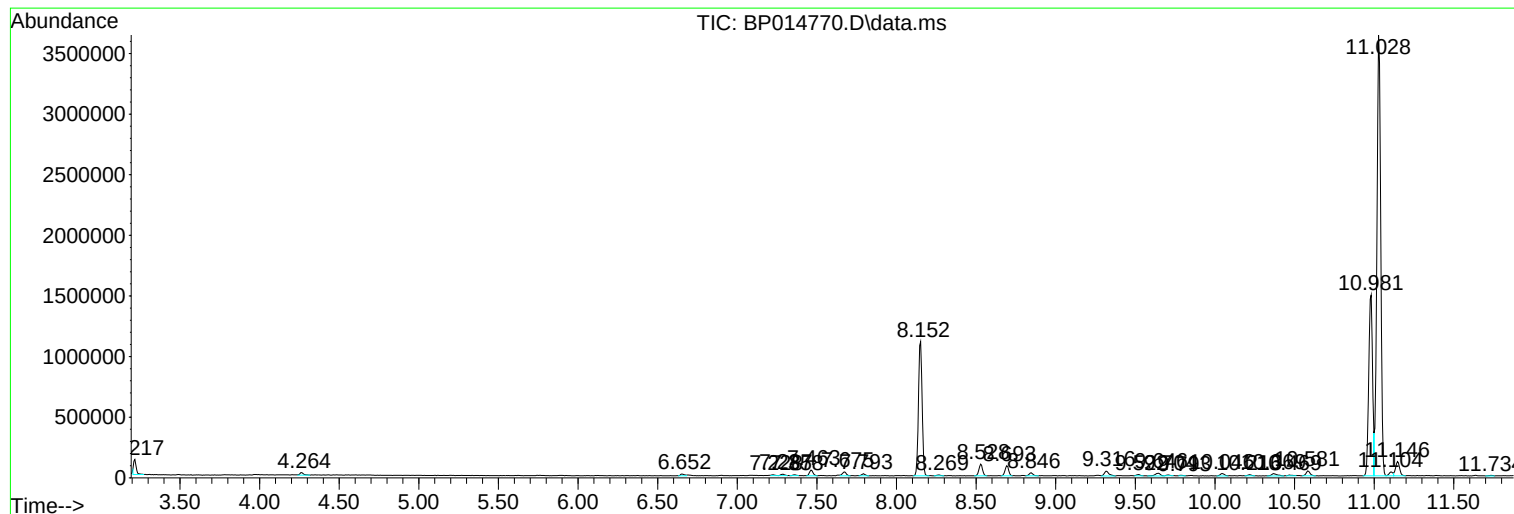

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014770.D
Acq On : 20 Apr 2023 22:59
Operator : CG/JU
Sample : 02296-06DL2 25X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCBK6DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014770.D
Acq On : 20 Apr 2023 22:59
Operator : CG/JU
Sample : 02296-06DL2 25X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCBK6DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
