

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014772.D
 Acq On : 21 Apr 2023 00:05
 Operator : CG/JU
 Sample : 02340-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014772.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	19	rVB	906273	965158	14.17%	1.682%
2	3.487	47	51	57	rBV	27924	38223	0.56%	0.067%
3	3.769	95	99	104	rBV	11802	18384	0.27%	0.032%
4	3.916	122	124	141	rBV	175809	272273	4.00%	0.475%
5	4.163	162	166	172	rVB4	7491	11826	0.17%	0.021%
6	4.263	178	183	189	rVB	24899	33988	0.50%	0.059%
7	4.634	243	246	252	rVB7	5921	8633	0.13%	0.015%
8	4.775	266	270	276	rVB	13070	17656	0.26%	0.031%
9	5.199	336	342	344	rBV5	4557	7031	0.10%	0.012%
10	6.034	481	484	492	rVB8	4887	8278	0.12%	0.014%
11	7.287	690	697	705	rBV	213324	336225	4.94%	0.586%
12	7.463	717	727	738	rBV	852894	1327729	19.49%	2.314%
13	7.669	756	762	770	rBV	779502	1244211	18.27%	2.169%
14	7.816	784	787	794	rVB5	8730	14924	0.22%	0.026%
15	8.152	836	844	850	rBV	847303	1339295	19.66%	2.334%
16	8.204	850	853	858	rVB3	7301	10625	0.16%	0.019%
17	8.846	954	962	972	rBV	604996	966252	14.19%	1.684%
18	8.975	979	984	990	rVB9	3385	7980	0.12%	0.014%
19	9.110	1003	1007	1012	rVB7	6365	9293	0.14%	0.016%
20	9.316	1035	1042	1051	rBV	885244	1429661	20.99%	2.492%
21	9.475	1063	1069	1074	rBV7	11788	19621	0.29%	0.034%
22	10.046	1159	1166	1176	rBV	617459	988586	14.51%	1.723%
23	10.151	1180	1184	1191	rVB3	11938	20515	0.30%	0.036%
24	10.581	1249	1257	1269	rBV	1023997	1732510	25.44%	3.020%
25	10.975	1316	1324	1331	rBV	1109445	1884581	27.67%	3.285%
26	11.104	1338	1346	1355	rBV	1021209	1659331	24.36%	2.892%
27	11.628	1430	1435	1442	rVB2	8092	13484	0.20%	0.024%
28	11.734	1447	1453	1463	rVV4	19840	37175	0.55%	0.065%
29	12.228	1531	1537	1544	rVB3	21510	37225	0.55%	0.065%
30	12.545	1586	1591	1596	rVB2	22183	32379	0.48%	0.056%
31	13.063	1670	1679	1682	rBV10	5660	13368	0.20%	0.023%
32	14.175	1862	1868	1880	rBV	2131123	2937682	43.13%	5.120%
33	14.475	1912	1919	1931	rVV	2483009	3579928	52.56%	6.239%
34	14.781	1961	1971	1978	rBV	1630213	2484507	36.48%	4.330%
35	14.845	1978	1982	1991	rVB10	5289	9067	0.13%	0.016%
36	14.939	1991	1998	2006	rBV	152585	233423	3.43%	0.407%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014772.D
 Acq On : 21 Apr 2023 00:05
 Operator : CG/JU
 Sample : 02340-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

37	15.181	2035	2039	2045	rVB7	7061	11421	0.17%	0.020%
38	15.445	2081	2084	2088	rVB2	8874	10599	0.16%	0.018%
39	15.569	2099	2105	2111	rVB8	9955	16401	0.24%	0.029%
40	15.769	2131	2139	2149	rBV	3272812	4536176	66.60%	7.906%
41	15.869	2150	2156	2168	rVV	663148	917535	13.47%	1.599%
42	16.010	2176	2180	2186	rVB2	13881	20391	0.30%	0.036%
43	16.128	2196	2200	2205	rVB8	4016	7367	0.11%	0.013%
44	16.222	2211	2216	2220	rVB7	5253	9546	0.14%	0.017%
45	16.557	2266	2273	2276	rVB9	4561	8304	0.12%	0.014%
46	16.904	2328	2332	2336	rVB7	5438	8389	0.12%	0.015%
47	17.110	2362	2367	2372	rBV7	8152	13963	0.21%	0.024%
48	17.316	2397	2402	2406	rBV5	5272	10360	0.15%	0.018%
49	17.527	2431	2438	2445	rBV	1995811	2788688	40.94%	4.860%
50	17.627	2448	2455	2471	rVV	4255507	5502167	80.78%	9.590%
51	17.792	2481	2483	2488	rVB6	5618	8805	0.13%	0.015%
52	18.075	2527	2531	2536	rBV4	8356	11428	0.17%	0.020%
53	18.175	2543	2548	2553	rBV3	40504	55033	0.81%	0.096%
54	18.375	2578	2582	2588	rBV3	32577	44662	0.66%	0.078%
55	18.951	2677	2680	2686	rVB6	23155	30046	0.44%	0.052%
56	19.204	2719	2723	2728	rBV6	44005	64190	0.94%	0.112%
57	19.422	2755	2760	2765	rBV	43822	61756	0.91%	0.108%
58	19.486	2766	2771	2776	rVV	47597	69575	1.02%	0.121%
59	19.598	2787	2790	2796	rVB4	27081	32319	0.47%	0.056%
60	19.839	2825	2831	2841	rBV	5069095	6418198	94.23%	11.186%
61	21.598	3125	3130	3137	rBV	2309448	2959495	43.45%	5.158%
62	24.004	3531	3539	3556	rVB2	3253015	6811201	100.00%	11.871%
63	24.168	3560	3567	3577	rVB2	1556144	3197480	46.94%	5.573%




Sum of corrected areas: 57376522

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014772.D
Acq On : 21 Apr 2023 00:05
Operator : CG/JU
Sample : 02340-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

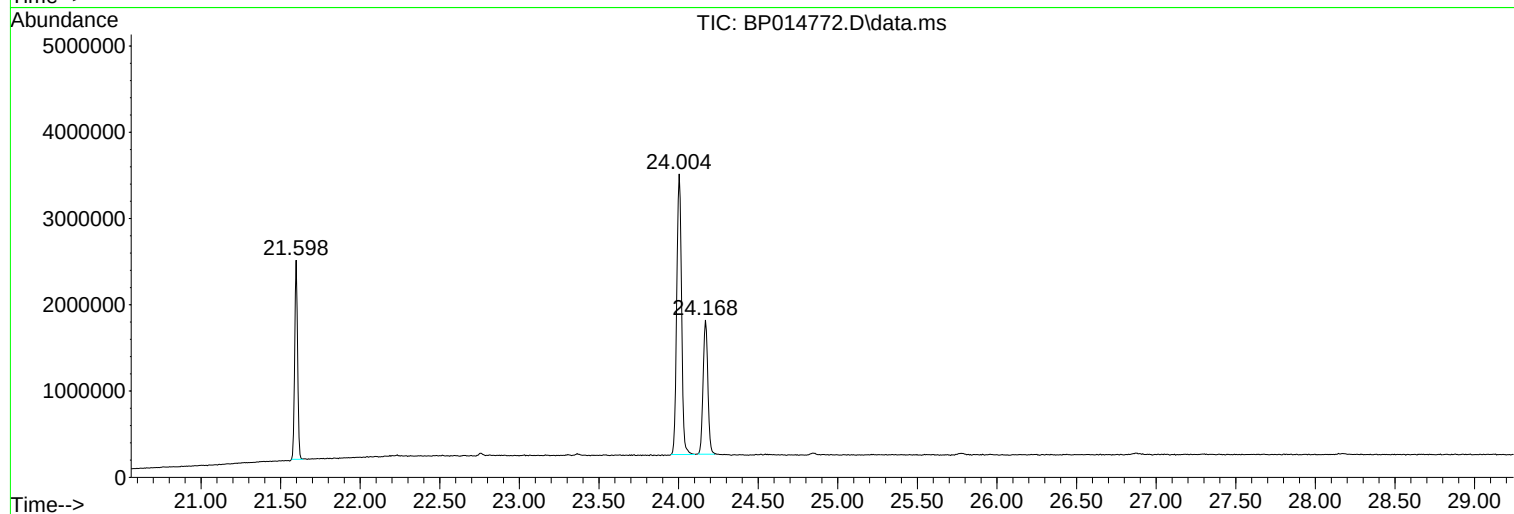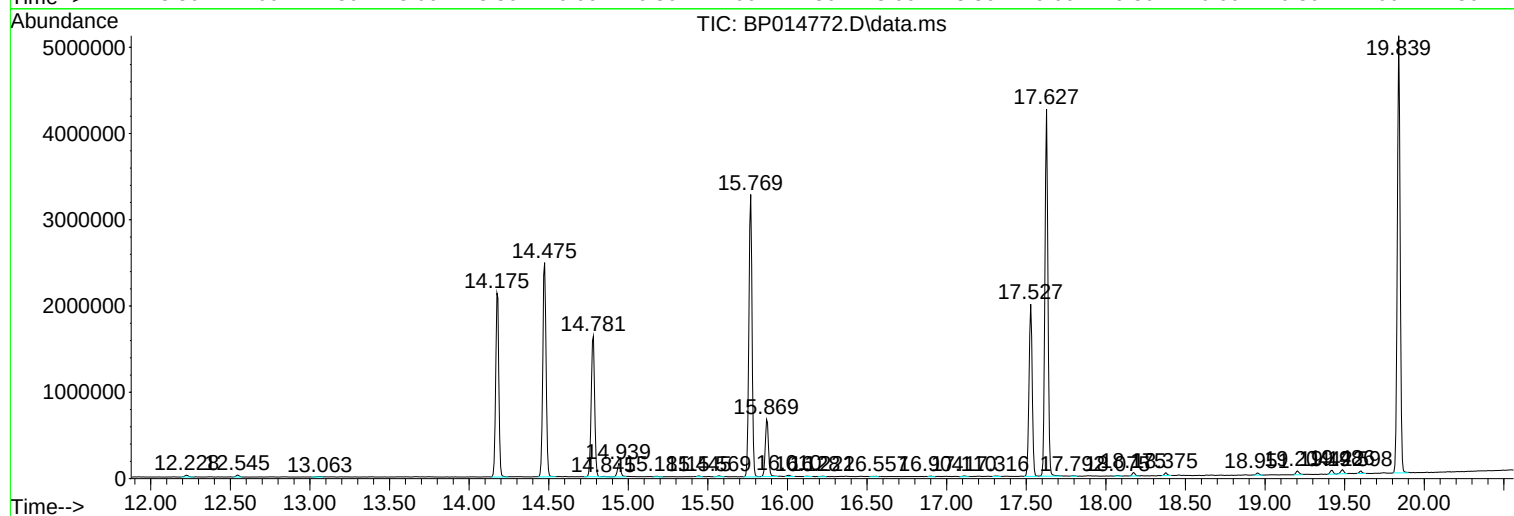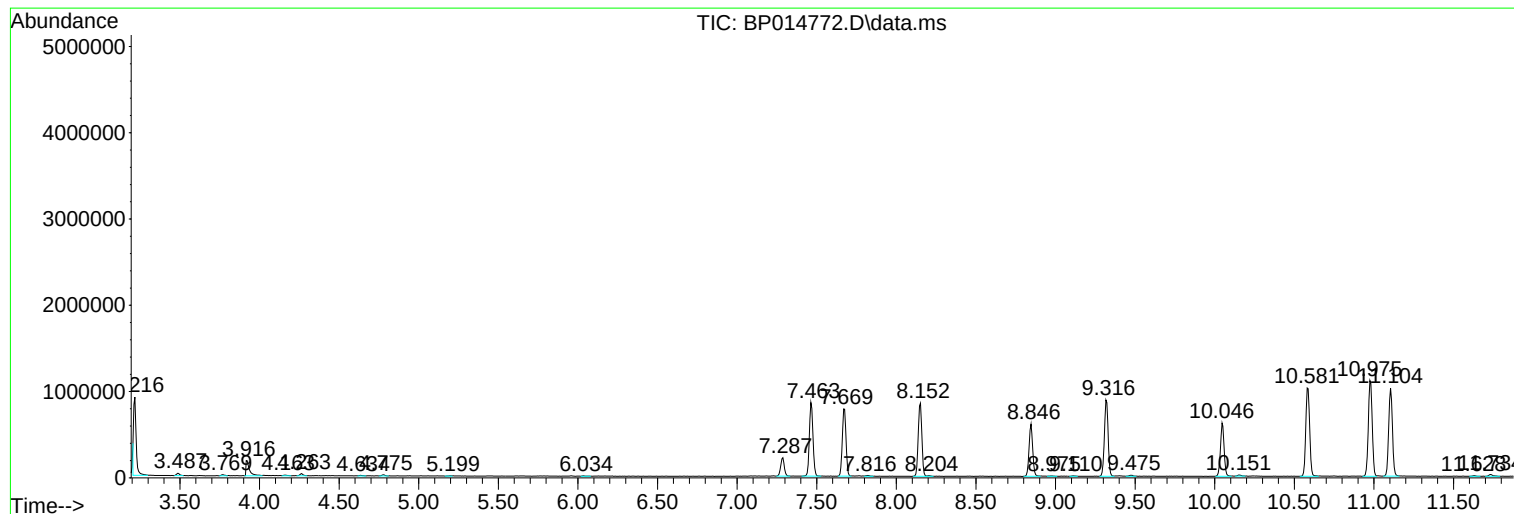

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014772.D
Acq On : 21 Apr 2023 00:05
Operator : CG/JU
Sample : 02340-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE17










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.216	14.41 ng/ul	965158	1,4-Dichlorobenzene-d4	8.152

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	43		
3	1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23		
5	Silane, tetramethyl-	88	C4H12Si	000075-76-3	17		

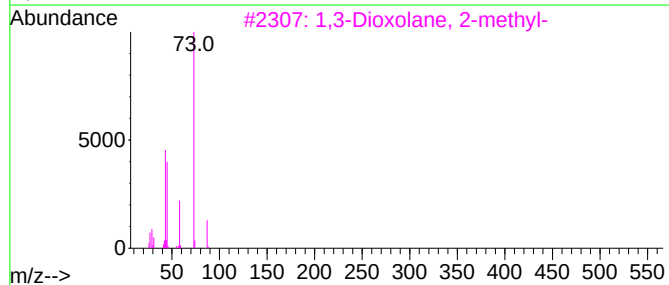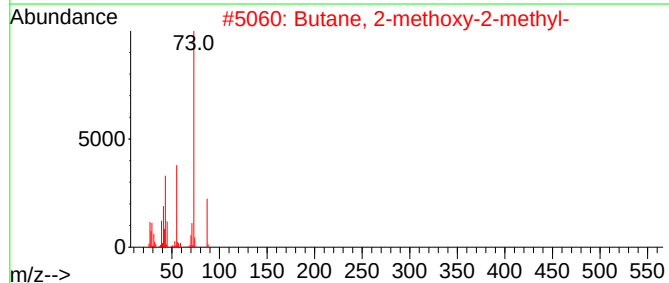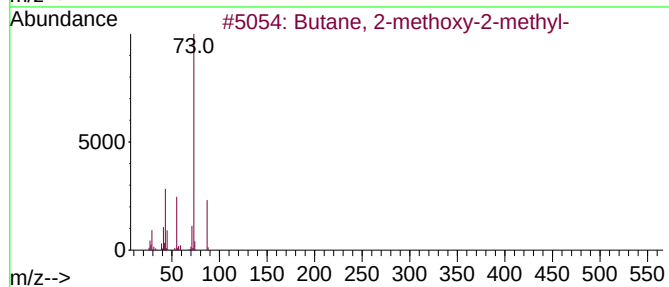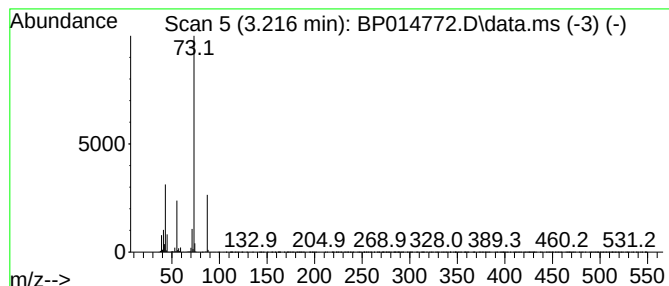

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014772.D
Acq On : 21 Apr 2023 00:05
Operator : CG/JU
Sample : 02340-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.216	14.4	ng/u1	965158	1	8.152	1339300	20.0