

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014774.D
 Acq On : 21 Apr 2023 01:12
 Operator : CG/JU
 Sample : 02340-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014774.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	3	5	22	rVB	1311720	1407499	20.40%	1.986%
2	3.458	42	46	50	rBV	171599	232556	3.37%	0.328%
3	3.522	55	57	68	rVB	26265	35111	0.51%	0.050%
4	3.764	94	98	105	rBV	20565	31803	0.46%	0.045%
5	3.917	121	124	141	rBV	303601	454760	6.59%	0.642%
6	4.164	162	166	171	rVB2	8439	11613	0.17%	0.016%
7	4.264	178	183	188	rBV	25431	33931	0.49%	0.048%
8	4.811	270	276	286	rVB	153357	226390	3.28%	0.319%
9	5.205	339	343	348	rBV5	5401	7752	0.11%	0.011%
10	7.287	688	697	706	rBV	311556	487394	7.06%	0.688%
11	7.463	719	727	740	rVB	1218862	1887515	27.36%	2.663%
12	7.675	755	763	772	rBV	1106215	1755130	25.44%	2.477%
13	7.763	775	778	783	rVB6	5340	8119	0.12%	0.011%
14	8.152	834	844	851	rBV	991210	1607133	23.29%	2.268%
15	8.746	939	945	952	rVB10	8253	14618	0.21%	0.021%
16	8.846	952	962	975	rBV	914952	1433855	20.78%	2.023%
17	9.322	1035	1043	1053	rBV	1281801	2090902	30.30%	2.950%
18	10.046	1158	1166	1179	rBV	935839	1517723	22.00%	2.142%
19	10.152	1180	1184	1191	rVB4	9414	18745	0.27%	0.026%
20	10.587	1248	1258	1275	rBV	1558517	2591483	37.56%	3.657%
21	10.975	1315	1324	1332	rBV	1413149	2350320	34.06%	3.316%
22	11.104	1338	1346	1355	rBV	1094417	1769583	25.65%	2.497%
23	11.734	1447	1453	1458	rBV9	7993	14087	0.20%	0.020%
24	12.357	1552	1559	1565	rBV9	5066	12168	0.18%	0.017%
25	12.546	1585	1591	1599	rVB2	30163	50926	0.74%	0.072%
26	12.640	1602	1607	1612	rBV8	5548	7969	0.12%	0.011%
27	12.763	1623	1628	1631	rBV7	4065	6965	0.10%	0.010%
28	13.663	1777	1781	1789	rBV7	6390	13107	0.19%	0.018%
29	13.781	1797	1801	1809	rVB	50092	70847	1.03%	0.100%
30	14.181	1862	1869	1885	rBV	3102683	4238963	61.43%	5.981%
31	14.304	1887	1890	1894	rVB6	6628	7713	0.11%	0.011%
32	14.357	1894	1899	1902	rBV	7660	11082	0.16%	0.016%
33	14.475	1912	1919	1927	rBV	3600939	5215197	75.58%	7.359%
34	14.781	1964	1971	1978	rVV	2156710	3130170	45.36%	4.417%
35	14.845	1978	1982	1987	rVB8	5515	8560	0.12%	0.012%
36	14.945	1993	1999	2004	rBV	208177	314631	4.56%	0.444%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014774.D
 Acq On : 21 Apr 2023 01:12
 Operator : CG/JU
 Sample : 02340-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

37	14.981	2004	2005	2012	rVB4	12356	15065	0.22%	0.021%
38	15.181	2034	2039	2041	rBV6	4899	8435	0.12%	0.012%
39	15.569	2099	2105	2108	rBV5	4568	8968	0.13%	0.013%
40	15.769	2131	2139	2148	rBV	4525629	6353620	92.08%	8.965%
41	15.869	2150	2156	2168	rVV	877057	1222195	17.71%	1.725%
42	16.010	2174	2180	2184	rVB2	20313	30678	0.44%	0.043%
43	16.128	2193	2200	2208	rBV	586002	772792	11.20%	1.090%
44	16.339	2230	2236	2242	rVB	5337	11047	0.16%	0.016%
45	16.545	2270	2271	2277	rVB7	6369	8610	0.12%	0.012%
46	16.692	2291	2296	2302	rBV2	38636	55510	0.80%	0.078%
47	17.269	2390	2394	2397	rBV6	5431	8060	0.12%	0.011%
48	17.310	2398	2401	2407	rVB5	7010	11123	0.16%	0.016%
49	17.528	2431	2438	2448	rBV	2473270	3409278	49.41%	4.811%
50	17.628	2448	2455	2471	rVV	4665954	6539639	94.78%	9.228%
51	18.233	2554	2558	2561	rBV6	7741	12984	0.19%	0.018%
52	18.381	2578	2583	2588	rBV2	51870	70519	1.02%	0.100%
53	19.416	2755	2759	2764	rBV2	54799	73036	1.06%	0.103%
54	19.486	2766	2771	2775	rVV	51567	73460	1.06%	0.104%
55	19.598	2787	2790	2794	rVB6	27757	31722	0.46%	0.045%
56	19.839	2825	2831	2837	rBV	5494760	6899993	100.00%	9.736%
57	21.269	3072	3074	3081	rBV5	40832	51565	0.75%	0.073%
58	21.598	3124	3130	3138	rBV	2207683	2907975	42.14%	4.103%
59	24.004	3531	3539	3555	rVB2	2970013	6212177	90.03%	8.766%
60	24.168	3560	3567	3585	rVB2	1384278	3005318	43.56%	4.241%




Sum of corrected areas: 70870089

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014774.D
Acq On : 21 Apr 2023 01:12
Operator : CG/JU
Sample : 02340-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

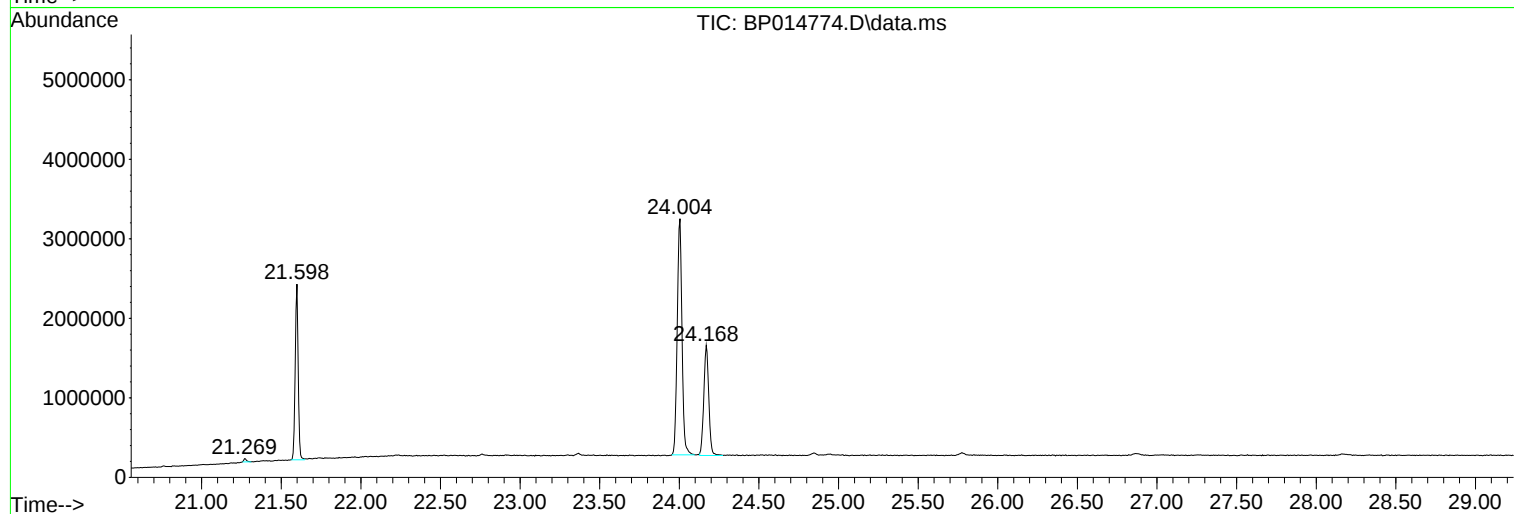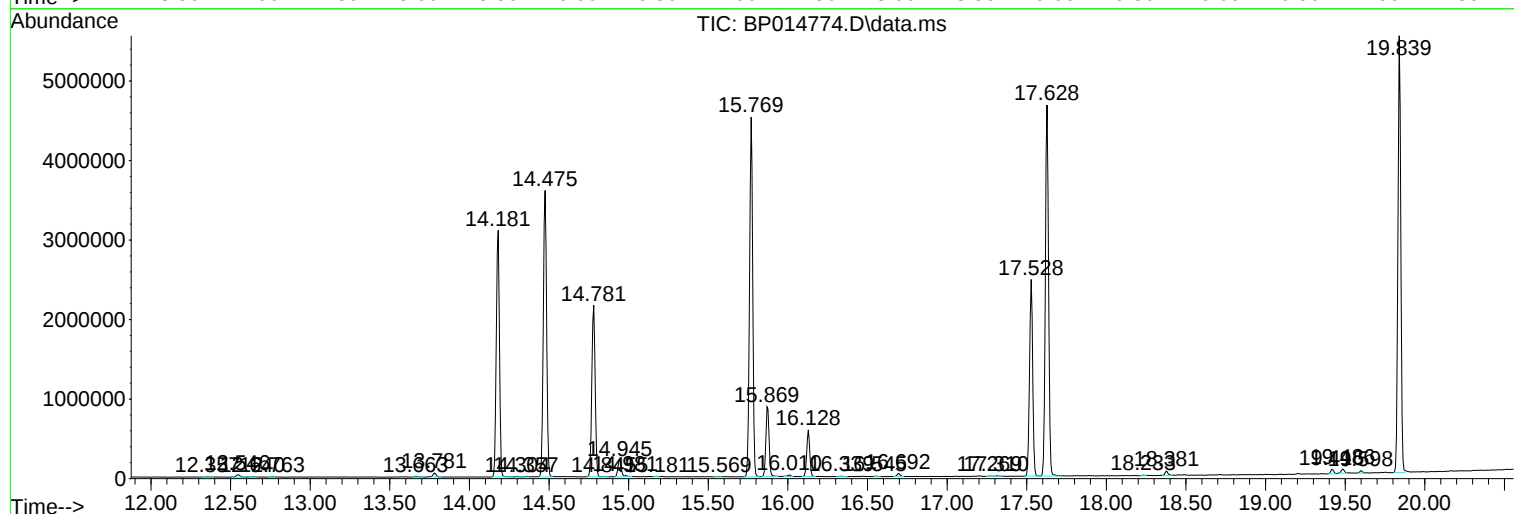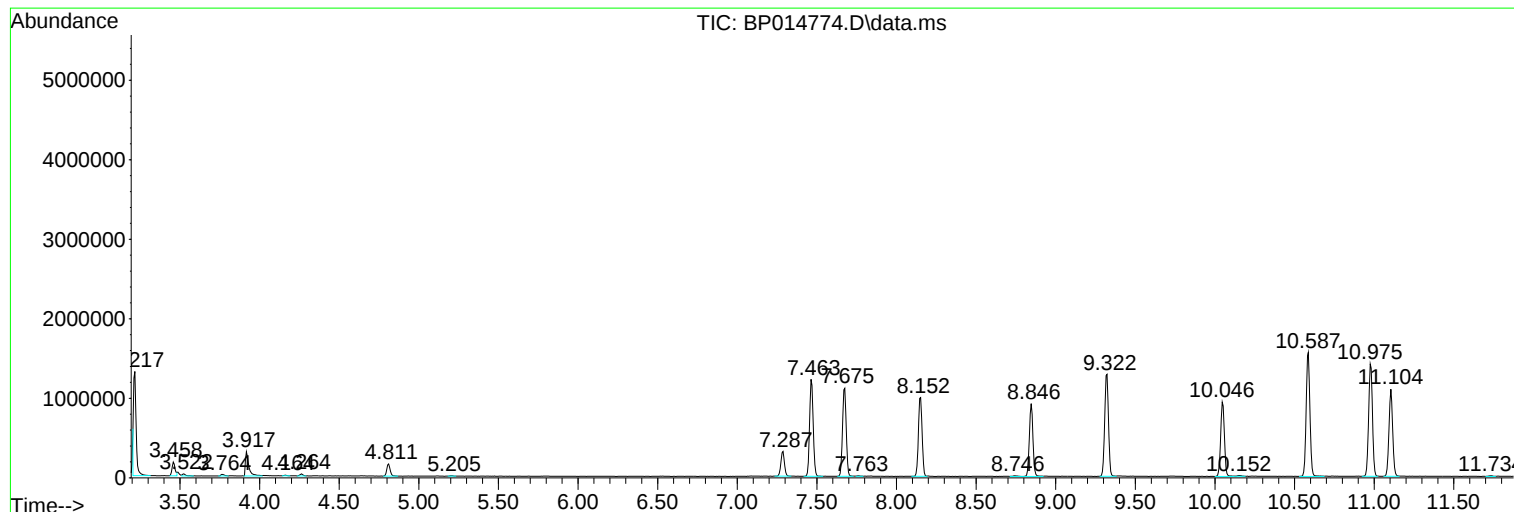

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014774.D
Acq On : 21 Apr 2023 01:12
Operator : CG/JU
Sample : 02340-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE20










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.217	17.52 ng/ul	1407500	1,4-Dichlorobenzene-d4	8.152

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	43		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40		
4	1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	23		
5	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17		

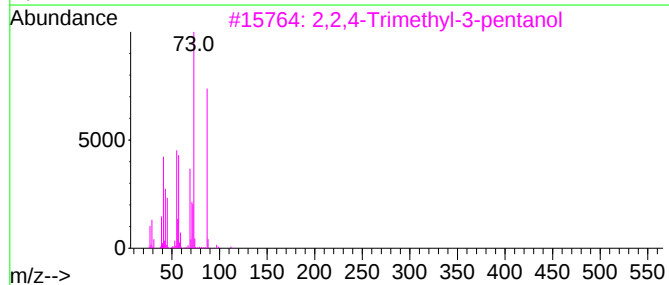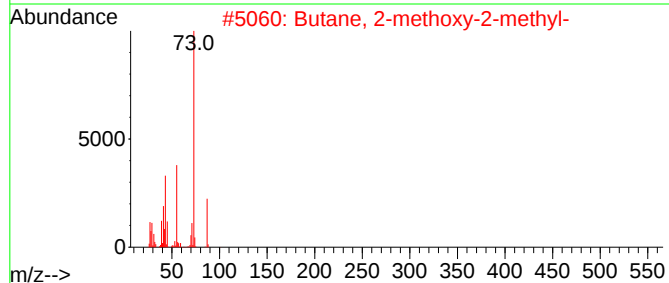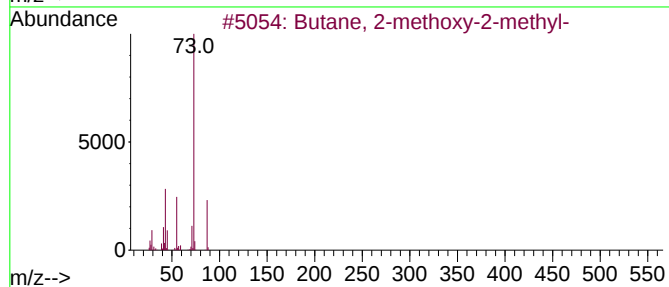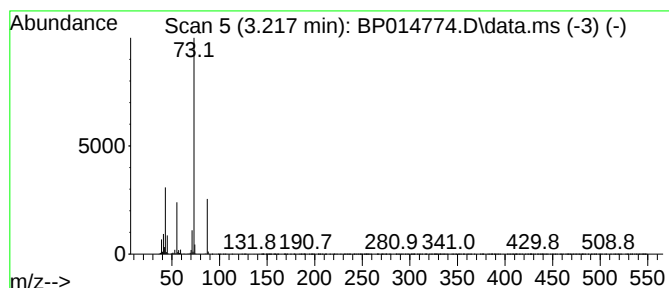

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014774.D
Acq On : 21 Apr 2023 01:12
Operator : CG/JU
Sample : 02340-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE20










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Benzophenone Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.128	4.94 ng/ul	772792	Acenaphthene-d10	14.781

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	95
3			Benzophenone	182	C13H10O	000119-61-9	94
4			Benzophenone	182	C13H10O	000119-61-9	93
5			Benzophenone	182	C13H10O	000119-61-9	91

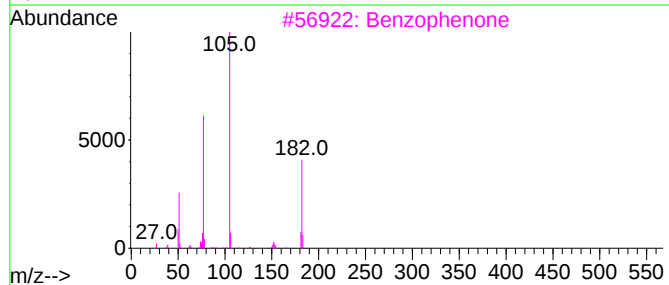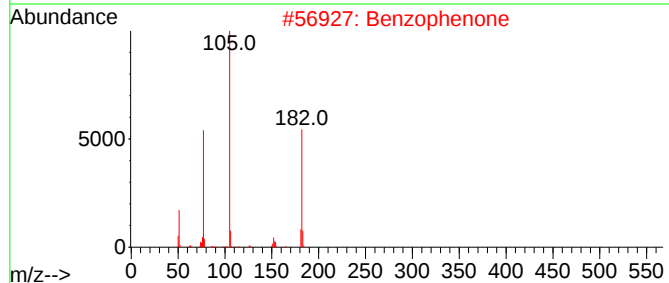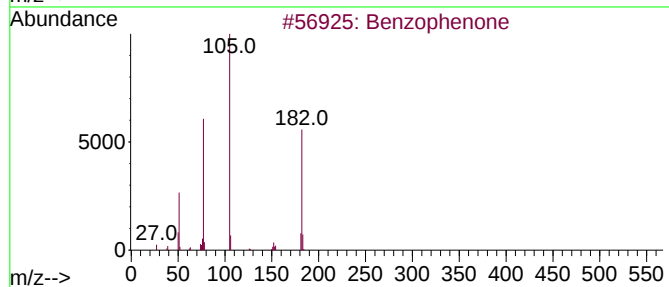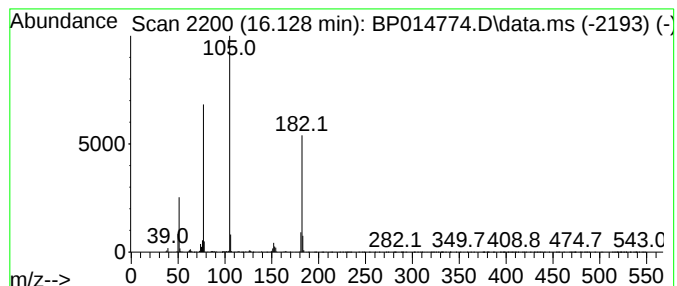

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014774.D
Acq On : 21 Apr 2023 01:12
Operator : CG/JU
Sample : 02340-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.217	17.5	ng/ul	1407500	1	8.152	1607130	20.0
Benzophenone	16.128	4.9	ng/ul	772792	3	14.781	3130170	20.0