

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
 Data File : BP014780.D
 Acq On : 21 Apr 2023 08:59
 Operator : CG/JU
 Sample : PB152276BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK276

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	10	rVB	59747	64317	1.23%	0.120%
2	3.493	47	52	60	rVB	70005	95896	1.83%	0.178%
3	3.916	121	124	144	rBV	646819	1014388	19.35%	1.885%
4	4.269	180	184	189	rBV2	17444	24470	0.47%	0.045%
5	7.293	691	698	709	rBV	934758	1487999	28.38%	2.765%
6	7.475	722	729	738	rBV	835082	1272792	24.28%	2.365%
7	7.681	757	764	772	rBV	979827	1536248	29.30%	2.855%
8	8.157	837	845	853	rBV	861883	1387321	26.46%	2.578%
9	8.857	957	964	974	rBV	1208558	1861656	35.51%	3.459%
10	9.328	1035	1044	1051	rBV	814877	1369195	26.12%	2.544%
11	10.057	1160	1168	1176	rBV	630128	1013257	19.33%	1.883%
12	10.598	1252	1260	1273	rBV	1102926	1819293	34.70%	3.381%
13	10.987	1318	1326	1335	rVB	1140135	1914619	36.52%	3.558%
14	11.116	1338	1348	1360	rBV	487389	811327	15.48%	1.508%
15	12.557	1588	1593	1598	rBV3	21888	35376	0.67%	0.066%
16	13.675	1776	1783	1791	rBV2	15642	27893	0.53%	0.052%
17	14.186	1863	1870	1881	rBV	1938254	2673743	51.00%	4.968%
18	14.486	1914	1921	1930	rBV	2313081	3333278	63.58%	6.194%
19	14.792	1966	1973	1980	rVB	1668839	2440877	46.56%	4.536%
20	14.957	1994	2001	2015	rBV	846711	1166759	22.26%	2.168%
21	15.198	2038	2042	2045	rVB6	4172	5469	0.10%	0.010%
22	15.722	2126	2131	2134	rBV7	8665	16618	0.32%	0.031%
23	15.780	2134	2141	2148	rVB	2941838	4038550	77.03%	7.504%
24	15.880	2153	2158	2166	rBV	576677	794291	15.15%	1.476%
25	16.022	2178	2182	2188	rVB4	14680	20561	0.39%	0.038%
26	16.169	2199	2207	2213	rBV5	7364	15086	0.29%	0.028%
27	16.563	2270	2274	2279	rVB8	5654	9741	0.19%	0.018%
28	16.816	2313	2317	2322	rBV8	6137	10347	0.20%	0.019%
29	16.998	2344	2348	2355	rVB5	11003	18504	0.35%	0.034%
30	17.322	2400	2403	2406	rBV5	6335	7803	0.15%	0.014%
31	17.363	2406	2410	2415	rVV5	7644	12463	0.24%	0.023%
32	17.539	2433	2440	2449	rBV	2062176	2779386	53.02%	5.165%
33	17.639	2450	2457	2470	rVV	3114695	4277517	81.59%	7.948%
34	17.910	2498	2503	2509	rBV8	9709	21590	0.41%	0.040%
35	18.069	2528	2530	2537	rVB7	8577	11289	0.22%	0.021%
36	18.386	2581	2584	2593	rBV7	16215	22733	0.43%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014780.D
Acq On : 21 Apr 2023 08:59
Operator : CG/JU
Sample : PB152276BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK276

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Title : SVOA CALIBRATION

37	18.974	2681	2684	2688	rBV5	10993	13165	0.25%	0.024%
38	19.427	2758	2761	2766	rBV3	35513	48010	0.92%	0.089%
39	19.498	2769	2773	2777	rBV	35081	54923	1.05%	0.102%
40	19.851	2827	2833	2843	rBV	3833602	4953524	94.49%	9.204%
41	21.610	3127	3132	3143	rBV	2250521	2954995	56.37%	5.491%
42	24.021	3534	3542	3562	rVB2	2547347	5242581	100.00%	9.742%
43	24.192	3564	3571	3584	rVB	1475617	3136529	59.83%	5.828%




Sum of corrected areas: 53816379

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014780.D
Acq On : 21 Apr 2023 08:59
Operator : CG/JU
Sample : PB152276BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK276

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

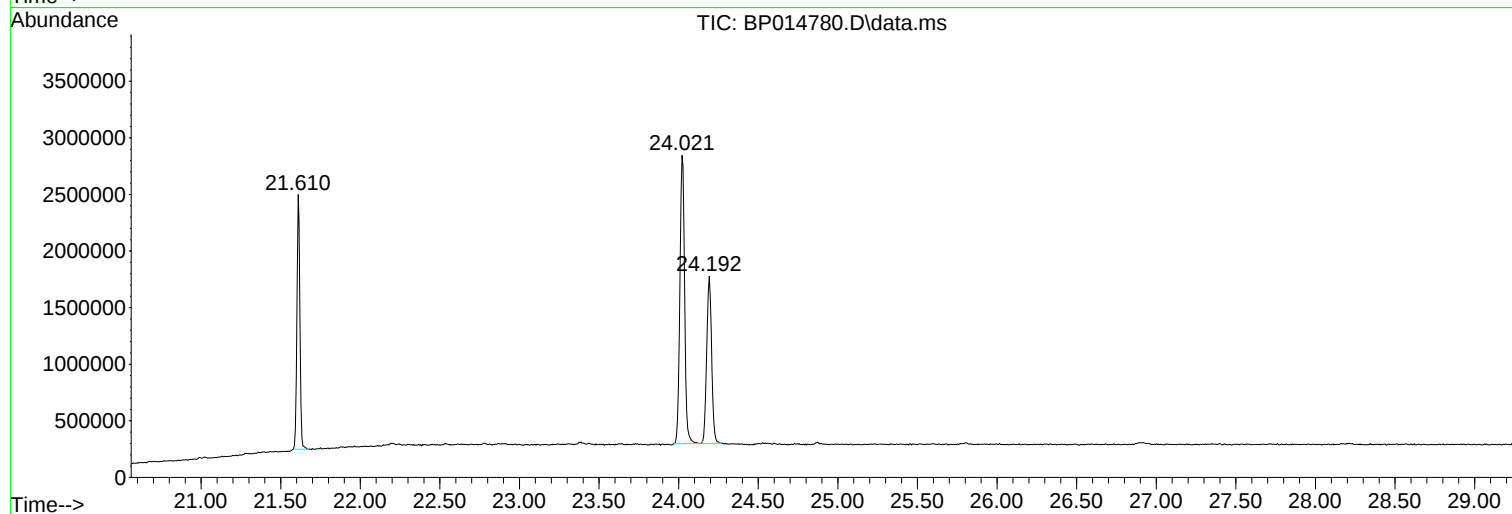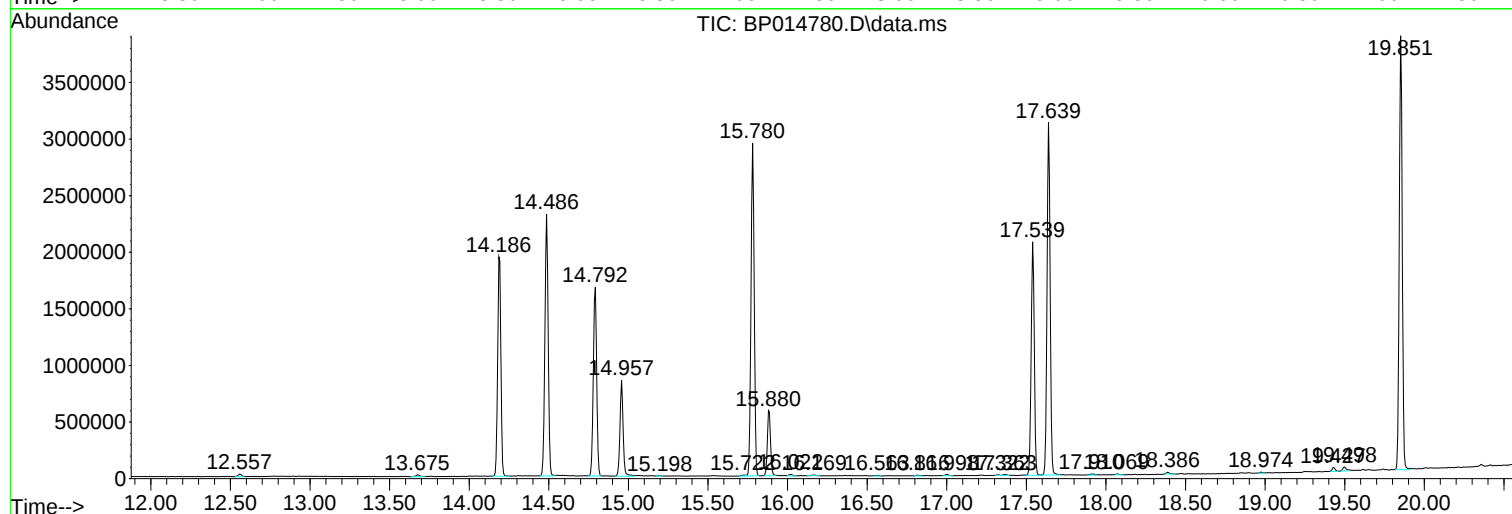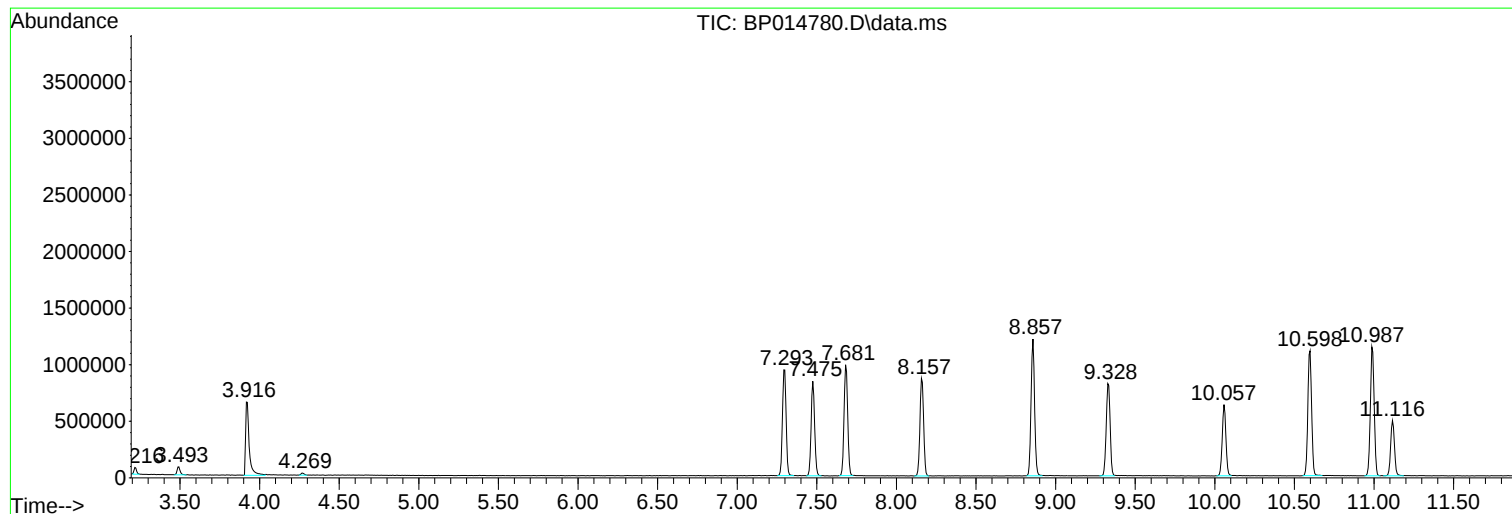

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014780.D
Acq On : 21 Apr 2023 08:59
Operator : CG/JU
Sample : PB152276BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK276

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042023\
Data File : BP014780.D
Acq On : 21 Apr 2023 08:59
Operator : CG/JU
Sample : PB152276BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK276

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc