

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010011.D
 Acq On : 21 Apr 2022 12:45
 Operator : CG/JU
 Sample : SST04026
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST040626

Quant Time: Apr 21 14:02:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 13:57:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	141370	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136	638869	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	453340	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	1021090	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.410	240	1084096	20.000	ng/ul	# 0.00
88) Perylene-d12	23.863	264	1013382	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	51104	16.133	ng/uL	0.00
4) Pyridine-d5	3.781	84	360925	41.326	ng/ul	0.00
7) Phenol-d5	7.105	99	507386	40.881	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	301463	40.799	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	384303	41.049	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	424621	40.983	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	207798	45.104	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	234161	46.360	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	439796	41.610	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	590574	39.231	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	1413581	39.696	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	1737655	41.188	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	266367	41.245	ng/ul	0.00
60) Fluorene-d10	15.569	176	1197581	39.977	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	263104	43.496	ng/ul	0.00
73) Anthracene-d10	17.428	188	1966473	40.223	ng/ul	0.00
81) Pyrene-d10	19.657	212	2407777	40.666	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.704	264	2145790	40.661	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.405	88	50261	15.565	ng/uL#	11
5) Pyridine	3.805	79	374865	41.138	ng/ul#	45
6) Benzaldehyde	7.075	77	310323	40.769	ng/ul	98
8) Phenol	7.128	94	507906	40.883	ng/ul#	93
10) Bis(2-Chloroethyl)ether	7.363	93	391721	40.479	ng/ul#	80
12) 2-Chlorophenol	7.505	128	387957	41.103	ng/ul	95
13) 2-Methylphenol	8.387	108	393398	40.608	ng/ul	99
14) 2,2'-oxybis(1-Chloropr...	8.475	45	579726	40.527	ng/ul#	85
16) Acetophenone	8.763	105	658060	40.312	ng/ul#	79
17) N-Nitroso-di-n-propyla...	8.757	70	350069	41.364	ng/ul#	74
18) 4-Methylphenol	8.716	108	436522	41.609	ng/ul	93
19) Hexachloroethane	9.028	117	160334	40.234	ng/ul#	81
22) Nitrobenzene	9.146	77	504223	42.639	ng/ul#	85
23) Isophorone	9.675	82	990496	40.648	ng/ul	97
25) 2-Nitrophenol	9.857	139	238889	44.344	ng/ul#	86
26) 2,4-Dimethylphenol	9.922	107	513695	40.182	ng/ul#	78
27) Bis(2-Chloroethoxy)met...	10.157	93	570025	39.844	ng/ul#	97
29) 2,4-Dichlorophenol	10.393	162	419156	40.906	ng/ul#	83
30) Naphthalene	10.799	128	1322501	40.250	ng/ul	97
32) 4-Chloroaniline	10.904	127	583949	39.199	ng/ul	98
33) Hexachlorobutadiene	11.093	225	286118	38.770	ng/ul	95
34) Caprolactam	11.675	113	82364	24.305	ng/ul#	10
35) 4-Chloro-3-methylphenol	12.028	107	507716	40.892	ng/ul#	71
36) 2-Methylnaphthalene	12.404	142	960578	40.017	ng/ul	93

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010011.D
 Acq On : 21 Apr 2022 12:45
 Operator : CG/JU
 Sample : SST04026
 Misc :
 ALS Vial : 6 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SST040626


Quant Time: Apr 21 14:02:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 13:57:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.622	142	968453	39.957	ng/ul#	95
39) 1,2,4,5-Tetrachloroben...	12.775	216	557465	40.192	ng/ul#	94
40) Hexachlorocyclopentadiene	12.757	237	312595	32.477	ng/ul	96
41) 2,4,6-Trichlorophenol	13.010	196	370334	41.810	ng/ul#	81
42) 2,4,5-Trichlorophenol	13.081	196	409507	42.781	ng/ul#	86
43) 1,1'-Biphenyl	13.410	154	1333483	40.314	ng/ul	94
44) 2-Chloronaphthalene	13.451	162	1026560	40.375	ng/ul	93
45) 2-Nitroaniline	13.651	65	359599	48.260	ng/ul#	80
47) Dimethylphthalate	14.028	163	1366945	39.883	ng/ul#	92
48) 2,6-Dinitrotoluene	14.145	165	296980	47.107	ng/ul	95
50) Acenaphthylene	14.298	152	1696397	40.745	ng/ul	95
51) 3-Nitroaniline	14.475	138	298679	45.572	ng/ul#	79
52) Acenaphthene	14.639	153	1092772	40.087	ng/ul	97
53) 2,4-Dinitrophenol	14.681	184	161191	42.300	ng/ul#	81
55) 4-Nitrophenol	14.787	109	235638	39.637	ng/ul#	50
56) Dibenzofuran	14.975	168	1604857	40.001	ng/ul	99
57) 2,4-Dinitrotoluene	14.934	165	429742	46.422	ng/ul#	84
58) 2,3,4,6-Tetrachlorophenol	15.198	232	361095	41.373	ng/ul#	86
59) Diethylphthalate	15.398	149	1400080	39.471	ng/ul	94
61) Fluorene	15.622	166	1321507	39.990	ng/ul	91
62) 4-Chlorophenyl-phenyle...	15.616	204	694290	39.513	ng/ul	97
63) 4-Nitroaniline	15.639	138	311615	47.470	ng/ul#	82
66) 4,6-Dinitro-2-methylph...	15.698	198	253663	42.188	ng/ul#	88
67) N-Nitrosodiphenylamine	15.828	169	1159388	39.665	ng/ul	94
68) 4-Bromophenyl-phenylether	16.516	248	431227	39.015	ng/ul	94
69) Hexachlorobenzene	16.633	284	497925	39.178	ng/ul#	89
70) Atrazine	16.786	200	475677	39.427	ng/ul	92
71) Pentachlorophenol	16.975	266	320174	37.218	ng/ul#	84
72) Phenanthrene	17.369	178	2192496	40.226	ng/ul	98
74) Anthracene	17.463	178	2223790	40.243	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.375	216	590996	40.033	ng/ul#	87
76) Pentachlorobenzene	14.898	250	573569	39.860	ng/ul	89
77) Carbazole	17.728	167	1987227	39.794	ng/ul#	96
78) Di-n-butylphthalate	18.280	149	2480765	40.397	ng/ul#	93
80) Fluoranthene	19.333	202	2741759	40.231	ng/ul#	95
82) Pyrene	19.686	202	2793712	40.432	ng/ul#	93
83) Butylbenzylphthalate	20.551	149	1199303	42.310	ng/ul#	81
84) 3,3'-Dichlorobenzidine	21.321	252	911587	39.460	ng/ul#	97
85) Benzo(a)anthracene	21.392	228	2752310	40.048	ng/ul	94
86) Bis(2-ethylhexyl)phtha...	21.316	149	1763599	41.364	ng/ul#	82
87) Chrysene	21.445	228	2687357	40.528	ng/ul	98
89) Di-n-octyl phthalate	22.257	149	3072460	43.274	ng/ul	100
90) Benzo(b)fluoranthene	23.116	252	2742520	40.733	ng/ul	99
91) Benzo(k)fluoranthene	23.163	252	2576153	41.931	ng/ul#	98
93) Benzo(a)pyrene	23.757	252	2554729	40.934	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.439	276	2622085	40.177	ng/ul#	93
95) Dibenzo(a,h)anthracene	26.451	278	2255675	39.860	ng/ul#	96
96) Benzo(g,h,i)perylene	27.221	276	2183425	40.575	ng/ul	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 21 14:02:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 13:57:49 2022
Response via : Initial Calibration







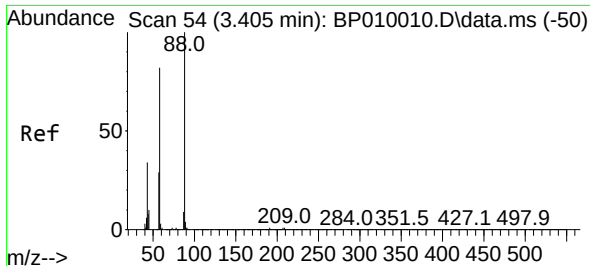

#2
1,4-Dioxane
Concen: 15.565 ng/uL
RT: 3.405 min Scan# 54
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion: 88 Resp: 50261
Ion Ratio Lower Upper
88 100
43 33.0 6.8 10.2#
58 90.1 28.4 42.6#

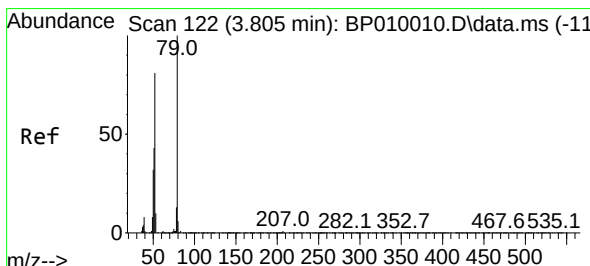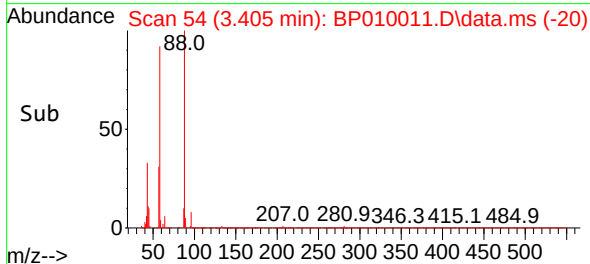

#5
Pyridine
Concen: 41.138 ng/uL
RT: 3.805 min Scan# 122
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion: 79 Resp: 374865
Ion Ratio Lower Upper
79 100
52 88.5 35.5 53.3#
51 41.7 20.2 30.4#


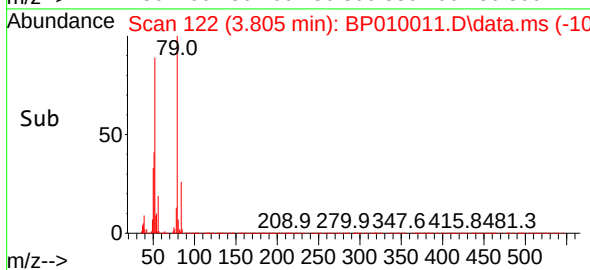






#6
Benzaldehyde
Concen: 40.769 ng/ul
RT: 7.075 min Scan# 611
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion: 77 Resp: 310323
Ion Ratio Lower Upper
77 100
105 96.2 77.0 115.4
106 92.7 77.0 115.4



#8
Phenol
Concen: 40.883 ng/ul
RT: 7.128 min Scan# 687
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion: 94 Resp: 507906
Ion Ratio Lower Upper
94 100
65 31.2 19.0 28.6#
66 45.2 34.6 51.8


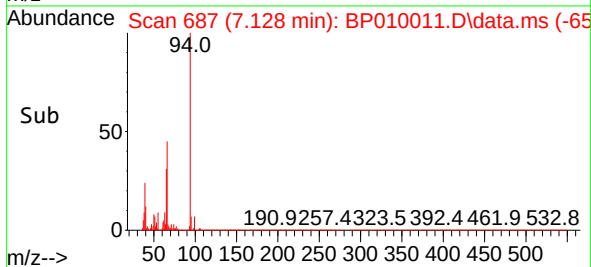

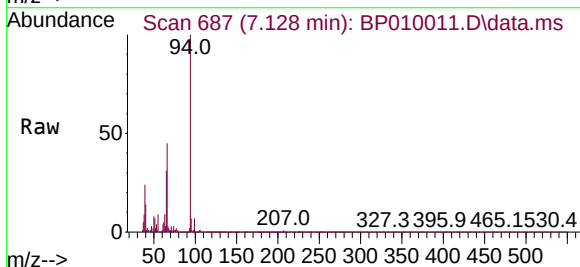




#10
 Bis(2-Chloroethyl)ether
 Concen: 40.479 ng/ul
 RT: 7.363 min Scan# 726
 Delta R.T. 0.006 min
 Lab File: BP010011.D
 Acq: 21 Apr 2022 12:45




Instrument :
 BNA_P
 ClientSampleId :
 SSTD040626


Tgt Ion: 93 Resp: 391721
 Ion Ratio Lower Upper
 93 100
 63 78.7 45.0 67.4#
 95 33.5 26.3 39.5

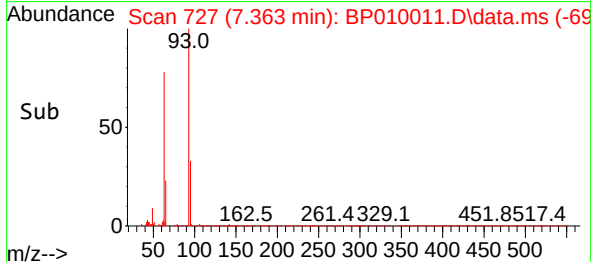

#12
 2-Chlorophenol
 Concen: 41.103 ng/ul
 RT: 7.505 min Scan# 751
 Delta R.T. 0.000 min
 Lab File: BP010011.D
 Acq: 21 Apr 2022 12:45

Tgt Ion: 128 Resp: 387957
 Ion Ratio Lower Upper
 128 100
 64 54.3 45.3 67.9
 130 32.4 29.0 43.6


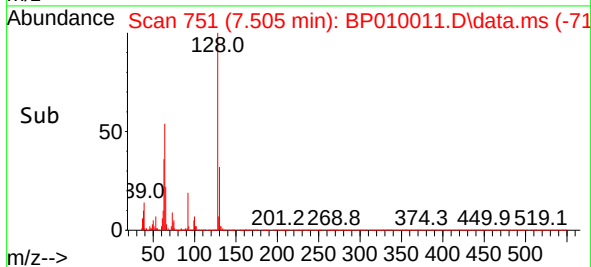

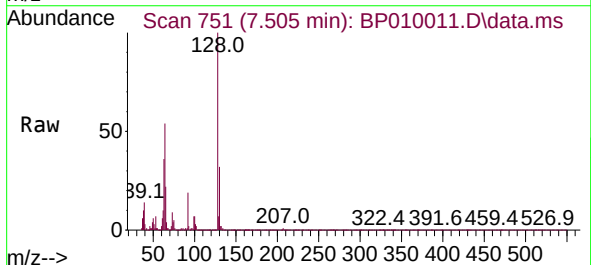




#13
2-Methylphenol
Concen: 40.608 ng/ul
RT: 8.387 min Scan# 900
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:108 Resp: 393398
Ion Ratio Lower Upper
108 100
107 89.2 70.8 106.2



#14
2,2'-oxybis(1-Chloropropane)
Concen: 40.527 ng/ul
RT: 8.475 min Scan# 916
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion: 45 Resp: 579726
Ion Ratio Lower Upper
45 100
77 14.1 17.1 25.7#
79 10.7 13.2 19.8#



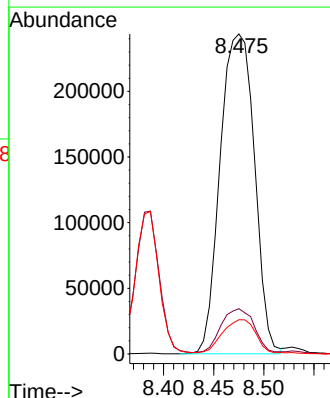





#16
Acetophenone
Concen: 40.312 ng/ul
RT: 8.763 min Scan# 965
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:105 Resp: 658060
Ion Ratio Lower Upper
105 100
77 81.3 53.4 80.2#
51 30.8 13.8 20.8#



#17
N-Nitroso-di-n-propylamine
Concen: 41.364 ng/ul
RT: 8.757 min Scan# 964
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion: 70 Resp: 350069
Ion Ratio Lower Upper
70 100
42 62.0 31.8 47.8#
101 10.1 15.6 23.4#
130 20.6 13.7 20.5#



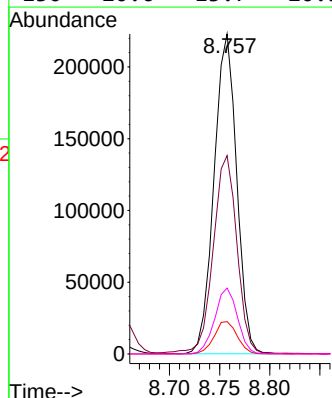





#18
4-Methylphenol
Concen: 41.609 ng/ul
RT: 8.716 min Scan# 91
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:108 Resp: 436522
Ion Ratio Lower Upper
108 100
107 111.3 83.6 125.4

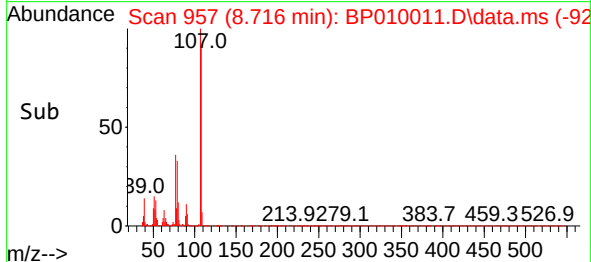

#19
Hexachloroethane
Concen: 40.234 ng/ul
RT: 9.028 min Scan# 1010
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:117 Resp: 160334
Ion Ratio Lower Upper
117 100
201 105.1 106.5 159.7#
199 65.6 59.0 88.6

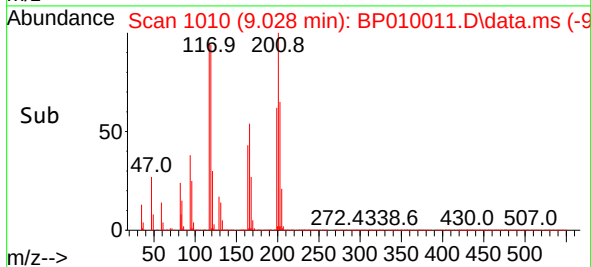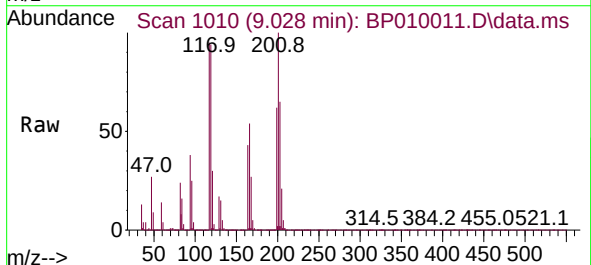



#22

Nitrobenzene

Concen: 42.639 ng/ul

RT: 9.146 min Scan# 110

Delta R.T. 0.006 min

Lab File: BP010011.D

Acq: 21 Apr 2022 12:45

Instrument :

BNA_P

ClientSampleId :

SSTD040626





Tgt Ion: 77 Resp: 504223

Ion Ratio Lower Upper

77 100

123 43.1 42.3 63.5

65 14.2 5.8 8.8#



#23

Isophorone

Concen: 40.648 ng/ul

RT: 9.675 min Scan# 1120

Delta R.T. 0.006 min

Lab File: BP010011.D

Acq: 21 Apr 2022 12:45




Tgt Ion: 82 Resp: 990496


Ion Ratio Lower Upper

82 100

95 8.2 7.8 11.8

138 17.0 12.9 19.3


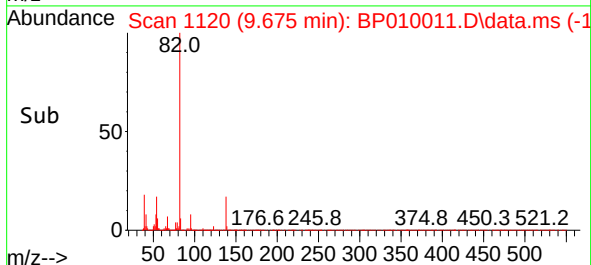
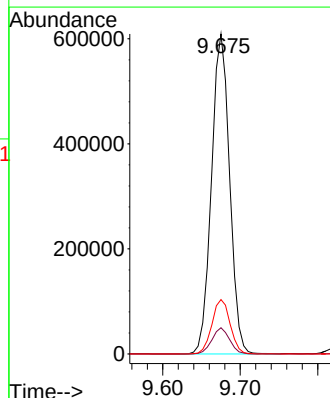
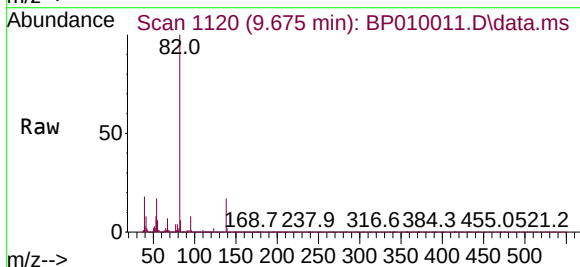




#25
2-Nitrophenol
Concen: 44.344 ng/ul
RT: 9.857 min Scan# 1151
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:139 Resp: 238889
Ion Ratio Lower Upper
139 100
65 59.6 49.4 74.2
109 36.1 44.7 67.1#



#26
2,4-Dimethylphenol
Concen: 40.182 ng/ul
RT: 9.922 min Scan# 1162
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:107 Resp: 513695
Ion Ratio Lower Upper
107 100
121 49.1 34.1 51.1
122 80.9 46.3 69.5#







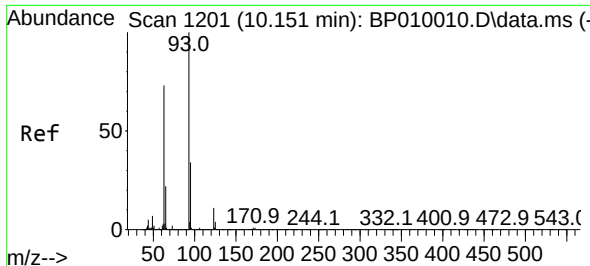

#27
Bis(2-Chloroethoxy)methane
Concen: 39.844 ng/ul
RT: 10.157 min Scan# 11
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion: 93 Resp: 570025
Ion Ratio Lower Upper
93 100
95 32.0 26.2 39.4
123 11.1 6.2 9.4#

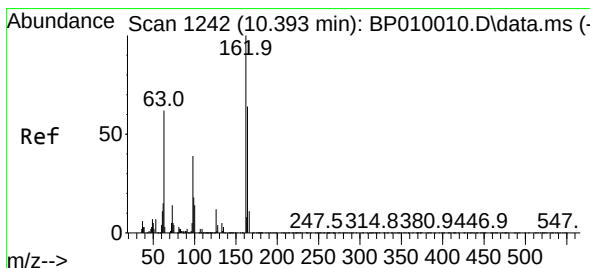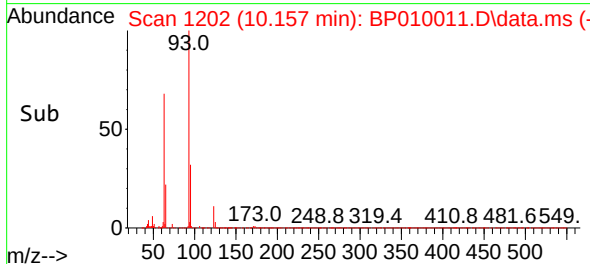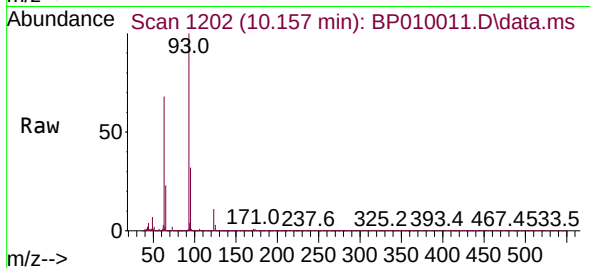

#29
2,4-Dichlorophenol
Concen: 40.906 ng/ul
RT: 10.393 min Scan# 1242
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:162 Resp: 419156
Ion Ratio Lower Upper
162 100
164 65.9 37.0 55.6#
98 39.9 31.0 46.6


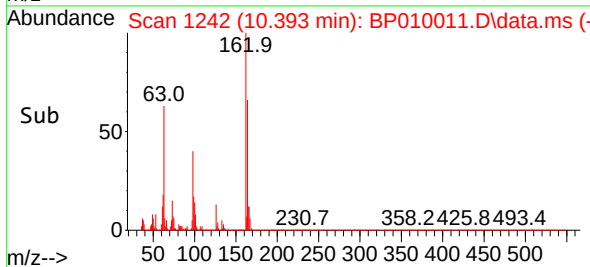

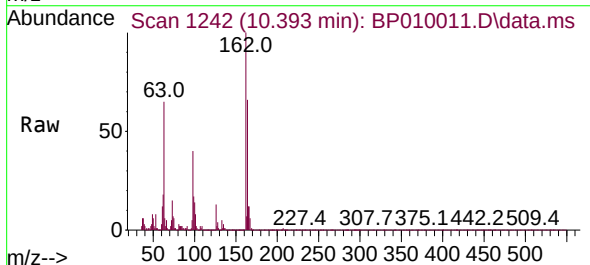




#30
Naphthalene
Concen: 40.250 ng/ul
RT: 10.799 min Scan# 1311
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:128 Resp: 1322501
Ion Ratio Lower Upper
128 100
129 10.7 8.6 13.0
127 12.9 12.2 18.4

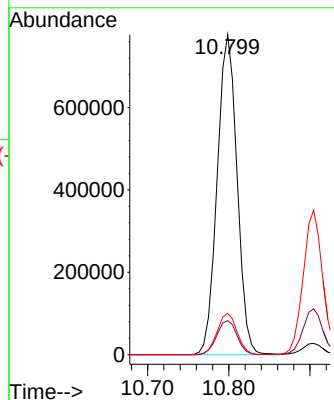

#32
4-Chloroaniline
Concen: 39.199 ng/ul
RT: 10.904 min Scan# 1329
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:127 Resp: 583949
Ion Ratio Lower Upper
127 100
129 31.8 24.6 37.0

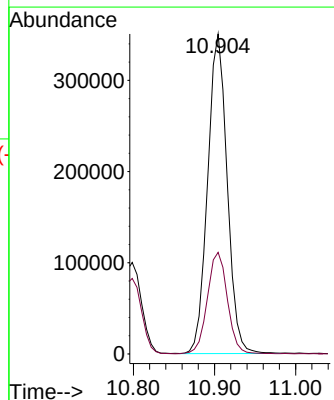



#33

Hexachlorobutadiene

Concen: 38.770 ng/ul

RT: 11.093 min Scan# 11

Delta R.T. 0.000 min

Lab File: BP010011.D

Acq: 21 Apr 2022 12:45

Instrument :

BNA_P

ClientSampleId :

SSTD040626





Tgt Ion:225 Resp: 286118

Ion Ratio Lower Upper

225 100

223 62.3 53.4 80.0

227 63.6 53.8 80.8



#34

Caprolactam

Concen: 24.305 ng/ul

RT: 11.675 min Scan# 1460

Delta R.T. 0.012 min

Lab File: BP010011.D

Acq: 21 Apr 2022 12:45




Tgt Ion:113 Resp: 82364


Ion Ratio Lower Upper

113 100

55 180.3 58.2 87.2#

56 137.6 68.6 103.0#









#35
4-Chloro-3-methylphenol
Concen: 40.892 ng/ul
RT: 12.028 min Scan# 1519
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:107 Resp: 507716
Ion Ratio Lower Upper
107 100
144 24.5 15.8 23.8#
142 73.2 38.9 58.3#



#36
2-Methylnaphthalene
Concen: 40.017 ng/ul
RT: 12.404 min Scan# 1584
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:142 Resp: 960578
Ion Ratio Lower Upper
142 100
141 87.0 64.3 96.5


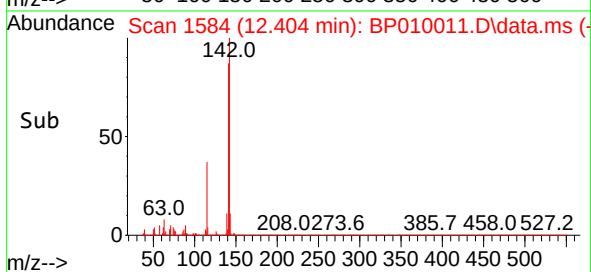






#37
1-Methylnaphthalene
Concen: 39.957 ng/ul
RT: 12.622 min Scan# 1621
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:142 Resp: 968453
Ion Ratio Lower Upper
142 100
141 91.9 69.8 104.8
116 4.1 5.6 8.4#

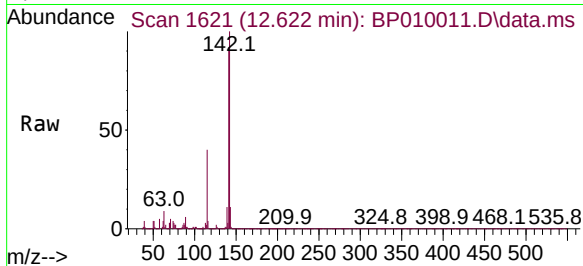

#39
1,2,4,5-Tetrachlorobenzene
Concen: 40.192 ng/ul
RT: 12.775 min Scan# 1647
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:216 Resp: 557465
Ion Ratio Lower Upper
216 100
214 77.2 58.2 87.2
179 21.3 14.2 21.2#
108 15.6 15.3 22.9




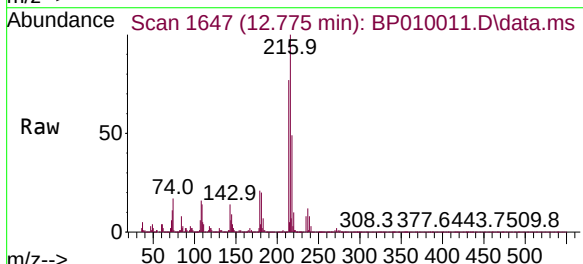




#40
Hexachlorocyclopentadiene
Concen: 32.477 ng/ul
RT: 12.757 min Scan# 1644
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:237 Resp: 312595
Ion Ratio Lower Upper
237 100
235 63.4 53.2 79.8
272 12.1 10.8 16.2

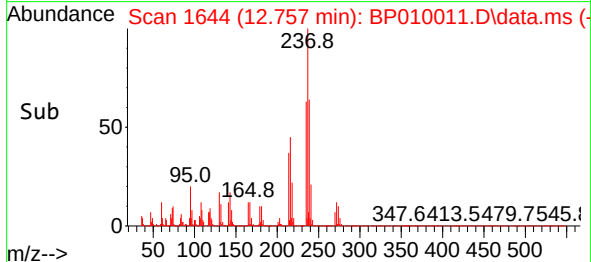

#41
2,4,6-Trichlorophenol
Concen: 41.810 ng/ul
RT: 13.010 min Scan# 1687
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:196 Resp: 370334
Ion Ratio Lower Upper
196 100
198 98.5 64.1 96.1#
200 31.1 19.9 29.9#





#42

2,4,5-Trichlorophenol

Concen: 42.781 ng/ul

RT: 13.081 min Scan# 1699

Delta R.T. 0.000 min

Lab File: BP010011.D

Acq: 21 Apr 2022 12:45

Instrument :

BNA_P

ClientSampleId :

SSTD040626





Tgt Ion:196 Resp: 409507

Ion Ratio Lower Upper

196 100

198 97.7 68.6 103.0

200 31.3 32.8 49.2#



#43

1,1'-Biphenyl

Concen: 40.314 ng/ul

RT: 13.410 min Scan# 1755

Delta R.T. 0.000 min

Lab File: BP010011.D

Acq: 21 Apr 2022 12:45




Tgt Ion:154 Resp: 1333483


Ion Ratio Lower Upper

154 100

153 39.6 28.6 43.0

76 12.2 8.5 12.7









#44
2-Chloronaphthalene
Concen: 40.375 ng/ul
RT: 13.451 min Scan# 1762
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:162 Resp: 1026560
Ion Ratio Lower Upper
162 100
164 32.5 27.5 41.3
127 40.5 37.1 55.7

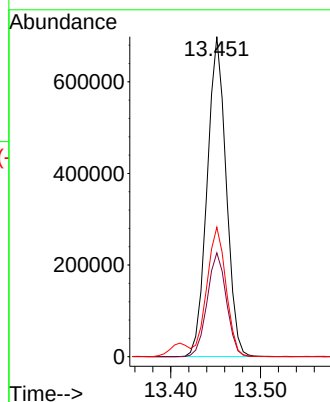

#45
2-Nitroaniline
Concen: 48.260 ng/ul
RT: 13.651 min Scan# 1796
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion: 65 Resp: 359599
Ion Ratio Lower Upper
65 100
92 65.1 77.9 116.9#
138 94.2 81.5 122.3



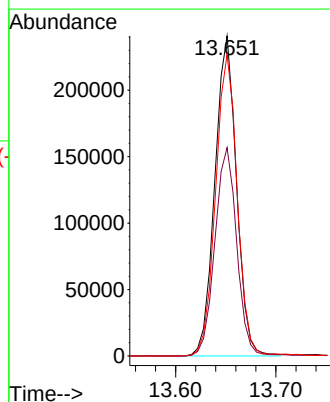





#47
Dimethylphthalate
Concen: 39.883 ng/ul
RT: 14.028 min Scan# 1860
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:163 Resp: 1366945
Ion Ratio Lower Upper
163 100
194 4.3 4.1 6.1
164 10.2 11.3 16.9#



#48
2,6-Dinitrotoluene
Concen: 47.107 ng/ul
RT: 14.145 min Scan# 1880
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:165 Resp: 296980
Ion Ratio Lower Upper
165 100
89 59.9 51.7 77.5
121 21.5 18.3 27.5


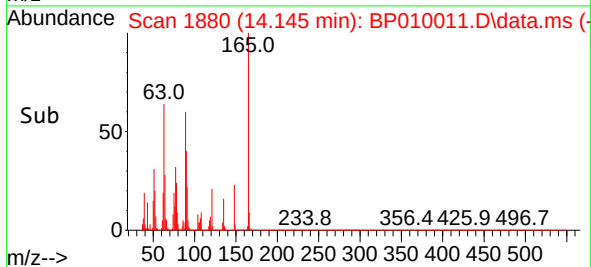

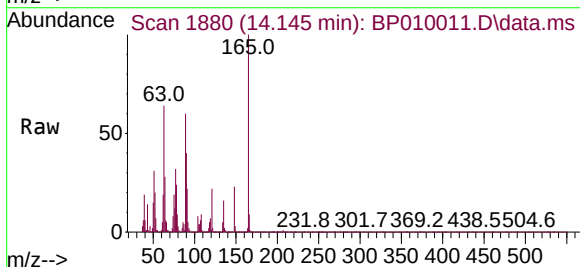




#50
Acenaphthylene
Concen: 40.745 ng/ul
RT: 14.298 min Scan# 1905
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:152 Resp: 1696397
Ion Ratio Lower Upper
152 100
151 19.7 18.3 27.5
153 12.9 11.0 16.6



#51
3-Nitroaniline
Concen: 45.572 ng/ul
RT: 14.475 min Scan# 1936
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:138 Resp: 298679
Ion Ratio Lower Upper
138 100
108 11.5 15.8 23.8#
92 119.3 117.1 175.7


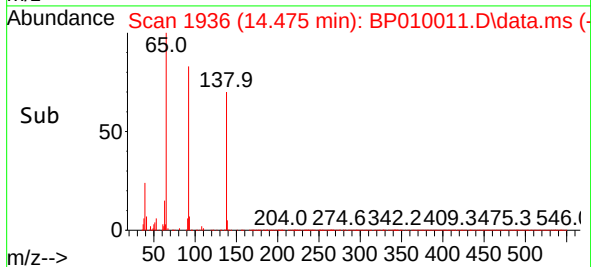

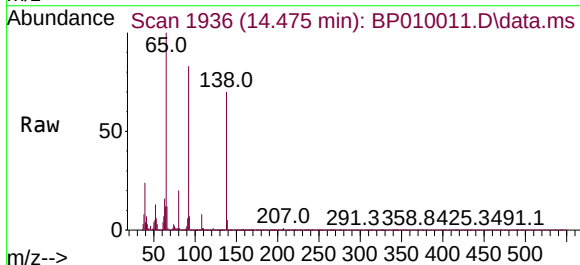


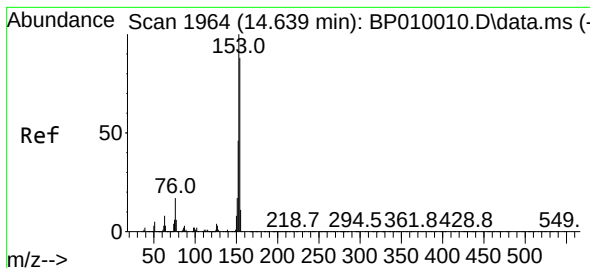

#52
Acenaphthene
Concen: 40.087 ng/ul
RT: 14.639 min Scan# 1964
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:153 Resp: 1092772
Ion Ratio Lower Upper
153 100
152 46.3 34.3 51.5
154 89.4 70.0 105.0

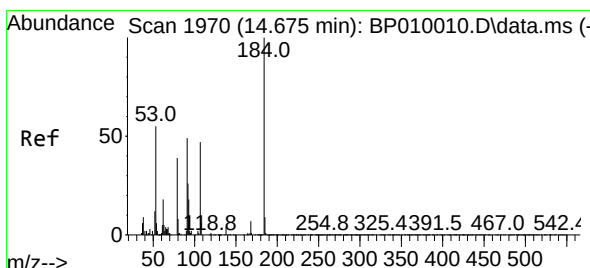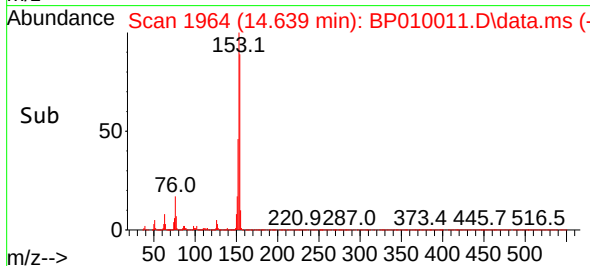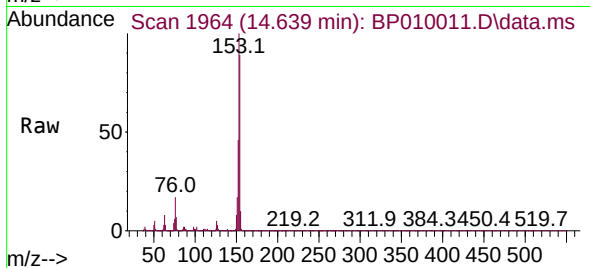

#53
2,4-Dinitrophenol
Concen: 42.300 ng/ul
RT: 14.681 min Scan# 1971
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:184 Resp: 161191
Ion Ratio Lower Upper
184 100
63 68.5 34.6 52.0#
154 66.4 57.7 86.5


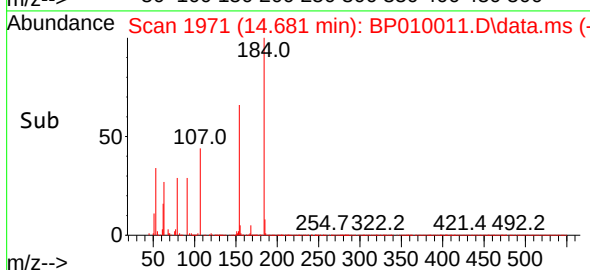

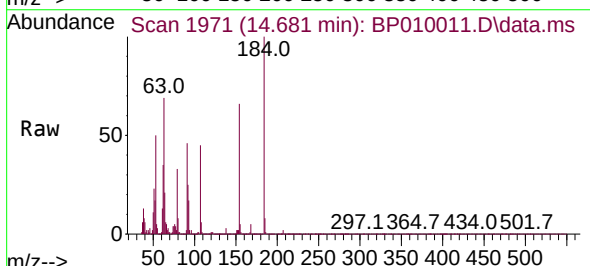




#55
4-Nitrophenol
Concen: 39.637 ng/ul
RT: 14.787 min Scan# 1987
Delta R.T. 0.012 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:109 Resp: 235638
Ion Ratio Lower Upper
109 100
139 117.8 61.4 92.2#
65 129.0 65.3 97.9#



#56
Dibenzofuran
Concen: 40.001 ng/ul
RT: 14.975 min Scan# 2021
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:168 Resp: 1604857
Ion Ratio Lower Upper
168 100
139 38.5 30.1 45.1









#57
2,4-Dinitrotoluene
Concen: 46.422 ng/ul
RT: 14.934 min Scan# 2014
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:165 Resp: 429742
Ion Ratio Lower Upper
165 100
63 47.4 29.5 44.3#
182 2.9 2.8 4.2



#58
2,3,4,6-Tetrachlorophenol
Concen: 41.373 ng/ul
RT: 15.198 min Scan# 2059
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:232 Resp: 361095
Ion Ratio Lower Upper
232 100
131 43.0 25.4 38.2#
130 2.3 4.2 6.2#
166 29.8 28.1 42.1



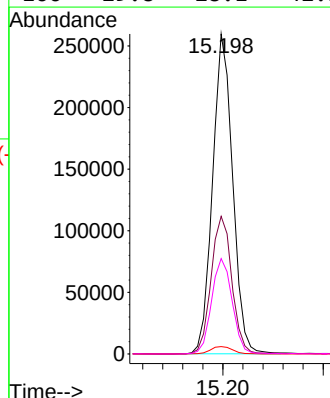





#59
Diethylphthalate
Concen: 39.471 ng/ul
RT: 15.398 min Scan# 2092
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:149 Resp: 1400080
Ion Ratio Lower Upper
149 100
177 23.2 22.0 33.0
150 12.7 10.2 15.2



#61
Fluorene
Concen: 39.990 ng/ul
RT: 15.622 min Scan# 2131
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:166 Resp: 1321507
Ion Ratio Lower Upper
166 100
165 97.3 70.3 105.5
167 13.4 9.5 14.3









#62
4-Chlorophenyl-phenylether
Concen: 39.513 ng/ul
RT: 15.616 min Scan# 2130
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:204 Resp: 694290
Ion Ratio Lower Upper
204 100
206 33.1 27.6 41.4
141 60.5 46.6 69.8



#63
4-Nitroaniline
Concen: 47.470 ng/ul
RT: 15.639 min Scan# 2134
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:138 Resp: 311615
Ion Ratio Lower Upper
138 100
92 57.0 41.6 62.4
108 96.2 97.6 146.4#


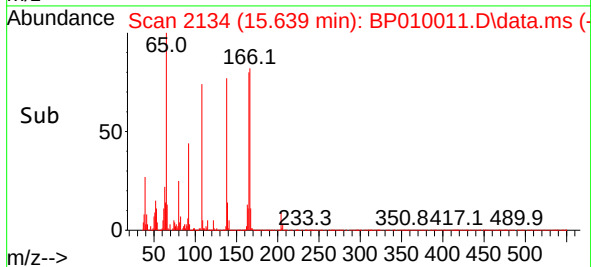

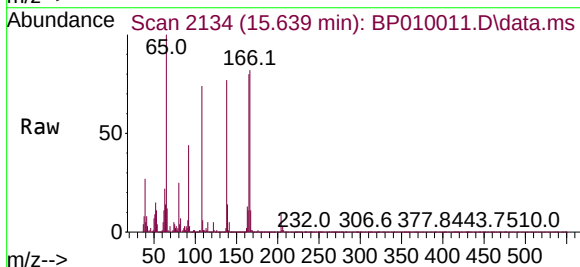




#66
4,6-Dinitro-2-methylphenol
Concen: 42.188 ng/ul
RT: 15.698 min Scan# 2144
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:198 Resp: 253663
Ion Ratio Lower Upper
198 100
182 3.9 6.0 9.0#
77 28.1 17.7 26.5#



#67
N-Nitrosodiphenylamine
Concen: 39.665 ng/ul
RT: 15.828 min Scan# 2166
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:169 Resp: 1159388
Ion Ratio Lower Upper
169 100
168 66.1 48.3 72.5
167 35.3 29.6 44.4









#68
4-Bromophenyl-phenylether
Concen: 39.015 ng/ul
RT: 16.516 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:248 Resp: 431227
Ion Ratio Lower Upper
248 100
250 97.7 79.4 119.0
141 72.8 67.2 100.8



#69
Hexachlorobenzene
Concen: 39.178 ng/ul
RT: 16.633 min Scan# 2303
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:284 Resp: 497925
Ion Ratio Lower Upper
284 100
142 34.8 19.2 28.8#
249 32.8 27.4 41.2









#70
Atrazine
Concen: 39.427 ng/ul
RT: 16.786 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:200 Resp: 475677
Ion Ratio Lower Upper
200 100
173 24.6 19.2 28.8
215 47.6 32.2 48.4



#71
Pentachlorophenol
Concen: 37.218 ng/ul
RT: 16.975 min Scan# 2361
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:266 Resp: 320174
Ion Ratio Lower Upper
266 100
264 63.1 57.3 85.9
268 62.9 65.7 98.5#









#72
Phenanthrene
Concen: 40.226 ng/ul
RT: 17.369 min Scan# 2428
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:178 Resp: 2192496
Ion Ratio Lower Upper
178 100
179 15.4 11.7 17.5
176 18.8 14.5 21.7

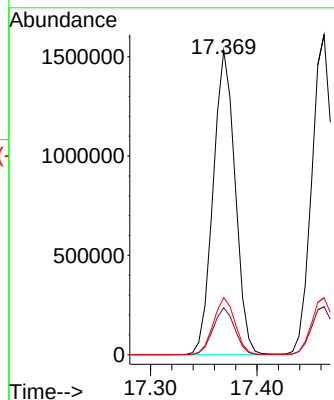

#74
Anthracene
Concen: 40.243 ng/ul
RT: 17.463 min Scan# 2444
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:178 Resp: 2223790
Ion Ratio Lower Upper
178 100
179 15.0 12.3 18.5
176 17.8 13.4 20.2



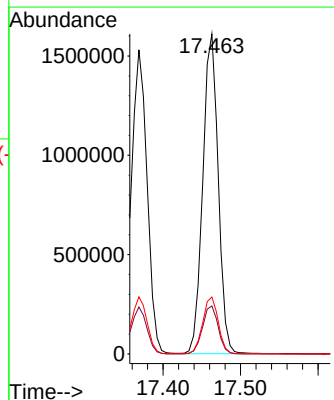





#75
1,2,3,4-Tetrachlorobenzene
Concen: 40.033 ng/uL
RT: 13.375 min Scan# 1749
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:216 Resp: 590996
Ion Ratio Lower Upper
216 100
214 78.0 50.4 75.6#
218 47.3 35.2 52.8



#76
Pentachlorobenzene
Concen: 39.860 ng/uL
RT: 14.898 min Scan# 2008
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:250 Resp: 573569
Ion Ratio Lower Upper
250 100
248 63.7 43.5 65.3
252 64.3 46.5 69.7









#77
Carbazole
Concen: 39.794 ng/ul
RT: 17.728 min Scan# 2488
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:167 Resp: 1987227
Ion Ratio Lower Upper
167 100
166 21.0 15.8 23.8
139 13.1 8.3 12.5#



#78
Di-n-butylphthalate
Concen: 40.397 ng/ul
RT: 18.280 min Scan# 2583
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:149 Resp: 2480765
Ion Ratio Lower Upper
149 100
150 9.2 9.6 14.4#
104 5.2 6.2 9.4#









#80
 Fluoranthene
 Concen: 40.231 ng/u1
 RT: 19.333 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP010011.D
 Acq: 21 Apr 2022 12:45




Instrument :
 BNA_P
 ClientSampleId :
 SSTD040626


Tgt Ion:202 Resp: 2741759
 Ion Ratio Lower Upper
 202 100
 101 9.1 9.6 14.4#
 100 7.2 6.3 9.5



#82
 Pyrene
 Concen: 40.432 ng/u1
 RT: 19.686 min Scan# 2822
 Delta R.T. 0.006 min
 Lab File: BP010011.D
 Acq: 21 Apr 2022 12:45

Tgt Ion:202 Resp: 2793712
 Ion Ratio Lower Upper
 202 100
 101 10.9 10.6 15.8
 100 9.3 9.8 14.6#





#83

Butylbenzylphthalate

Concen: 42.310 ng/ul

RT: 20.551 min Scan# 2969

Delta R.T. 0.000 min

Lab File: BP010011.D

Acq: 21 Apr 2022 12:45

Instrument :

BNA_P

ClientSampleId :

SSTD040626





Tgt Ion:149 Resp: 1199303

Ion Ratio Lower Upper

149 100

91 73.2 71.1 106.7

206 22.5 28.8 43.2#



#84

3,3'-Dichlorobenzidine

Concen: 39.460 ng/ul

RT: 21.321 min Scan# 3100

Delta R.T. 0.000 min

Lab File: BP010011.D

Acq: 21 Apr 2022 12:45




Tgt Ion:252 Resp: 911587


Ion Ratio Lower Upper

252 100

254 64.0 49.8 74.6

126 9.7 4.3 6.5#





#85

Benzo(a)anthracene

Concen: 40.048 ng/ul

RT: 21.392 min Scan# 3112

Delta R.T. 0.000 min

Lab File: BP010011.D

Acq: 21 Apr 2022 12:45

Instrument :

BNA_P

ClientSampleId :

SSTD040626





Tgt Ion:228 Resp: 2752310

Ion Ratio Lower Upper

228 100

229 19.5 18.2 27.2

226 26.0 22.8 34.2



#86

Bis(2-ethylhexyl)phthalate

Concen: 41.364 ng/ul

RT: 21.316 min Scan# 3099

Delta R.T. 0.000 min

Lab File: BP010011.D

Acq: 21 Apr 2022 12:45




Tgt Ion:149 Resp: 1763599


Ion Ratio Lower Upper

149 100

167 28.7 32.8 49.2#

279 5.1 5.6 8.4#









#87
Chrysene
Concen: 40.528 ng/ul
RT: 21.445 min Scan# 3121
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:228 Resp: 2687357
Ion Ratio Lower Upper
228 100
226 29.1 22.7 34.1
229 20.1 15.2 22.8



#89
Di-n-octyl phthalate
Concen: 43.274 ng/ul
RT: 22.257 min Scan# 3259
Delta R.T. 0.000 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:149 Resp: 3072460









#90
Benzo(b)fluoranthene
Concen: 40.733 ng/ul
RT: 23.116 min Scan# 3404
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45




Instrument :
BNA_P
ClientSampleId :
SSTD040626


Tgt Ion:252 Resp: 2742520
Ion Ratio Lower Upper
252 100
253 22.3 17.4 26.0
125 8.4 7.3 10.9

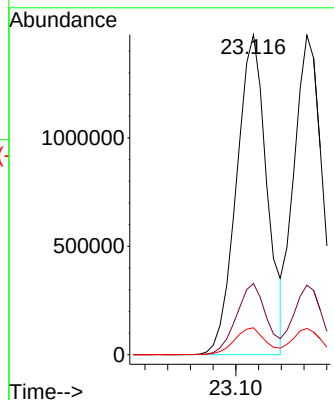

#91
Benzo(k)fluoranthene
Concen: 41.931 ng/ul
RT: 23.163 min Scan# 3413
Delta R.T. 0.006 min
Lab File: BP010011.D
Acq: 21 Apr 2022 12:45

Tgt Ion:252 Resp: 2576153
Ion Ratio Lower Upper
252 100
253 21.8 17.9 26.9
125 8.2 5.1 7.7#

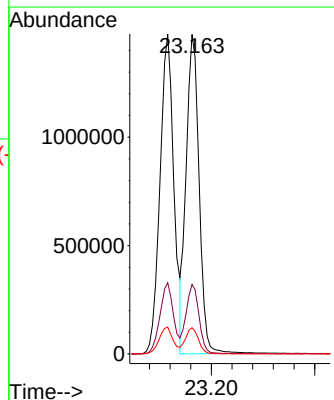



#93

Benzo(a)pyrene

Concen: 40.934 ng/ul

RT: 23.757 min Scan# 3

Delta R.T. 0.006 min

Lab File: BP010011.D

Acq: 21 Apr 2022 12:45

Instrument :

BNA_P

ClientSampleId :

SSTD040626





Tgt Ion:252 Resp: 2554729

Ion Ratio Lower Upper

252 100

253 21.6 17.5 26.3

125 9.3 6.4 9.6



#94

Indeno(1,2,3-cd)pyrene

Concen: 40.177 ng/ul

RT: 26.439 min Scan# 3970

Delta R.T. 0.012 min

Lab File: BP010011.D

Acq: 21 Apr 2022 12:45




Tgt Ion:276 Resp: 2622085


Ion Ratio Lower Upper

276 100

138 20.4 12.3 18.5

277 25.8 19.3 28.9









#95
 Dibenzo(a,h)anthracene
 Concen: 39.860 ng/ul
 RT: 26.451 min Scan# 3970
 Delta R.T. 0.012 min
 Lab File: BP010011.D
 Acq: 21 Apr 2022 12:45

Instrument :
 BNA_P
 ClientSampleId :
 SSTD040626

Tgt Ion:278 Resp: 2255675
 Ion Ratio Lower Upper
 278 100
 139 13.0 6.6 10.0#
 279 23.4 18.4 27.6



#96
 Benzo(g,h,i)perylene
 Concen: 40.575 ng/ul
 RT: 27.221 min Scan# 4103
 Delta R.T. 0.012 min
 Lab File: BP010011.D
 Acq: 21 Apr 2022 12:45

Tgt Ion:276 Resp: 2183425
 Ion Ratio Lower Upper
 276 100
 138 17.0 11.6 17.4
 277 23.5 15.9 23.9

