

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010014.D
 Acq On : 21 Apr 2022 15:03
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV629

Quant Time: Apr 21 19:00:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	154042	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	701982	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	508662	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	1106760	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.410	240	1055162	20.000	ng/ul	# 0.00
88) Perylene-d12	23.863	264	910119	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	29282	8.289	ng/uL	0.00
4) Pyridine-d5	3.787	84	204992	20.628	ng/ul	0.00
7) Phenol-d5	7.105	99	286216	20.427	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	177573	21.121	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	224219	21.608	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	244072	21.024	ng/ul	0.00
21) Nitrobenzene-d5	9.105	128	118704	21.261	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	134319	22.028	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	253385	21.346	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	373150	21.924	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	826047	20.877	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	1012549	21.144	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	146799	20.153	ng/ul	0.00
60) Fluorene-d10	15.569	176	702512	20.640	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	138576	19.802	ng/ul	0.00
73) Anthracene-d10	17.428	188	1127415	21.056	ng/ul	0.00
81) Pyrene-d10	19.657	212	1332955	22.213	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.704	264	1034546	21.682	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.405	88	29685	8.087	ng/uL#	18
5) Pyridine	3.805	79	212583	20.579	ng/ul#	42
6) Benzaldehyde	7.075	77	159707	21.329	ng/ul	94
8) Phenol	7.128	94	290045	20.602	ng/ul#	93
10) Bis(2-Chloroethyl)ether	7.364	93	230189	21.222	ng/ul#	79
12) 2-Chlorophenol	7.505	128	222057	21.215	ng/ul	95
13) 2-Methylphenol	8.387	108	223841	20.731	ng/ul	98
14) 2,2'-oxybis(1-Chloropr...	8.475	45	346676	21.540	ng/ul#	85
16) Acetophenone	8.764	105	387030	21.368	ng/ul#	77
17) N-Nitroso-di-n-propyla...	8.752	70	208831	22.006	ng/ul#	74
18) 4-Methylphenol	8.711	108	247723	20.838	ng/ul	88
19) Hexachloroethane	9.028	117	94207	21.420	ng/ul#	82
22) Nitrobenzene	9.146	77	292100	21.354	ng/ul#	87
23) Isophorone	9.675	82	579651	21.454	ng/ul	96
25) 2-Nitrophenol	9.858	139	139585	21.614	ng/ul#	85
26) 2,4-Dimethylphenol	9.922	107	298206	21.328	ng/ul#	79
27) Bis(2-Chloroethoxy)met...	10.158	93	338017	21.345	ng/ul#	98
29) 2,4-Dichlorophenol	10.393	162	245090	21.479	ng/ul#	83
30) Naphthalene	10.799	128	779650	21.220	ng/ul	97
32) 4-Chloroaniline	10.905	127	368357	21.962	ng/ul	97
33) Hexachlorobutadiene	11.093	225	168487	20.834	ng/ul	96
34) Caprolactam	11.669	113	49653	12.097	ng/ul#	1
35) 4-Chloro-3-methylphenol	12.028	107	297316	21.569	ng/ul#	71
36) 2-Methylnaphthalene	12.404	142	563728	21.156	ng/ul	91

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010014.D
 Acq On : 21 Apr 2022 15:03
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 9 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SICV629


Quant Time: Apr 21 19:00:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.622	142	569130	21.035	ng/ul#	94
39) 1,2,4,5-Tetrachloroben...	12.775	216	329201	20.948	ng/ul#	92
40) Hexachlorocyclopentadiene	12.757	237	172545	19.482	ng/ul	95
41) 2,4,6-Trichlorophenol	13.010	196	213941	21.041	ng/ul#	81
42) 2,4,5-Trichlorophenol	13.081	196	237947	21.508	ng/ul#	87
43) 1,1'-Biphenyl	13.410	154	789670	21.049	ng/ul	93
44) 2-Chloronaphthalene	13.451	162	612367	21.092	ng/ul	93
45) 2-Nitroaniline	13.651	65	200783	21.328	ng/ul#	84
47) Dimethylphthalate	14.028	163	802072	20.857	ng/ul#	93
48) 2,6-Dinitrotoluene	14.146	165	166827	21.139	ng/ul	95
50) Acenaphthylene	14.299	152	1010550	21.304	ng/ul	95
51) 3-Nitroaniline	14.475	138	109123	15.264	ng/ul#	84
52) Acenaphthene	14.640	153	648046	21.010	ng/ul	98
53) 2,4-Dinitrophenol	14.681	184	77703	17.620	ng/ul#	81
55) 4-Nitrophenol	14.781	109	125921	19.897	ng/ul#	48
56) Dibenzofuran	14.975	168	952479	20.854	ng/ul	98
57) 2,4-Dinitrotoluene	14.934	165	244843	21.237	ng/ul#	84
58) 2,3,4,6-Tetrachlorophenol	15.198	232	206893	21.038	ng/ul#	86
59) Diethylphthalate	15.393	149	821165	20.994	ng/ul	93
61) Fluorene	15.622	166	780851	20.823	ng/ul	92
62) 4-Chlorophenyl-phenyle...	15.616	204	406399	20.592	ng/ul	95
63) 4-Nitroaniline	15.634	138	101635	14.610	ng/ul#	78
66) 4,6-Dinitro-2-methylph...	15.698	198	136959	20.284	ng/ul#	92
67) N-Nitrosodiphenylamine	15.828	169	683092	21.511	ng/ul	94
68) 4-Bromophenyl-phenylether	16.516	248	252262	21.369	ng/ul	94
69) Hexachlorobenzene	16.640	284	286979	20.943	ng/ul#	92
70) Atrazine	16.787	200	270637	20.963	ng/ul	91
71) Pentachlorophenol	16.975	266	173600	19.893	ng/ul#	83
72) Phenanthrene	17.369	178	1253302	20.834	ng/ul	98
74) Anthracene	17.463	178	1287530	21.250	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.381	216	348914	21.595	ng/ul#	87
76) Pentachlorobenzene	14.898	250	334434	21.107	ng/ul#	88
77) Carbazole	17.728	167	1109379	20.691	ng/ul#	95
78) Di-n-butylphthalate	18.281	149	1412870	21.419	ng/ul#	93
80) Fluoranthene	19.334	202	1526958	22.560	ng/ul#	95
82) Pyrene	19.686	202	1545889	22.169	ng/ul#	93
83) Butylbenzylphthalate	20.551	149	660524	22.915	ng/ul#	81
84) 3,3'-Dichlorobenzidine	21.322	252	364899	19.220	ng/ul#	96
85) Benzo(a)anthracene	21.392	228	1429999	21.355	ng/ul	95
86) Bis(2-ethylhexyl)phtha...	21.316	149	946583	22.157	ng/ul#	82
87) Chrysene	21.451	228	1402446	21.270	ng/ul	99
89) Di-n-octyl phthalate	22.257	149	1576105	22.276	ng/ul	100
90) Benzo(b)fluoranthene	23.116	252	1332552	21.779	ng/ul	100
91) Benzo(k)fluoranthene	23.163	252	1258488	21.714	ng/ul#	98
93) Benzo(a)pyrene	23.757	252	1220236	21.566	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.427	276	1200528	21.329	ng/ul#	93
95) Dibenzo(a,h)anthracene	26.451	278	1019929	21.177	ng/ul#	95
96) Benzo(g,h,i)perylene	27.210	276	1009012	21.246	ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 21 19:00:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration









#2
 1,4-Dioxane
 Concen: 8.087 ng/uL
 RT: 3.405 min Scan# 54
 Delta R.T. -0.000 min
 Lab File: BP010014.D
 Acq: 21 Apr 2022 15:03




Instrument :
 BNA_P
 ClientSampleId :
 SICV629


Tgt Ion: 88 Resp: 29685
 Ion Ratio Lower Upper
 88 100
 43 35.1 6.8 10.2#
 58 84.3 28.4 42.6#

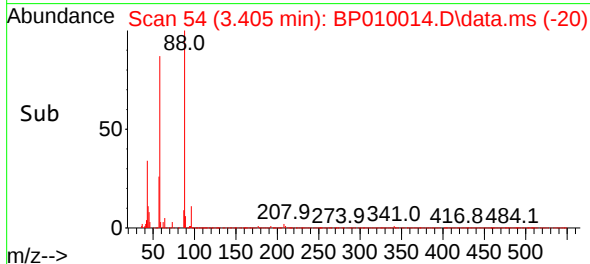

#5
 Pyridine
 Concen: 20.579 ng/uL
 RT: 3.805 min Scan# 122
 Delta R.T. 0.000 min
 Lab File: BP010014.D
 Acq: 21 Apr 2022 15:03

Tgt Ion: 79 Resp: 212583
 Ion Ratio Lower Upper
 79 100
 52 90.8 35.5 53.3#
 51 43.3 20.2 30.4#


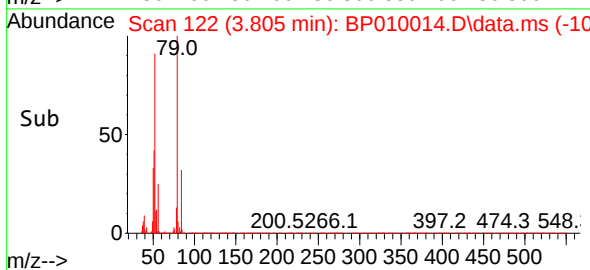

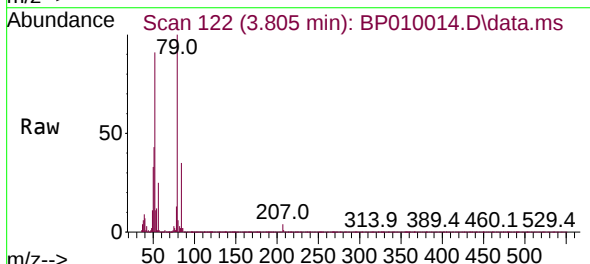




#6
Benzaldehyde
Concen: 21.329 ng/ul
RT: 7.075 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion: 77 Resp: 159707
Ion Ratio Lower Upper
77 100
105 94.9 77.0 115.4
106 86.3 77.0 115.4



#8
Phenol
Concen: 20.602 ng/ul
RT: 7.128 min Scan# 687
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion: 94 Resp: 290045
Ion Ratio Lower Upper
94 100
65 32.6 19.0 28.6#
66 44.3 34.6 51.8









#10
Bis(2-Chloroethyl)ether
Concen: 21.222 ng/ul
RT: 7.364 min Scan# 71
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion: 93 Resp: 230189
Ion Ratio Lower Upper
93 100
63 80.7 45.0 67.4#
95 32.7 26.3 39.5

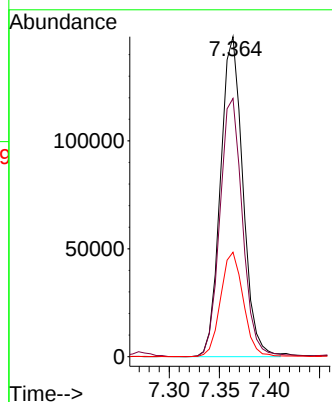

#12
2-Chlorophenol
Concen: 21.215 ng/ul
RT: 7.505 min Scan# 751
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:128 Resp: 222057
Ion Ratio Lower Upper
128 100
64 53.8 45.3 67.9
130 33.0 29.0 43.6

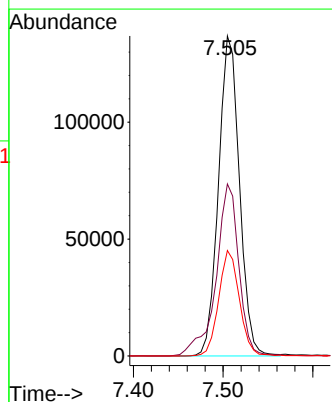



#13

2-Methylphenol

Concen: 20.731 ng/ul

RT: 8.387 min Scan# 900

Delta R.T. 0.006 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03

Instrument :

BNA_P

ClientSampleId :





SICV629

Tgt Ion:108 Resp: 223841

Ion Ratio Lower Upper

108 100

107 90.3 70.8 106.2

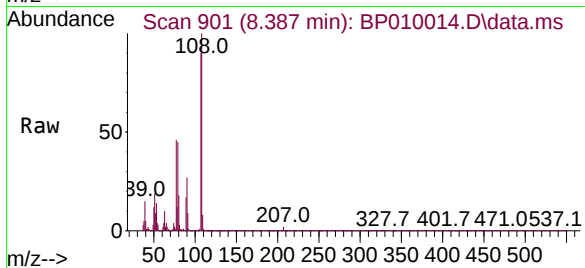

#14

2,2'-oxybis(1-Chloropropane)

Concen: 21.540 ng/ul

RT: 8.475 min Scan# 916

Delta R.T. 0.006 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03




Tgt Ion: 45 Resp: 346676


Ion Ratio Lower Upper

45 100

77 13.7 17.1 25.7#

79 10.3 13.2 19.8#


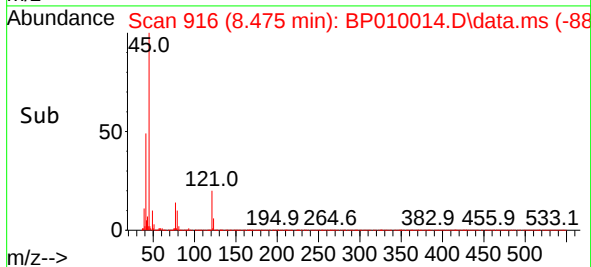

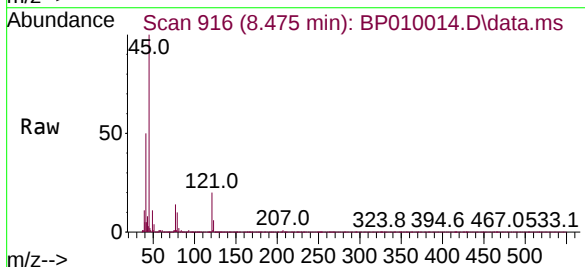




#16
Acetophenone
Concen: 21.368 ng/ul
RT: 8.764 min Scan# 90
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:105 Resp: 387030
Ion Ratio Lower Upper
105 100
77 83.5 53.4 80.2#
51 30.8 13.8 20.8#



#17
N-Nitroso-di-n-propylamine
Concen: 22.006 ng/ul
RT: 8.752 min Scan# 963
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion: 70 Resp: 208831
Ion Ratio Lower Upper
70 100
42 61.8 31.8 47.8#
101 9.9 15.6 23.4#
130 20.2 13.7 20.5









#18
4-Methylphenol
Concen: 20.838 ng/ul
RT: 8.711 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:108 Resp: 247723
Ion Ratio Lower Upper
108 100
107 116.4 83.6 125.4



#19
Hexachloroethane
Concen: 21.420 ng/ul
RT: 9.028 min Scan# 1010
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:117 Resp: 94207
Ion Ratio Lower Upper
117 100
201 105.6 106.5 159.7#
199 67.0 59.0 88.6









#22
Nitrobenzene
Concen: 21.354 ng/ul
RT: 9.146 min Scan# 1100
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion: 77 Resp: 292100
Ion Ratio Lower Upper
77 100
123 44.4 42.3 63.5
65 14.8 5.8 8.8#



#23
Isophorone
Concen: 21.454 ng/ul
RT: 9.675 min Scan# 1120
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion: 82 Resp: 579651
Ion Ratio Lower Upper
82 100
95 7.9 7.8 11.8
138 17.2 12.9 19.3



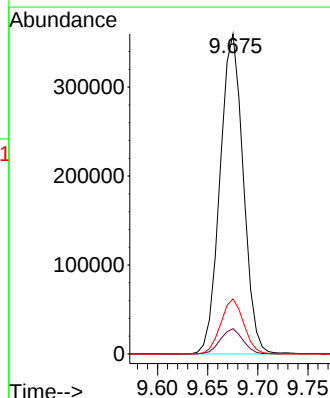





#25
2-Nitrophenol
Concen: 21.614 ng/ul
RT: 9.858 min Scan# 1151
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:139 Resp: 139585
Ion Ratio Lower Upper
139 100
65 59.2 49.4 74.2
109 35.5 44.7 67.1#



#26
2,4-Dimethylphenol
Concen: 21.328 ng/ul
RT: 9.922 min Scan# 1162
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:107 Resp: 298206
Ion Ratio Lower Upper
107 100
121 47.3 34.1 51.1
122 80.4 46.3 69.5#









#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.345 ng/ul
 RT: 10.158 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: BP010014.D
 Acq: 21 Apr 2022 15:03




Instrument :
 BNA_P
 ClientSampleId :
 SICV629


Tgt Ion: 93 Resp: 338017
 Ion Ratio Lower Upper
 93 100
 95 32.8 26.2 39.4
 123 11.2 6.2 9.4#

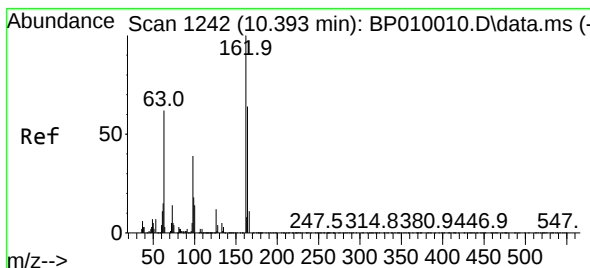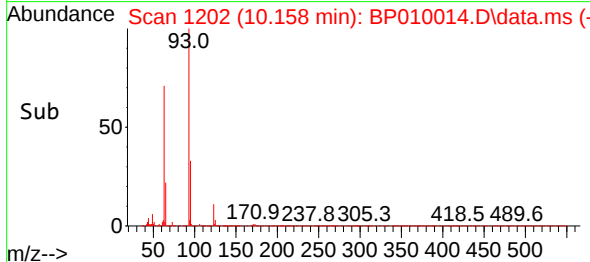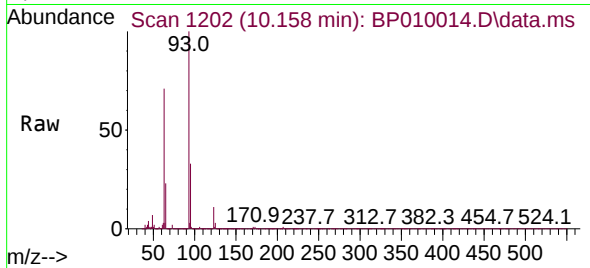

#29
 2,4-Dichlorophenol
 Concen: 21.479 ng/ul
 RT: 10.393 min Scan# 1242
 Delta R.T. 0.000 min
 Lab File: BP010014.D
 Acq: 21 Apr 2022 15:03

Tgt Ion:162 Resp: 245090
 Ion Ratio Lower Upper
 162 100
 164 66.4 37.0 55.6#
 98 38.6 31.0 46.6


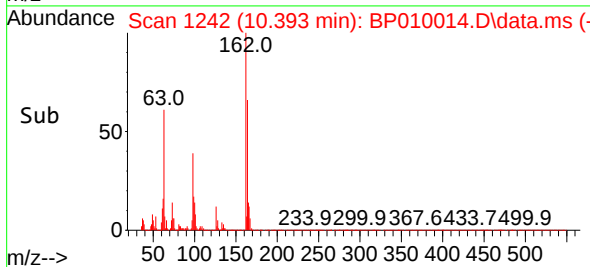

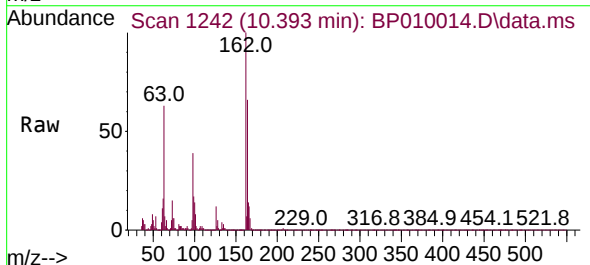




#30
Naphthalene
Concen: 21.220 ng/ul
RT: 10.799 min Scan# 1311
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:128 Resp: 779650
Ion Ratio Lower Upper
128 100
129 10.9 8.6 13.0
127 13.1 12.2 18.4

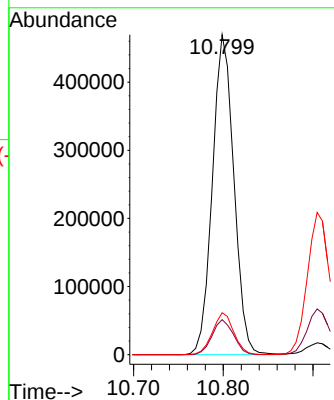

#32
4-Chloroaniline
Concen: 21.962 ng/ul
RT: 10.905 min Scan# 1329
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:127 Resp: 368357
Ion Ratio Lower Upper
127 100
129 32.2 24.6 37.0



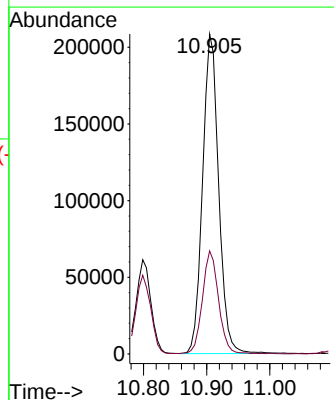





#33
Hexachlorobutadiene
Concen: 20.834 ng/ul
RT: 11.093 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:225 Resp: 168487
Ion Ratio Lower Upper
225 100
223 63.9 53.4 80.0
227 63.1 53.8 80.8



#34
Caprolactam
Concen: 12.097 ng/ul
RT: 11.669 min Scan# 1459
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:113 Resp: 49653
Ion Ratio Lower Upper
113 100
55 187.8 58.2 87.2#
56 153.0 68.6 103.0#









#35
4-Chloro-3-methylphenol
Concen: 21.569 ng/ul
RT: 12.028 min Scan# 1519
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:107 Resp: 297316
Ion Ratio Lower Upper
107 100
144 24.6 15.8 23.8#
142 73.7 38.9 58.3#

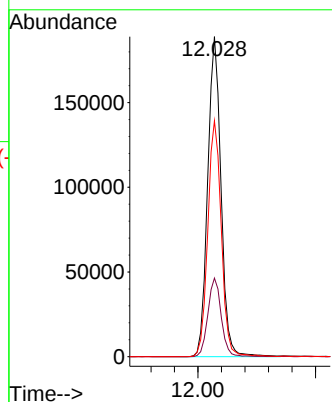

#36
2-Methylnaphthalene
Concen: 21.156 ng/ul
RT: 12.404 min Scan# 1584
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:142 Resp: 563728
Ion Ratio Lower Upper
142 100
141 88.8 64.3 96.5



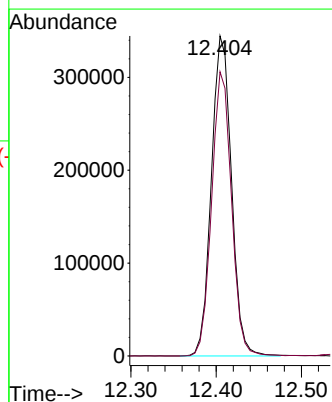





#37
1-Methylnaphthalene
Concen: 21.035 ng/ul
RT: 12.622 min Scan# 1621
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:142 Resp: 569130
Ion Ratio Lower Upper
142 100
141 92.7 69.8 104.8
116 4.3 5.6 8.4#



#39
1,2,4,5-Tetrachlorobenzene
Concen: 20.948 ng/ul
RT: 12.775 min Scan# 1647
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:216 Resp: 329201
Ion Ratio Lower Upper
216 100
214 79.1 58.2 87.2
179 22.0 14.2 21.2#
108 16.4 15.3 22.9


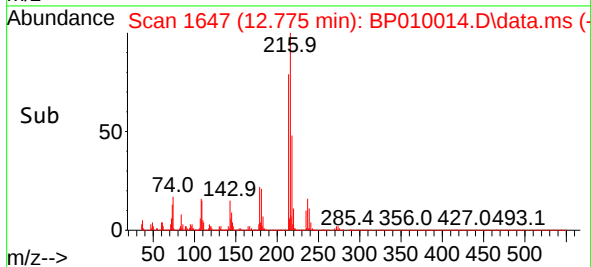

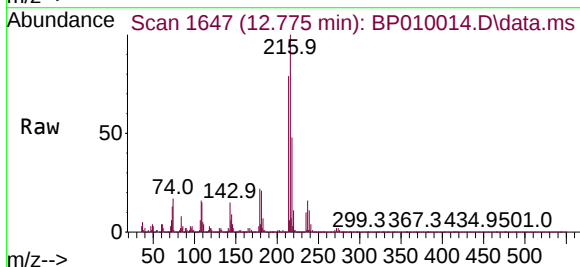




#40
Hexachlorocyclopentadiene
Concen: 19.482 ng/ul
RT: 12.757 min Scan# 1644
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:237 Resp: 172545
Ion Ratio Lower Upper
237 100
235 61.5 53.2 79.8
272 13.6 10.8 16.2



#41
2,4,6-Trichlorophenol
Concen: 21.041 ng/ul
RT: 13.010 min Scan# 1687
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:196 Resp: 213941
Ion Ratio Lower Upper
196 100
198 98.5 64.1 96.1#
200 31.6 19.9 29.9#





#42

2,4,5-Trichlorophenol

Concen: 21.508 ng/ul

RT: 13.081 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03

Instrument :

BNA_P

ClientSampleId :

SICV629





Tgt Ion:196 Resp: 237947

Ion Ratio Lower Upper

196 100

198 95.4 68.6 103.0

200 30.1 32.8 49.2#

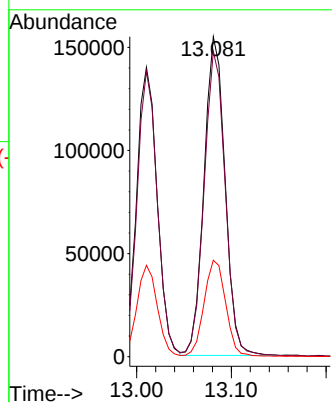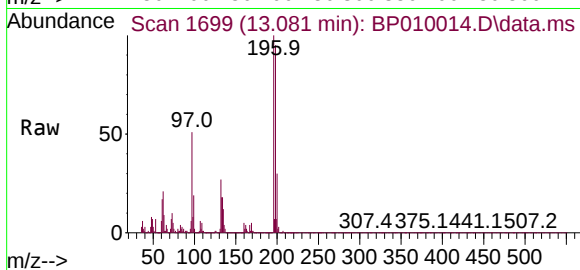

#43

1,1'-Biphenyl

Concen: 21.049 ng/ul

RT: 13.410 min Scan# 1755

Delta R.T. 0.000 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03




Tgt Ion:154 Resp: 789670


Ion Ratio Lower Upper

154 100

153 40.2 28.6 43.0

76 12.2 8.5 12.7



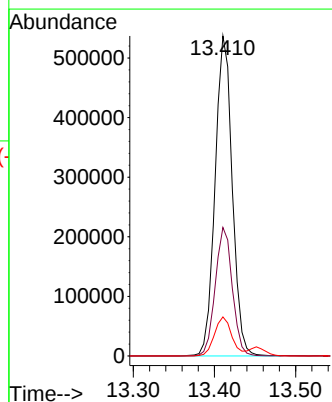
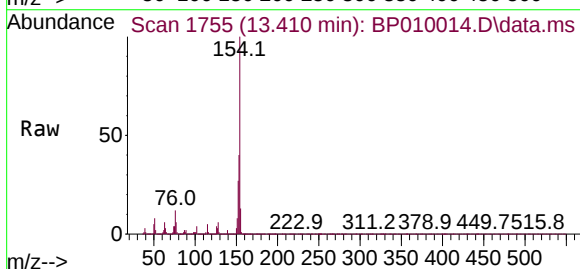




#44
2-Chloronaphthalene
Concen: 21.092 ng/ul
RT: 13.451 min Scan# 1762
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:162 Resp: 612367
Ion Ratio Lower Upper
162 100
164 32.7 27.5 41.3
127 39.5 37.1 55.7

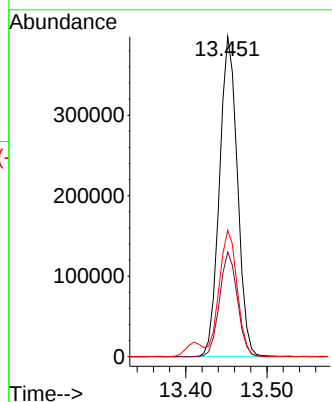

#45
2-Nitroaniline
Concen: 21.328 ng/ul
RT: 13.651 min Scan# 1796
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion: 65 Resp: 200783
Ion Ratio Lower Upper
65 100
92 67.3 77.9 116.9#
138 99.3 81.5 122.3





#47

Dimethylphthalate

Concen: 20.857 ng/ul

RT: 14.028 min Scan# 1860

Delta R.T. 0.000 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03

Instrument :

BNA_P

ClientSampleId :

SICV629





Tgt Ion:163 Resp: 802072

Ion Ratio Lower Upper

163 100

194 4.4 4.1 6.1

164 10.4 11.3 16.9#



#48

2,6-Dinitrotoluene

Concen: 21.139 ng/ul

RT: 14.146 min Scan# 1880

Delta R.T. 0.000 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03




Tgt Ion:165 Resp: 166827


Ion Ratio Lower Upper

165 100

89 60.6 51.7 77.5

121 21.2 18.3 27.5


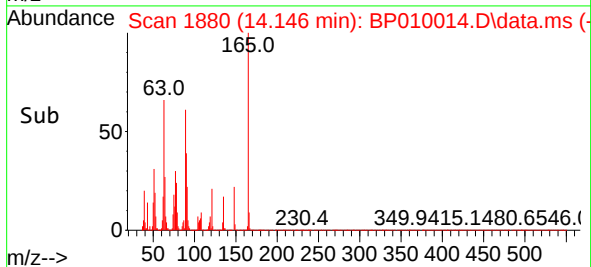

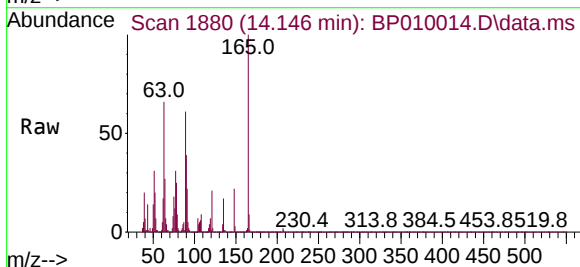




#50
Acenaphthylene
Concen: 21.304 ng/ul
RT: 14.299 min Scan# 1906
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:152 Resp: 1010550
Ion Ratio Lower Upper
152 100
151 19.7 18.3 27.5
153 12.9 11.0 16.6

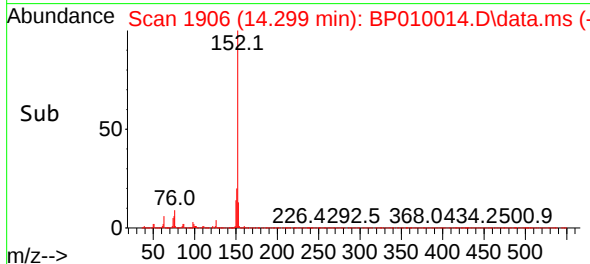

#51
3-Nitroaniline
Concen: 15.264 ng/ul
RT: 14.475 min Scan# 1936
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:138 Resp: 109123
Ion Ratio Lower Upper
138 100
108 12.2 15.8 23.8#
92 126.6 117.1 175.7

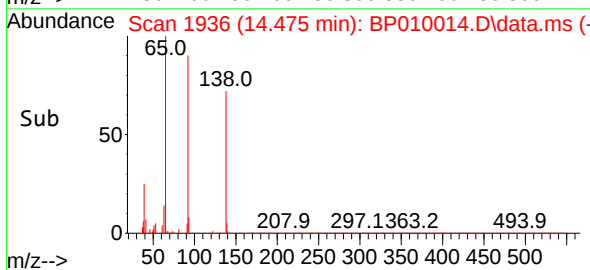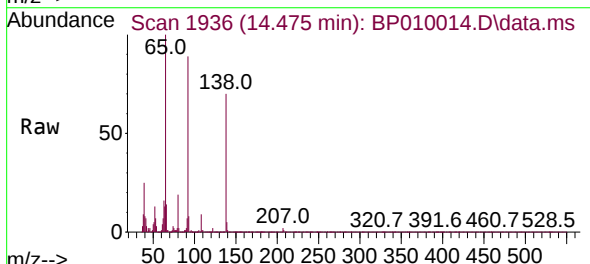

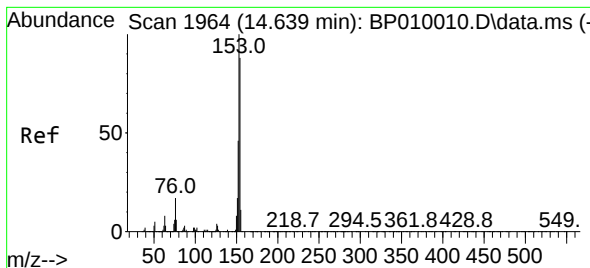

#52

Acenaphthene

Concen: 21.010 ng/ul

RT: 14.640 min Scan# 1964

Delta R.T. 0.000 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03

Instrument :

BNA_P

ClientSampleId :

SICV629





Tgt Ion:153 Resp: 648046

Ion Ratio Lower Upper

153 100

152 46.3 34.3 51.5

154 88.4 70.0 105.0

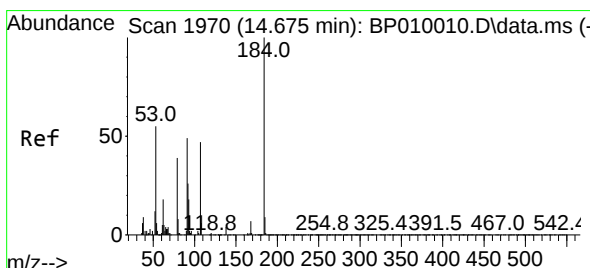

#53

2,4-Dinitrophenol

Concen: 17.620 ng/ul

RT: 14.681 min Scan# 1971

Delta R.T. 0.006 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03




Tgt Ion:184 Resp: 77703


Ion Ratio Lower Upper

184 100

63 70.1 34.6 52.0#

154 68.3 57.7 86.5


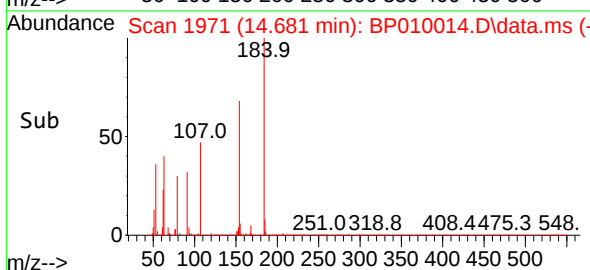






#55
4-Nitrophenol
Concen: 19.897 ng/ul
RT: 14.781 min Scan# 1987
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:109 Resp: 125921
Ion Ratio Lower Upper
109 100
139 117.7 61.4 92.2#
65 132.3 65.3 97.9#



#56
Dibenzofuran
Concen: 20.854 ng/ul
RT: 14.975 min Scan# 2021
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:168 Resp: 952479
Ion Ratio Lower Upper
168 100
139 38.6 30.1 45.1









#57
2,4-Dinitrotoluene
Concen: 21.237 ng/ul
RT: 14.934 min Scan# 2014
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:165 Resp: 244843
Ion Ratio Lower Upper
165 100
63 47.1 29.5 44.3#
182 3.2 2.8 4.2



#58
2,3,4,6-Tetrachlorophenol
Concen: 21.038 ng/ul
RT: 15.198 min Scan# 2059
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:232 Resp: 206893
Ion Ratio Lower Upper
232 100
131 45.1 25.4 38.2#
130 2.6 4.2 6.2#
166 31.4 28.1 42.1









#59
Diethylphthalate
Concen: 20.994 ng/ul
RT: 15.393 min Scan# 2092
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:149 Resp: 821165
Ion Ratio Lower Upper
149 100
177 22.2 22.0 33.0
150 12.7 10.2 15.2

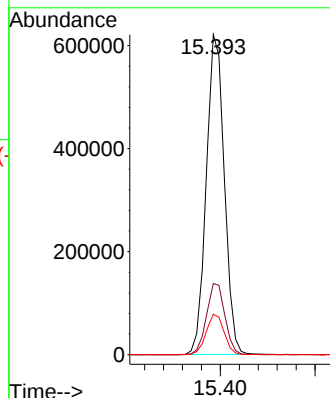

#61
Fluorene
Concen: 20.823 ng/ul
RT: 15.622 min Scan# 2131
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:166 Resp: 780851
Ion Ratio Lower Upper
166 100
165 96.2 70.3 105.5
167 13.4 9.5 14.3



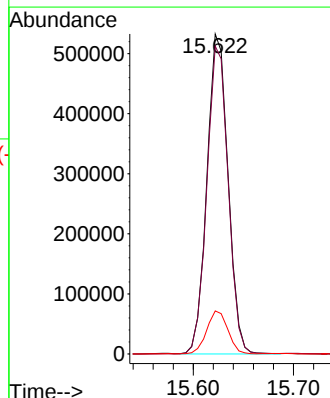





#62
4-Chlorophenyl-phenylether
Concen: 20.592 ng/ul
RT: 15.616 min Scan# 2130
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:204 Resp: 406399
Ion Ratio Lower Upper
204 100
206 32.2 27.6 41.4
141 61.9 46.6 69.8

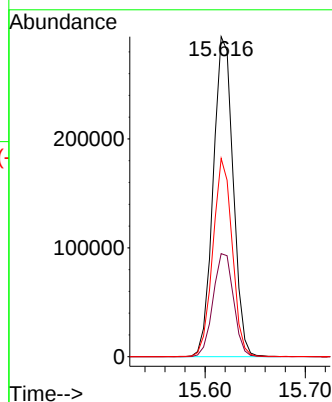

#63
4-Nitroaniline
Concen: 14.610 ng/ul
RT: 15.634 min Scan# 2133
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:138 Resp: 101635
Ion Ratio Lower Upper
138 100
92 51.9 41.6 62.4
108 86.8 97.6 146.4#









#66
4,6-Dinitro-2-methylphenol
Concen: 20.284 ng/ul
RT: 15.698 min Scan# 2144
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:198 Resp: 136959
Ion Ratio Lower Upper
198 100
182 3.9 6.0 9.0#
77 25.8 17.7 26.5

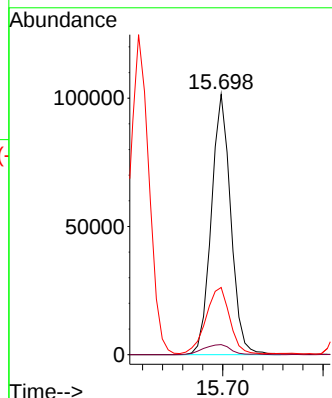

#67
N-Nitrosodiphenylamine
Concen: 21.511 ng/ul
RT: 15.828 min Scan# 2166
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:169 Resp: 683092
Ion Ratio Lower Upper
169 100
168 65.8 48.3 72.5
167 34.0 29.6 44.4



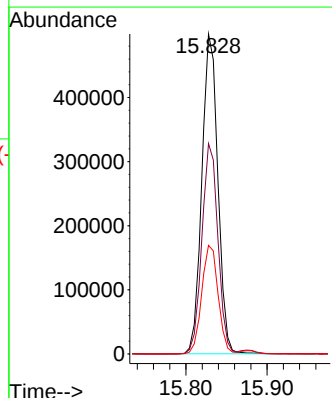





#68
4-Bromophenyl-phenylether
Concen: 21.369 ng/ul
RT: 16.516 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:248 Resp: 252262
Ion Ratio Lower Upper
248 100
250 97.0 79.4 119.0
141 73.7 67.2 100.8



#69
Hexachlorobenzene
Concen: 20.943 ng/ul
RT: 16.640 min Scan# 2304
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:284 Resp: 286979
Ion Ratio Lower Upper
284 100
142 31.4 19.2 28.8#
249 32.7 27.4 41.2









#70
Atrazine
Concen: 20.963 ng/ul
RT: 16.787 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:200 Resp: 270637
Ion Ratio Lower Upper
200 100
173 25.6 19.2 28.8
215 48.3 32.2 48.4

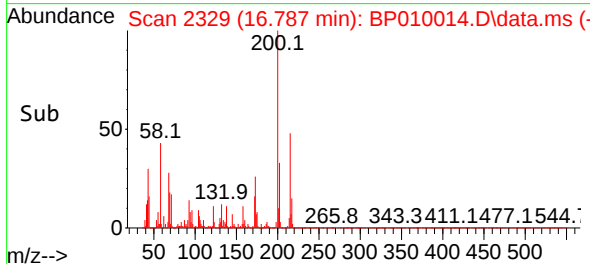

#71
Pentachlorophenol
Concen: 19.893 ng/ul
RT: 16.975 min Scan# 2361
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:266 Resp: 173600
Ion Ratio Lower Upper
266 100
264 63.4 57.3 85.9
268 61.8 65.7 98.5#


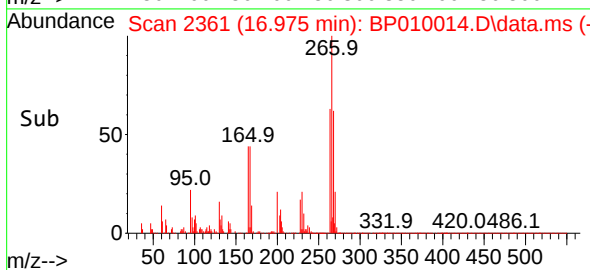

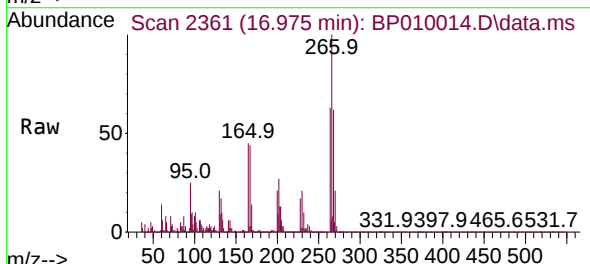




#72
Phenanthrene
Concen: 20.834 ng/ul
RT: 17.369 min Scan# 2428
Delta R.T. 0.000 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:178 Resp: 1253302
Ion Ratio Lower Upper
178 100
179 15.8 11.7 17.5
176 18.8 14.5 21.7



#74
Anthracene
Concen: 21.250 ng/ul
RT: 17.463 min Scan# 2444
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:178 Resp: 1287530
Ion Ratio Lower Upper
178 100
179 15.2 12.3 18.5
176 17.5 13.4 20.2





#75

1,2,3,4-Tetrachlorobenzene

Concen: 21.595 ng/uL

RT: 13.381 min Scan# 1750

Delta R.T. 0.006 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03

Instrument :

BNA_P

ClientSampleId :

SICV629





Tgt Ion:216 Resp: 348914

Ion Ratio Lower Upper

216 100

214 76.9 50.4 75.6#

218 47.1 35.2 52.8

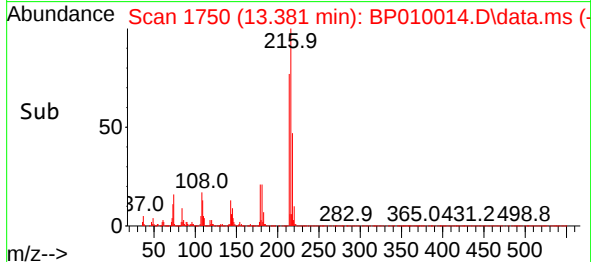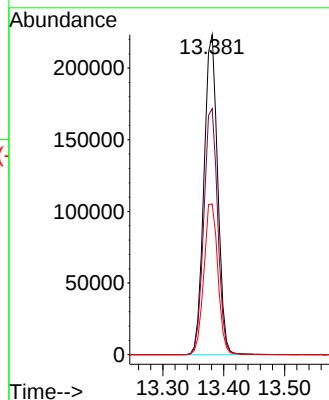

#76

Pentachlorobenzene

Concen: 21.107 ng/uL

RT: 14.898 min Scan# 2008

Delta R.T. 0.000 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03




Tgt Ion:250 Resp: 334434


Ion Ratio Lower Upper

250 100

248 65.7 43.5 65.3#

252 65.0 46.5 69.7

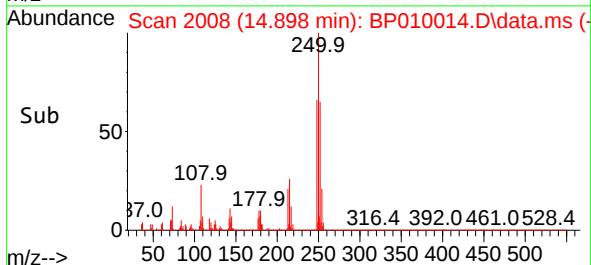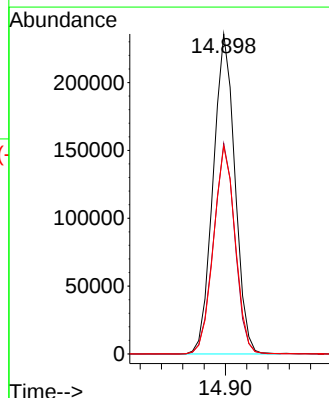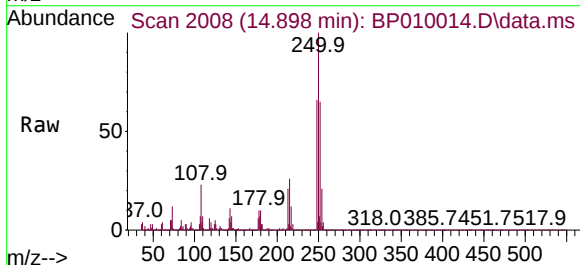



#77

Carbazole

Concen: 20.691 ng/ul

RT: 17.728 min Scan# 2488

Delta R.T. 0.006 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03

Instrument :

BNA_P

ClientSampleId :

SICV629





Tgt Ion:167 Resp: 1109379

Ion Ratio Lower Upper

167 100

166 21.5 15.8 23.8

139 13.0 8.3 12.5#



#78

Di-n-butylphthalate

Concen: 21.419 ng/ul

RT: 18.281 min Scan# 2583

Delta R.T. 0.006 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03




Tgt Ion:149 Resp: 1412870


Ion Ratio Lower Upper

149 100

150 9.1 9.6 14.4#

104 5.5 6.2 9.4#



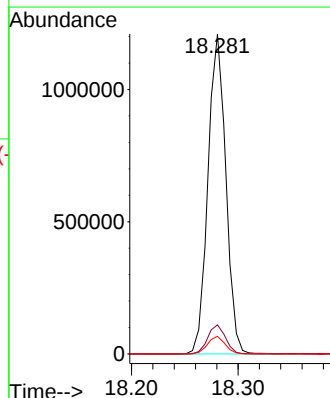





#80
Fluoranthene
Concen: 22.560 ng/u1
RT: 19.334 min Scan# 21
Delta R.T. 0.007 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:202 Resp: 1526958
Ion Ratio Lower Upper
202 100
101 9.4 9.6 14.4#
100 7.4 6.3 9.5

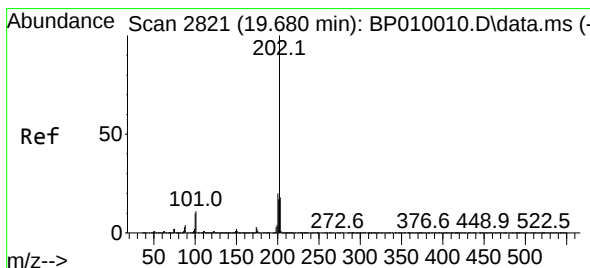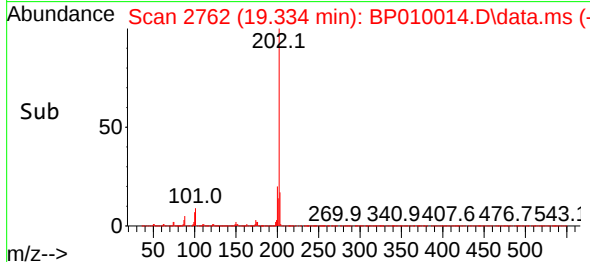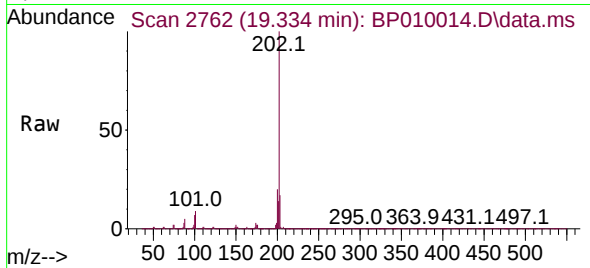

#82
Pyrene
Concen: 22.169 ng/u1
RT: 19.686 min Scan# 2822
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:202 Resp: 1545889
Ion Ratio Lower Upper
202 100
101 10.9 10.6 15.8
100 9.2 9.8 14.6#

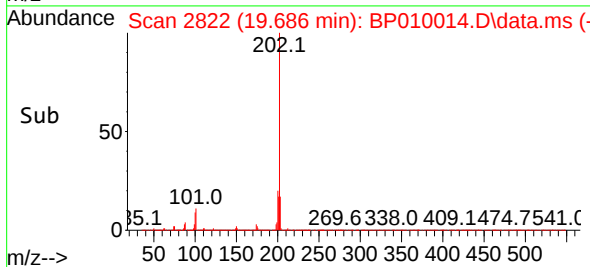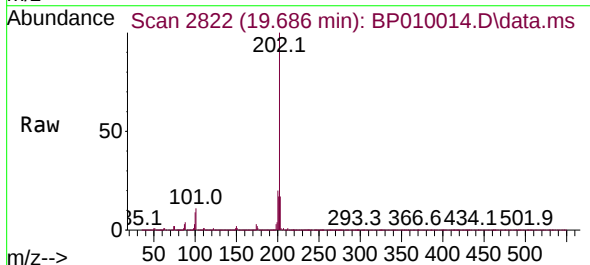



#83

Butylbenzylphthalate

Concen: 22.915 ng/ul

RT: 20.551 min Scan# 2969

Delta R.T. 0.000 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03

Instrument :

BNA_P

ClientSampleId :

SICV629





Tgt Ion:149 Resp: 660524

Ion Ratio Lower Upper

149 100

91 73.2 71.1 106.7

206 21.1 28.8 43.2#



#84

3,3'-Dichlorobenzidine

Concen: 19.220 ng/ul

RT: 21.322 min Scan# 3100

Delta R.T. 0.000 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03




Tgt Ion:252 Resp: 364899


Ion Ratio Lower Upper

252 100

254 64.6 49.8 74.6

126 9.6 4.3 6.5#

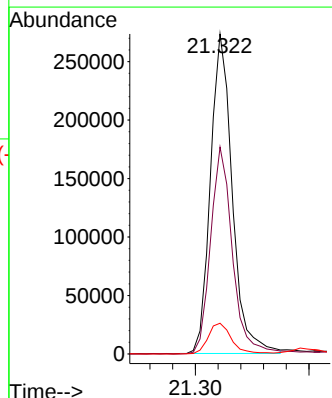



#85

Benzo(a)anthracene

Concen: 21.355 ng/ul

RT: 21.392 min Scan# 3112

Delta R.T. 0.000 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03

Instrument :

BNA_P

ClientSampleId :

SICV629





Tgt Ion:228 Resp: 1429999

Ion Ratio Lower Upper

228 100

229 19.5 18.2 27.2

226 26.6 22.8 34.2

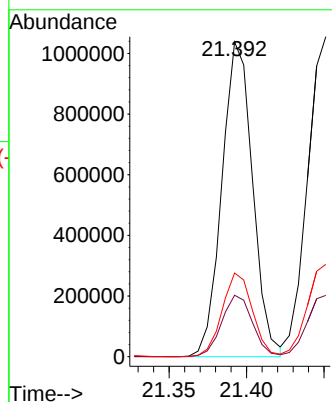

#86

Bis(2-ethylhexyl)phthalate

Concen: 22.157 ng/ul

RT: 21.316 min Scan# 3099

Delta R.T. 0.000 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03




Tgt Ion:149 Resp: 946583


Ion Ratio Lower Upper

149 100

167 28.5 32.8 49.2#

279 4.7 5.6 8.4#





#87

Chrysene

Concen: 21.270 ng/ul

RT: 21.451 min Scan# 3121

Delta R.T. 0.006 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03

Instrument :

BNA_P

ClientSampleId :

SICV629





Tgt Ion:228 Resp: 1402446

Ion Ratio Lower Upper

228 100

226 28.8 22.7 34.1

229 19.1 15.2 22.8



#89

Di-n-octyl phthalate

Concen: 22.276 ng/ul




RT: 22.257 min Scan# 3259


Delta R.T. 0.000 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03

Tgt Ion:149 Resp: 1576105


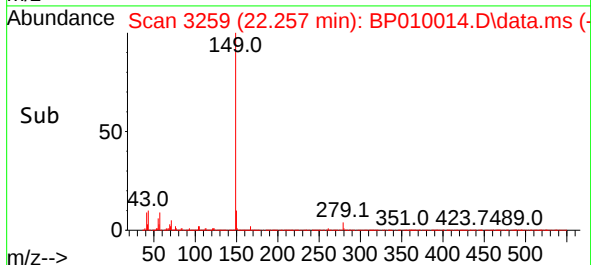
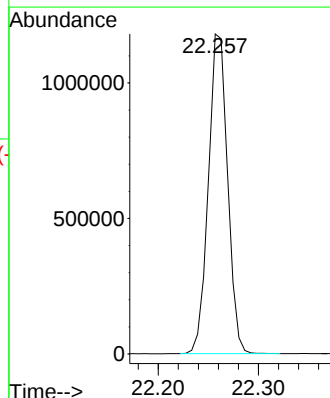
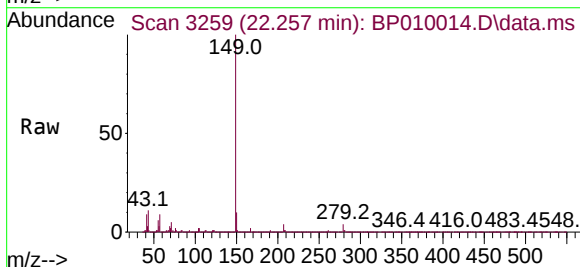




#90
Benzo(b)fluoranthene
Concen: 21.779 ng/ul
RT: 23.116 min Scan# 3404
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03




Instrument :
BNA_P
ClientSampleId :
SICV629


Tgt Ion:252 Resp: 1332552
Ion Ratio Lower Upper
252 100
253 21.7 17.4 26.0
125 8.5 7.3 10.9



#91
Benzo(k)fluoranthene
Concen: 21.714 ng/ul
RT: 23.163 min Scan# 3413
Delta R.T. 0.006 min
Lab File: BP010014.D
Acq: 21 Apr 2022 15:03

Tgt Ion:252 Resp: 1258488
Ion Ratio Lower Upper
252 100
253 21.9 17.9 26.9
125 8.3 5.1 7.7#





#93

Benzo(a)pyrene

Concen: 21.566 ng/ul

RT: 23.757 min Scan# 3514

Delta R.T. 0.006 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03

Instrument :

BNA_P

ClientSampleId :

SICV629





Tgt Ion:252 Resp: 1220236

Ion Ratio Lower Upper

252 100

253 21.7 17.5 26.3

125 9.2 6.4 9.6



#94

Indeno(1,2,3-cd)pyrene

Concen: 21.329 ng/ul

RT: 26.427 min Scan# 3968

Delta R.T. 0.000 min

Lab File: BP010014.D

Acq: 21 Apr 2022 15:03




Tgt Ion:276 Resp: 1200528


Ion Ratio Lower Upper

276 100

138 20.4 12.3 18.5

277 25.6 19.3 28.9


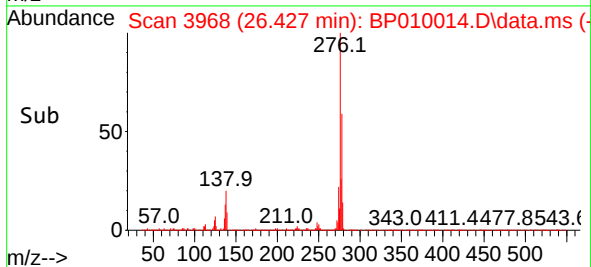

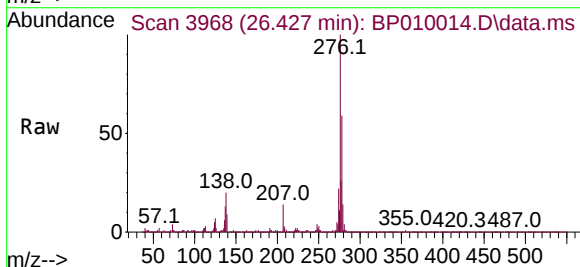




#95
 Dibenzo(a,h)anthracene
 Concen: 21.177 ng/ul
 RT: 26.451 min Scan# 3970
 Delta R.T. 0.012 min
 Lab File: BP010014.D
 Acq: 21 Apr 2022 15:03

Instrument :
 BNA_P
 ClientSampleId :
 SICV629

Tgt Ion:278 Resp: 1019929
 Ion Ratio Lower Upper
 278 100
 139 13.2 6.6 10.0#
 279 23.6 18.4 27.6



#96
 Benzo(g,h,i)perylene
 Concen: 21.246 ng/ul
 RT: 27.210 min Scan# 4101
 Delta R.T. 0.000 min
 Lab File: BP010014.D
 Acq: 21 Apr 2022 15:03

Tgt Ion:276 Resp: 1009012
 Ion Ratio Lower Upper
 276 100
 138 17.9 11.6 17.4#
 277 24.0 15.9 23.9#

