




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010018.D
 Acq On : 21 Apr 2022 17:19
 Operator : CG/JU
 Sample : PB144259BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK259

Manual IntegrationsAPPROVED

Quant Time: Apr 22 04:18:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

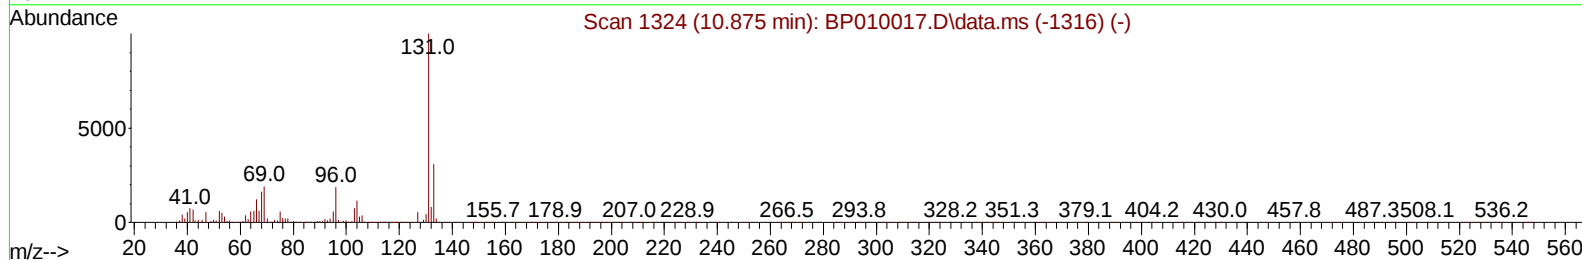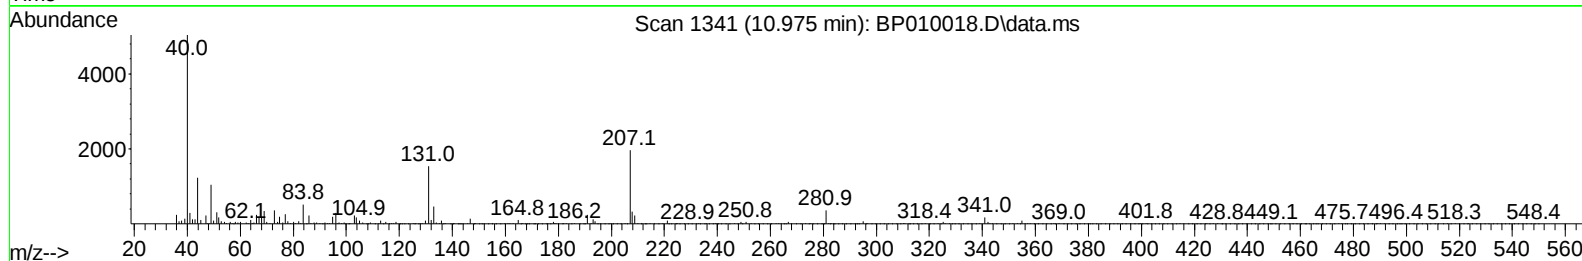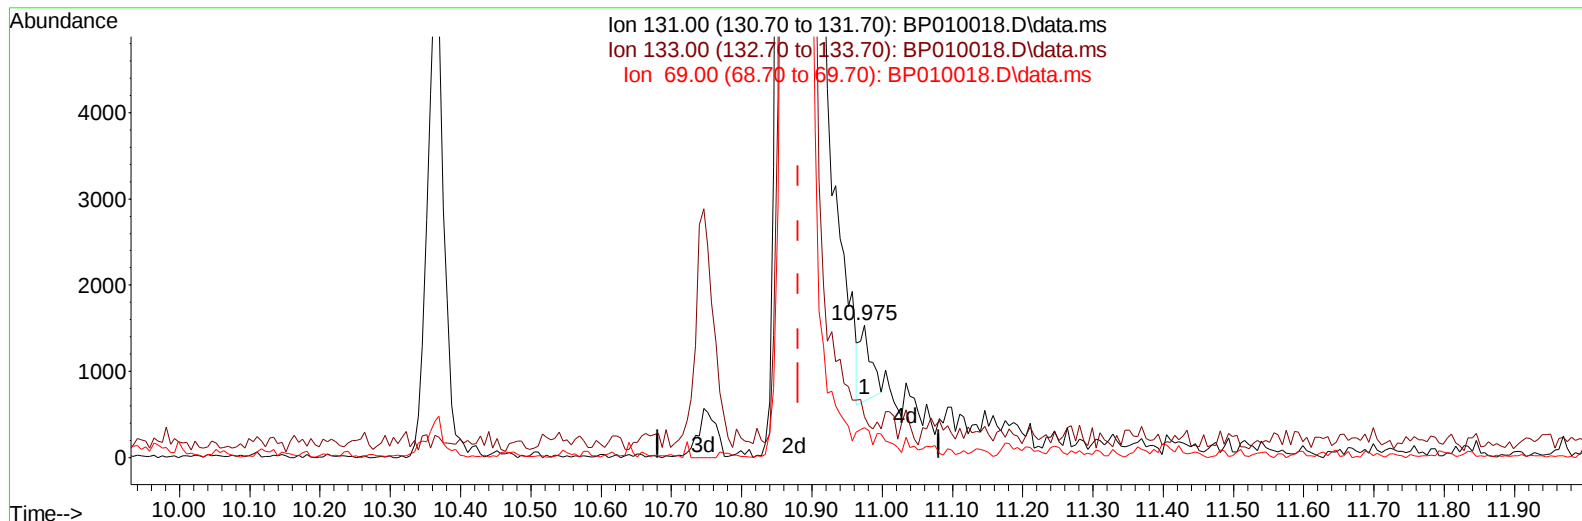

TIC: BP010018.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.975min (+ 0.094) 0.07 ng/ul

response 976

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	30.49
69.00	26.10	22.43
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010018.D
 Acq On : 21 Apr 2022 17:19
 Operator : CG/JU
 Sample : PB144259BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK259

Manual IntegrationsAPPROVED

Quant Time: Apr 22 04:18:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

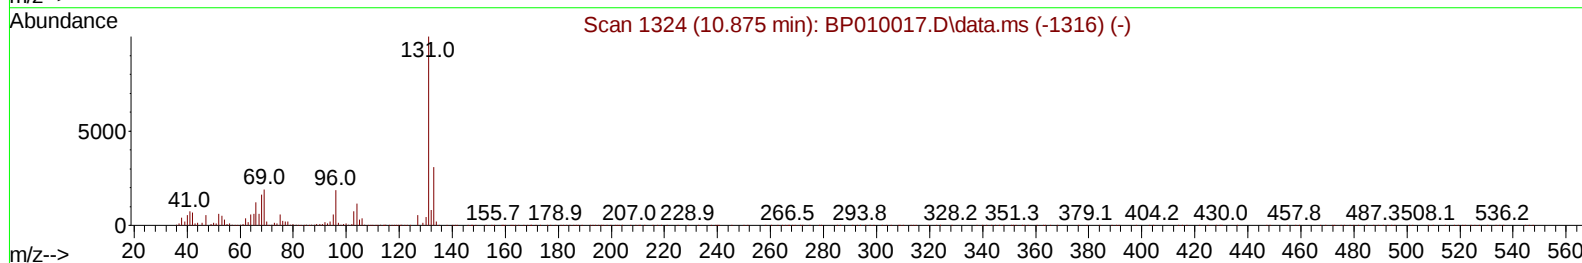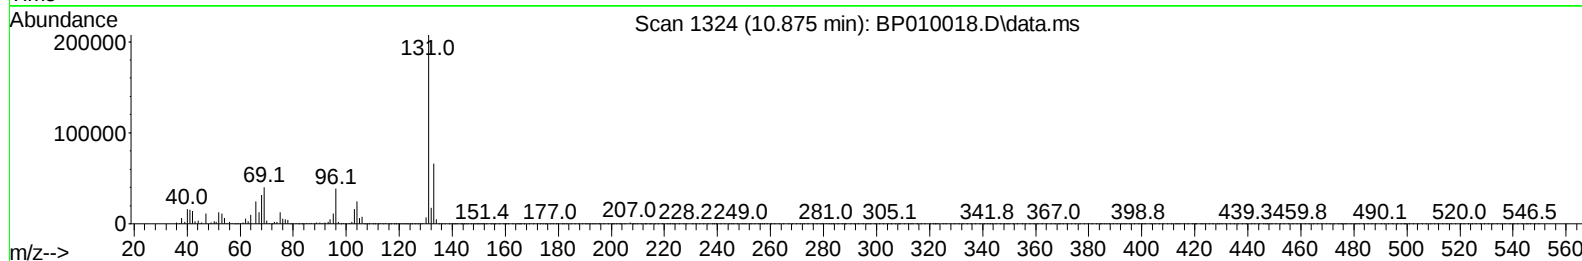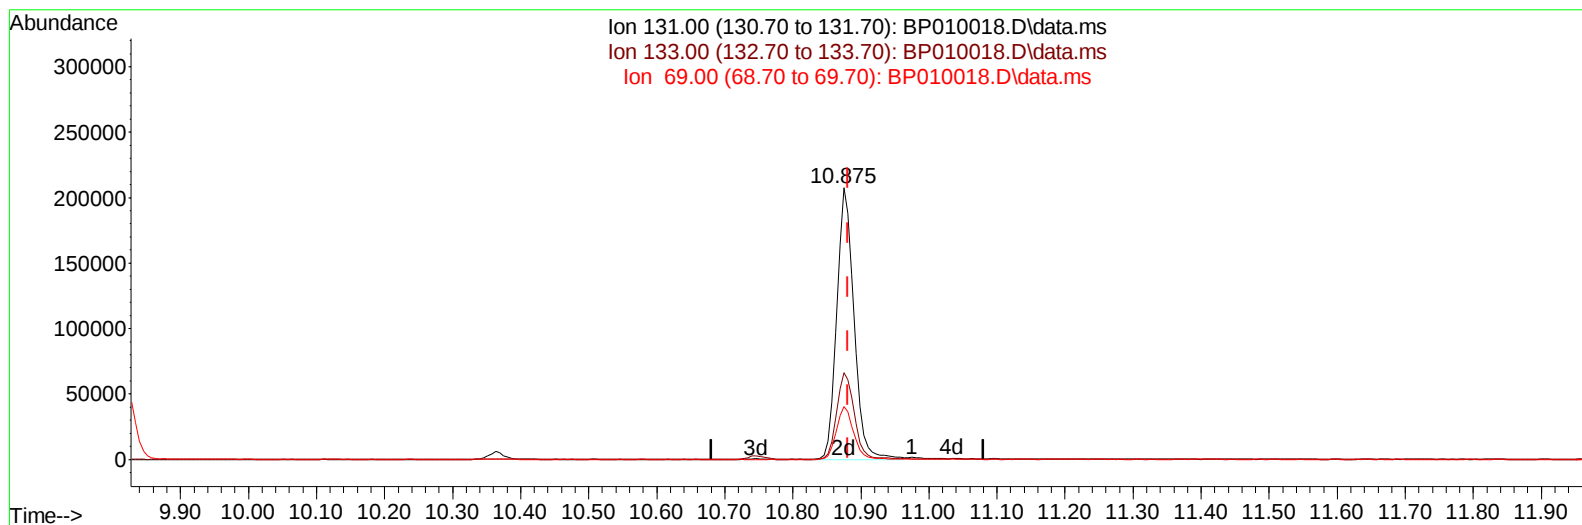

TIC: BP010018.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.875min (-0.006) 24.66 ng/ul m

response 365461

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	31.98
69.00	26.10	19.43#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010018.D
 Acq On : 21 Apr 2022 17:19
 Operator : CG/JU
 Sample : PB144259BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK259

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 04:18:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	133167	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136	611290	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	454920	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	1028281	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	993278	20.000	ng/ul	# 0.00
88) Perylene-d12	23.857	264	879834	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	17130	5.609	ng/uL	0.00
4) Pyridine-d5	3.787	84	218882	25.478	ng/ul	0.00
7) Phenol-d5	7.099	99	285656	23.583	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	196468	27.031	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	231987	25.861	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	253597	25.269	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	125883	25.892	ng/ul	0.00
24) 2-Nitrophenol-d4	9.822	143	139787	26.326	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	241663	23.379	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	365461m	24.658	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	978694	27.656	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160	1058834	24.722	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	144425	22.169	ng/ul	0.00
60) Fluorene-d10	15.563	176	829047	27.235	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	131942	20.293	ng/ul	0.00
73) Anthracene-d10	17.422	188	1329658	26.728	ng/ul	0.00
81) Pyrene-d10	19.651	212	1601075	28.344	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1249422	27.087	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010018.D
Acq On : 21 Apr 2022 17:19
Operator : CG/JU
Sample : PB144259BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK259

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/22/2022
Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 04:18:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

