




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010033.D
 Acq On : 22 Apr 2022 01:44
 Operator : CG/JU
 Sample : N2473-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J41

Manual IntegrationsAPPROVED

Quant Time: Apr 22 04:22:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

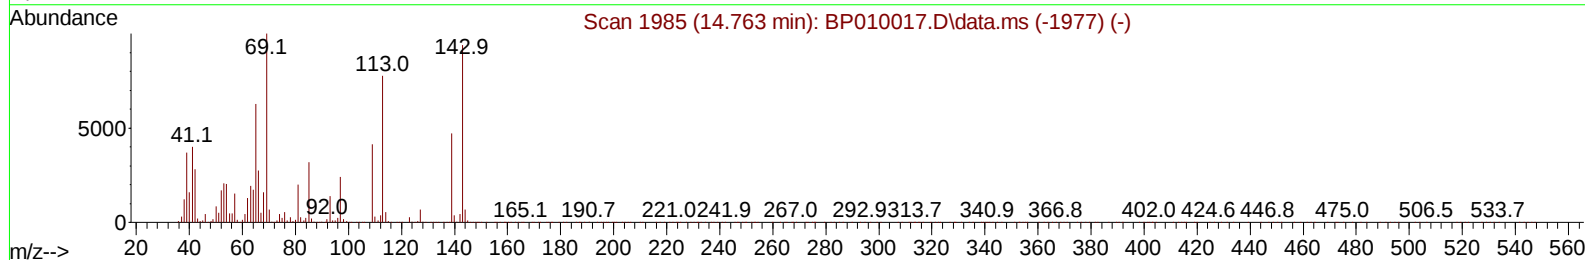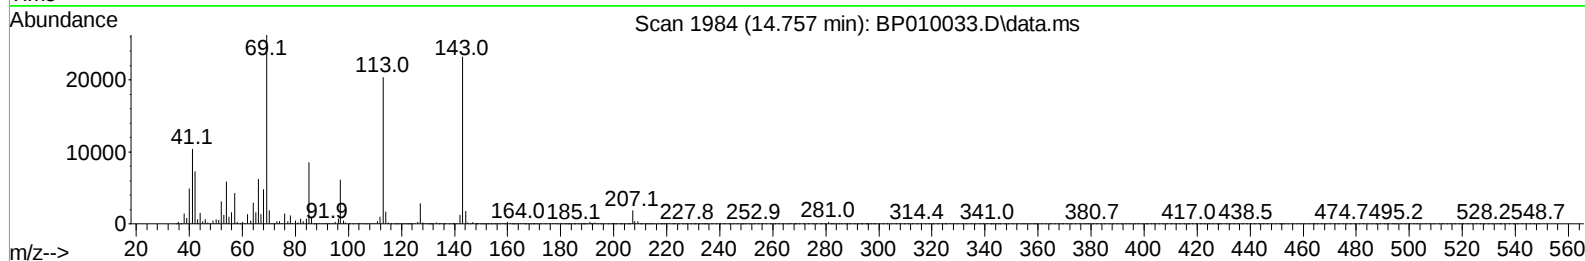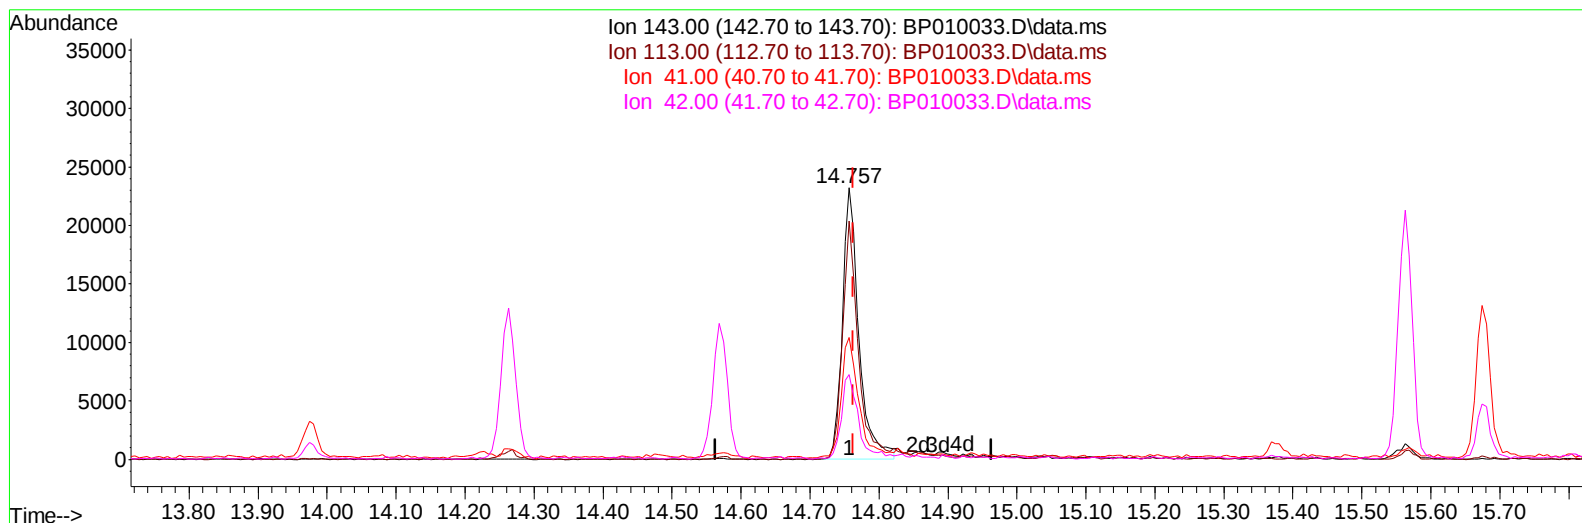

TIC: BP010033.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (-0.006) 5.40 ng/u1

response 38552

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	87.94#
41.00	23.20	44.94#
42.00	18.00	31.27#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010033.D
 Acq On : 22 Apr 2022 01:44
 Operator : CG/JU
 Sample : N2473-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J41

Manual IntegrationsAPPROVED

Quant Time: Apr 22 04:22:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

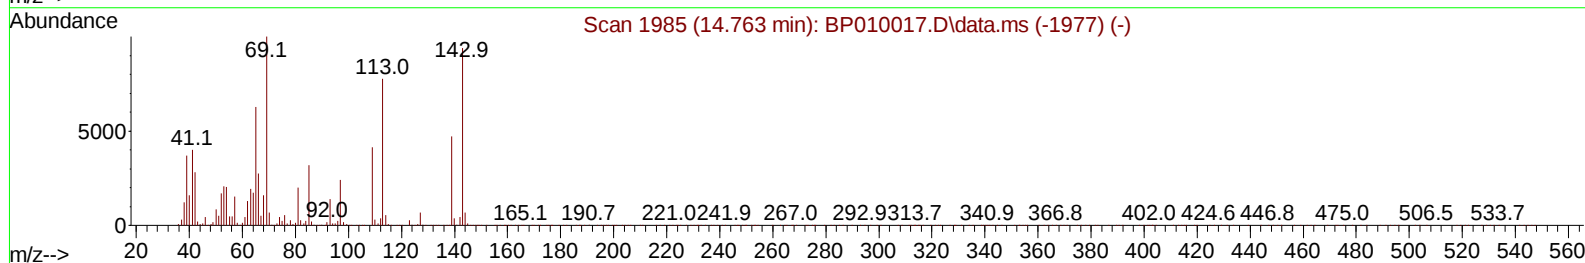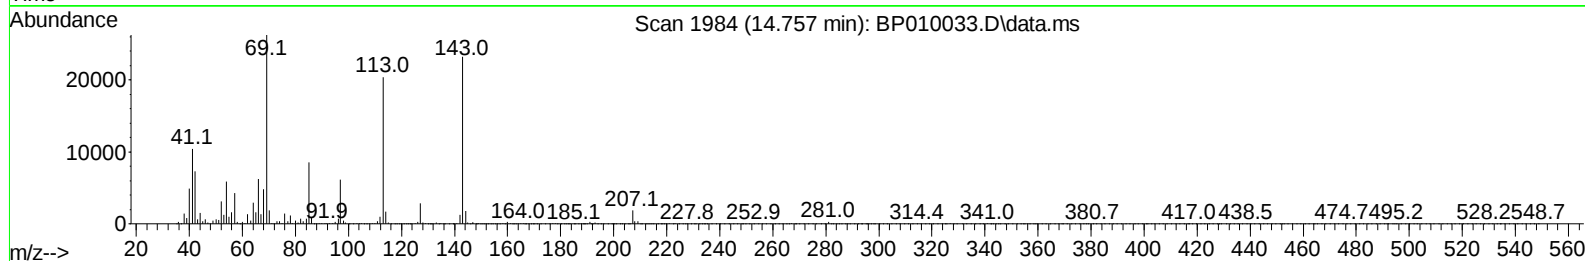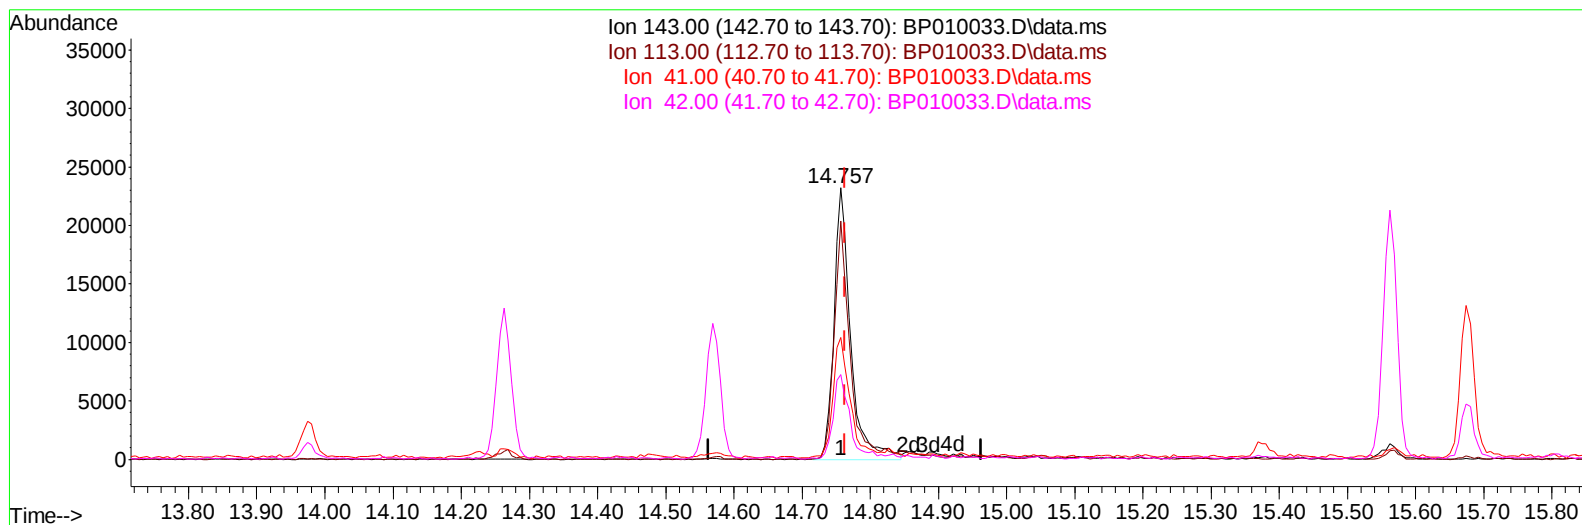

TIC: BP010033.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (-0.006) 5.53 ng/ul m

response 39487

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	87.94#
41.00	23.20	44.94#
42.00	18.00	31.27#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010033.D
 Acq On : 22 Apr 2022 01:44
 Operator : CG/JU
 Sample : N2473-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J41

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/22/2022
 Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 04:22:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	146399	20.000	ng/ul	0.00
20) Naphthalene-d8	10.745	136	682856	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	498808	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	1099426	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	1003962	20.000	ng/ul	# 0.00
88) Perylene-d12	23.851	264	898745	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	15979	4.760	ng/uL	0.00
4) Pyridine-d5	3.799	84	34056	3.606	ng/ul	0.01
7) Phenol-d5	7.099	99	83531	6.273	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	258958	32.409	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	238535	24.187	ng/ul	0.00
15) 4-Methylphenol-d8	8.645	113	171646	15.558	ng/ul	0.00
21) Nitrobenzene-d5	9.098	128	169058	31.128	ng/ul	0.00
24) 2-Nitrophenol-d4	9.822	143	179426	30.250	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	298915	25.887	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	194932	11.774	ng/ul	0.00
46) Dimethylphthalate-d6	13.980	166	1319825	34.015	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160	1439999	30.664	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	39487m	5.528	ng/ul	0.00
60) Fluorene-d10	15.563	176	1136417	34.047	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	211584	30.436	ng/ul	0.00
73) Anthracene-d10	17.422	188	2021757	38.011	ng/ul	0.00
81) Pyrene-d10	19.651	212	2393650	41.923	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1835177	38.949	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010033.D
Acq On : 22 Apr 2022 01:44
Operator : CG/JU
Sample : N2473-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J41

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/22/2022
Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 04:22:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

