




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010050.D
 Acq On : 22 Apr 2022 11:49
 Operator : CG/JU
 Sample : N2473-13DL 20X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HX2DL

Manual IntegrationsAPPROVED

Quant Time: Apr 22 23:26:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/25/2022
 Supervised By :mohammad ahmed 04/26/2022

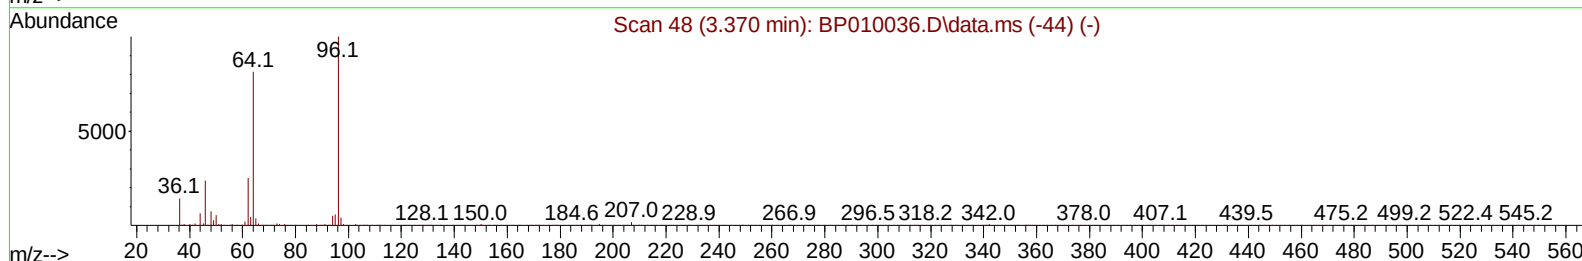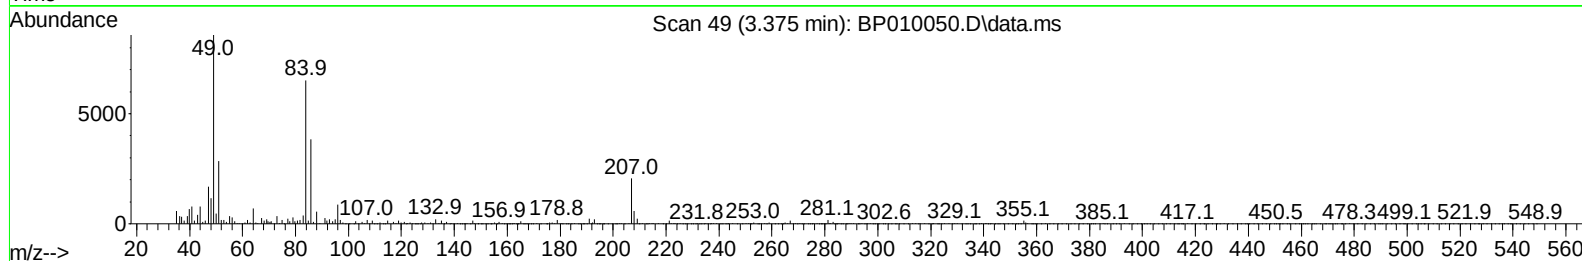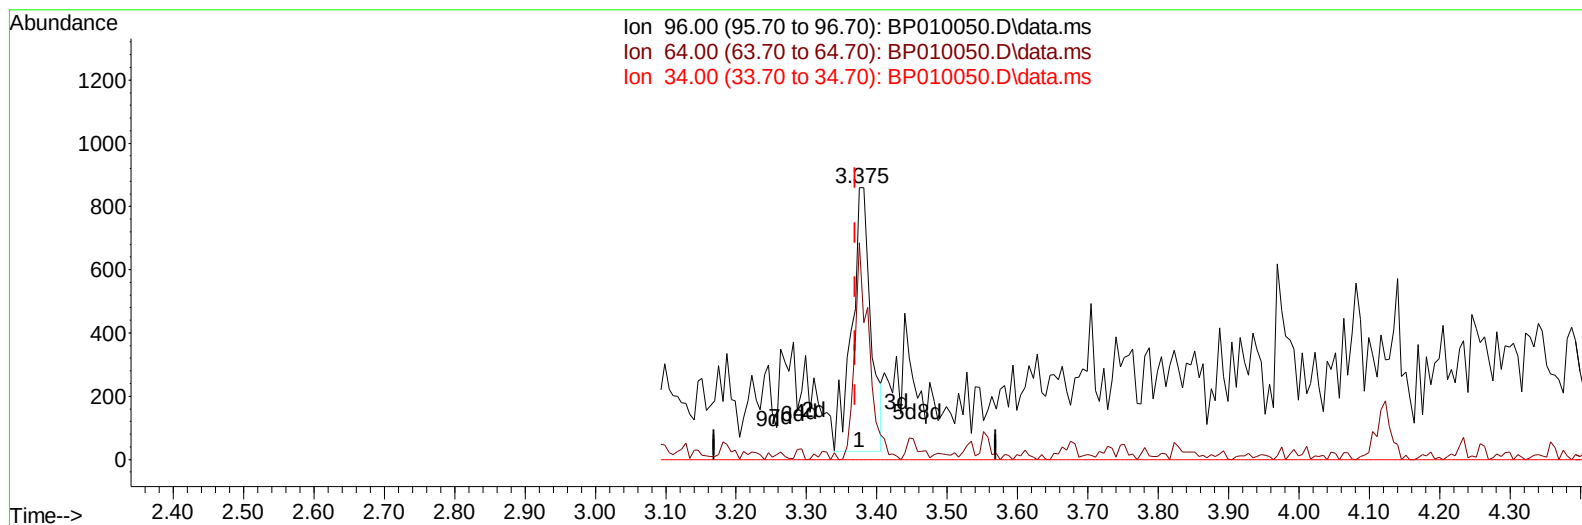

TIC: BP010050.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.375min (+ 0.006) 0.31 ng/uL

response 1561

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	79.74#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010050.D
 Acq On : 22 Apr 2022 11:49
 Operator : CG/JU
 Sample : N2473-13DL 20X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HX2DL

Manual IntegrationsAPPROVED

Quant Time: Apr 22 23:26:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/25/2022
 Supervised By :mohammad ahmed 04/26/2022

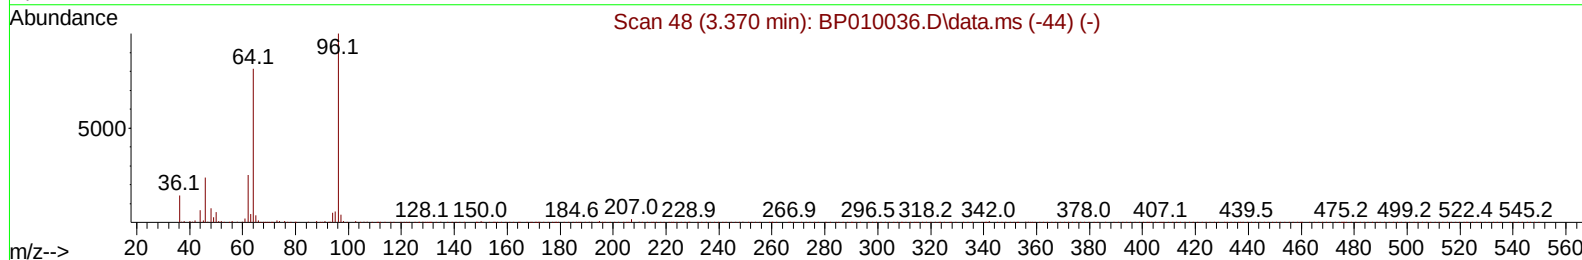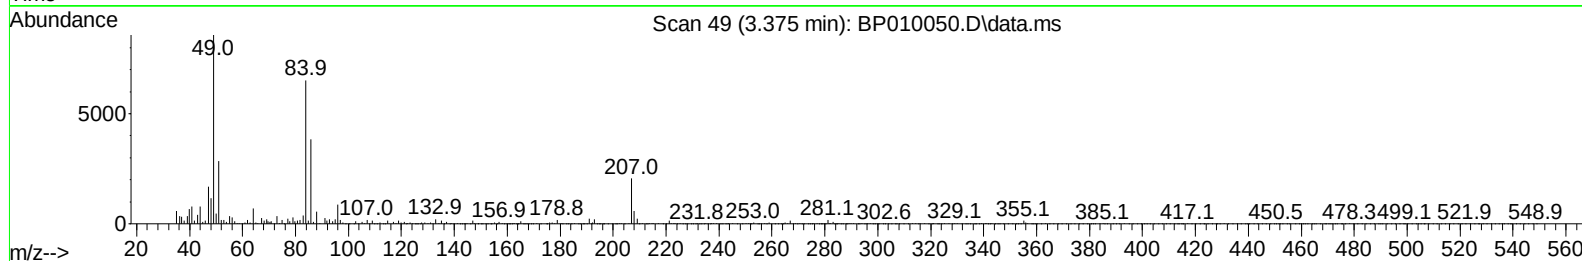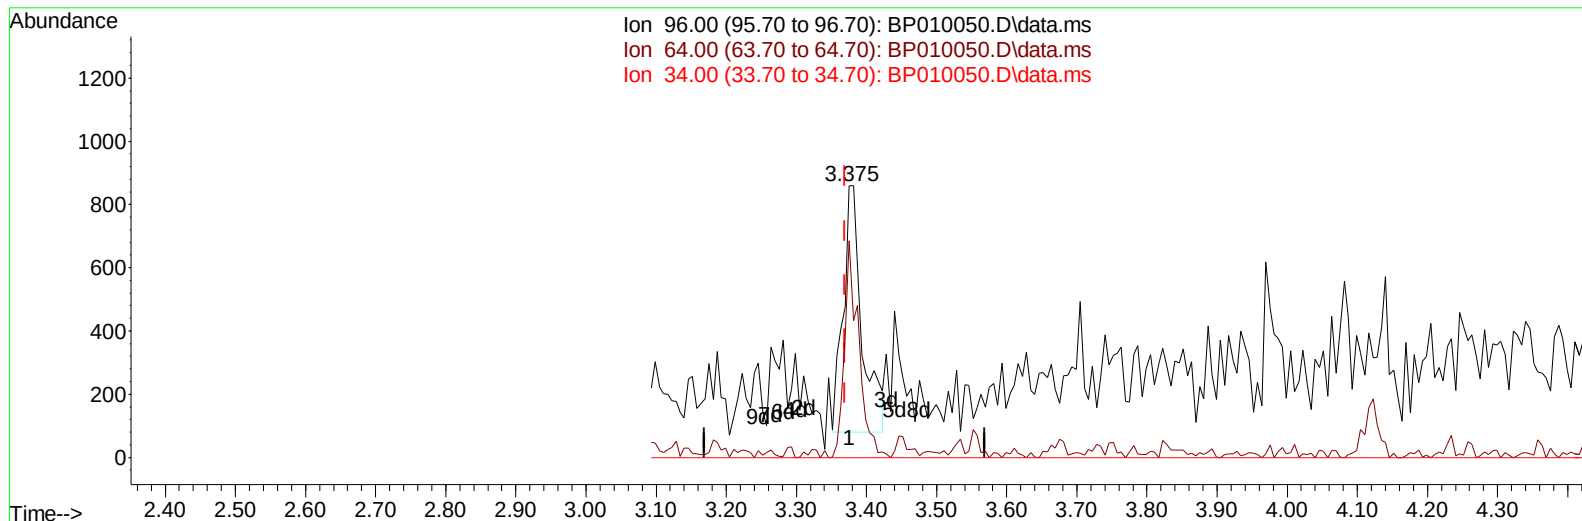

TIC: BP010050.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.375min (+ 0.006) 0.29 ng/uL m

response 1457

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	79.74#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010050.D
 Acq On : 22 Apr 2022 11:49
 Operator : CG/JU
 Sample : N2473-13DL 20X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HX2DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/25/2022
 Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 23:26:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	218777	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136	981039	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	686999	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	1445910	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	1129041	20.000	ng/ul	# 0.00
88) Perylene-d12	23.857	264	969300	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	1457m	0.290	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.105	99	8166	0.410	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	20280	1.698	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	21122	1.433	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	15117	0.917	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	13482	1.728	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	13659	1.603	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	24290	1.464	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	28644	1.204	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	93160	1.743	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160	104178	1.611	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.563	176	81904	1.782	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.422	188	135683	1.940	ng/ul	0.00
81) Pyrene-d10	19.651	212	148526	2.313	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	93537	1.841	ng/ul	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.146	77	1005203	52.582	ng/ul#	87
75) 1,2,3,4-Tetrachloroben...	13.375	216	21323	1.010	ng/uL	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010050.D
Acq On : 22 Apr 2022 11:49
Operator : CG/JU
Sample : N2473-13DL 20X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HX2DL

Manual IntegrationsAPPROVED

Quant Time: Apr 22 23:26:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/25/2022
Supervised By :mohammad ahmed 04/26/2022

