




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010055.D
 Acq On : 22 Apr 2022 14:37
 Operator : CG/JU
 Sample : N2473-18
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ9

Manual IntegrationsAPPROVED

Quant Time: Apr 22 23:28:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/25/2022
 Supervised By :mohammad ahmed 04/26/2022

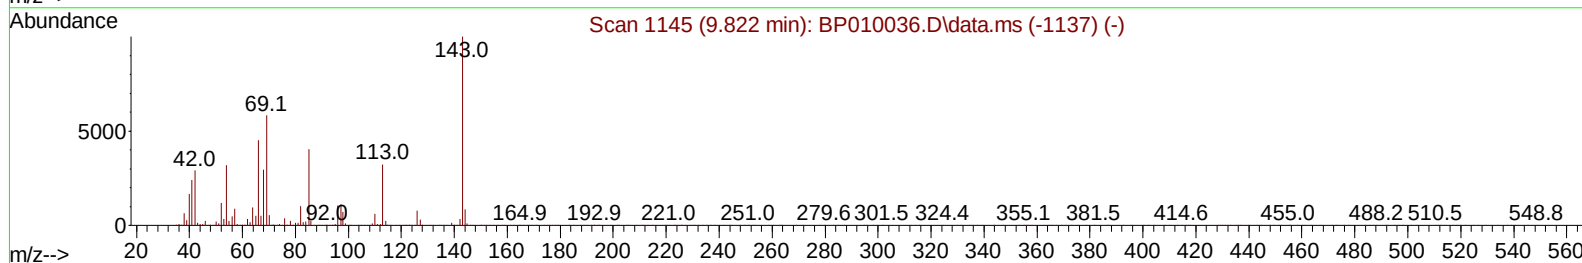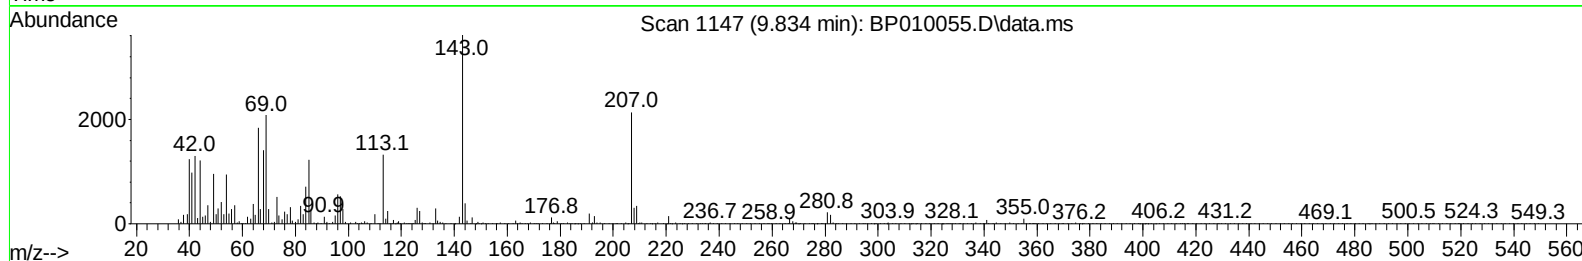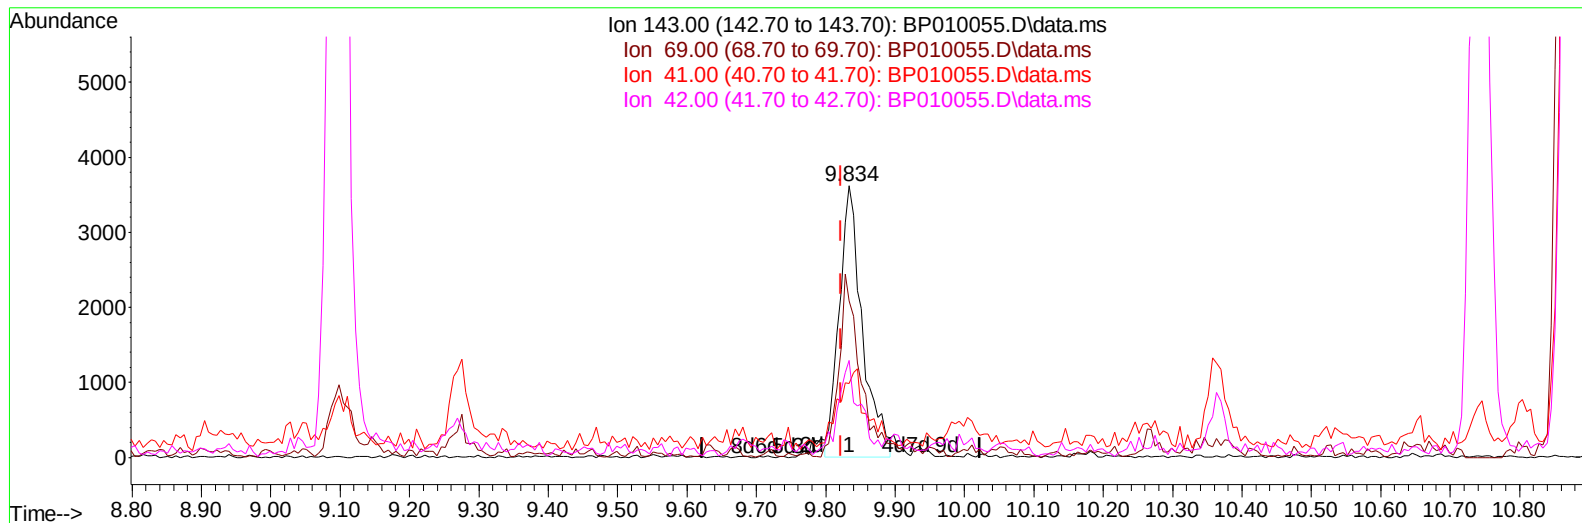

TIC: BP010055.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.834min (+ 0.012) 1.24 ng/ul

response 8357

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	47.10	57.55#
41.00	16.70	27.25#
42.00	20.70	35.82#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010055.D
 Acq On : 22 Apr 2022 14:37
 Operator : CG/JU
 Sample : N2473-18
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ9

Manual IntegrationsAPPROVED

Quant Time: Apr 22 23:28:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/25/2022
 Supervised By :mohammad ahmed 04/26/2022

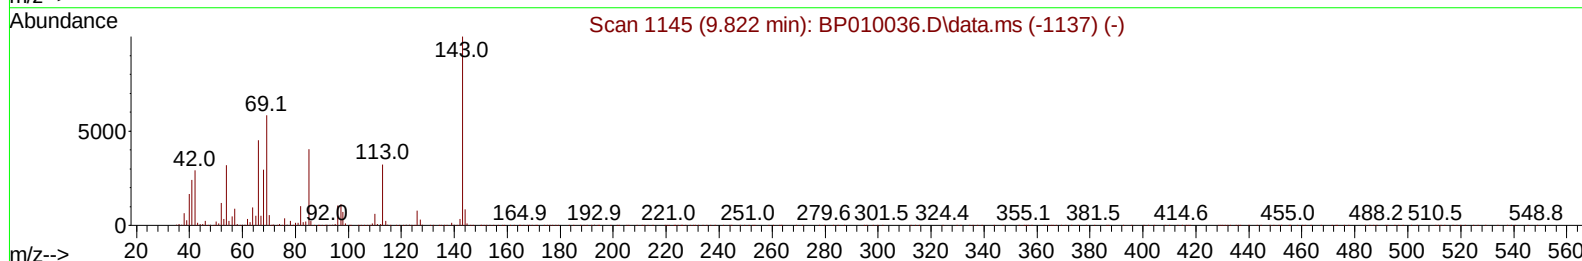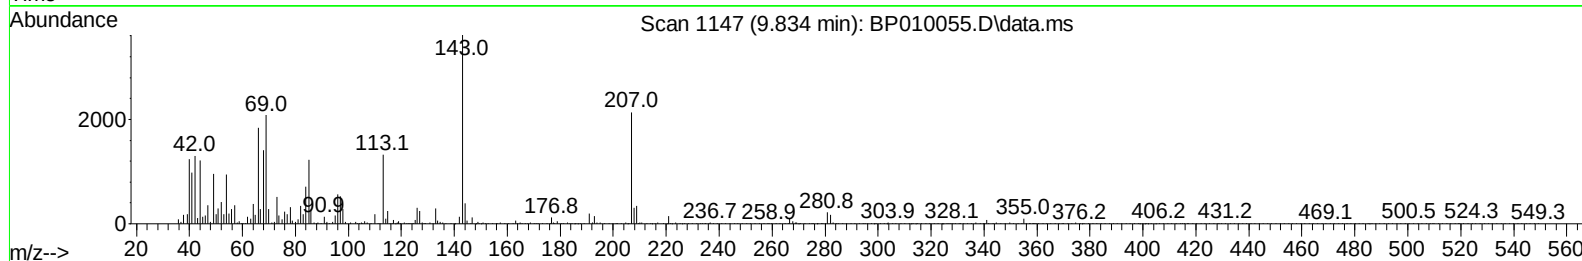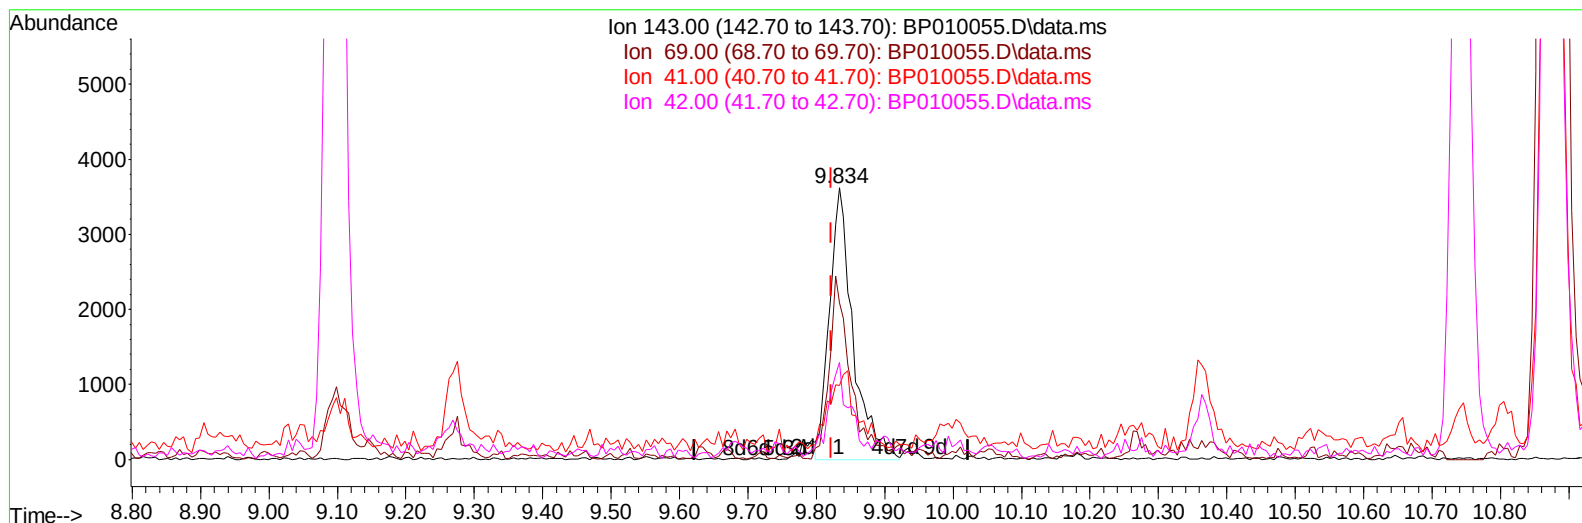

TIC: BP010055.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.834min (+ 0.012) 1.28 ng/ul m

response 8622

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	47.10	57.55#
41.00	16.70	27.25#
42.00	20.70	35.82#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010055.D
Acq On : 22 Apr 2022 14:37
Operator : CG/JU
Sample : N2473-18
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9

Manual IntegrationsAPPROVED

Quant Time: Apr 22 23:28:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/25/2022
Supervised By :mohammad ahmed 04/26/2022

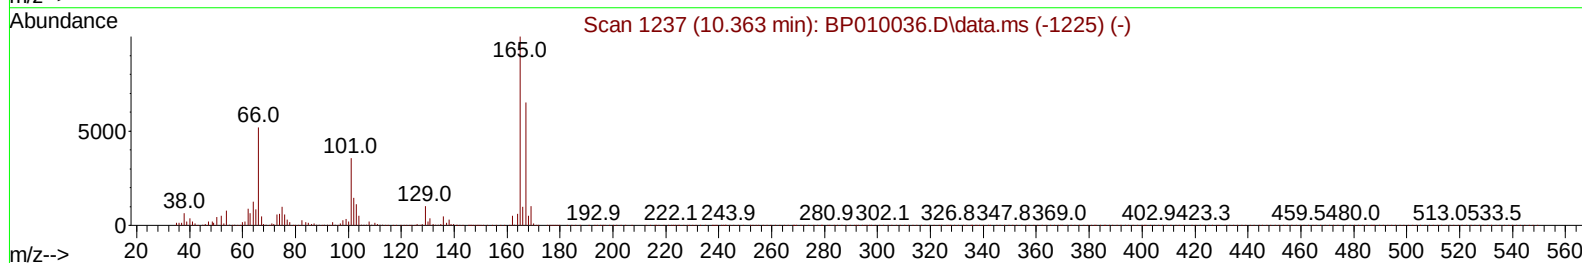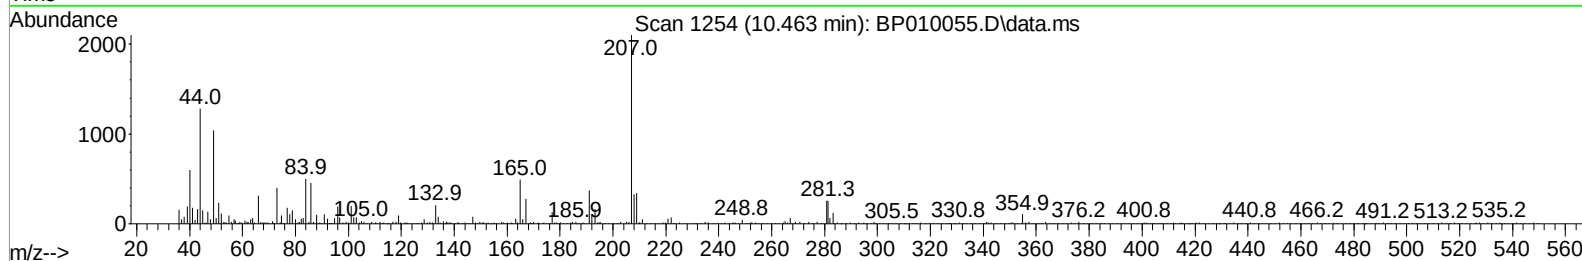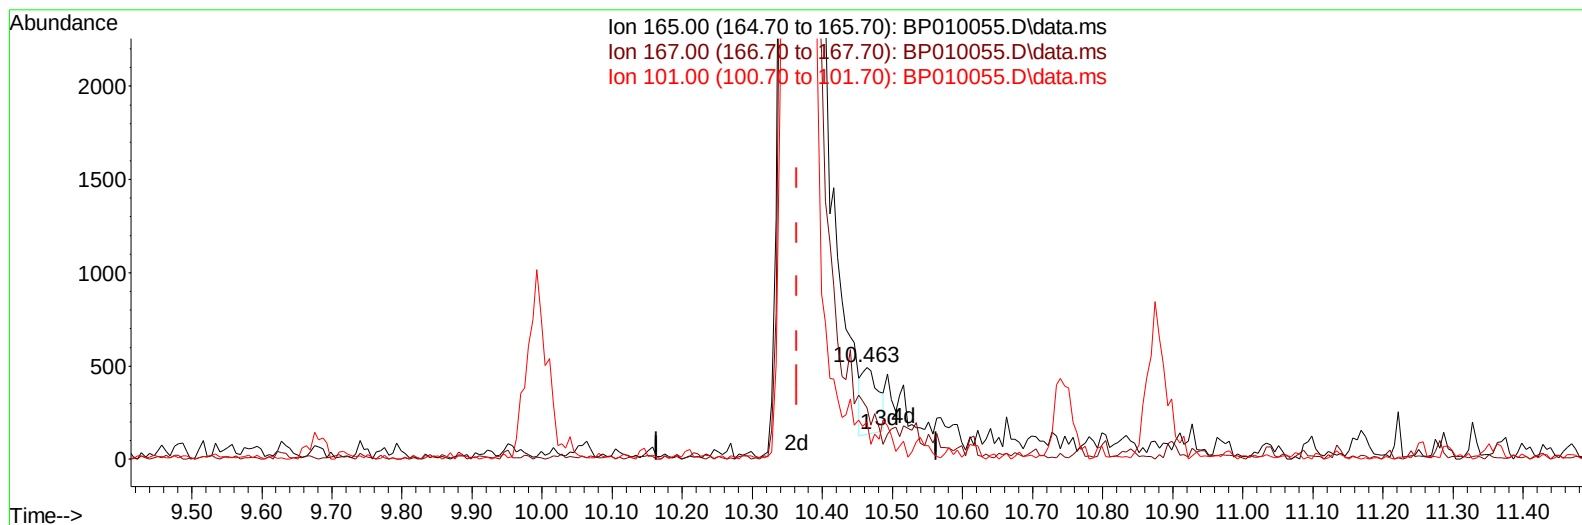

TIC: BP010055.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.463min (+ 0.100) 0.05 ng/ul

response 601

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	56.10
101.00	49.80	40.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010055.D
 Acq On : 22 Apr 2022 14:37
 Operator : CG/JU
 Sample : N2473-18
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ9

Manual IntegrationsAPPROVED

Quant Time: Apr 22 23:28:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/25/2022
 Supervised By :mohammad ahmed 04/26/2022

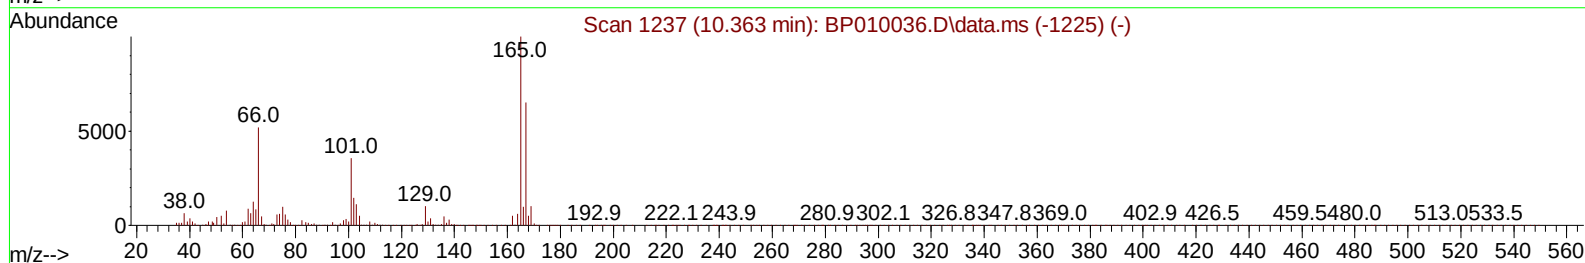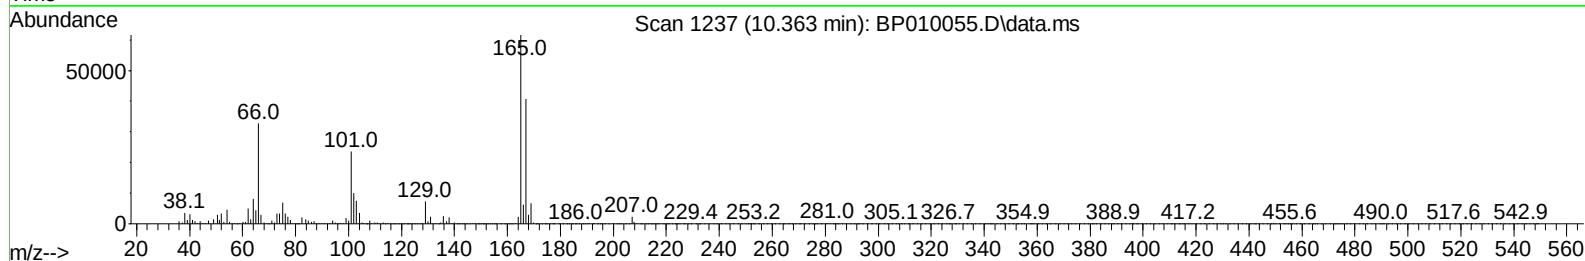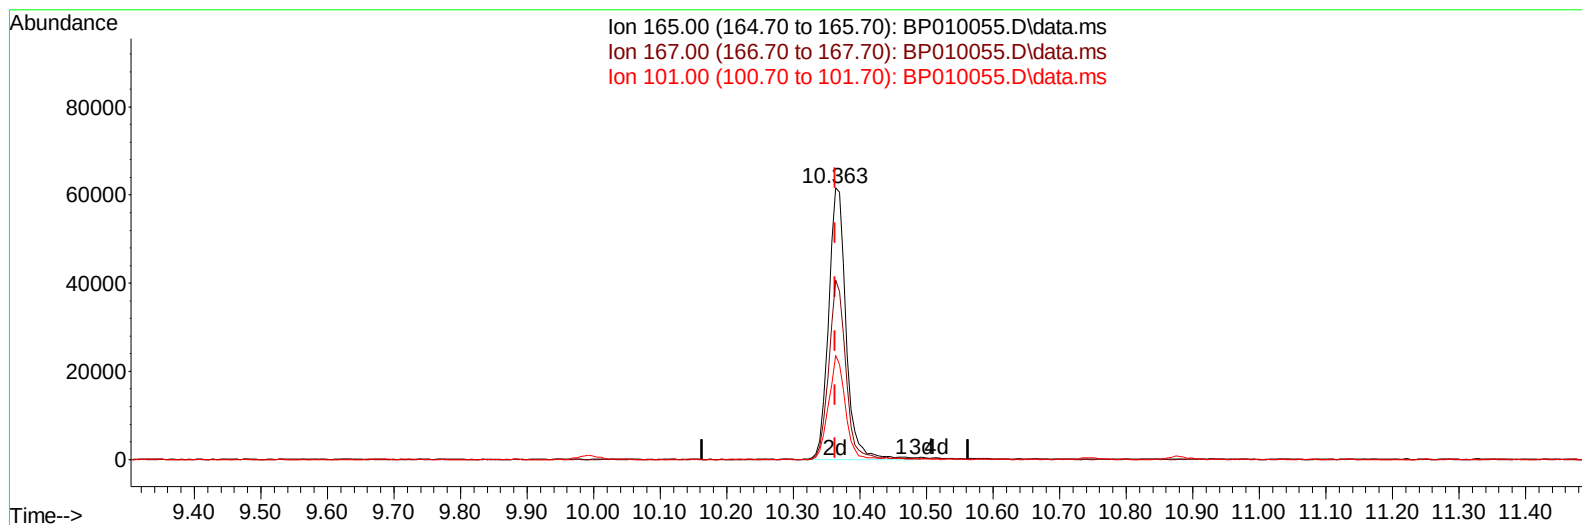

TIC: BP010055.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.363min (+ 0.000) 8.66 ng/ul m

response 113240

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	66.17
101.00	49.80	38.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010055.D
Acq On : 22 Apr 2022 14:37
Operator : CG/JU
Sample : N2473-18
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9

Manual IntegrationsAPPROVED

Quant Time: Apr 22 23:28:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/25/2022
Supervised By :mohammad ahmed 04/26/2022

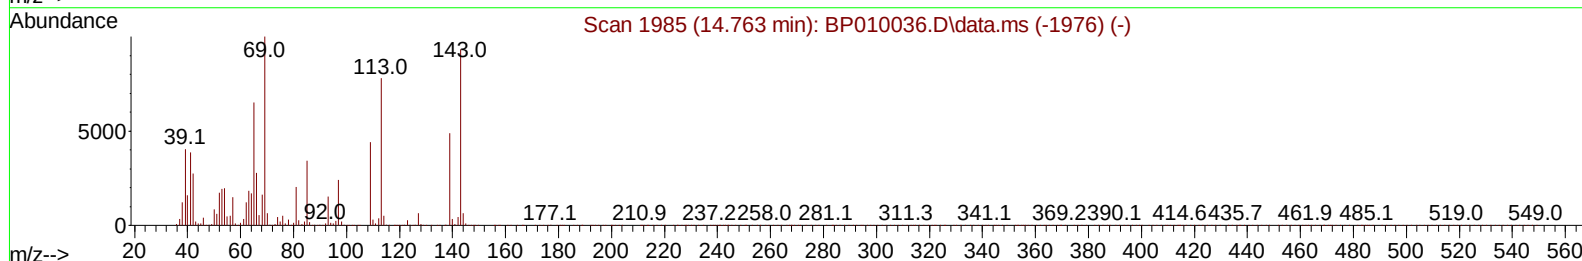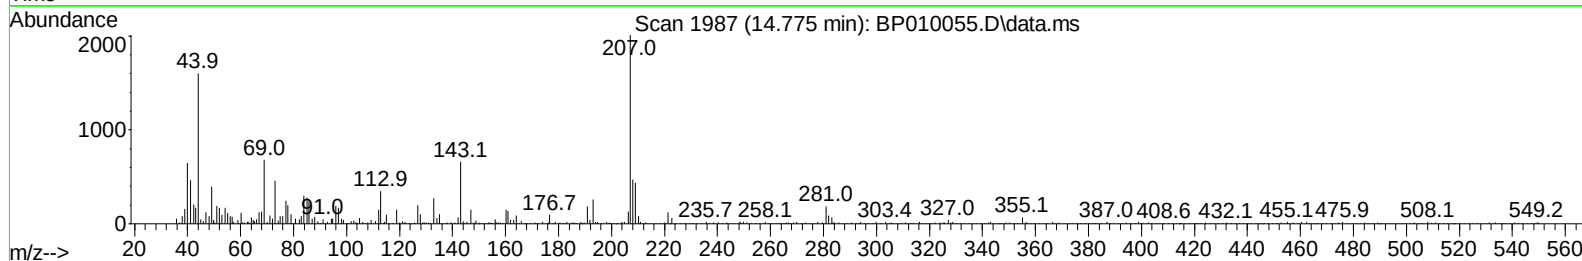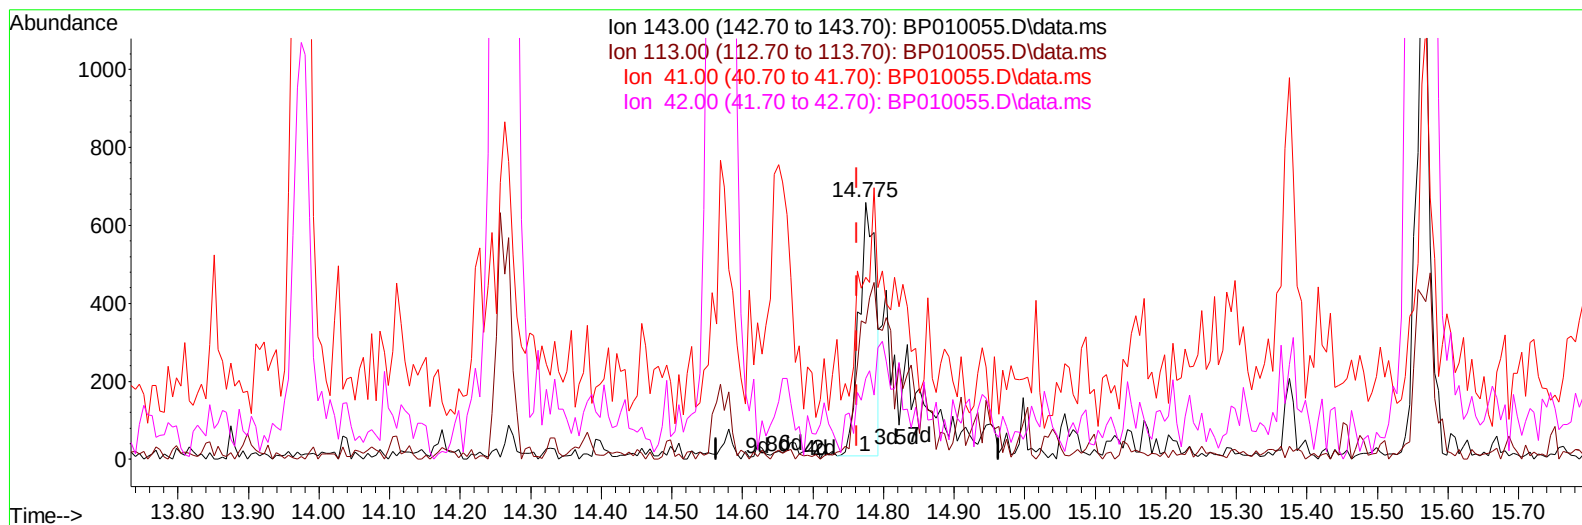

TIC: BP010055.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.775min (+ 0.012) 0.13 ng/ul

response 1069

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	54.32#
41.00	23.20	70.86#
42.00	18.00	31.56#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010055.D
Acq On : 22 Apr 2022 14:37
Operator : CG/JU
Sample : N2473-18
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9

Manual IntegrationsAPPROVED

Quant Time: Apr 22 23:28:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/25/2022
Supervised By :mohammad ahmed 04/26/2022

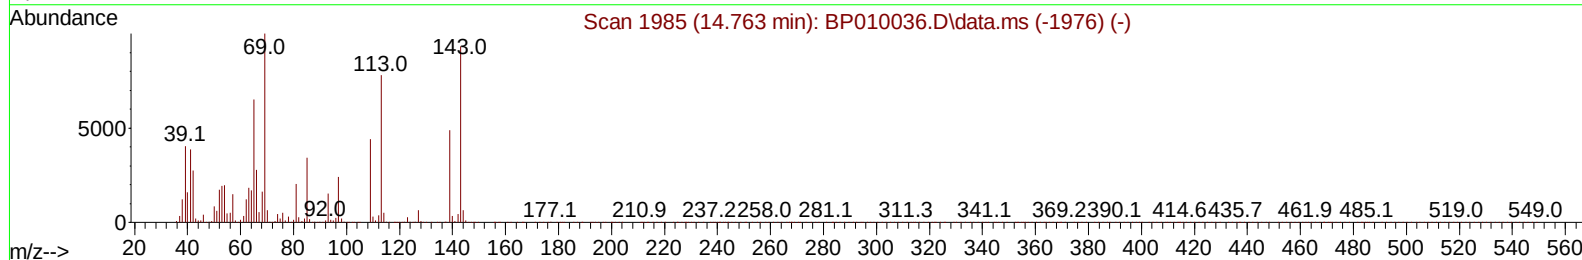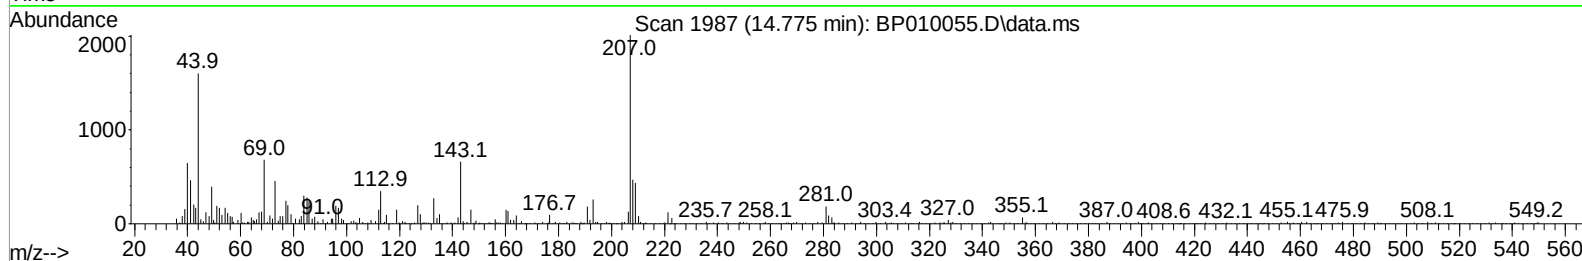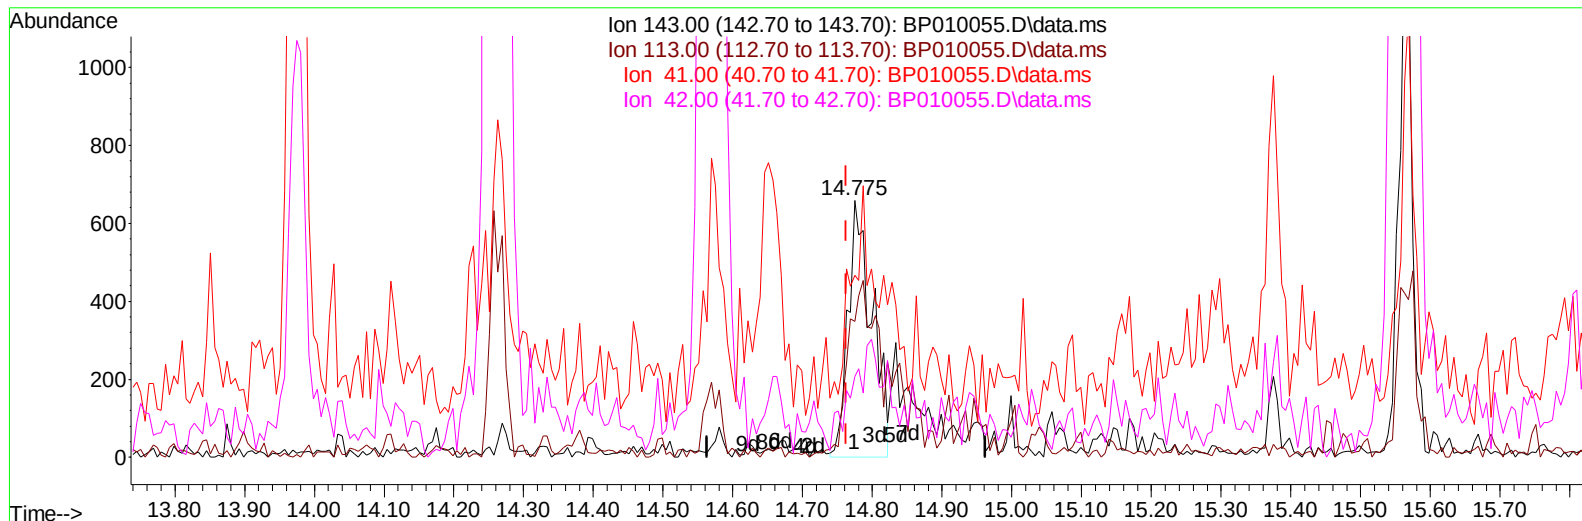

TIC: BP010055.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.775min (+ 0.012) 0.20 ng/ul m

response 1565

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	52.81#
41.00	23.20	70.86#
42.00	18.00	31.56#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010055.D
 Acq On : 22 Apr 2022 14:37
 Operator : CG/JU
 Sample : N2473-18
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/25/2022
 Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 23:28:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	166393	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136	773266	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	558418	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	1186685	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	1063469	20.000	ng/ul	0.00
88) Perylene-d12	23.863	264	887655	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	21630	5.669	ng/uL	0.00
4) Pyridine-d5	3.793	84	91143	8.491	ng/ul	0.00
7) Phenol-d5	7.099	99	24003	1.586	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	256264	28.218	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	103392	9.224	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	45036	3.591	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	172156	27.992	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	8622m	1.284	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.363	165	113240m	8.660	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	453533	24.190	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	1294899	29.810	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160	1400035	26.630	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	1565m	0.196	ng/ul	0.01
60) Fluorene-d10	15.563	176	1075607	28.786	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	30	0.004	ng/ul	-0.01
73) Anthracene-d10	17.422	188	1819639	31.695	ng/ul	0.00
81) Pyrene-d10	19.651	212	2107212	34.842	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1503820	32.315	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010055.D
Acq On : 22 Apr 2022 14:37
Operator : CG/JU
Sample : N2473-18
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/25/2022
Supervised By :mohammad ahmed 04/26/2022

Quant Time: Apr 22 23:28:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

