




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010074.D
Acq On : 23 Apr 2022 02:10
Operator : CG/JU
Sample : N2475-06
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BP0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:56:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

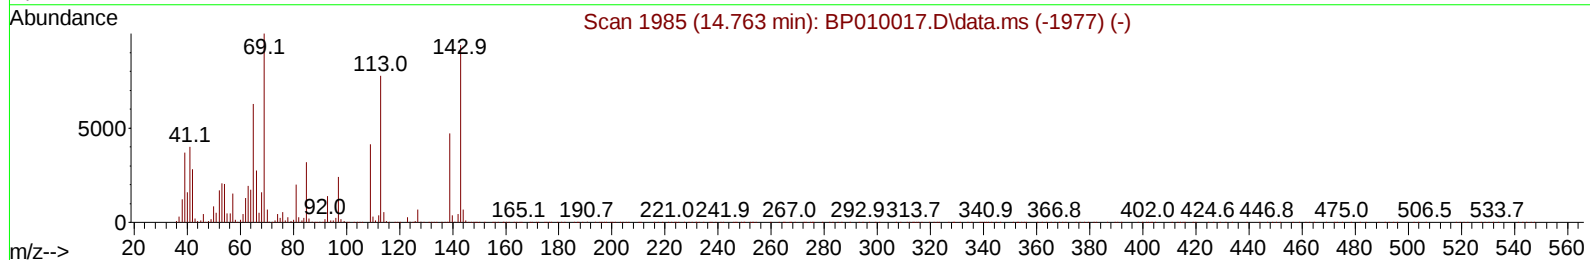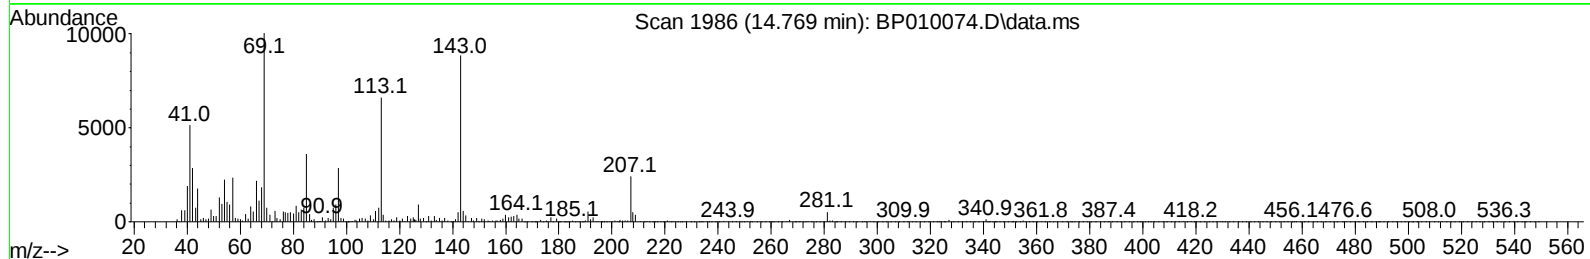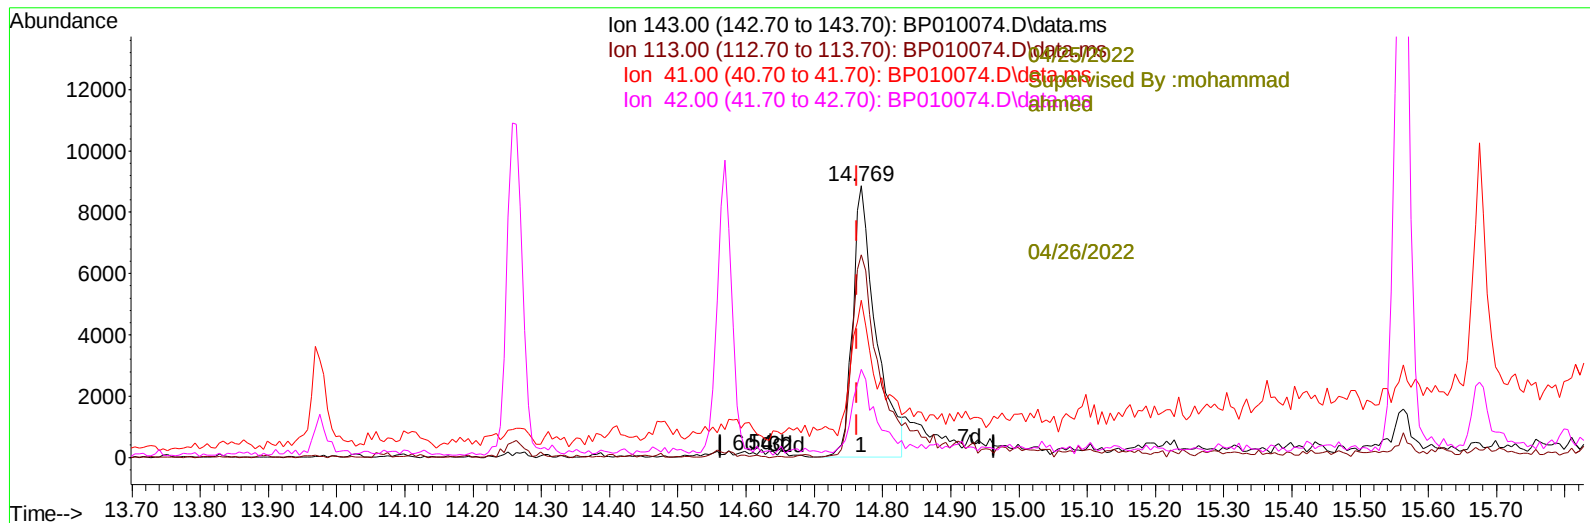

TIC: BP010074.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.769min (+ 0.006) 3.15 ng/u1

response 20839

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	74.70#
41.00	23.20	57.93#
42.00	18.00	32.36#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010074.D
Acq On : 23 Apr 2022 02:10
Operator : CG/JU
Sample : N2475-06
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BP0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:56:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

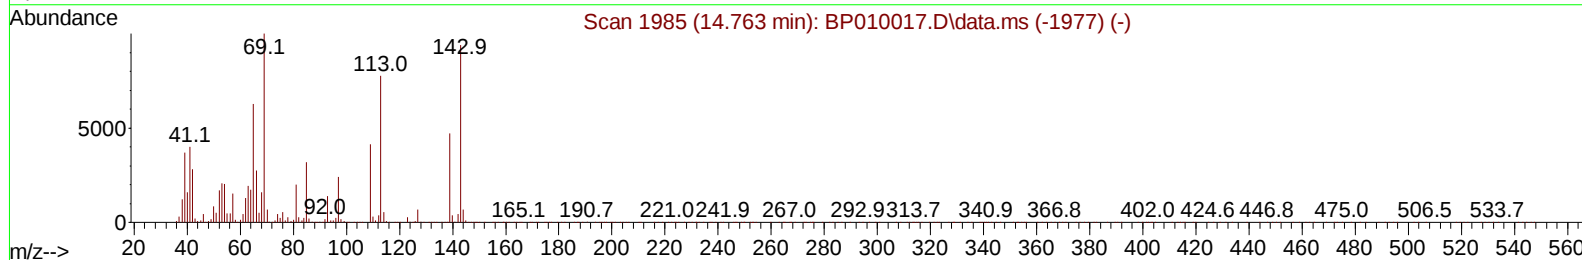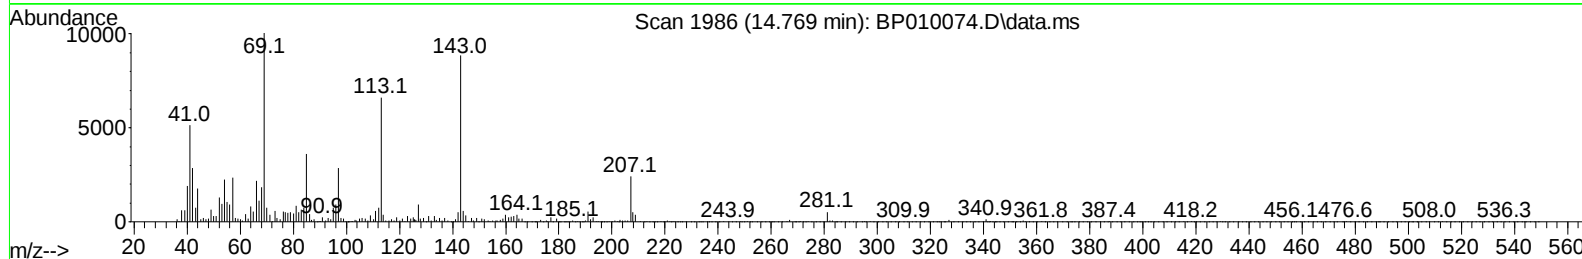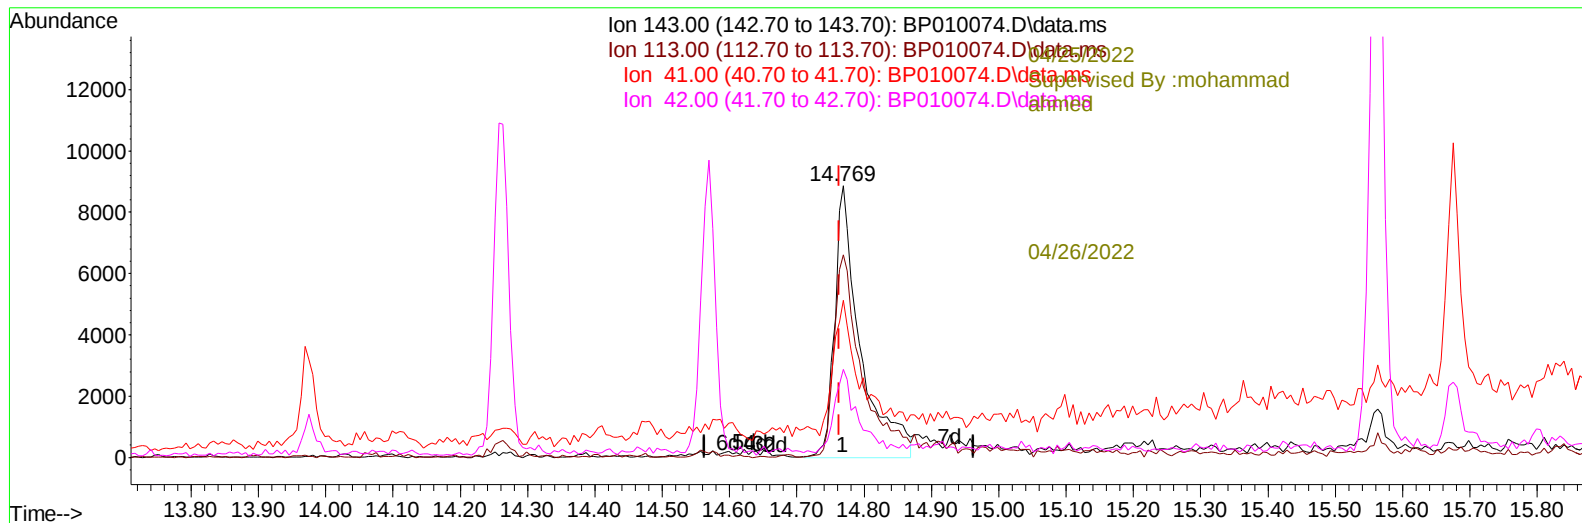

TIC: BP010074.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.769min (+ 0.006) 3.54 ng/ul m

response 23471

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	74.70#
41.00	23.20	57.93#
42.00	18.00	32.36#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010074.D
 Acq On : 23 Apr 2022 02:10
 Operator : CG/JU
 Sample : N2475-06
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BP0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 03:56:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----04/25/2022							
Supervised By :mohammad ali med							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.940	152		134645	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136		637980	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164		462554	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188		978676	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.398	240		784067	20.000	ng/ul	#-0.01
88) Perylene-d12	23.857	264		682289	20.000	ng/ul	0.00
-----04/26/2022							
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.370	96		13521	4.379	ng/uL	0.00
4) Pyridine-d5	3.799	84		61308	7.058	ng/ul	0.01
7) Phenol-d5	7.099	99		78314	6.394	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.264	67		241184	32.819	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132		232018	25.580	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113		161772	15.943	ng/ul	-0.01
21) Nitrobenzene-d5	9.099	128		161361	31.801	ng/ul	0.00
24) 2-Nitrophenol-d4	9.822	143		165652	29.892	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165		294160	27.267	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131		364304	23.551	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166		1247023	34.657	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160		1394261	32.017	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143		23471m	3.543	ng/ul	0.00
60) Fluorene-d10	15.563	176		1117831	36.116	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200		124897	20.183	ng/ul	0.00
73) Anthracene-d10	17.422	188		1814224	38.317	ng/ul	0.00
81) Pyrene-d10	19.651	212		2106203	47.235	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264		1439004	40.230	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010074.D
Acq On : 23 Apr 2022 02:10
Operator : CG/JU
Sample : N2475-06
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BP0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut
Upadhyay

Quant Time: Apr 23 03:56:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

