

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010019.D
 Acq On : 21 Apr 2022 17:53
 Operator : CG/JU
 Sample : PB144260BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	57	rVB	35377	50682	1.17%	0.124%
2	3.787	115	119	140	rBV	403201	724490	16.77%	1.775%
3	4.116	172	175	181	rVB2	11081	16953	0.39%	0.042%
4	7.099	675	682	694	rBV	547519	905125	20.95%	2.217%
5	7.263	704	710	725	rVB	446650	739880	17.13%	1.812%
6	7.469	738	745	759	rVB	572278	931632	21.56%	2.282%
7	7.940	817	825	835	rBV	449643	727565	16.84%	1.782%
8	8.646	934	945	957	rBV	731282	1234489	28.57%	3.024%
9	9.099	1014	1022	1035	rBV	601290	1027693	23.79%	2.517%
10	9.822	1136	1145	1160	rBV	508206	875228	20.26%	2.144%
11	10.363	1227	1237	1250	rBV	723136	1254988	29.05%	3.074%
12	10.746	1293	1302	1316	rBV	679921	1130539	26.17%	2.769%
13	10.875	1316	1324	1339	rBV	743272	1350395	31.26%	3.308%
14	12.328	1567	1571	1577	rBV3	14118	25431	0.59%	0.062%
15	12.545	1605	1608	1612	rBV6	2978	4848	0.11%	0.012%
16	13.310	1736	1738	1744	rVB7	3427	6275	0.15%	0.015%
17	13.545	1774	1778	1782	rBV7	2487	4391	0.10%	0.011%
18	13.975	1844	1851	1862	rBV	1632826	2320921	53.72%	5.685%
19	14.075	1866	1868	1877	rVB9	3457	6138	0.14%	0.015%
20	14.263	1891	1900	1914	rBV	1663194	2491363	57.67%	6.103%
21	14.569	1944	1952	1963	rBV	1123144	1718683	39.78%	4.210%
22	14.757	1978	1984	1998	rBV	691190	1092122	25.28%	2.675%
23	15.216	2055	2062	2063	rBV7	3107	5839	0.14%	0.014%
24	15.563	2114	2121	2134	rBV	2272365	3277295	75.86%	8.028%
25	15.675	2134	2140	2152	rBV	748570	1061196	24.56%	2.599%
26	15.804	2157	2162	2172	rVB	29927	47059	1.09%	0.115%
27	16.257	2232	2239	2240	rBV7	2783	4844	0.11%	0.012%
28	16.351	2248	2255	2261	rBV5	9832	17630	0.41%	0.043%
29	16.998	2362	2365	2369	rVB6	4766	6887	0.16%	0.017%
30	17.110	2377	2384	2388	rBV4	7131	12746	0.30%	0.031%
31	17.322	2413	2420	2429	rBV	1449823	2167684	50.17%	5.310%
32	17.422	2430	2437	2452	rVB	2477714	3641027	84.28%	8.919%
33	17.992	2532	2534	2539	rVB6	4136	4441	0.10%	0.011%
34	18.269	2578	2581	2586	rBV7	3779	4870	0.11%	0.012%
35	19.227	2740	2744	2751	rBV3	30265	41065	0.95%	0.101%
36	19.298	2752	2756	2763	rVB	33286	43497	1.01%	0.107%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010019.D
Acq On : 21 Apr 2022 17:53
Operator : CG/JU
Sample : PB144260BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK260

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

37	19.651	2810	2816	2833	rBV	3215584	4320388	100.00%	10.583%
38	21.404	3109	3114	3127	rBV	1642165	2212314	51.21%	5.419%
39	23.698	3497	3504	3511	rBV2	1655342	3317680	76.79%	8.127%
40	23.857	3524	3531	3546	rVB2	923784	1997032	46.22%	4.892%




Sum of corrected areas: 40823325

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010019.D
Acq On : 21 Apr 2022 17:53
Operator : CG/JU
Sample : PB144260BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

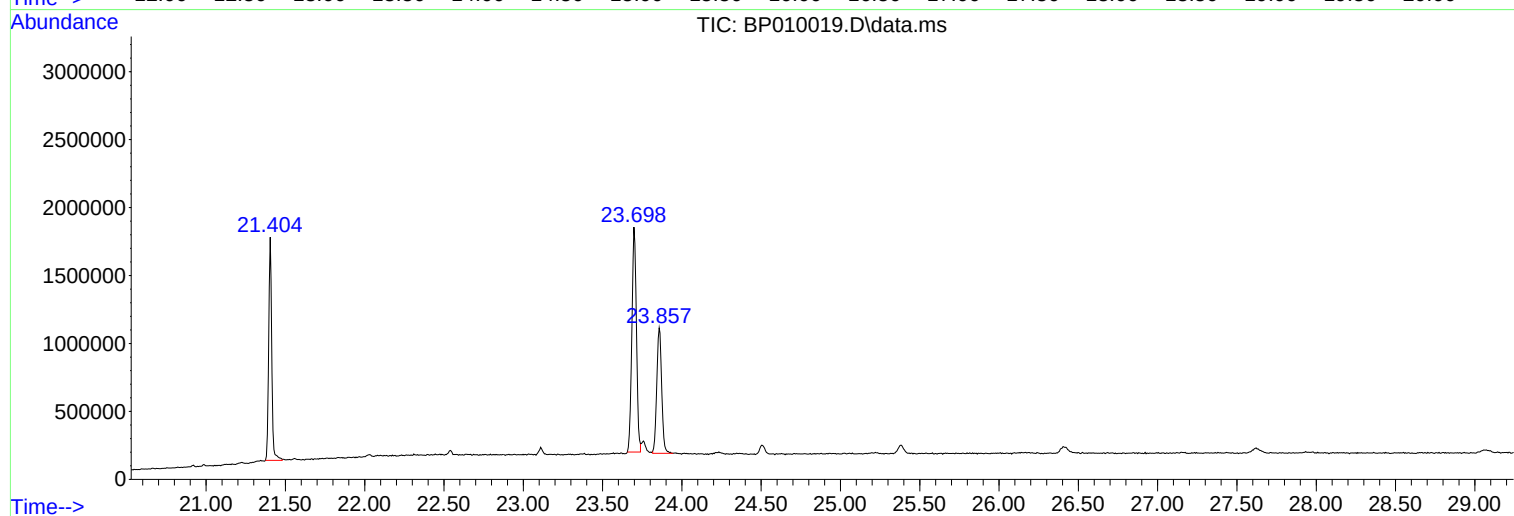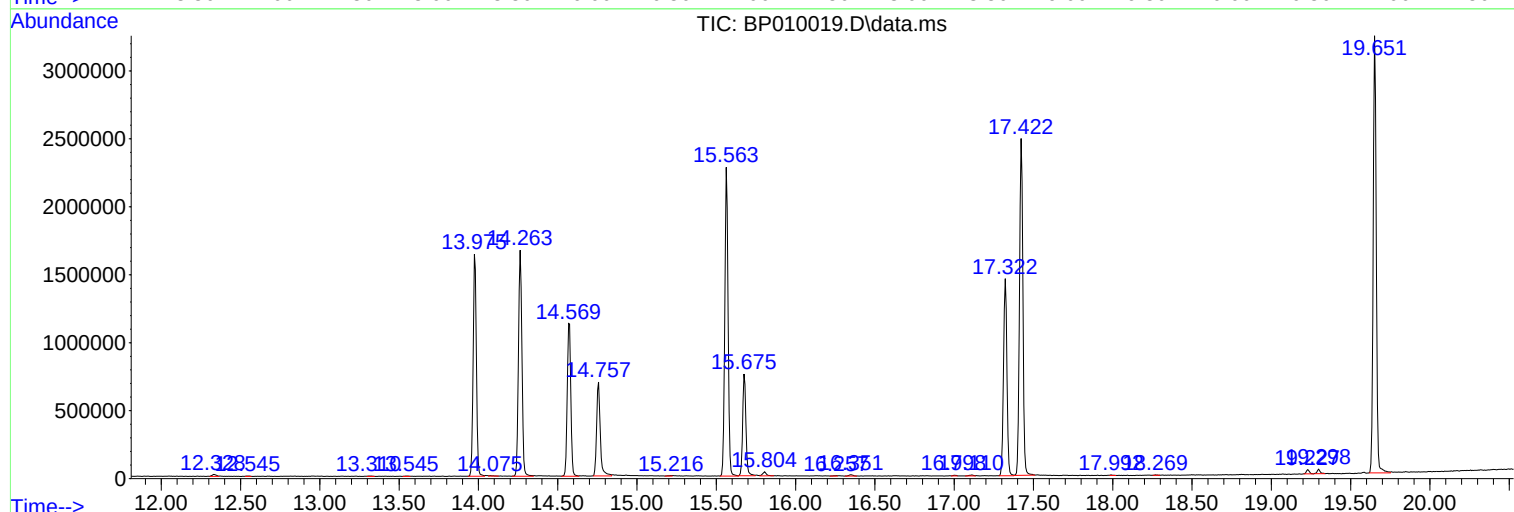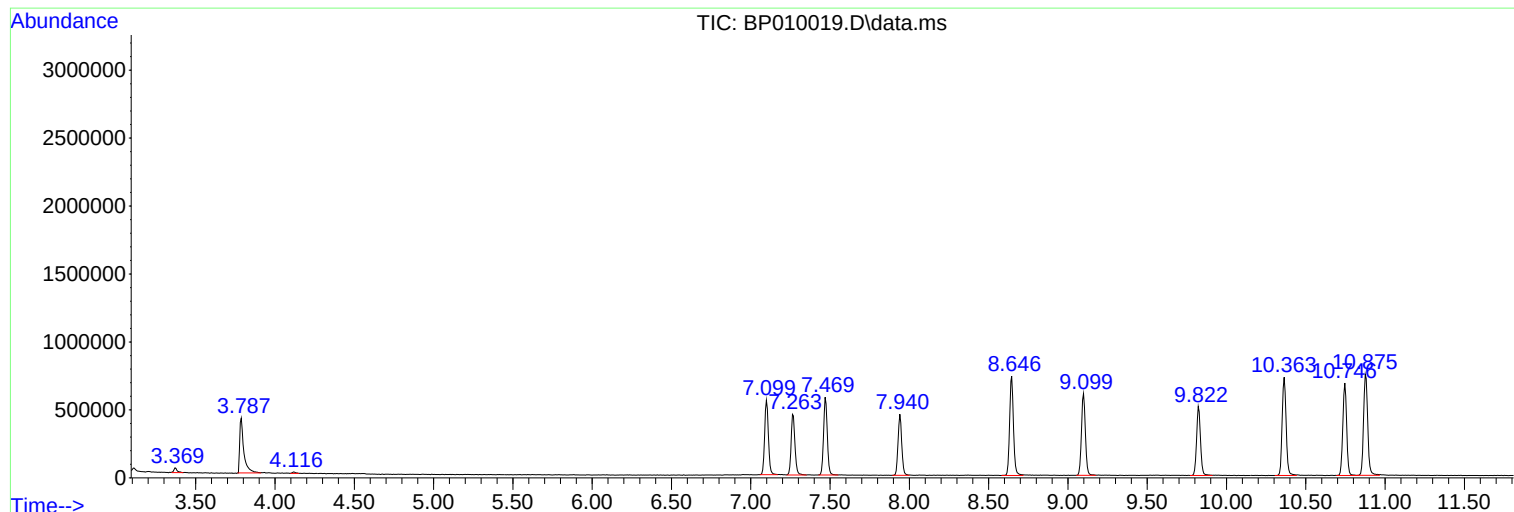

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010019.D
Acq On : 21 Apr 2022 17:53
Operator : CG/JU
Sample : PB144260BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010019.D
Acq On : 21 Apr 2022 17:53
Operator : CG/JU
Sample : PB144260BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------