

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010023.D
 Acq On : 21 Apr 2022 20:07
 Operator : CG/JU
 Sample : N2373-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	45	48	56	rVB	22054	29630	0.80%	0.083%
2	3.481	64	67	68	rBV3	3999	3715	0.10%	0.010%
3	3.787	116	119	134	rBV	262619	512203	13.86%	1.430%
4	4.117	173	175	181	rVB7	5657	9946	0.27%	0.028%
5	6.822	630	635	638	rBV7	2253	3870	0.10%	0.011%
6	7.099	675	682	693	rBV	454865	750241	20.30%	2.095%
7	7.263	704	710	720	rBV	356487	592080	16.02%	1.653%
8	7.469	738	745	756	rBV	476849	765023	20.70%	2.136%
9	7.940	818	825	835	rVV	358853	598268	16.19%	1.671%
10	8.005	835	836	842	rVB4	6559	8365	0.23%	0.023%
11	8.252	872	878	884	rBV10	7261	13917	0.38%	0.039%
12	8.646	936	945	958	rBV	617941	1043071	28.22%	2.913%
13	9.099	1014	1022	1033	rBV	481747	833171	22.54%	2.326%
14	9.552	1093	1099	1104	rVB2	21403	34937	0.95%	0.098%
15	9.822	1136	1145	1157	rBV	411953	702703	19.01%	1.962%
16	10.240	1214	1216	1223	rVB7	2824	4951	0.13%	0.014%
17	10.363	1230	1237	1248	rBV	610923	1053819	28.51%	2.943%
18	10.557	1268	1270	1275	rVB6	3345	4906	0.13%	0.014%
19	10.746	1293	1302	1311	rBV	552541	939993	25.43%	2.625%
20	10.875	1317	1324	1341	rBV	592583	1091172	29.52%	3.047%
21	11.793	1475	1480	1485	rVB7	3580	6789	0.18%	0.019%
22	12.175	1540	1545	1553	rVB3	14303	23843	0.65%	0.067%
23	12.334	1566	1572	1579	rBV3	11294	23290	0.63%	0.065%
24	12.810	1647	1653	1656	rBV8	2833	5400	0.15%	0.015%
25	12.851	1656	1660	1666	rVB8	2870	5351	0.14%	0.015%
26	12.987	1681	1683	1686	rVB4	3570	3764	0.10%	0.011%
27	13.075	1694	1698	1702	rVB7	3872	6044	0.16%	0.017%
28	13.128	1702	1707	1711	rVV7	5119	8858	0.24%	0.025%
29	13.193	1714	1718	1722	rVB6	3553	5594	0.15%	0.016%
30	13.304	1735	1737	1742	rBV6	2714	3741	0.10%	0.010%
31	13.410	1748	1755	1762	rVB2	14912	22041	0.60%	0.062%
32	13.851	1823	1830	1831	rBV7	3341	3807	0.10%	0.011%
33	13.975	1845	1851	1862	rBV	1255414	1782319	48.22%	4.977%
34	14.263	1892	1900	1912	rBV	1337733	2022642	54.72%	5.648%
35	14.569	1943	1952	1964	rBV	934918	1408160	38.10%	3.932%
36	14.757	1976	1984	2005	rBV	477991	828236	22.41%	2.313%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010023.D
 Acq On : 21 Apr 2022 20:07
 Operator : CG/JU
 Sample : N2373-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	14.987	2019	2023	2030	rVB10	5638	10033	0.27%	0.028%
38	15.381	2086	2090	2095	rBV6	5037	7774	0.21%	0.022%
39	15.563	2114	2121	2134	rBV	1823867	2646166	71.59%	7.389%
40	15.675	2134	2140	2150	rBV	493878	683449	18.49%	1.908%
41	15.804	2157	2162	2172	rVB2	21145	36931	1.00%	0.103%
42	16.010	2194	2197	2200	rVB5	4080	6020	0.16%	0.017%
43	16.128	2216	2217	2222	rVB5	3571	4721	0.13%	0.013%
44	16.292	2241	2245	2249	rVB7	5245	8594	0.23%	0.024%
45	16.357	2249	2256	2261	rVB7	6800	12828	0.35%	0.036%
46	16.522	2280	2284	2288	rVV2	17802	25370	0.69%	0.071%
47	17.004	2363	2366	2371	rVB6	6555	9640	0.26%	0.027%
48	17.116	2381	2385	2388	rVV6	4120	7626	0.21%	0.021%
49	17.322	2412	2420	2431	rBV	1242121	1807643	48.90%	5.047%
50	17.422	2431	2437	2446	rBV	2037939	2911532	78.77%	8.130%
51	17.910	2518	2520	2523	rVB4	4609	4927	0.13%	0.014%
52	17.939	2523	2525	2528	rBV4	3379	4359	0.12%	0.012%
53	17.992	2531	2534	2538	rVB2	14311	17977	0.49%	0.050%
54	18.063	2544	2546	2547	rBV2	5646	4120	0.11%	0.012%
55	18.204	2565	2570	2578	rBV	98232	156157	4.22%	0.436%
56	19.181	2732	2736	2739	rVB6	13724	19329	0.52%	0.054%
57	19.228	2741	2744	2752	rVB3	32074	41363	1.12%	0.115%
58	19.298	2752	2756	2759	rBV	30769	42713	1.16%	0.119%
59	19.381	2766	2770	2774	rVB4	12898	18502	0.50%	0.052%
60	19.651	2810	2816	2831	rBV	2706020	3696238	100.00%	10.321%
61	20.139	2897	2899	2905	rBV6	14764	20584	0.56%	0.057%
62	21.110	3059	3064	3073	rBV	514479	671704	18.17%	1.876%
63	21.404	3108	3114	3128	rVB	1496553	2127877	57.57%	5.942%
64	23.110	3400	3404	3408	rBV	88270	125464	3.39%	0.350%
65	23.698	3496	3504	3510	rBV2	1670423	3293506	89.10%	9.196%
66	23.857	3523	3531	3541	rVB2	944397	2009792	54.37%	5.612%
67	24.504	3637	3641	3648	rVB	112663	224626	6.08%	0.627%




Sum of corrected areas: 35813425

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010023.D
Acq On : 21 Apr 2022 20:07
Operator : CG/JU
Sample : N2373-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

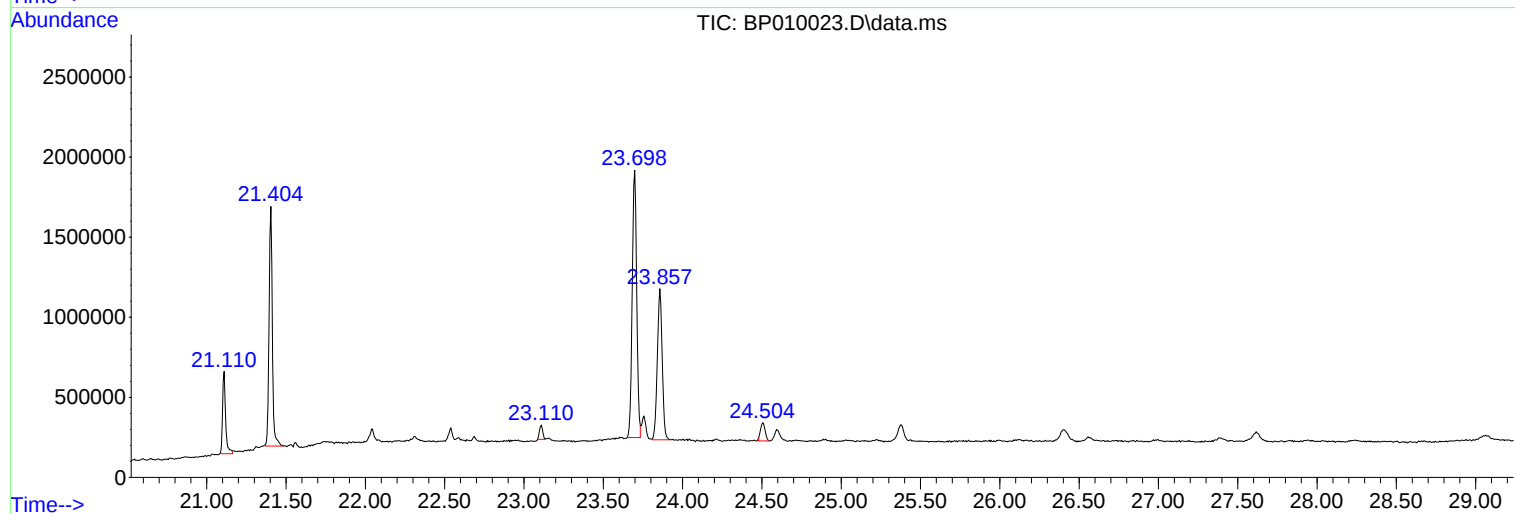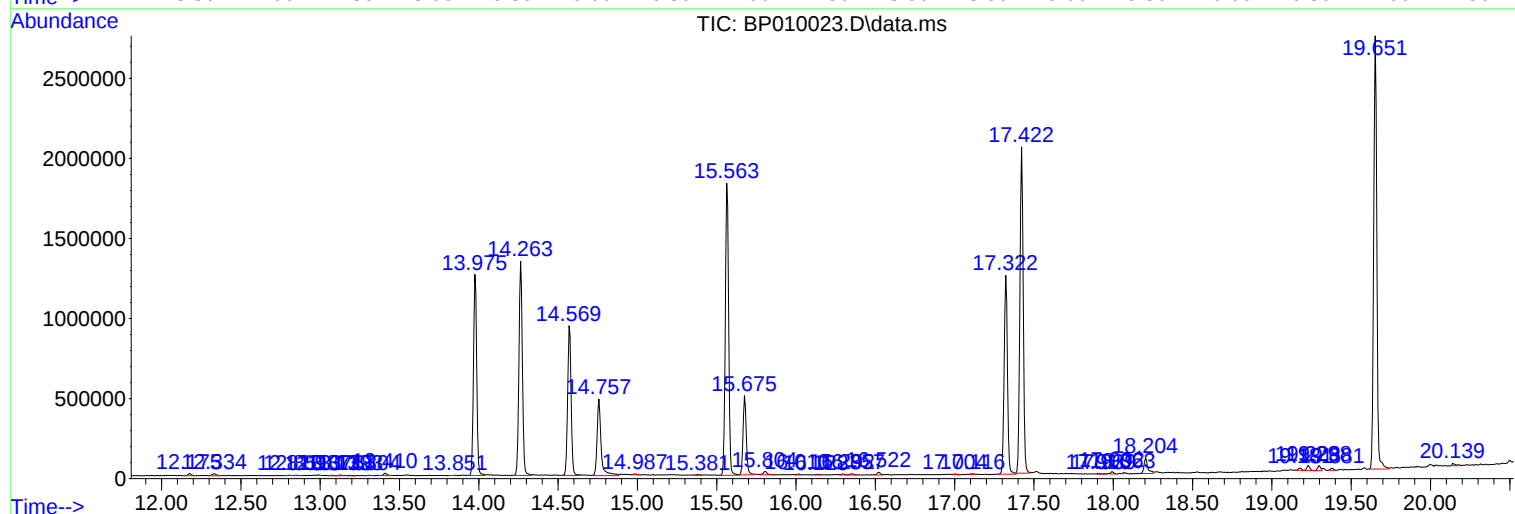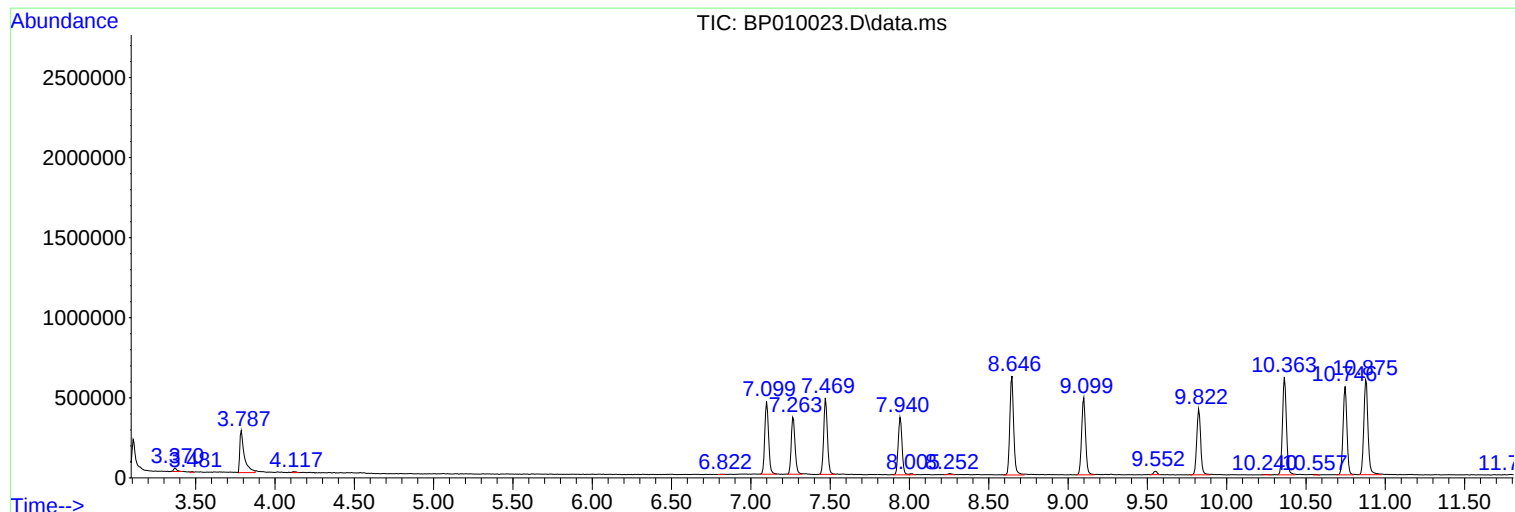

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010023.D
Acq On : 21 Apr 2022 20:07
Operator : CG/JU
Sample : N2373-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFD3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.110	6.31 ng/ul	671704	Chrysene-d12	21.404

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Eicosene, (E)-			280	C20H40	074685-33-9	96
2	1-Heneicosanol			312	C21H44O	015594-90-8	95
3	Cycloeicosane			280	C20H40	000296-56-0	94
4	1-Tetracosene			336	C24H48	010192-32-2	94
5	1-Hexacosene			364	C26H52	018835-33-1	94

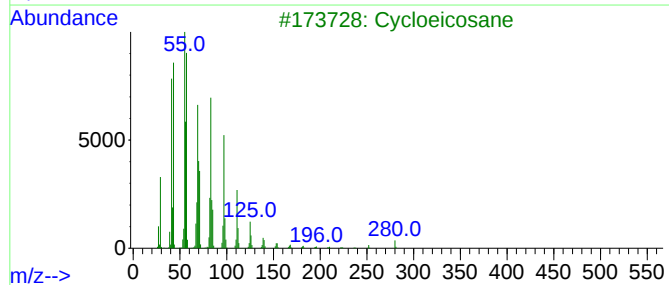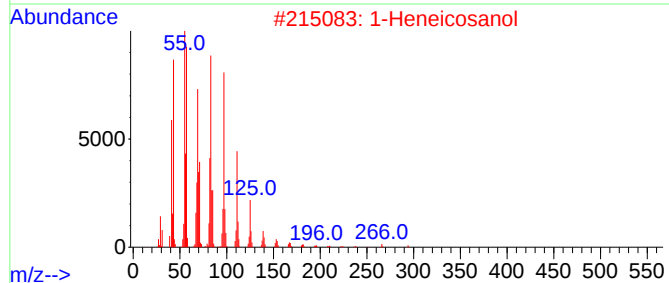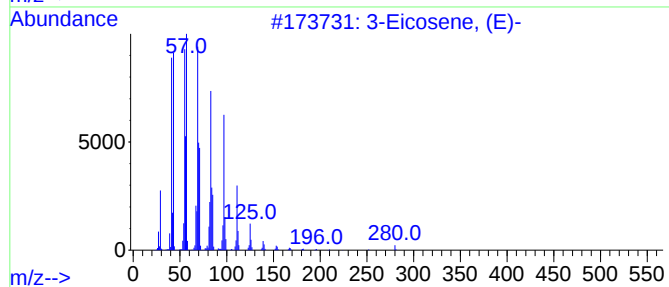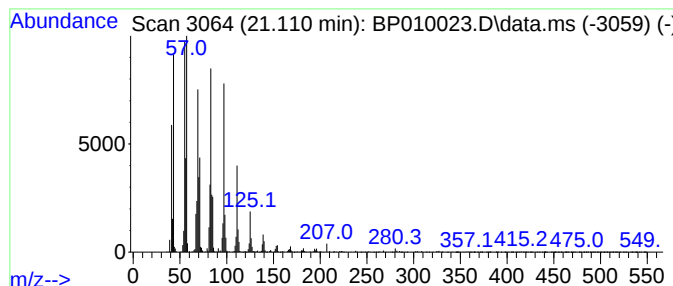

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010023.D
Acq On : 21 Apr 2022 20:07
Operator : CG/JU
Sample : N2373-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFD3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.504	2.24 ng/ul	224626	Perylene-d12	23.857

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Heptadecane, 9-octyl-	352	C25H52	007225-64-1	93
2		Heneicosane	296	C21H44	000629-94-7	93
3		Heneicosane, 11-decyl-	437	C31H64	055320-06-4	93
4		Tricosane	324	C23H48	000638-67-5	93
5		Heneicosane	296	C21H44	000629-94-7	91

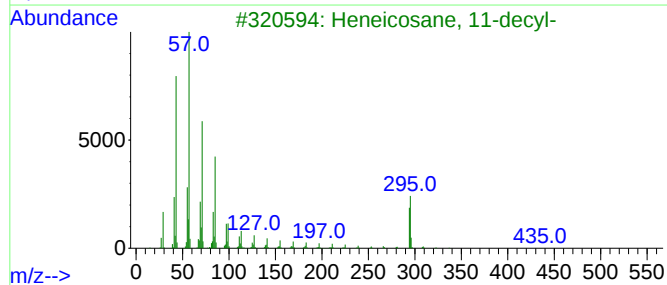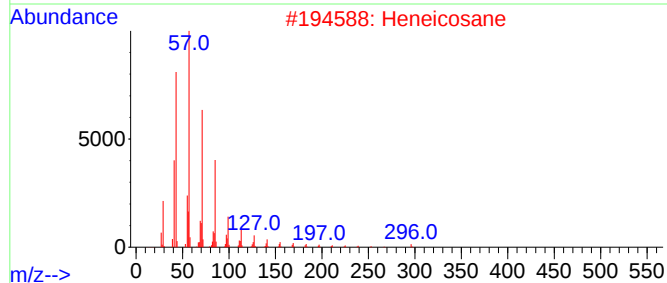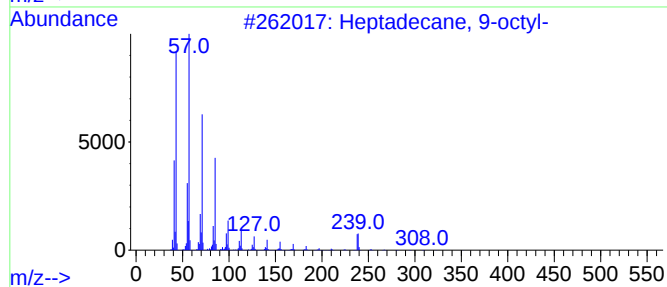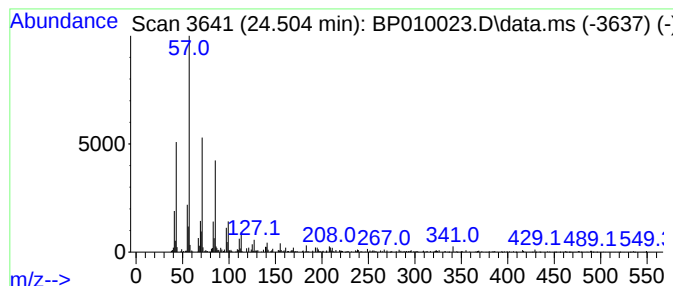

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010023.D
Acq On : 21 Apr 2022 20:07
Operator : CG/JU
Sample : N2373-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.110	6.3	ng/u1	671704	5	21.404	2127880	20.0
(DEL) Alkane: S...	24.504	2.2	ng/u1	224626	6	23.857	2009790	20.0