

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010033.D
 Acq On : 22 Apr 2022 01:44
 Operator : CG/JU
 Sample : N2473-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	53	rVB	27425	37367	0.62%	0.075%
2	3.663	96	98	106	rVB5	6309	11961	0.20%	0.024%
3	3.799	117	121	134	rBV	55490	107705	1.78%	0.216%
4	4.116	172	175	183	rVB5	10093	18257	0.30%	0.037%
5	5.052	331	334	340	rBV7	6626	9427	0.16%	0.019%
6	6.946	653	656	660	rBV5	5337	6360	0.10%	0.013%
7	7.099	675	682	692	rBV	155533	262035	4.32%	0.525%
8	7.263	704	710	722	rBV	569037	916958	15.12%	1.839%
9	7.469	737	745	755	rBV	552881	903979	14.90%	1.813%
10	7.828	801	806	812	rVB2	23997	39578	0.65%	0.079%
11	7.940	816	825	835	rBV	558038	917304	15.12%	1.839%
12	8.004	835	836	842	rVB6	6481	7701	0.13%	0.015%
13	8.293	878	885	894	rBV2	22661	40176	0.66%	0.081%
14	8.645	938	945	956	rBV	471571	797400	13.14%	1.599%
15	9.098	1011	1022	1034	rBV	766381	1304326	21.50%	2.615%
16	9.545	1093	1098	1104	rVB2	24102	41166	0.68%	0.083%
17	9.822	1135	1145	1156	rBV	606430	1039321	17.13%	2.084%
18	10.363	1228	1237	1250	rBV	864647	1465383	24.16%	2.938%
19	10.610	1272	1279	1285	rBV	100560	162866	2.68%	0.327%
20	10.745	1294	1302	1316	rVB	862492	1452146	23.94%	2.912%
21	10.875	1316	1324	1337	rBV	357434	682966	11.26%	1.369%
22	11.134	1361	1368	1376	rVB	26946	48211	0.79%	0.097%
23	12.039	1520	1522	1530	rBV8	6014	11191	0.18%	0.022%
24	12.175	1540	1545	1553	rBV9	6878	14787	0.24%	0.030%
25	12.334	1565	1572	1581	rVB3	19187	37829	0.62%	0.076%
26	12.875	1661	1664	1667	rVB5	5200	6271	0.10%	0.013%
27	12.945	1671	1676	1680	rVV8	4506	8687	0.14%	0.017%
28	12.998	1680	1685	1692	rVV10	7004	16066	0.26%	0.032%
29	13.192	1712	1718	1723	rVB10	5646	10260	0.17%	0.021%
30	13.375	1744	1749	1752	rBV2	14138	24152	0.40%	0.048%
31	13.410	1752	1755	1758	rVB3	10068	12679	0.21%	0.025%
32	13.975	1840	1851	1868	rBV	2016620	2949801	48.63%	5.915%
33	14.110	1871	1874	1879	rVB7	4995	6532	0.11%	0.013%
34	14.263	1888	1900	1913	rBV	2156397	3191735	52.61%	6.400%
35	14.569	1943	1952	1962	rBV	1461462	2173089	35.82%	4.357%
36	14.657	1965	1967	1974	rVB8	5126	8442	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010033.D
 Acq On : 22 Apr 2022 01:44
 Operator : CG/JU
 Sample : N2473-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	14.757	1978	1984	1998	rBV	164799	283824	4.68%	0.569%
38	14.892	2002	2007	2011	rVV5	11409	15594	0.26%	0.031%
39	15.051	2029	2034	2043	rBV5	4437	8286	0.14%	0.017%
40	15.210	2056	2061	2064	rBV7	3901	6413	0.11%	0.013%
41	15.380	2084	2090	2095	rBV	26825	40389	0.67%	0.081%
42	15.563	2114	2121	2134	rBV	2983716	4245202	69.98%	8.512%
43	15.675	2134	2140	2153	rVV	1071782	1540118	25.39%	3.088%
44	15.804	2157	2162	2168	rVB2	34903	56317	0.93%	0.113%
45	16.139	2215	2219	2223	rVB7	4536	6802	0.11%	0.014%
46	16.351	2248	2255	2261	rVB3	12180	21053	0.35%	0.042%
47	16.998	2361	2365	2370	rVB5	7482	10037	0.17%	0.020%
48	17.104	2377	2383	2394	rBV4	9874	24894	0.41%	0.050%
49	17.322	2413	2420	2430	rBV	1937907	2701941	44.54%	5.418%
50	17.422	2430	2437	2453	rVV	3568103	5213578	85.94%	10.454%
51	17.933	2520	2524	2528	rBV7	4254	7126	0.12%	0.014%
52	17.992	2530	2534	2540	rVB2	34864	45031	0.74%	0.090%
53	18.204	2565	2570	2577	rBV4	48166	72841	1.20%	0.146%
54	18.274	2579	2582	2587	rVB4	8392	12183	0.20%	0.024%
55	18.810	2671	2673	2677	rVB5	5653	6618	0.11%	0.013%
56	19.227	2740	2744	2750	rVB2	47294	64157	1.06%	0.129%
57	19.298	2752	2756	2762	rVB	48151	66240	1.09%	0.133%
58	19.580	2801	2804	2809	rVB5	13347	15664	0.26%	0.031%
59	19.651	2810	2816	2834	rVV	4570265	6066405	100.00%	12.164%
60	20.145	2897	2900	2903	rVB4	15092	17982	0.30%	0.036%
61	21.104	3059	3063	3070	rBV	486319	622868	10.27%	1.249%
62	21.404	3108	3114	3127	rBV	1897103	2687611	44.30%	5.389%
63	23.104	3400	3403	3409	rVB	76684	108334	1.79%	0.217%
64	23.698	3496	3504	3511	rBV2	2356312	4763228	78.52%	9.551%
65	23.856	3523	3531	3542	rVB2	1120421	2396963	39.51%	4.806%




Sum of corrected areas: 49871813

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010033.D
Acq On : 22 Apr 2022 01:44
Operator : CG/JU
Sample : N2473-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J41

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

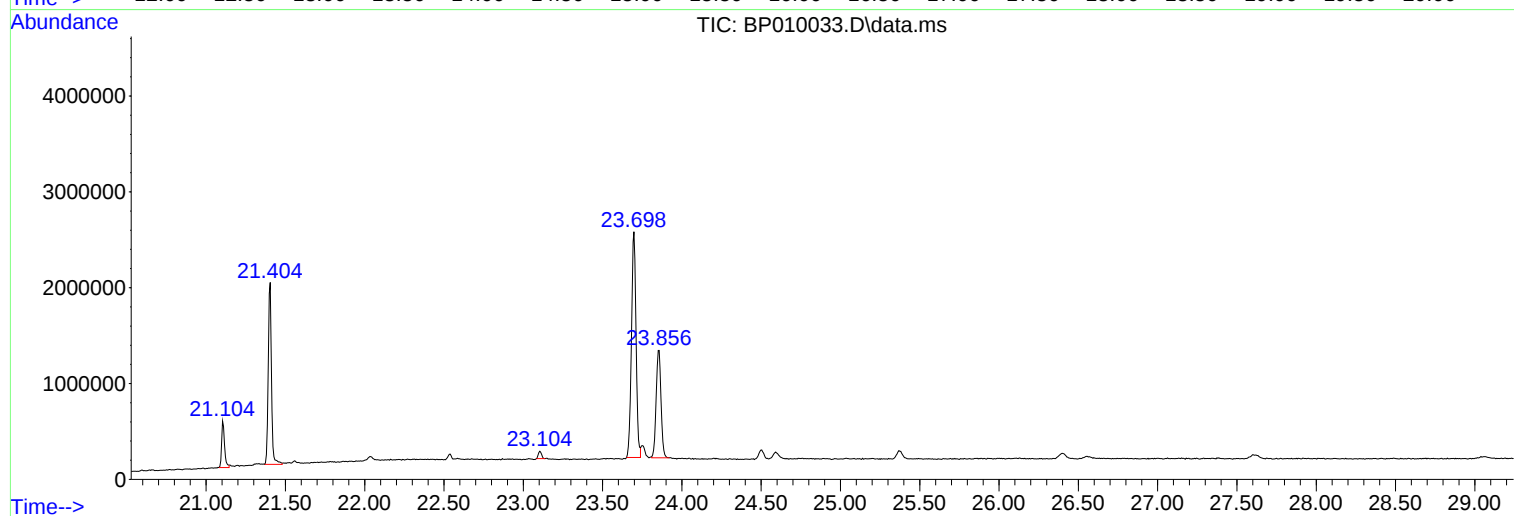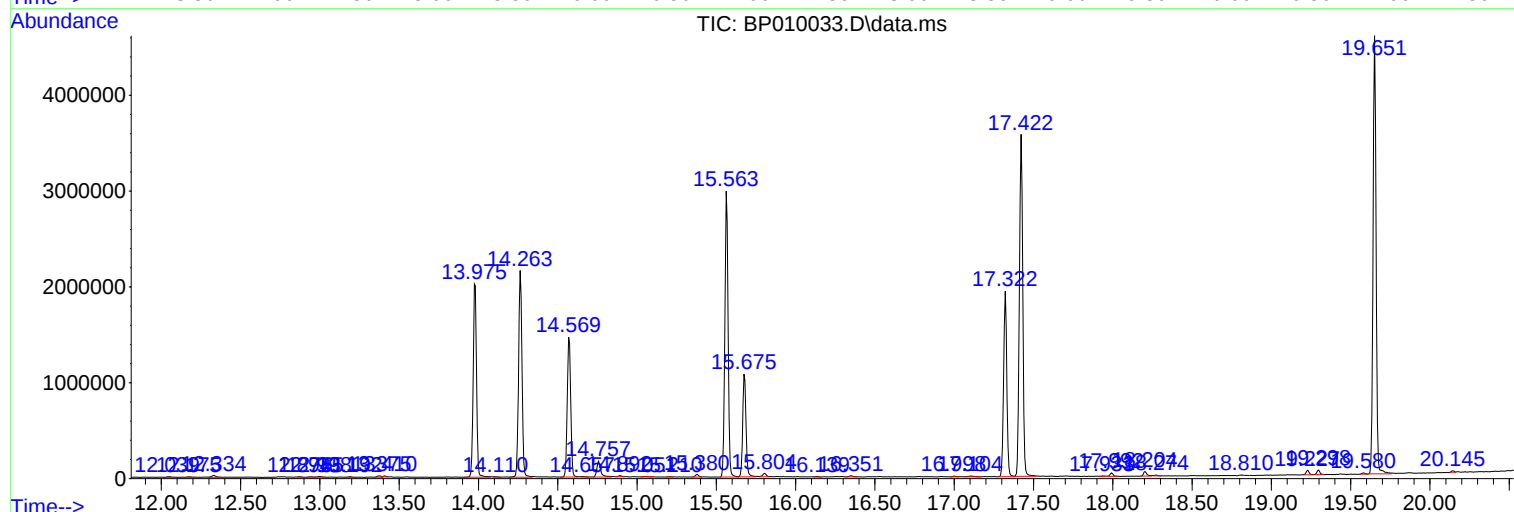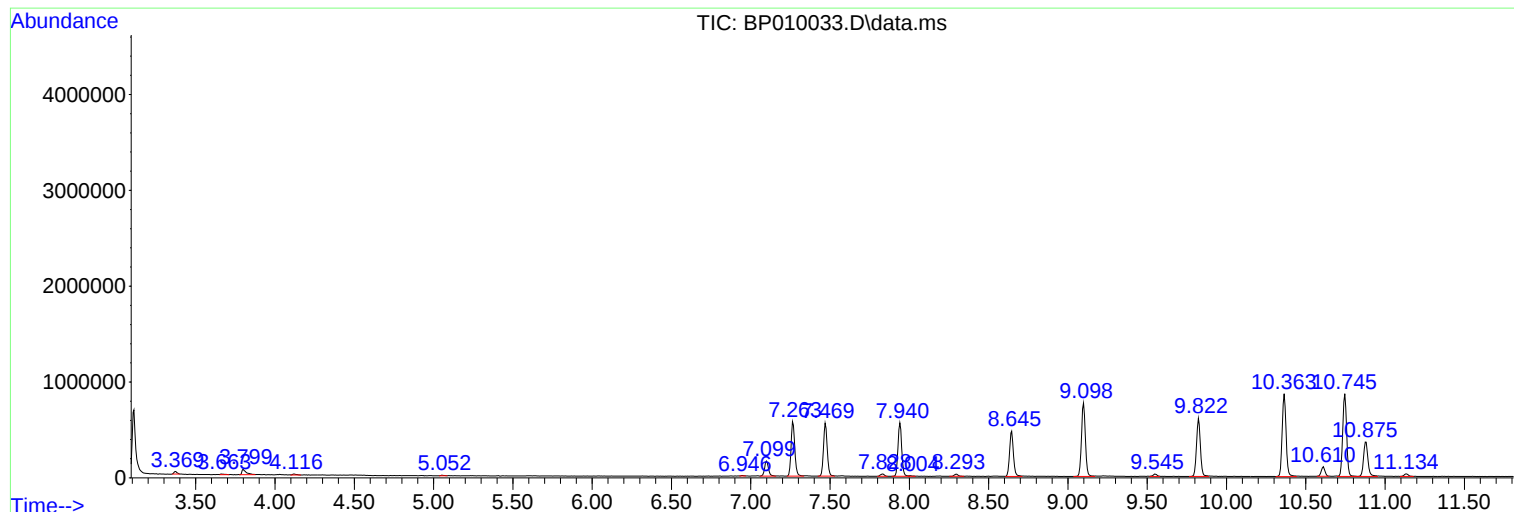

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010033.D
Acq On : 22 Apr 2022 01:44
Operator : CG/JU
Sample : N2473-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J41










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,3,5-trichloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.610	2.24 ng/ul	162866	Naphthalene-d8	10.745

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
2			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
3			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
4			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	97
5			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	97

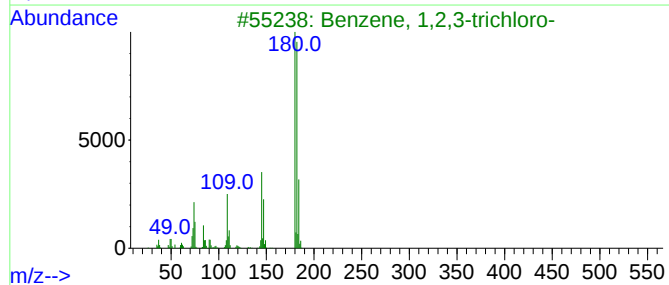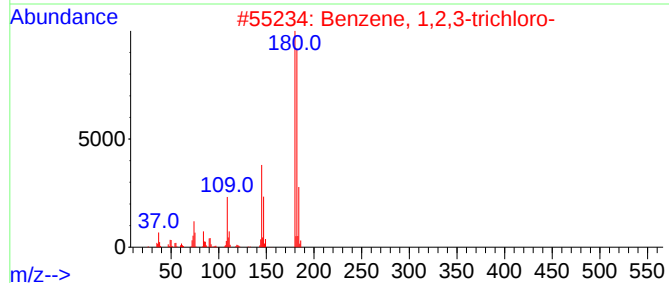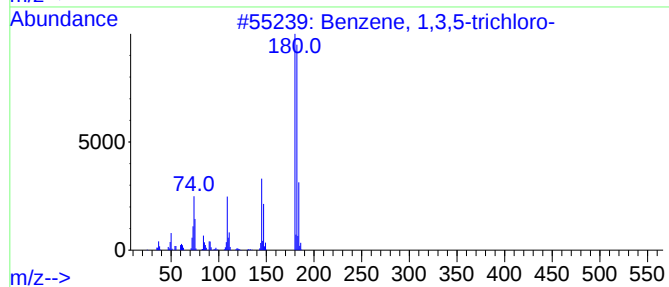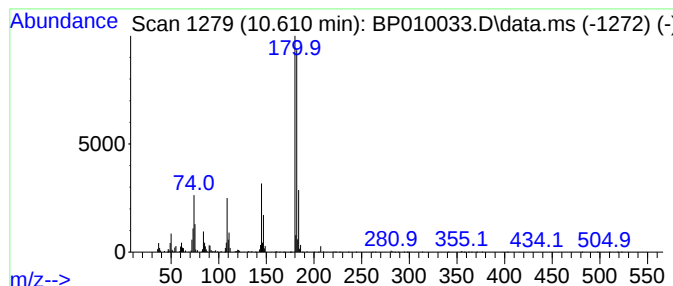

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010033.D
Acq On : 22 Apr 2022 01:44
Operator : CG/JU
Sample : N2473-06
Misc :
ALS Vial : 28 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
C0J41

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.104	4.64 ng/ul	622868	Chrysene-d12		21.404	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Tetracosene		336	C24H48	010192-32-2	94
2	1-Heneicosanol		312	C21H44O	015594-90-8	94
3	Pentacos-1-ene		350	C25H50	016980-85-1	94
4	Trifluoroacetoxy hexadecane		338	C18H33F3O2	006222-03-3	93
5	1-Hexacosene		364	C26H52	018835-33-1	93

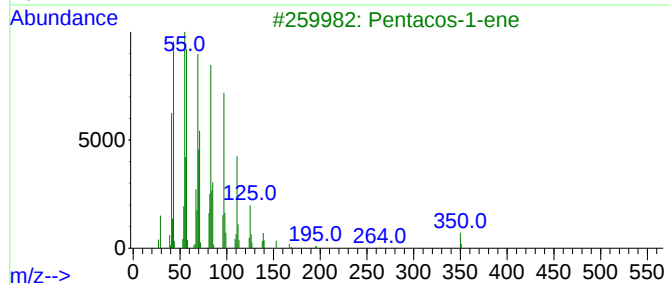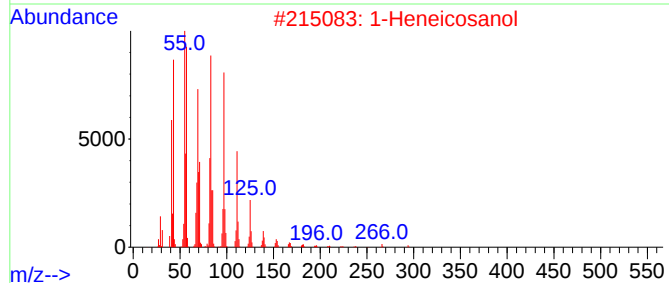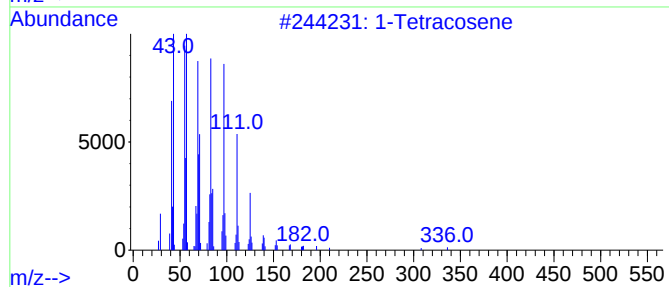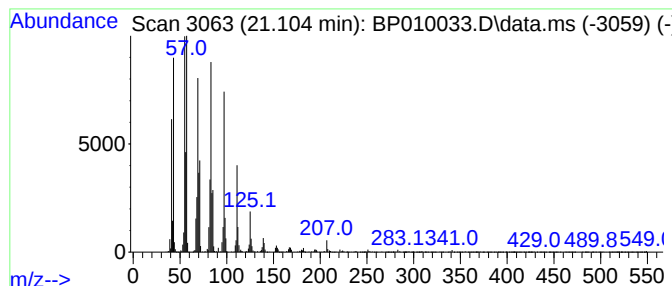

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010033.D
Acq On : 22 Apr 2022 01:44
Operator : CG/JU
Sample : N2473-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J41

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,3,5-...	10.610	2.2	ng/u1	162866	2	10.745	1452150	20.0
(DEL) Alkane: S...	21.104	4.6	ng/u1	622868	5	21.404	2687610	20.0