

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010037.D
 Acq On : 22 Apr 2022 04:32
 Operator : CG/JU
 Sample : PB144266BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	45	48	59	rVB	40711	62743	1.27%	0.131%
2	3.787	115	119	131	rBV	457361	825597	16.66%	1.725%
3	4.122	173	176	182	rVB4	9455	14134	0.29%	0.030%
4	7.099	675	682	693	rBV	648123	1069149	21.57%	2.233%
5	7.264	704	710	722	rVB	524444	864571	17.45%	1.806%
6	7.469	738	745	759	rBV	687512	1101596	22.23%	2.301%
7	7.940	818	825	842	rVB	583978	952817	19.23%	1.990%
8	8.646	937	945	958	rBV	870459	1451049	29.28%	3.031%
9	9.099	1014	1022	1034	rBV	708099	1187030	23.95%	2.480%
10	9.822	1138	1145	1155	rBV	593952	997177	20.12%	2.083%
11	10.363	1229	1237	1254	rBV	855086	1492051	30.11%	3.117%
12	10.746	1293	1302	1315	rBV	863026	1484037	29.95%	3.100%
13	10.875	1317	1324	1339	rBV	874446	1571632	31.71%	3.283%
14	12.328	1566	1571	1579	rBV4	16718	31706	0.64%	0.066%
15	13.546	1772	1778	1781	rBV8	3095	5197	0.10%	0.011%
16	13.851	1825	1830	1835	rBV8	3922	5905	0.12%	0.012%
17	13.975	1844	1851	1862	rBV	1867047	2607270	52.61%	5.446%
18	14.263	1891	1900	1917	rBV	1933649	2885415	58.22%	6.027%
19	14.569	1945	1952	1964	rBV	1534619	2253976	45.48%	4.708%
20	14.651	1964	1966	1975	rVB10	4042	7789	0.16%	0.016%
21	14.757	1975	1984	1999	rBV	758521	1224509	24.71%	2.558%
22	14.922	2010	2012	2016	rVB5	3531	5317	0.11%	0.011%
23	15.563	2114	2121	2133	rBV	2548857	3722394	75.11%	7.776%
24	15.675	2133	2140	2153	rVV	838793	1149972	23.20%	2.402%
25	15.804	2156	2162	2171	rVB2	31552	55276	1.12%	0.115%
26	16.351	2248	2255	2260	rBV6	10914	19634	0.40%	0.041%
27	17.004	2360	2366	2372	rBV9	5608	12000	0.24%	0.025%
28	17.104	2381	2383	2387	rVB3	6748	8825	0.18%	0.018%
29	17.322	2413	2420	2430	rBV	1938380	2778155	56.06%	5.803%
30	17.422	2430	2437	2451	rVV2	2856450	4201744	84.78%	8.777%
31	17.763	2491	2495	2500	rVB7	3606	5576	0.11%	0.012%
32	19.228	2740	2744	2749	rBV3	35296	51079	1.03%	0.107%
33	19.298	2751	2756	2760	rBV2	37947	51747	1.04%	0.108%
34	19.580	2802	2804	2807	rBV3	9969	9570	0.19%	0.020%
35	19.651	2810	2816	2830	rBV	3734084	4955835	100.00%	10.352%
36	21.404	3108	3114	3126	rBV	2013317	2735457	55.20%	5.714%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010037.D
Acq On : 22 Apr 2022 04:32
Operator : CG/JU
Sample : PB144266BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK266

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

37	23.692	3496	3503	3511	rBV2	1779187	3689927	74.46%	7.708%
38	23.851	3523	3530	3540	rVB2	1139804	2325302	46.92%	4.857%




Sum of corrected areas: 47873160

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010037.D
Acq On : 22 Apr 2022 04:32
Operator : CG/JU
Sample : PB144266BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK266

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

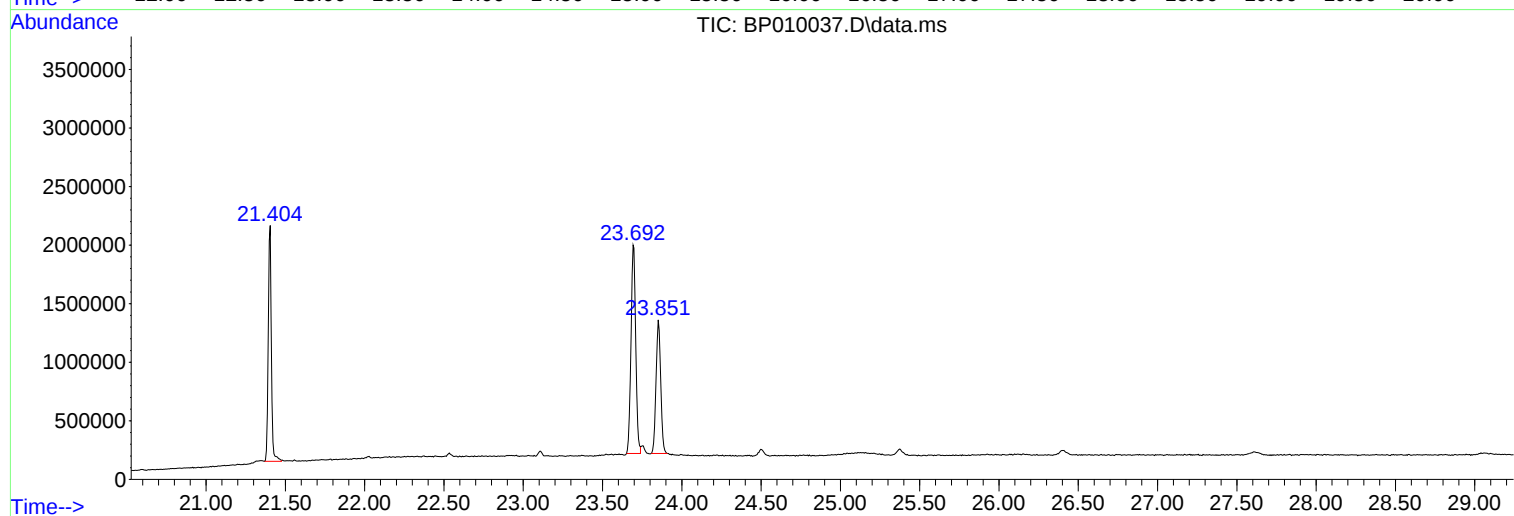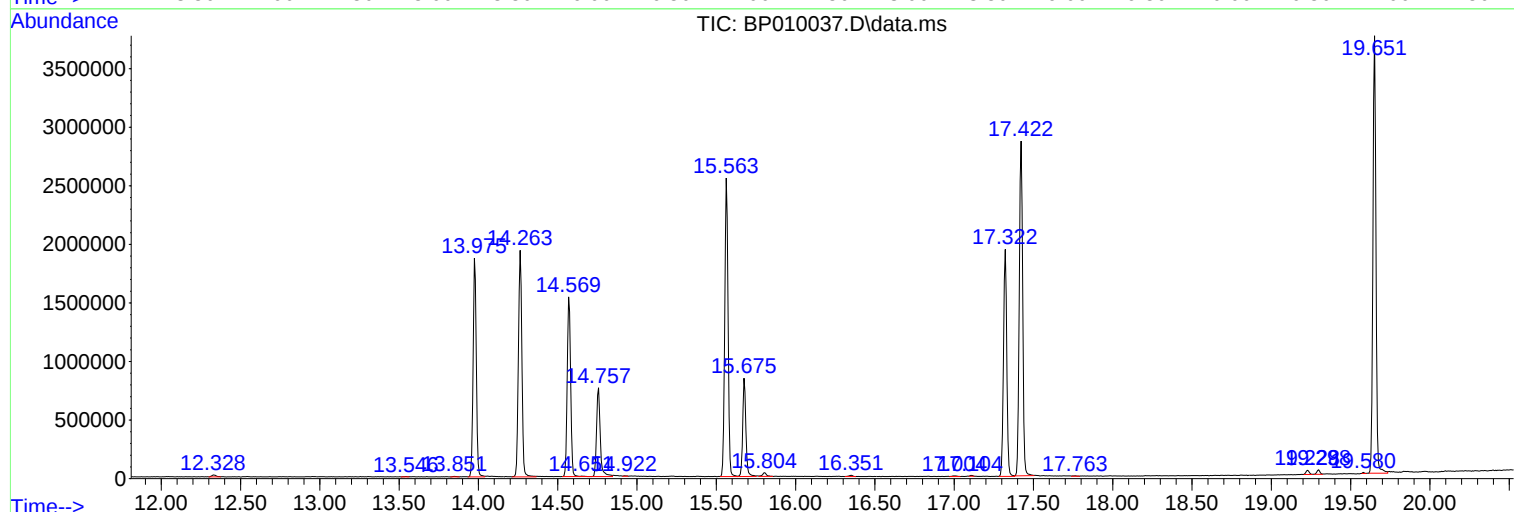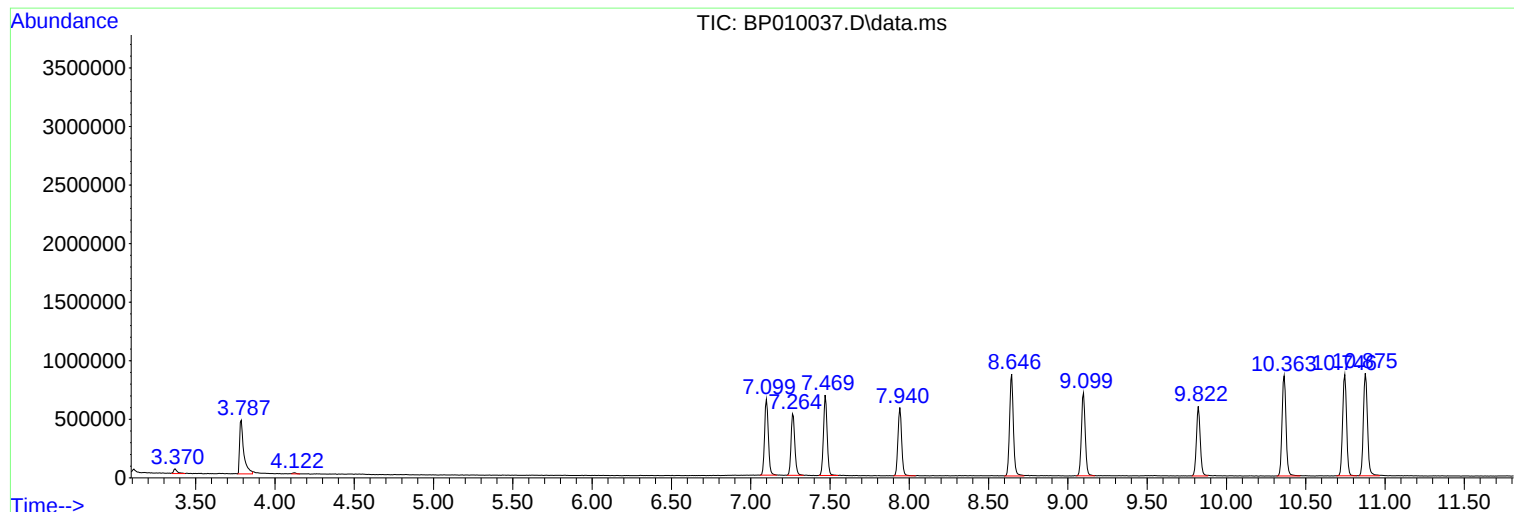

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010037.D
Acq On : 22 Apr 2022 04:32
Operator : CG/JU
Sample : PB144266BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK266

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010037.D
Acq On : 22 Apr 2022 04:32
Operator : CG/JU
Sample : PB144266BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK266

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------