

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010046.D
 Acq On : 22 Apr 2022 09:35
 Operator : CG/JU
 Sample : PB144261BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK261

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	54	rBV	29750	39746	0.96%	0.099%
2	3.787	115	119	141	rBV	372897	713330	17.26%	1.769%
3	4.117	173	175	182	rVB4	8543	11840	0.29%	0.029%
4	7.099	676	682	694	rBV	519792	837518	20.27%	2.077%
5	7.263	704	710	725	rVB	416520	681157	16.48%	1.690%
6	7.469	738	745	755	rBV	530414	876184	21.20%	2.173%
7	7.940	818	825	835	rBV	485823	796892	19.28%	1.977%
8	8.646	937	945	959	rBV	681857	1152298	27.88%	2.858%
9	9.099	1014	1022	1032	rBV	537223	938882	22.72%	2.329%
10	9.822	1136	1145	1155	rBV	455895	787779	19.06%	1.954%
11	10.363	1228	1237	1253	rBV	686112	1182345	28.61%	2.933%
12	10.746	1292	1302	1315	rBV	737863	1275743	30.87%	3.164%
13	10.875	1316	1324	1338	rBV	698365	1263996	30.59%	3.135%
14	11.369	1403	1408	1418	rBV	2516	6186	0.15%	0.015%
15	12.328	1566	1571	1582	rBV2	13209	26622	0.64%	0.066%
16	12.963	1671	1679	1684	rVB2	2676	6344	0.15%	0.016%
17	13.857	1825	1831	1835	rBV8	3375	6627	0.16%	0.016%
18	13.975	1844	1851	1862	rBV	1490453	2077205	50.26%	5.152%
19	14.263	1893	1900	1914	rBV	1567307	2307135	55.83%	5.723%
20	14.569	1945	1952	1965	rBV	1300766	1931012	46.73%	4.790%
21	14.757	1977	1984	1998	rBV	555147	952289	23.04%	2.362%
22	15.563	2113	2121	2134	rBV	2089453	3033517	73.41%	7.524%
23	15.675	2134	2140	2153	rVV	639562	881726	21.34%	2.187%
24	15.804	2157	2162	2167	rVB3	22883	37280	0.90%	0.092%
25	16.345	2250	2254	2259	rVB7	8494	12222	0.30%	0.030%
26	16.828	2332	2336	2340	rVB7	2623	4359	0.11%	0.011%
27	16.998	2360	2365	2369	rVB8	4623	7224	0.17%	0.018%
28	17.110	2378	2384	2389	rVB3	8188	14709	0.36%	0.036%
29	17.322	2413	2420	2430	rBV	1698210	2462661	59.59%	6.108%
30	17.422	2430	2437	2450	rVV	2262209	3409929	82.51%	8.458%
31	18.804	2670	2672	2677	rVV6	4961	6404	0.15%	0.016%
32	19.227	2739	2744	2750	rBV3	29443	48587	1.18%	0.121%
33	19.298	2752	2756	2761	rVV	27693	39971	0.97%	0.099%
34	19.580	2801	2804	2808	rVV6	8133	10985	0.27%	0.027%
35	19.651	2810	2816	2830	rBV	3093646	4132545	100.00%	10.251%
36	21.404	3108	3114	3133	rVB	1827317	2584209	62.53%	6.410%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010046.D
Acq On : 22 Apr 2022 09:35
Operator : CG/JU
Sample : PB144261BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

37	23.104	3400	3403	3408	rVB	60082	82191	1.99%	0.204%
38	23.692	3496	3503	3510	rBV2	1613552	3244870	78.52%	8.049%
39	23.857	3523	3531	3542	rVB2	1058903	2288243	55.37%	5.676%
40	24.504	3637	3641	3647	rVB3	74224	142609	3.45%	0.354%




Sum of corrected areas: 40315371

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010046.D
Acq On : 22 Apr 2022 09:35
Operator : CG/JU
Sample : PB144261BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

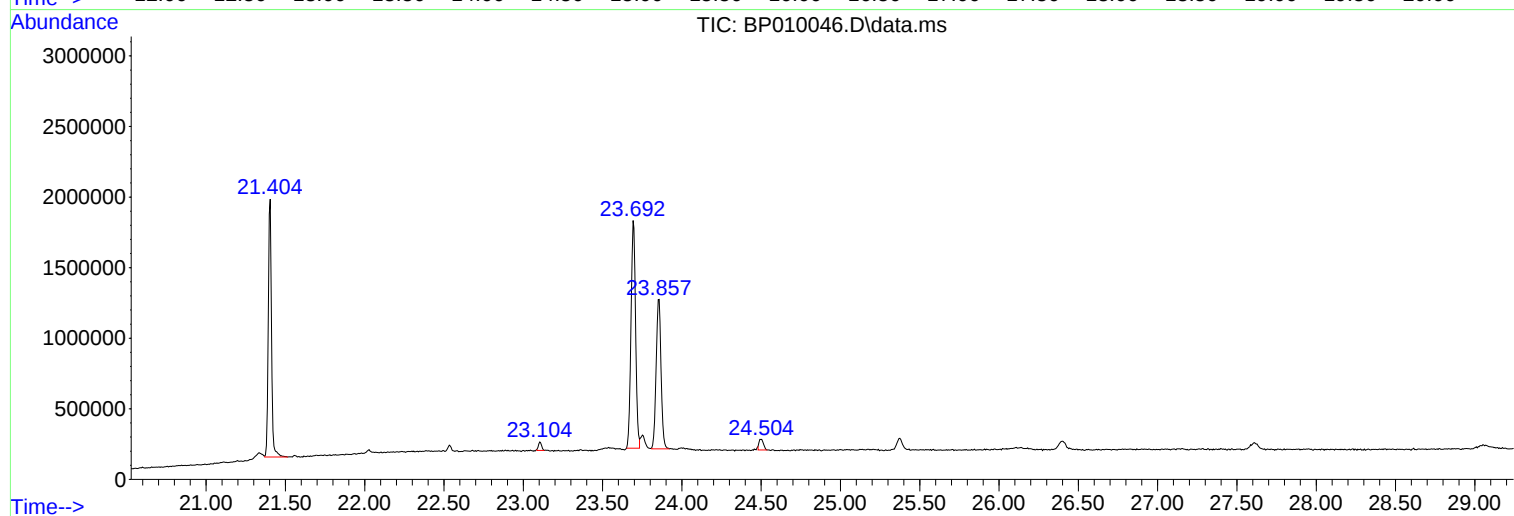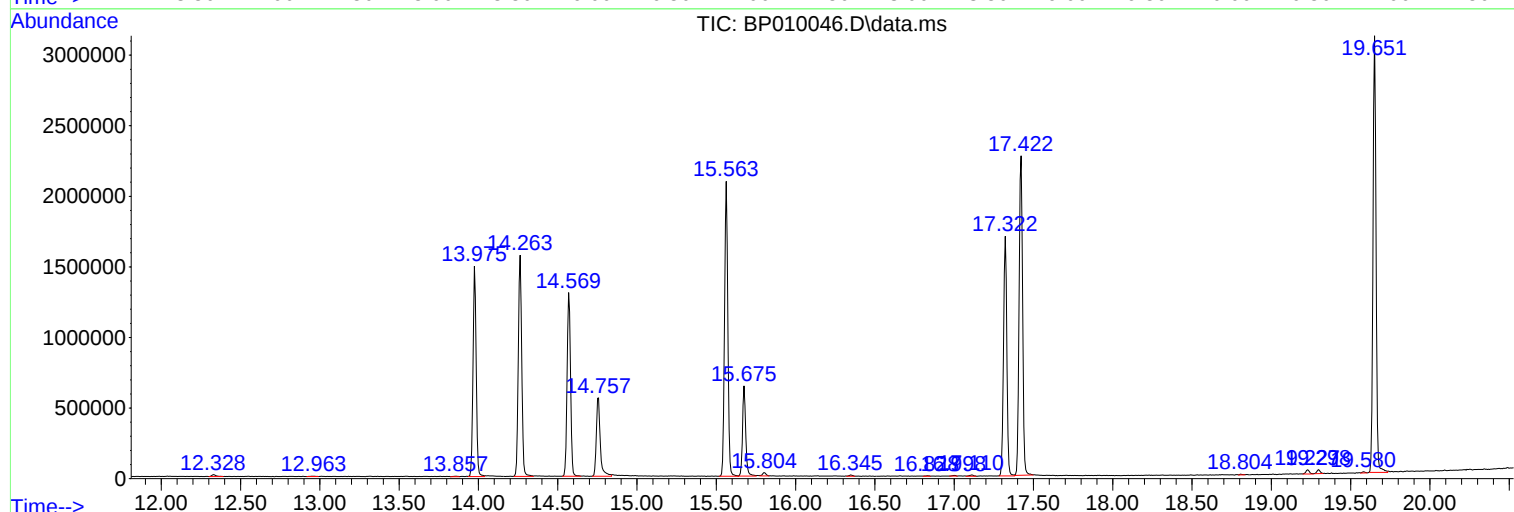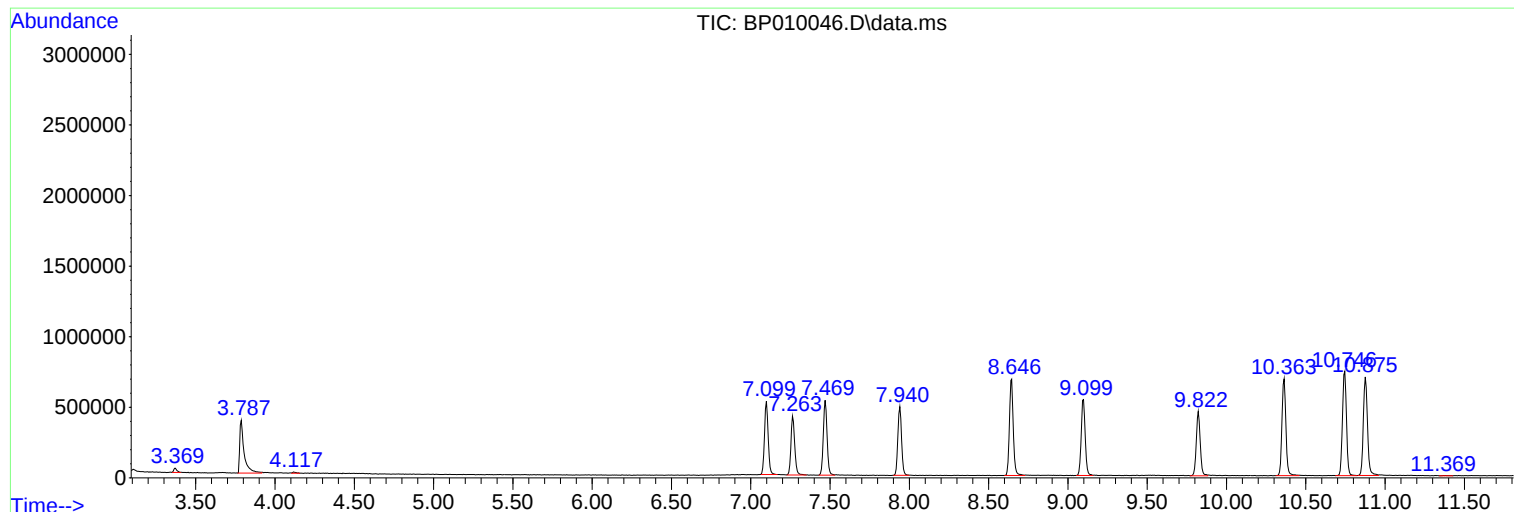

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010046.D
Acq On : 22 Apr 2022 09:35
Operator : CG/JU
Sample : PB144261BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010046.D
Acq On : 22 Apr 2022 09:35
Operator : CG/JU
Sample : PB144261BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc