

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010052.D
 Acq On : 22 Apr 2022 12:56
 Operator : CG/JU
 Sample : N2473-07DL 5X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J50DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010052.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.264	360	370	399	rBV	31589689	57802384	50.54%	14.643%
2	6.622	595	601	609	rVB	89218	146983	0.13%	0.037%
3	7.269	704	711	719	rBV	169615	278398	0.24%	0.071%
4	7.475	736	746	756	rBV	168073	282621	0.25%	0.072%
5	7.846	798	809	820	rBV	14555411	27049012	23.65%	6.852%
6	8.016	820	838	842	rBV2	38179144	99068320	86.62%	25.097%
7	8.346	878	894	899	rBV2	38704233	114373755	100.00%	28.974%
8	8.646	939	945	956	rVB	136482	229914	0.20%	0.058%
9	9.099	1014	1022	1024	rBV	207578	332507	0.29%	0.084%
10	9.146	1024	1030	1041	rVB	1916496	3242904	2.84%	0.822%
11	9.440	1073	1080	1089	rBV	227322	372362	0.33%	0.094%
12	9.757	1129	1134	1140	rVB	150076	262304	0.23%	0.066%
13	9.822	1140	1145	1155	rBV2	156756	311375	0.27%	0.079%
14	10.369	1230	1238	1251	rBV	242485	425694	0.37%	0.108%
15	10.628	1270	1282	1296	rBV	22522582	43224779	37.79%	10.950%
16	10.752	1296	1303	1315	rVV	1272398	2085615	1.82%	0.528%
17	10.881	1318	1325	1333	rVB	148396	271506	0.24%	0.069%
18	11.140	1359	1369	1385	rBV	9363479	16873106	14.75%	4.274%
19	11.346	1394	1404	1421	rVB	2207705	3770752	3.30%	0.955%
20	11.557	1432	1440	1453	rBV	555130	964854	0.84%	0.244%
21	12.034	1511	1521	1537	rVB2	66731	142616	0.12%	0.036%
22	12.769	1642	1646	1654	rVB	469353	752641	0.66%	0.191%
23	13.151	1704	1711	1725	rBV	128284	209453	0.18%	0.053%
24	13.375	1742	1749	1761	rBV	1468110	2297167	2.01%	0.582%
25	13.975	1843	1851	1857	rBV	557248	877730	0.77%	0.222%
26	14.263	1889	1900	1911	rBV	587308	875878	0.77%	0.222%
27	14.575	1946	1953	1970	rBV	1992468	3059060	2.67%	0.775%
28	15.563	2114	2121	2134	rBV	761264	1166875	1.02%	0.296%
29	15.681	2135	2141	2152	rVB	189217	291958	0.26%	0.074%
30	17.322	2414	2420	2430	rBV	2564940	3709044	3.24%	0.940%
31	17.422	2430	2437	2447	rVB	845925	1228909	1.07%	0.311%
32	19.651	2811	2816	2821	rBV	1112749	1417760	1.24%	0.359%
33	21.404	3109	3114	3121	rBV	2503084	3384400	2.96%	0.857%
34	23.110	3401	3404	3410	rVB2	93772	139544	0.12%	0.035%
35	23.698	3498	3504	3510	rBV2	424477	855549	0.75%	0.217%
36	23.857	3524	3531	3545	rVB2	1425501	2968523	2.60%	0.752%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION




Sum of corrected areas: 394746252

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

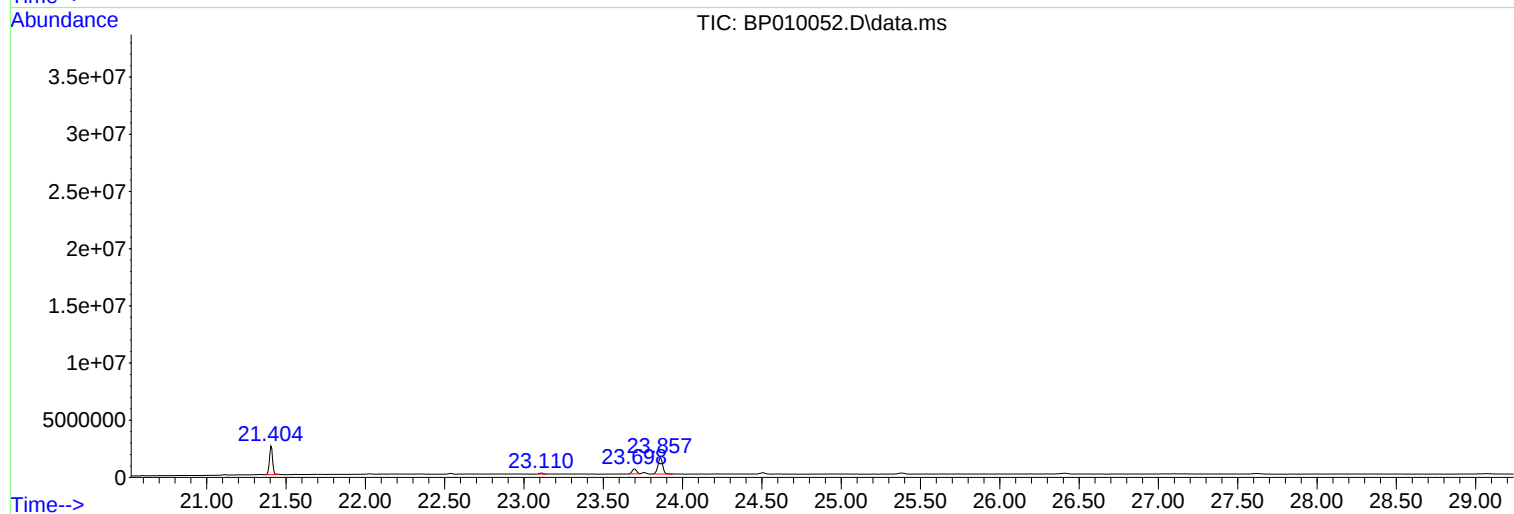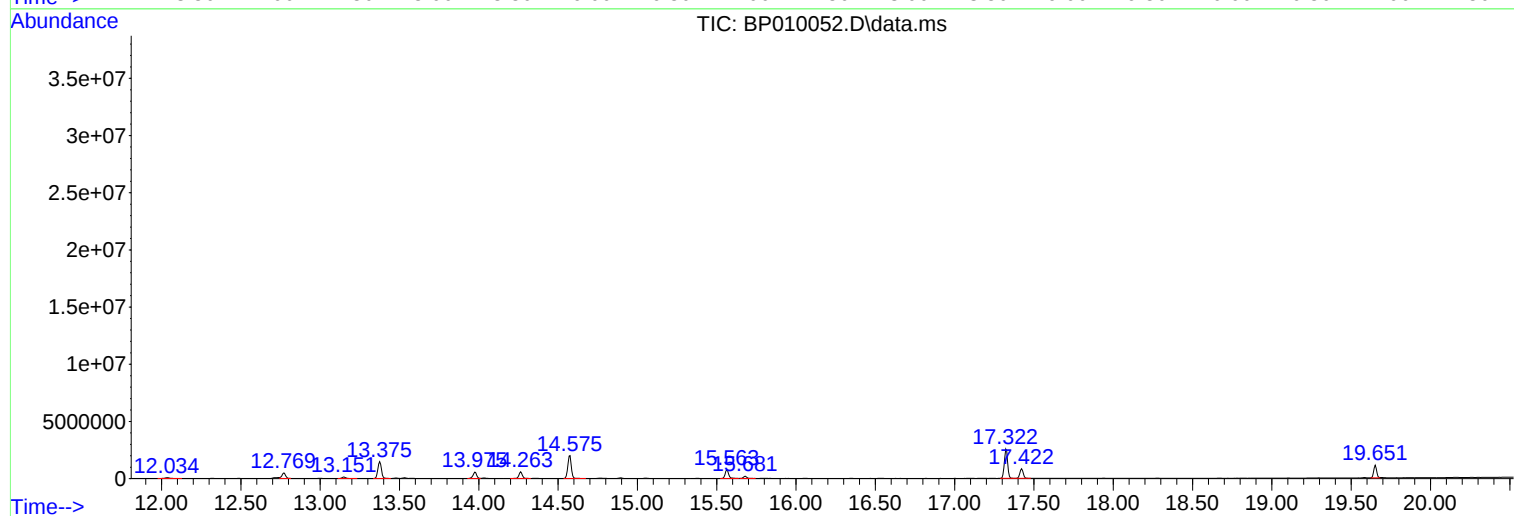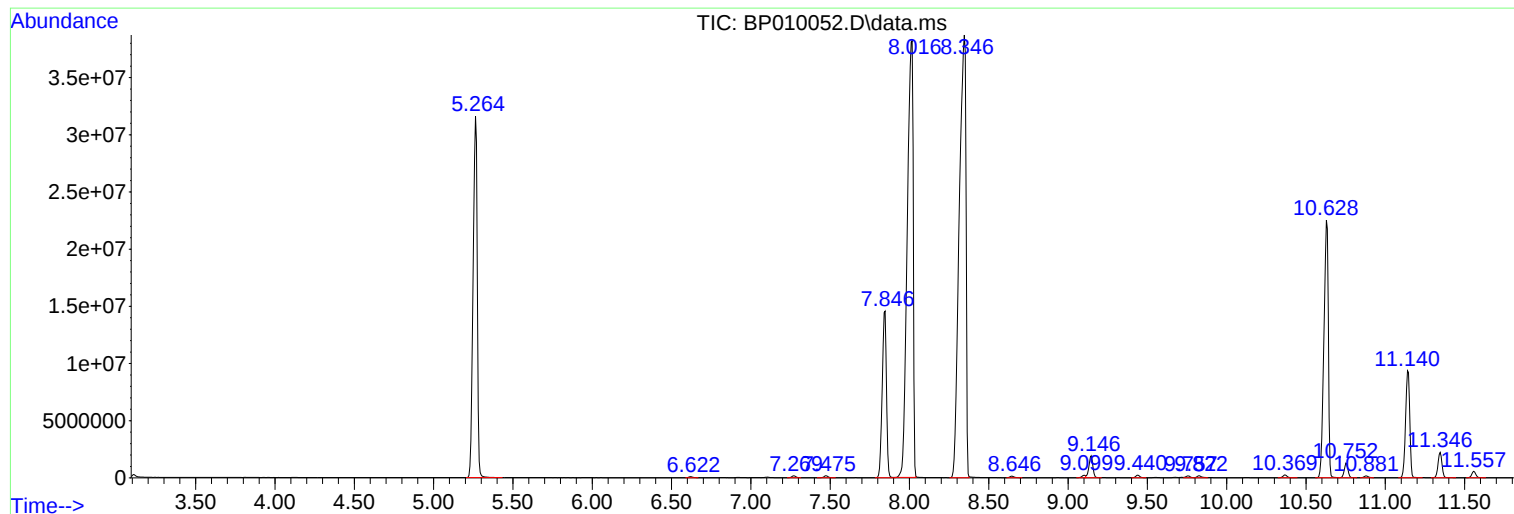

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, chloro- Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.264	11.67 ng/ul	57802400	1,4-Dichlorobenzene-d4	7.958

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, chloro-	112	C6H5Cl	000108-90-7	97
2			Benzene, chloro-	112	C6H5Cl	000108-90-7	96
3			Benzene, chloro-	112	C6H5Cl	000108-90-7	95
4			Benzene, chloro-	112	C6H5Cl	000108-90-7	94
5			Benzene, chloro-	112	C6H5Cl	000108-90-7	94

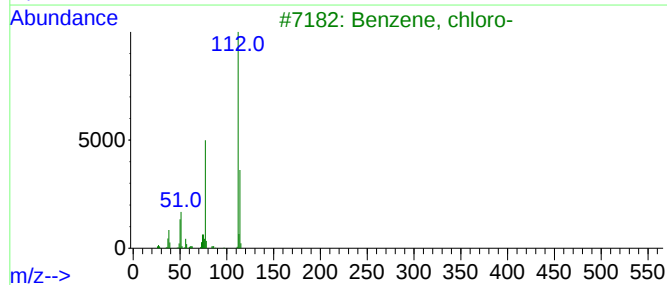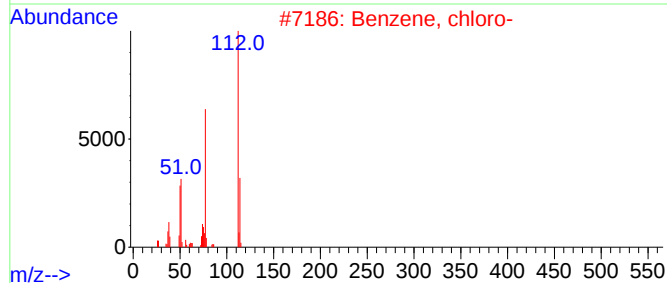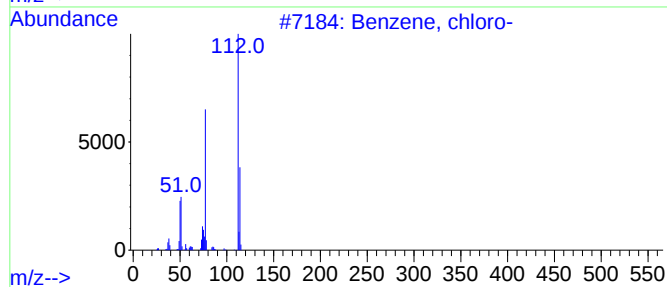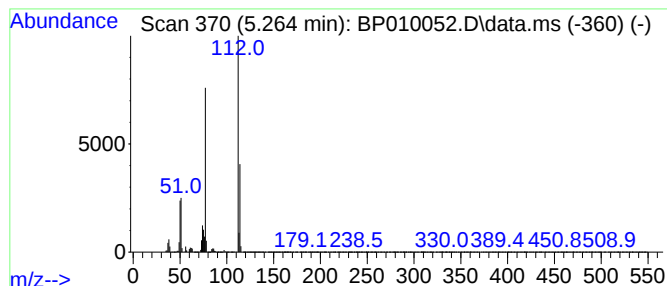

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, 1,4-dichloro- Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.846	5.46 ng/ul	27049000	1,4-Dichlorobenzene-d4	7.958

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	98
2			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	98
3			Benzene, 1,2-dichloro-	146	C6H4Cl2	000095-50-1	98
4			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	96
5			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	96

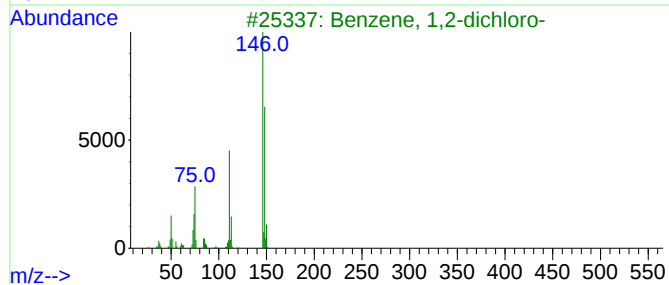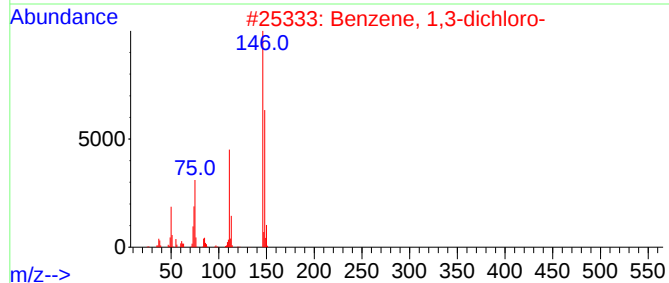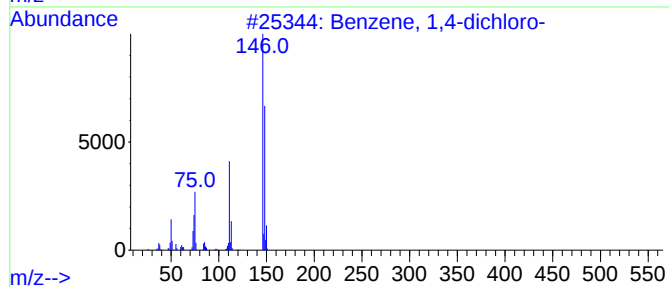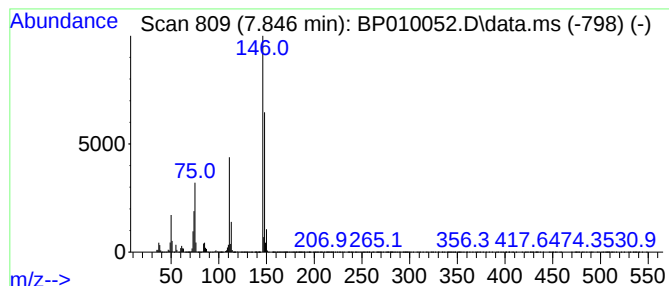

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Benzene, 1,2-dichloro- Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.016	20.00 ng/ul	99068300	1,4-Dichlorobenzene-d4	7.958

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	98
2			Benzene, 1,2-dichloro-	146	C6H4Cl2	000095-50-1	98
3			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	98
4			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	97
5			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	97

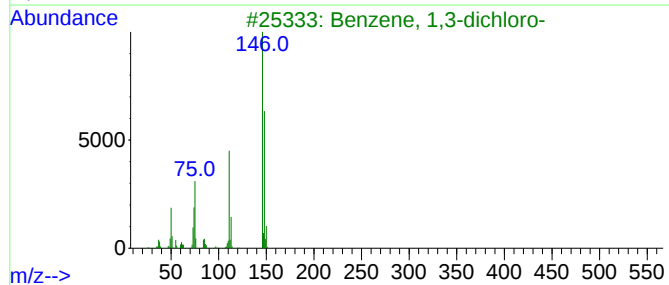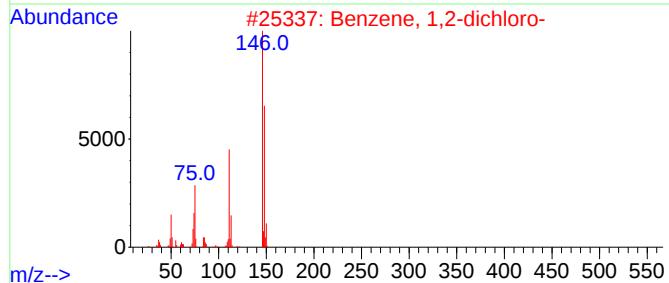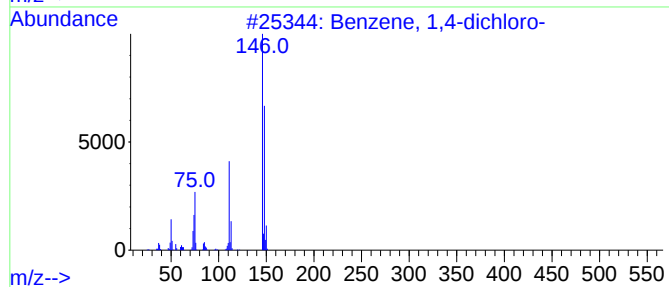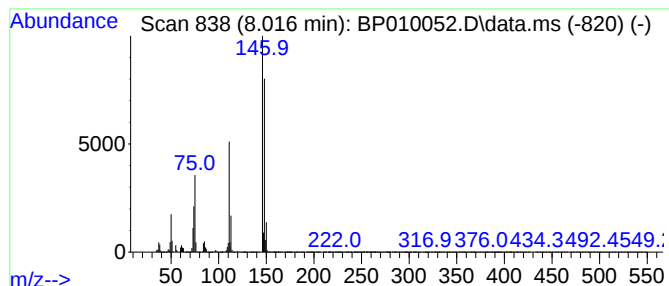

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Benzene, 1,3-dichloro- Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.346	23.09 ng/ul	114374000	1,4-Dichlorobenzene-d4	7.958

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	98
2			Benzene, 1,2-dichloro-	146	C6H4Cl2	000095-50-1	98
3			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	98
4			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	96
5			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	96

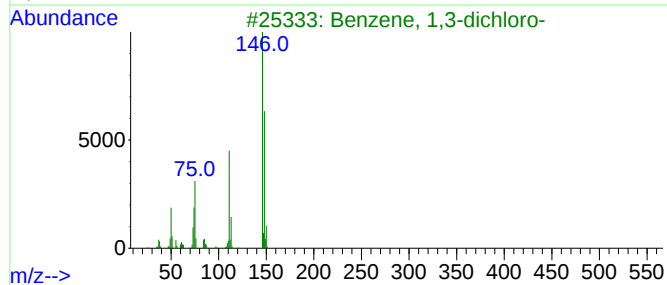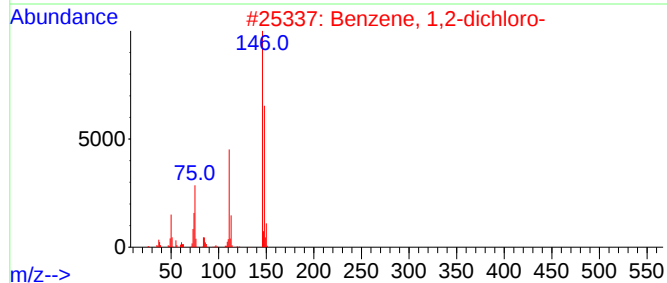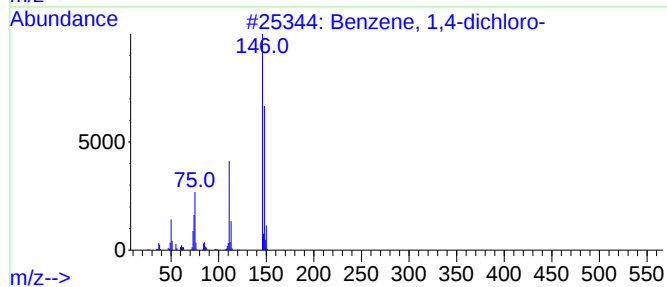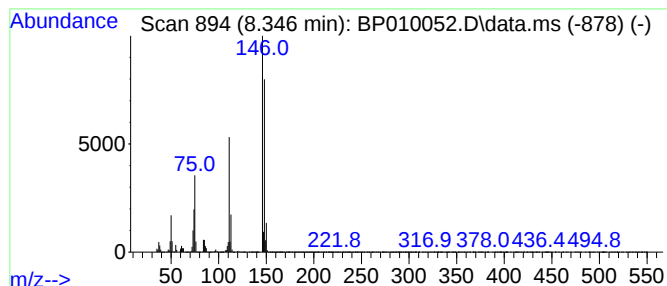

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 Benzene, 1-bromo-4-chloro- Concentration Rank 9

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.440	3.57 ng/ul	372362	Naphthalene-d8	10.752

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1-bromo-4-chloro-	190	C6H4BrCl	000106-39-8	98
2			Benzene, 1-bromo-2-chloro-	190	C6H4BrCl	000694-80-4	97
3			Benzene, 1-bromo-3-chloro-	190	C6H4BrCl	000108-37-2	95
4			Benzene, 1-bromo-4-chloro-	190	C6H4BrCl	000106-39-8	95
5			Benzene, 1-bromo-2-chloro-	190	C6H4BrCl	000694-80-4	95

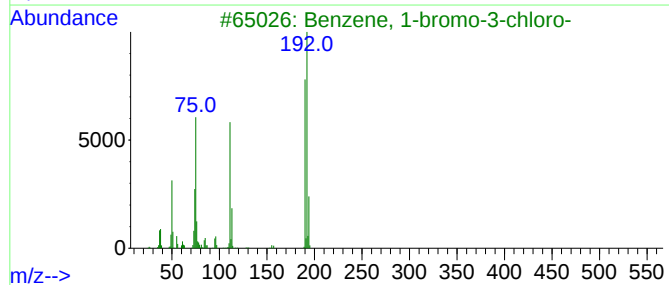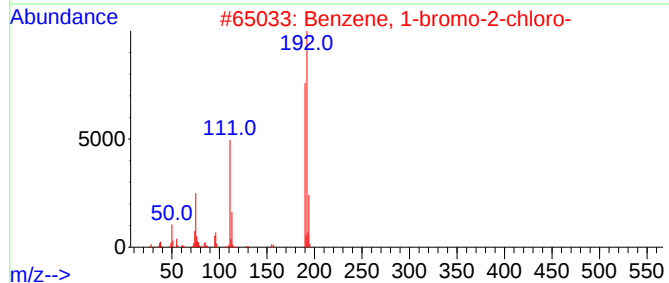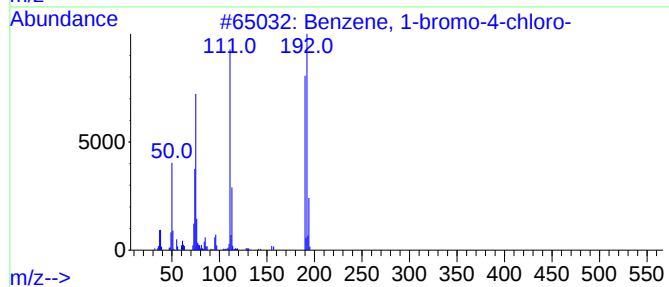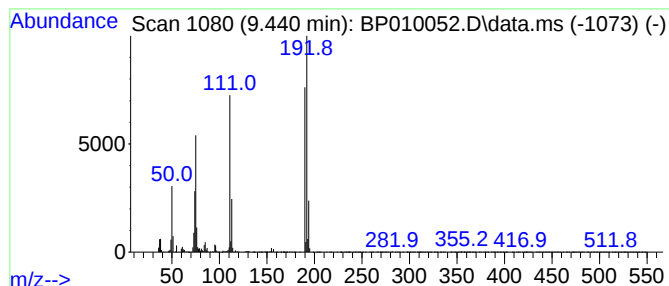

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 Benzene, 1-bromo-2-chloro- Concentration Rank 10

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.757	2.52 ng/ul	262304	Naphthalene-d8	10.752

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1-bromo-4-chloro-	190	C6H4BrCl	000106-39-8	97
2			Benzene, 1-bromo-2-chloro-	190	C6H4BrCl	000694-80-4	95
3			Benzene, 1-bromo-4-chloro-	190	C6H4BrCl	000106-39-8	95
4			Benzene, 1-bromo-3-chloro-	190	C6H4BrCl	000108-37-2	94
5			Benzene, 1-bromo-2-chloro-	190	C6H4BrCl	000694-80-4	94

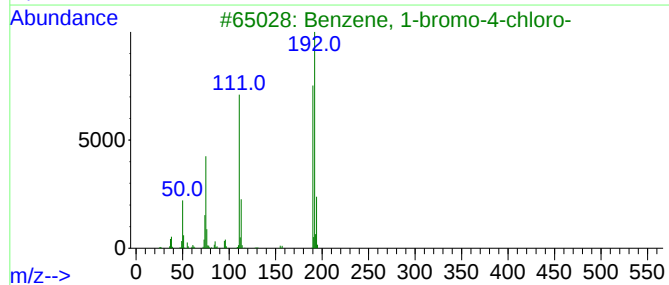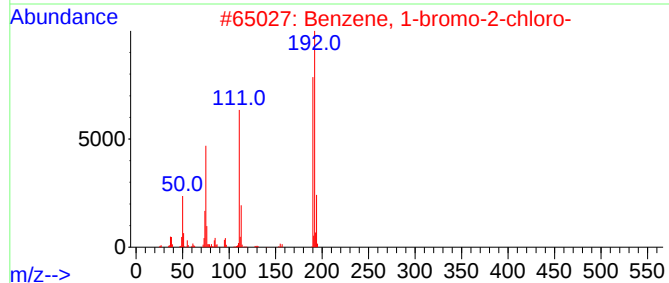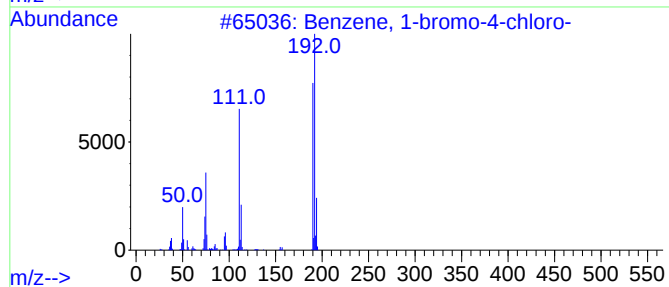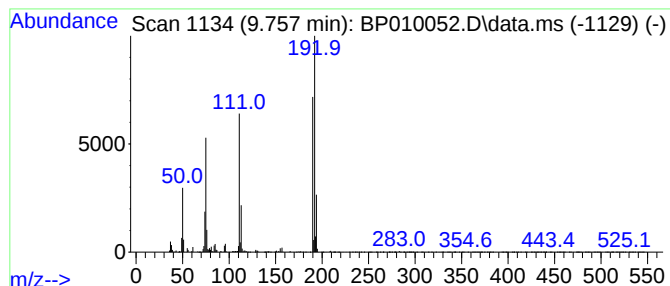

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 Benzene, 1,2,3-trichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.628	414.50 ng/ul	43224800	Naphthalene-d8	10.752

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	99
2			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
3			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
4			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	97
5			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	97

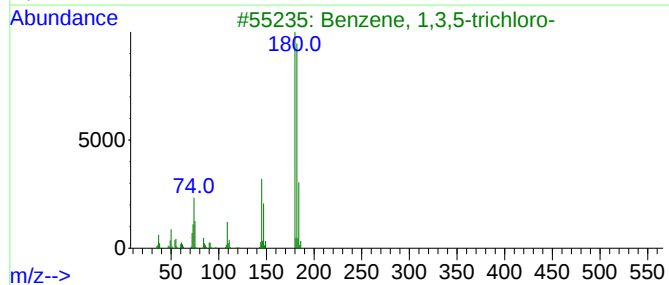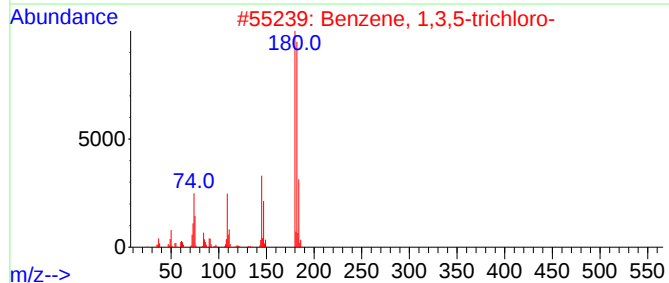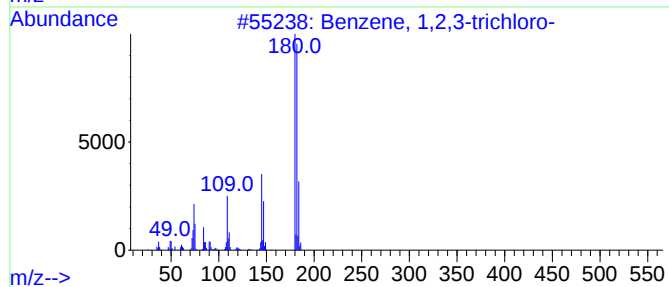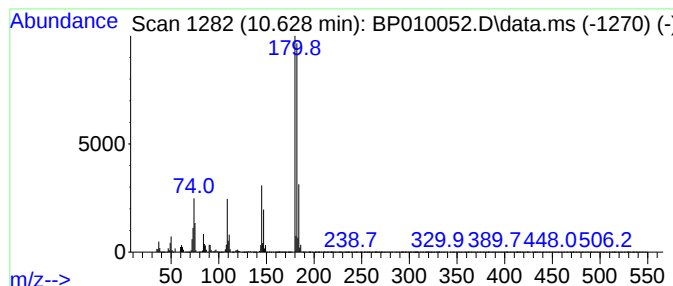

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 8 Benzene, 1,2,4-trichloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.140	161.81 ng/ul	16873100	Naphthalene-d8	10.752

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	98
2			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
3			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
4			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
5			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	97

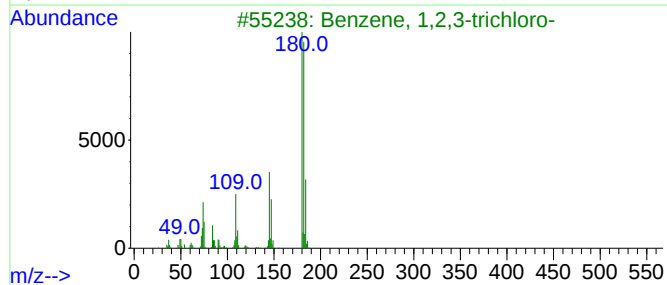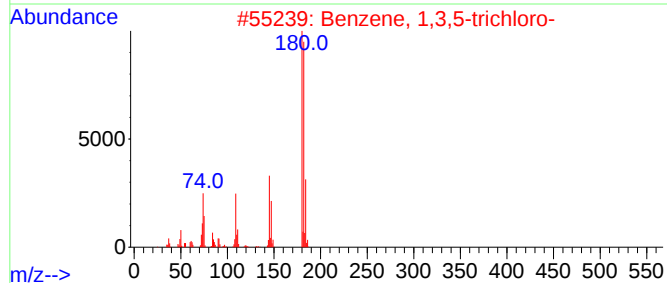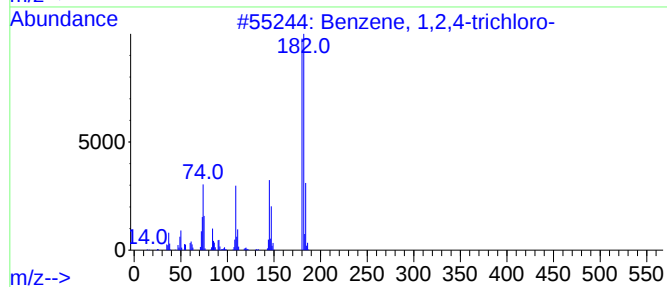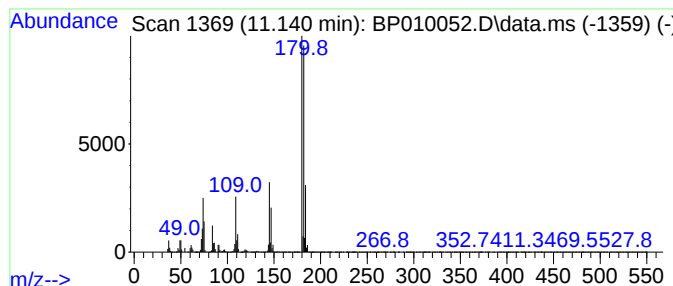

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 9 Benzene, 1-chloro-3-nitro- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.346	36.16 ng/ul	3770750	Naphthalene-d8	10.752

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1-chloro-3-nitro-	157	C6H4ClNO2	000121-73-3	96
2			Benzene, 1-chloro-3-nitro-	157	C6H4ClNO2	000121-73-3	95
3			Benzene, 1-chloro-4-nitro-	157	C6H4ClNO2	000100-00-5	94
4			Benzene, 1-chloro-4-nitro-	157	C6H4ClNO2	000100-00-5	94
5			Benzene, 1-chloro-3-nitro-	157	C6H4ClNO2	000121-73-3	93

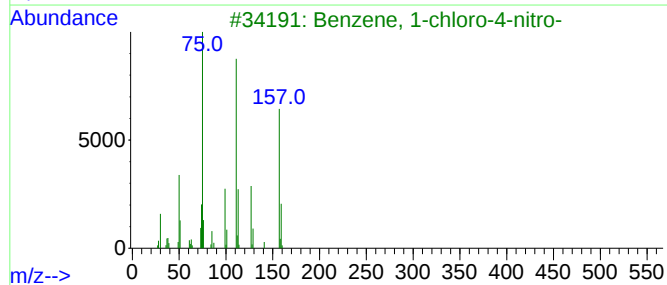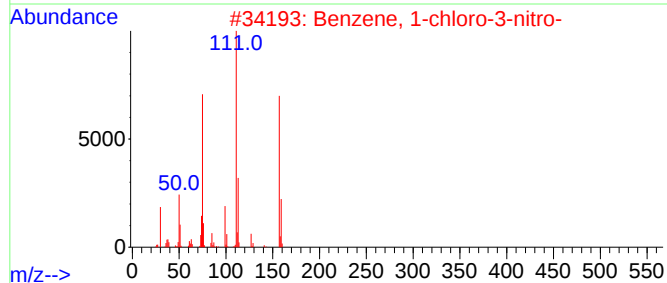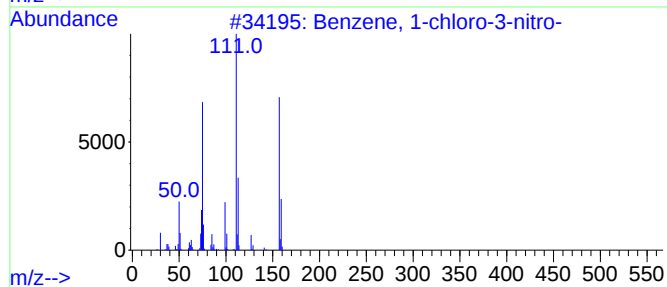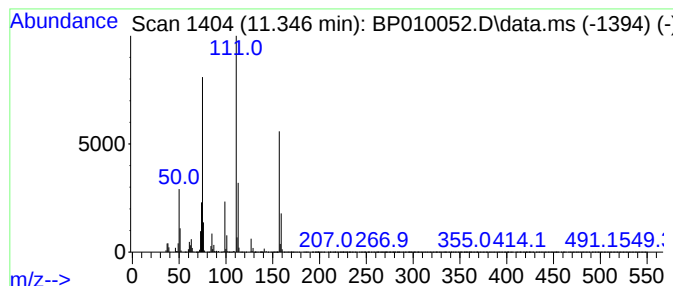

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 10 Benzene, 1-chloro-2-nitro- Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.557	9.25 ng/ul	964854	Naphthalene-d8	10.752

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1-chloro-2-nitro-	157	C6H4ClNO2	000088-73-3	98
2			Benzene, 1-chloro-2-nitro-	157	C6H4ClNO2	000088-73-3	97
3			Benzene, 1-chloro-4-nitro-	157	C6H4ClNO2	000100-00-5	97
4			Benzene, 1-chloro-2-nitro-	157	C6H4ClNO2	000088-73-3	96
5			Benzene, 1-chloro-4-nitro-	157	C6H4ClNO2	000100-00-5	96

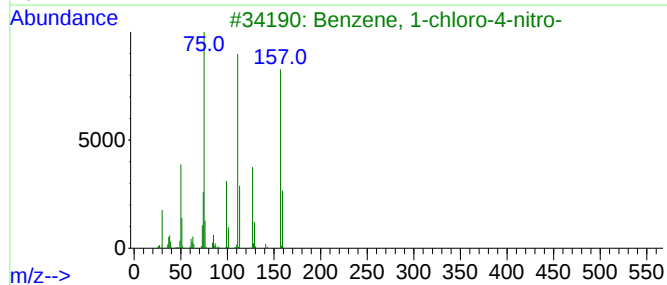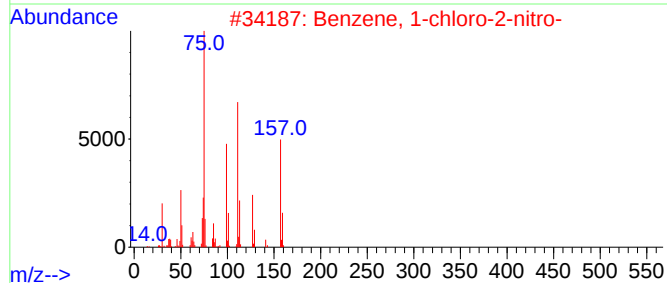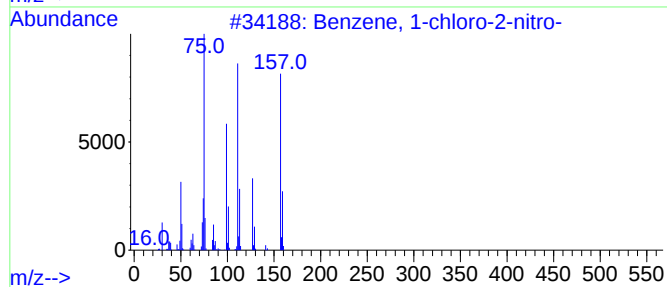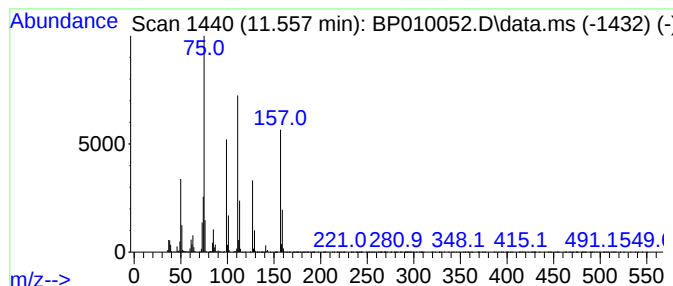

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010052.D
Acq On : 22 Apr 2022 12:56
Operator : CG/JU
Sample : N2473-07DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J50DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, chloro-	5.264	11.7	ng/ul	57802400	1	7.958	99068300	20.0
Benzene, 1,4-di...	7.846	5.5	ng/ul	27049000	1	7.958	99068300	20.0
Benzene, 1,2-di...	8.016	20.0	ng/ul	99068300	1	7.958	99068300	20.0
Benzene, 1,3-di...	8.346	23.1	ng/ul	114374000	1	7.958	99068300	20.0
Benzene, 1-brom...	9.440	3.6	ng/ul	372362	2	10.752	2085620	20.0
Benzene, 1-brom...	9.757	2.5	ng/ul	262304	2	10.752	2085620	20.0
Benzene, 1,2,3-...	10.628	414.5	ng/ul	43224800	2	10.752	2085620	20.0
Benzene, 1,2,4-...	11.140	161.8	ng/ul	16873100	2	10.752	2085620	20.0
Benzene, 1-chlo...	11.346	36.2	ng/ul	3770750	2	10.752	2085620	20.0
Benzene, 1-chlo...	11.557	9.3	ng/ul	964854	2	10.752	2085620	20.0