

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010055.D
 Acq On : 22 Apr 2022 14:37
 Operator : CG/JU
 Sample : N2473-18
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	59	rVB	42764	69089	1.29%	0.157%
2	3.793	117	120	134	rBV	153311	289628	5.39%	0.659%
3	4.017	155	158	163	rBV6	7364	16347	0.30%	0.037%
4	4.122	173	176	182	rVB3	10390	16164	0.30%	0.037%
5	5.981	487	492	499	rBV7	9271	19569	0.36%	0.045%
6	7.040	668	672	675	rBV6	5471	7707	0.14%	0.018%
7	7.099	675	682	691	rVB	46031	87415	1.63%	0.199%
8	7.263	701	710	726	rVB	560713	913275	17.00%	2.078%
9	7.469	739	745	755	rBV	228394	389193	7.25%	0.885%
10	7.940	817	825	832	rBV	621876	1006996	18.75%	2.291%
11	8.010	832	837	845	rVB	32010	54607	1.02%	0.124%
12	8.187	863	867	871	rBV7	5349	9268	0.17%	0.021%
13	8.646	938	945	957	rBV	117095	213382	3.97%	0.485%
14	8.757	957	964	970	rVB3	9992	19897	0.37%	0.045%
15	9.040	1006	1012	1016	rBV	50105	86886	1.62%	0.198%
16	9.099	1016	1022	1036	rVB	728494	1271421	23.67%	2.893%
17	9.269	1045	1051	1059	rVB10	11322	22735	0.42%	0.052%
18	9.546	1094	1098	1105	rVB4	7956	12590	0.23%	0.029%
19	9.669	1115	1119	1123	rBV7	3568	6552	0.12%	0.015%
20	9.834	1140	1147	1155	rBV5	20586	47373	0.88%	0.108%
21	9.993	1168	1174	1179	rVB9	3870	8730	0.16%	0.020%
22	10.263	1211	1220	1223	rBV10	4635	10548	0.20%	0.024%
23	10.363	1229	1237	1253	rBV	301518	548058	10.20%	1.247%
24	10.651	1280	1286	1294	rBV2	17920	37076	0.69%	0.084%
25	10.746	1294	1302	1309	rBV	944830	1615603	30.08%	3.676%
26	10.804	1309	1312	1316	rVB3	14817	19729	0.37%	0.045%
27	10.875	1317	1324	1339	rBV	858048	1529803	28.48%	3.481%
28	11.404	1409	1414	1421	rVB4	8389	16864	0.31%	0.038%
29	11.546	1435	1438	1444	rVB8	5178	8341	0.16%	0.019%
30	11.916	1495	1501	1506	rBV7	6491	12267	0.23%	0.028%
31	12.046	1516	1523	1528	rBV6	14263	28945	0.54%	0.066%
32	12.140	1534	1539	1545	rVB9	5398	10267	0.19%	0.023%
33	12.328	1564	1571	1577	rBV2	20273	33888	0.63%	0.077%
34	12.775	1640	1647	1651	rBV9	4400	9374	0.17%	0.021%
35	12.869	1661	1663	1670	rVB8	4550	8436	0.16%	0.019%
36	12.940	1670	1675	1685	rBV8	8730	19328	0.36%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010055.D
 Acq On : 22 Apr 2022 14:37
 Operator : CG/JU
 Sample : N2473-18
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	13.187	1710	1717	1726	rVB6	13382	25572	0.48%	0.058%
38	13.892	1832	1837	1841	rVV7	10795	16023	0.30%	0.036%
39	13.975	1845	1851	1863	rVV	2022548	2822838	52.55%	6.422%
40	14.104	1870	1873	1880	rVB8	7138	10678	0.20%	0.024%
41	14.263	1890	1900	1919	rBV	2106224	3101104	57.73%	7.056%
42	14.569	1943	1952	1963	rBV	1629473	2419897	45.05%	5.506%
43	14.651	1963	1966	1971	rVB5	9353	13680	0.25%	0.031%
44	14.787	1983	1989	1992	rBV8	5328	9529	0.18%	0.022%
45	14.828	1995	1996	2005	rVB9	4382	6749	0.13%	0.015%
46	15.375	2085	2089	2096	rVB2	16277	27554	0.51%	0.063%
47	15.563	2114	2121	2134	rBV	2838301	4002454	74.51%	9.106%
48	15.804	2155	2162	2167	rBV	33009	51421	0.96%	0.117%
49	15.928	2179	2183	2186	rBV5	8768	14139	0.26%	0.032%
50	16.139	2213	2219	2224	rBV10	6353	14217	0.26%	0.032%
51	16.351	2251	2255	2261	rVB6	11088	17487	0.33%	0.040%
52	17.004	2361	2366	2370	rVB8	5795	7729	0.14%	0.018%
53	17.110	2380	2384	2387	rBV2	7448	11422	0.21%	0.026%
54	17.322	2413	2420	2430	rBV	1984992	2886723	53.74%	6.568%
55	17.422	2430	2437	2452	rVB	3259059	4679767	87.12%	10.647%
56	17.610	2465	2469	2477	rVB	12567	17649	0.33%	0.040%
57	17.986	2528	2533	2541	rVB	212750	266917	4.97%	0.607%
58	18.275	2578	2582	2586	rBV	17576	24208	0.45%	0.055%
59	19.227	2740	2744	2749	rBV2	42344	62902	1.17%	0.143%
60	19.298	2751	2756	2764	rVV	41066	63576	1.18%	0.145%
61	19.580	2801	2804	2809	rBV6	16558	19213	0.36%	0.044%
62	19.651	2810	2816	2830	rVV	3958099	5371604	100.00%	12.221%
63	21.404	3109	3114	3129	rVB	2076628	2797950	52.09%	6.366%
64	22.539	3304	3307	3313	rVB2	70286	96320	1.79%	0.219%
65	23.110	3400	3404	3411	rVB2	100807	158328	2.95%	0.360%
66	23.698	3497	3504	3511	rBV2	1903788	3872125	72.09%	8.810%
67	23.863	3524	3532	3545	rVB2	1117233	2371586	44.15%	5.396%
68	24.504	3638	3641	3649	rVB2	111506	214186	3.99%	0.487%


Sum of corrected areas: 43952898

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010055.D
Acq On : 22 Apr 2022 14:37
Operator : CG/JU
Sample : N2473-18
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

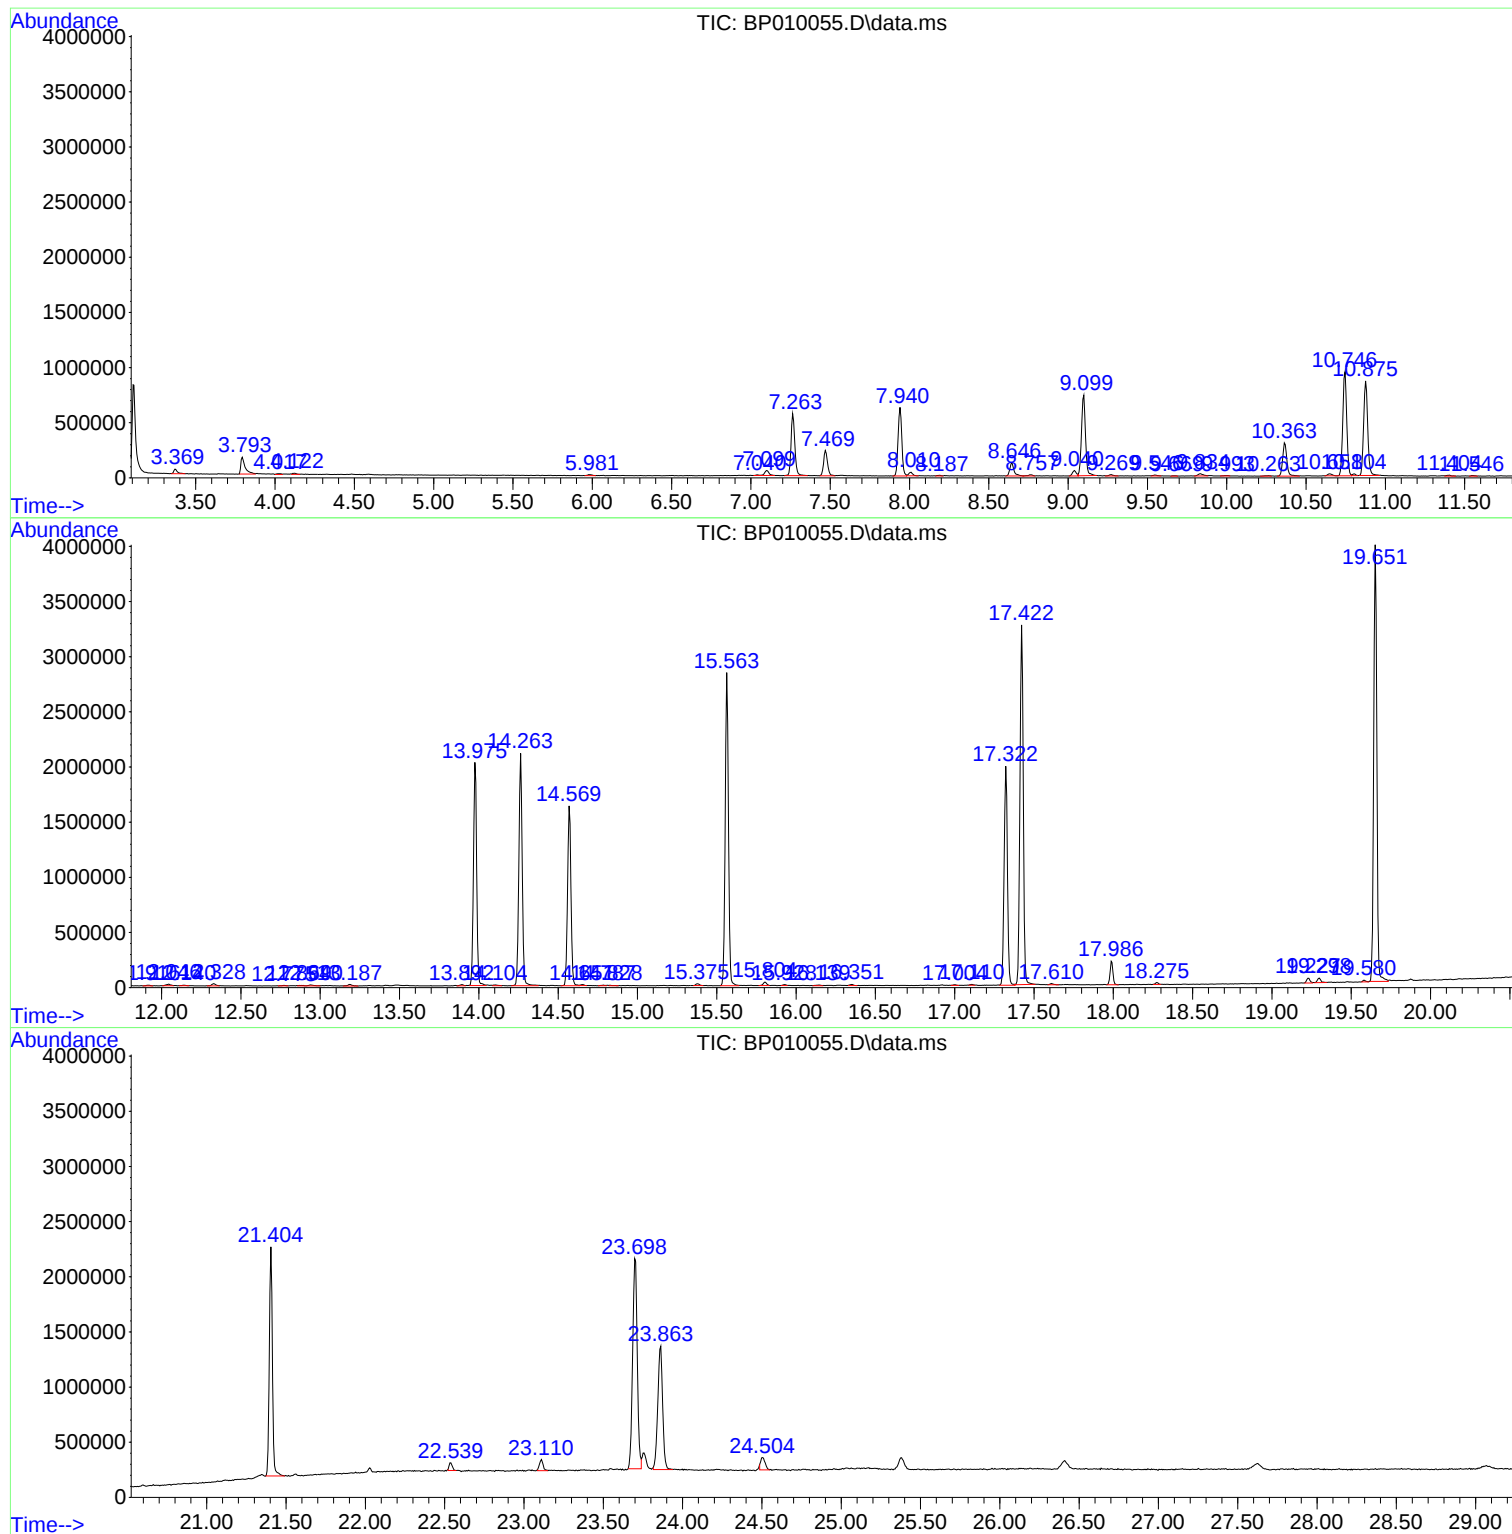

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010055.D
Acq On : 22 Apr 2022 14:37
Operator : CG/JU
Sample : N2473-18
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010055.D
Acq On : 22 Apr 2022 14:37
Operator : CG/JU
Sample : N2473-18
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc