

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010068.D
 Acq On : 22 Apr 2022 22:48
 Operator : CG/JU
 Sample : N2490-11
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010068.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	52	rBV	21475	29994	0.59%	0.070%
2	3.652	92	96	98	rBV4	8836	12749	0.25%	0.030%
3	3.799	118	121	136	rBV	104221	242711	4.77%	0.566%
4	4.116	171	175	180	rVB3	8989	14527	0.29%	0.034%
5	5.252	362	368	377	rBV2	20285	39182	0.77%	0.091%
6	6.487	574	578	581	rBV6	3868	5339	0.10%	0.012%
7	7.099	676	682	692	rVB	126355	220183	4.33%	0.514%
8	7.263	700	710	721	rBV	526622	853977	16.78%	1.992%
9	7.340	721	723	728	rVB4	4468	6797	0.13%	0.016%
10	7.469	738	745	754	rBV	488701	823534	16.19%	1.921%
11	7.575	760	763	768	rVB7	3451	5158	0.10%	0.012%
12	7.828	800	806	813	rVB2	27826	48307	0.95%	0.113%
13	7.940	817	825	835	rBV	497700	889095	17.47%	2.074%
14	8.293	879	885	891	rBV	74119	126649	2.49%	0.295%
15	8.646	935	945	958	rBV	393304	693487	13.63%	1.618%
16	9.099	1011	1022	1035	rBV	720161	1256222	24.69%	2.930%
17	9.546	1092	1098	1106	rVB2	47135	74833	1.47%	0.175%
18	9.822	1137	1145	1154	rBV	506117	851164	16.73%	1.986%
19	10.363	1228	1237	1257	rBV	780157	1414391	27.80%	3.299%
20	10.516	1260	1263	1269	rVB8	4750	8742	0.17%	0.020%
21	10.610	1269	1279	1282	rBV	75521	145371	2.86%	0.339%
22	10.746	1294	1302	1316	rVB	797117	1377072	27.06%	3.212%
23	10.875	1317	1324	1347	rBV	551833	1132058	22.25%	2.641%
24	11.134	1361	1368	1374	rVB3	31499	59709	1.17%	0.139%
25	12.045	1516	1523	1527	rBV6	7613	18116	0.36%	0.042%
26	12.175	1539	1545	1553	rVB5	8169	15825	0.31%	0.037%
27	12.328	1566	1571	1578	rBV2	16962	29431	0.58%	0.069%
28	12.940	1672	1675	1678	rBV5	4183	5974	0.12%	0.014%
29	13.187	1714	1717	1722	rVB7	4604	7646	0.15%	0.018%
30	13.381	1741	1750	1752	rBV6	11291	21307	0.42%	0.050%
31	13.404	1752	1754	1760	rVB	17407	23552	0.46%	0.055%
32	13.604	1781	1788	1793	rBV6	9389	19318	0.38%	0.045%
33	13.975	1844	1851	1865	rBV	1851373	2708398	53.23%	6.318%
34	14.263	1890	1900	1917	rBV	1999611	3025895	59.47%	7.059%
35	14.481	1932	1937	1942	rVB7	5338	8357	0.16%	0.019%
36	14.569	1944	1952	1968	rBV	1370352	2069077	40.66%	4.827%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010068.D
 Acq On : 22 Apr 2022 22:48
 Operator : CG/JU
 Sample : N2490-11
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	14.775	1980	1987	1997	rBV2	46161	120709	2.37%	0.282%
38	14.892	2004	2007	2011	rVB6	6578	8237	0.16%	0.019%
39	14.981	2019	2022	2025	rBV5	4142	5229	0.10%	0.012%
40	15.234	2059	2065	2068	rBV7	6104	12711	0.25%	0.030%
41	15.375	2083	2089	2094	rBV3	18402	31072	0.61%	0.072%
42	15.563	2114	2121	2135	rBV	2764450	4100582	80.59%	9.566%
43	15.675	2135	2140	2152	rVV	388525	596064	11.71%	1.390%
44	15.804	2156	2162	2168	rVB	32625	56040	1.10%	0.131%
45	15.998	2193	2195	2201	rVB7	4748	7090	0.14%	0.017%
46	16.133	2215	2218	2221	rBV5	3359	5288	0.10%	0.012%
47	16.239	2233	2236	2237	rBV3	5067	6518	0.13%	0.015%
48	16.351	2250	2255	2259	rVB6	11221	16720	0.33%	0.039%
49	16.998	2362	2365	2370	rBV7	4825	7836	0.15%	0.018%
50	17.086	2376	2380	2381	rBV3	6092	7169	0.14%	0.017%
51	17.110	2381	2384	2390	rVV3	8168	15360	0.30%	0.036%
52	17.192	2394	2398	2400	rBV5	4615	5928	0.12%	0.014%
53	17.322	2413	2420	2430	rBV	1698582	2508014	49.29%	5.851%
54	17.422	2430	2437	2456	rVV	3043739	4520832	88.85%	10.546%
55	17.992	2530	2534	2537	rVB5	9874	14172	0.28%	0.033%
56	18.204	2563	2570	2577	rBV6	26323	46044	0.90%	0.107%
57	18.275	2579	2582	2586	rVB3	10776	14938	0.29%	0.035%
58	18.810	2670	2673	2677	rBV6	6079	7899	0.16%	0.018%
59	19.227	2740	2744	2750	rVB2	38230	51937	1.02%	0.121%
60	19.298	2752	2756	2760	rVV	38636	48823	0.96%	0.114%
61	19.574	2801	2803	2807	rBV4	10663	12068	0.24%	0.028%
62	19.651	2810	2816	2833	rBV	3813941	5088134	100.00%	11.870%
63	21.104	3060	3063	3072	rBV	94780	147414	2.90%	0.344%
64	21.404	3108	3114	3127	rBV	1388837	2049085	40.27%	4.780%
65	23.698	3496	3504	3511	rBV	1560003	3269660	64.26%	7.627%
66	23.857	3524	3531	3548	rVB2	795925	1801498	35.41%	4.203%




Sum of corrected areas: 42867218

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010068.D
Acq On : 22 Apr 2022 22:48
Operator : CG/JU
Sample : N2490-11
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J34

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

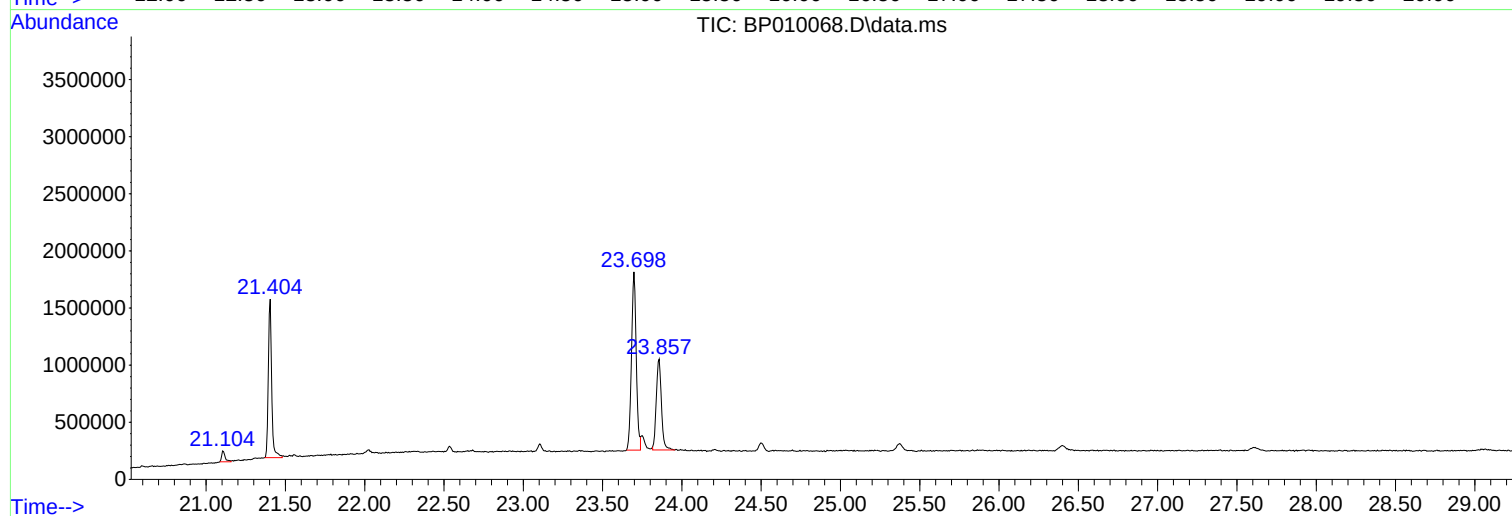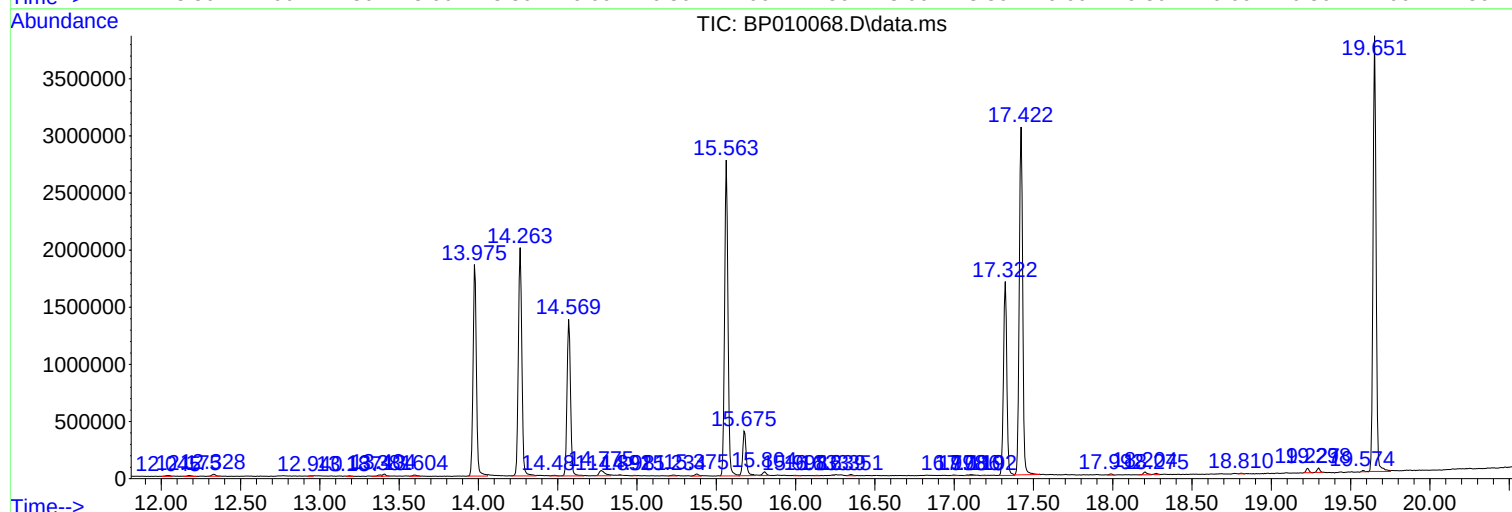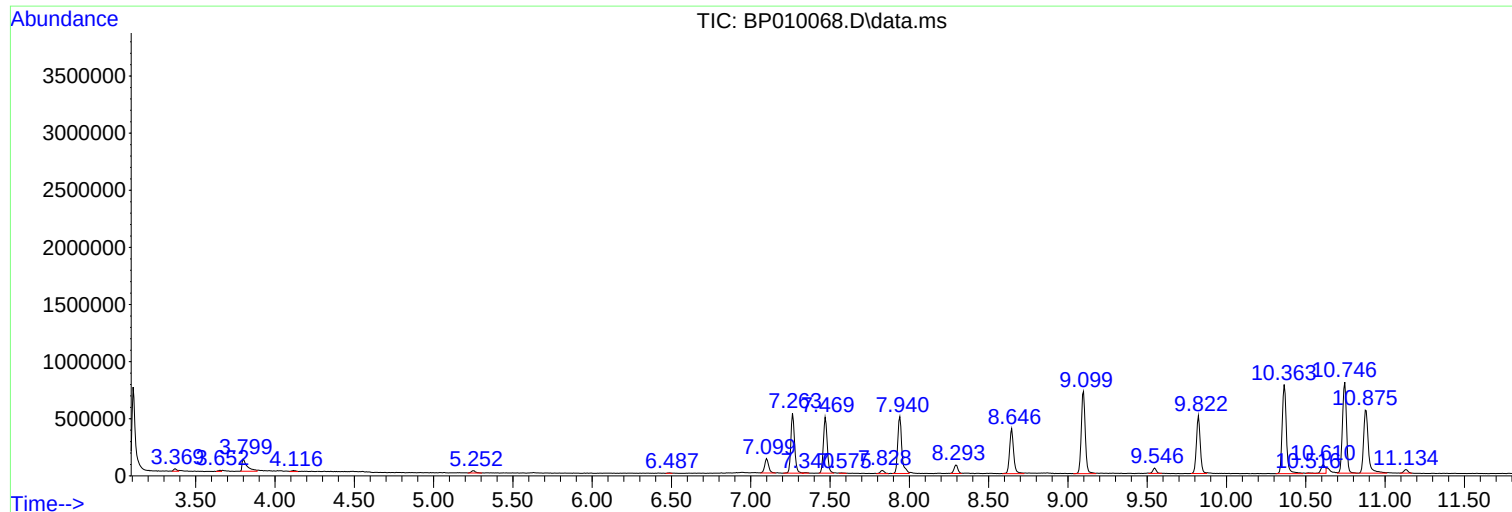

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010068.D
Acq On : 22 Apr 2022 22:48
Operator : CG/JU
Sample : N2490-11
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J34










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,3-dichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.293	2.85 ng/ul	126649	1,4-Dichlorobenzene-d4	7.940

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	98
2			Benzene, 1,2-dichloro-	146	C6H4Cl2	000095-50-1	98
3			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	98
4			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	97
5			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	96

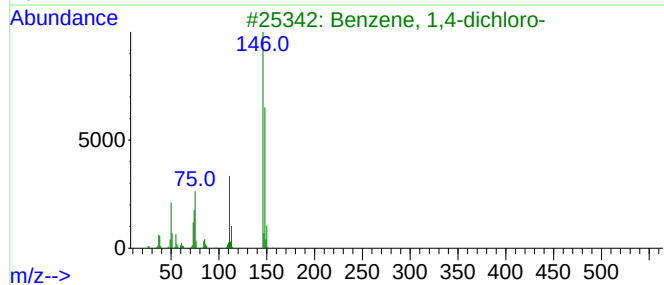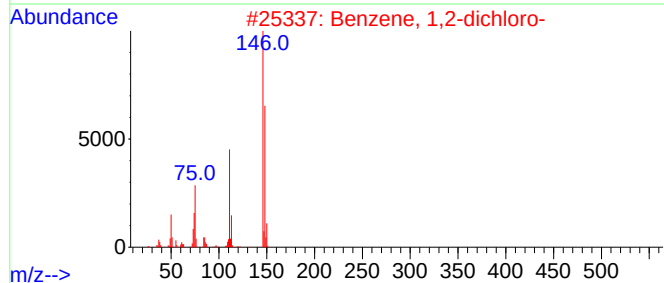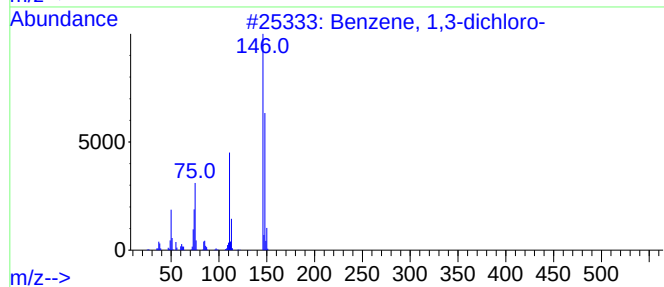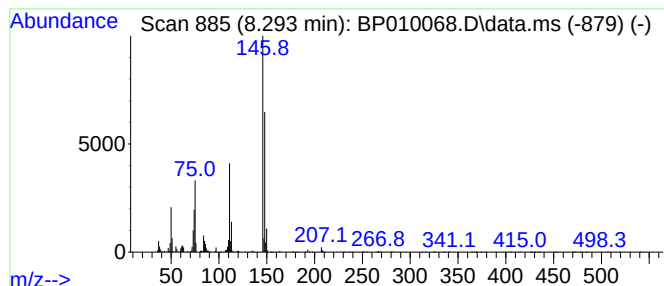

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010068.D
Acq On : 22 Apr 2022 22:48
Operator : CG/JU
Sample : N2490-11
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J34










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, 1,3,5-trichloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.610	2.11 ng/ul	145371	Naphthalene-d8	10.746

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
2			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
3			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	96
4			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	95
5			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	94

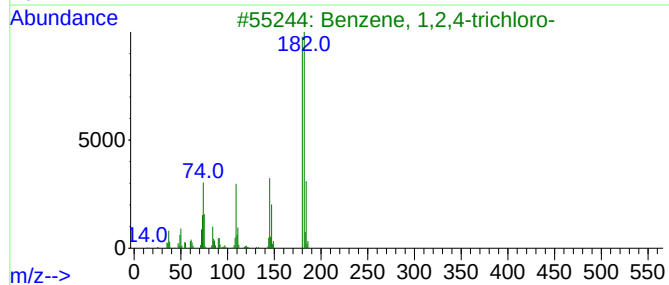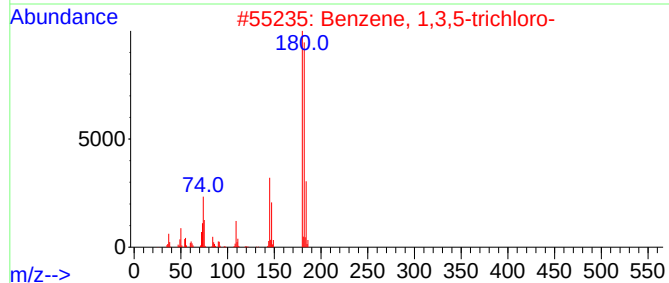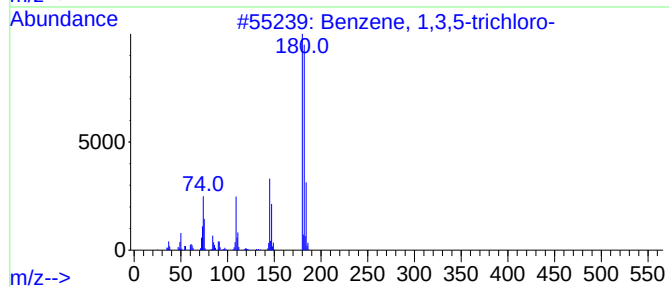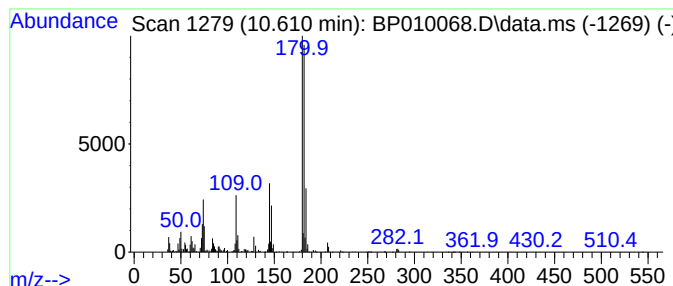

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010068.D
Acq On : 22 Apr 2022 22:48
Operator : CG/JU
Sample : N2490-11
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J34

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,3-di...	8.293	2.9	ng/ul	126649	1	7.940	889095	20.0
Benzene, 1,3,5-...	10.610	2.1	ng/ul	145371	2	10.746	1377070	20.0