

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010070.D
 Acq On : 22 Apr 2022 23:55
 Operator : CG/JU
 Sample : N2475-05
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	44	48	62	rVB2	27538	58465	1.18%	0.135%
2	3.652	92	96	105	rBV3	14538	35994	0.73%	0.083%
3	3.805	118	122	128	rBV	68981	135029	2.73%	0.311%
4	4.117	173	175	179	rVB3	6350	6431	0.13%	0.015%
5	5.640	428	434	437	rBV8	3901	7529	0.15%	0.017%
6	5.981	487	492	497	rBV9	5925	12125	0.24%	0.028%
7	6.481	574	577	583	rVB8	3340	5707	0.12%	0.013%
8	7.099	676	682	692	rVB	134778	232947	4.70%	0.536%
9	7.264	701	710	721	rBV	514768	840857	16.97%	1.936%
10	7.469	736	745	754	rBV	507318	853550	17.23%	1.965%
11	7.940	817	825	833	rBV	531561	867241	17.50%	1.997%
12	8.011	833	837	841	rVB2	11153	18383	0.37%	0.042%
13	8.363	892	897	899	rBV6	3880	4969	0.10%	0.011%
14	8.646	937	945	957	rBV	434522	739652	14.93%	1.703%
15	8.763	961	965	971	rVB6	5097	11016	0.22%	0.025%
16	9.046	1008	1013	1015	rBV5	4960	9580	0.19%	0.022%
17	9.099	1015	1022	1035	rVB	703225	1222884	24.68%	2.815%
18	9.499	1083	1090	1092	rBV8	3946	5349	0.11%	0.012%
19	9.546	1092	1098	1107	rVB4	15259	30809	0.62%	0.071%
20	9.822	1138	1145	1162	rBV	521249	893933	18.04%	2.058%
21	10.363	1227	1237	1251	rBV	804298	1446955	29.20%	3.331%
22	10.693	1288	1293	1294	rBV5	4590	5439	0.11%	0.013%
23	10.746	1294	1302	1313	rVB	822347	1427661	28.81%	3.287%
24	10.875	1317	1324	1344	rBV	578383	1177606	23.77%	2.711%
25	12.040	1519	1522	1529	rBV8	6378	11244	0.23%	0.026%
26	12.175	1541	1545	1552	rBV7	8461	13959	0.28%	0.032%
27	12.334	1563	1572	1576	rBV3	18070	35237	0.71%	0.081%
28	12.375	1576	1579	1587	rVB4	12286	23541	0.48%	0.054%
29	12.763	1641	1645	1649	rBV7	4871	10052	0.20%	0.023%
30	12.957	1668	1678	1680	rBV7	4565	9768	0.20%	0.022%
31	13.116	1701	1705	1710	rVB6	8174	14137	0.29%	0.033%
32	13.193	1710	1718	1724	rVB6	5358	14383	0.29%	0.033%
33	13.299	1731	1736	1737	rBV5	5784	7355	0.15%	0.017%
34	13.416	1749	1756	1762	rBV	124864	190570	3.85%	0.439%
35	13.469	1762	1765	1770	rBV6	3891	6003	0.12%	0.014%
36	13.975	1843	1851	1868	rBV	1852299	2689636	54.28%	6.192%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010070.D
 Acq On : 22 Apr 2022 23:55
 Operator : CG/JU
 Sample : N2475-05
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	14.263	1890	1900	1916	rBV	2026508	2998714	60.52%	6.904%
38	14.475	1934	1936	1942	rVB6	5544	6164	0.12%	0.014%
39	14.569	1942	1952	1973	rBV	1395901	2165753	43.71%	4.986%
40	14.769	1981	1986	2004	rBV4	52914	149479	3.02%	0.344%
41	15.204	2054	2060	2072	rBV2	40646	70931	1.43%	0.163%
42	15.316	2074	2079	2084	rVB2	11625	18131	0.37%	0.042%
43	15.387	2084	2091	2096	rBV3	15602	30106	0.61%	0.069%
44	15.563	2113	2121	2134	rBV	2711552	3998888	80.70%	9.207%
45	15.675	2134	2140	2152	rVB	469140	695078	14.03%	1.600%
46	15.804	2157	2162	2169	rVB2	33273	54873	1.11%	0.126%
47	15.981	2188	2192	2199	rVB4	22955	33351	0.67%	0.077%
48	16.187	2224	2227	2231	rVB5	4412	7011	0.14%	0.016%
49	16.251	2234	2238	2240	rBV5	4275	6128	0.12%	0.014%
50	16.351	2251	2255	2259	rVB7	9387	13487	0.27%	0.031%
51	16.463	2269	2274	2275	rBV5	4290	6402	0.13%	0.015%
52	16.492	2275	2279	2283	rVV5	7955	11785	0.24%	0.027%
53	16.828	2333	2336	2340	rVB6	5831	8272	0.17%	0.019%
54	17.004	2362	2366	2371	rVB8	5438	8838	0.18%	0.020%
55	17.192	2393	2398	2403	rBV9	8202	16710	0.34%	0.038%
56	17.322	2413	2420	2430	rBV	1860666	2623245	52.94%	6.040%
57	17.422	2430	2437	2454	rVB	2978152	4395170	88.70%	10.119%
58	17.898	2515	2518	2523	rVB7	6309	6756	0.14%	0.016%
59	17.986	2529	2533	2539	rBV7	15539	23322	0.47%	0.054%
60	18.198	2565	2569	2574	rBV4	35182	57627	1.16%	0.133%
61	18.645	2643	2645	2647	rBV3	5688	5474	0.11%	0.013%
62	19.228	2740	2744	2750	rBV2	40450	56098	1.13%	0.129%
63	19.298	2751	2756	2770	rVV	38119	67004	1.35%	0.154%
64	19.433	2776	2779	2781	rBV3	9920	8740	0.18%	0.020%
65	19.575	2800	2803	2809	rVB7	14987	20685	0.42%	0.048%
66	19.651	2810	2816	2830	rBV	3677856	4955155	100.00%	11.408%
67	21.080	3056	3059	3060	rBV	52933	52966	1.07%	0.122%
68	21.104	3060	3063	3069	rVB	107625	140588	2.84%	0.324%
69	21.404	3108	3114	3126	rBV	1527504	2246333	45.33%	5.172%
70	23.698	3496	3504	3521	rBV2	1534182	3510225	70.84%	8.082%
71	23.857	3523	3531	3545	rVB2	851934	1889208	38.13%	4.350%




Sum of corrected areas: 43434693

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010070.D
Acq On : 22 Apr 2022 23:55
Operator : CG/JU
Sample : N2475-05
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BN6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

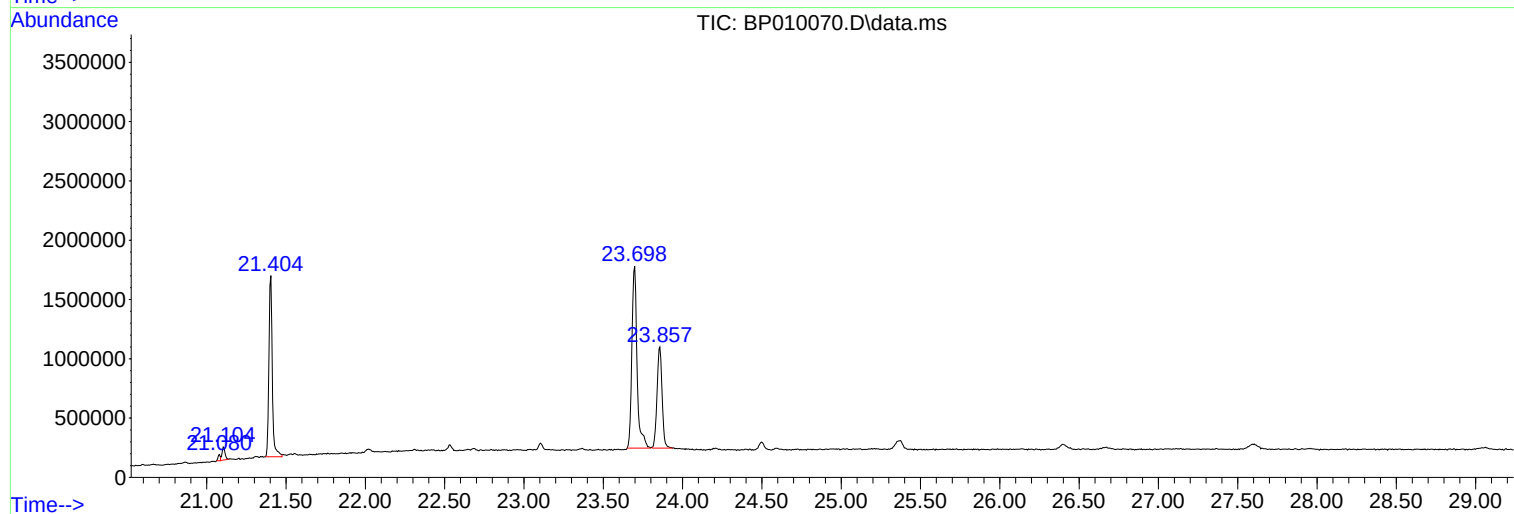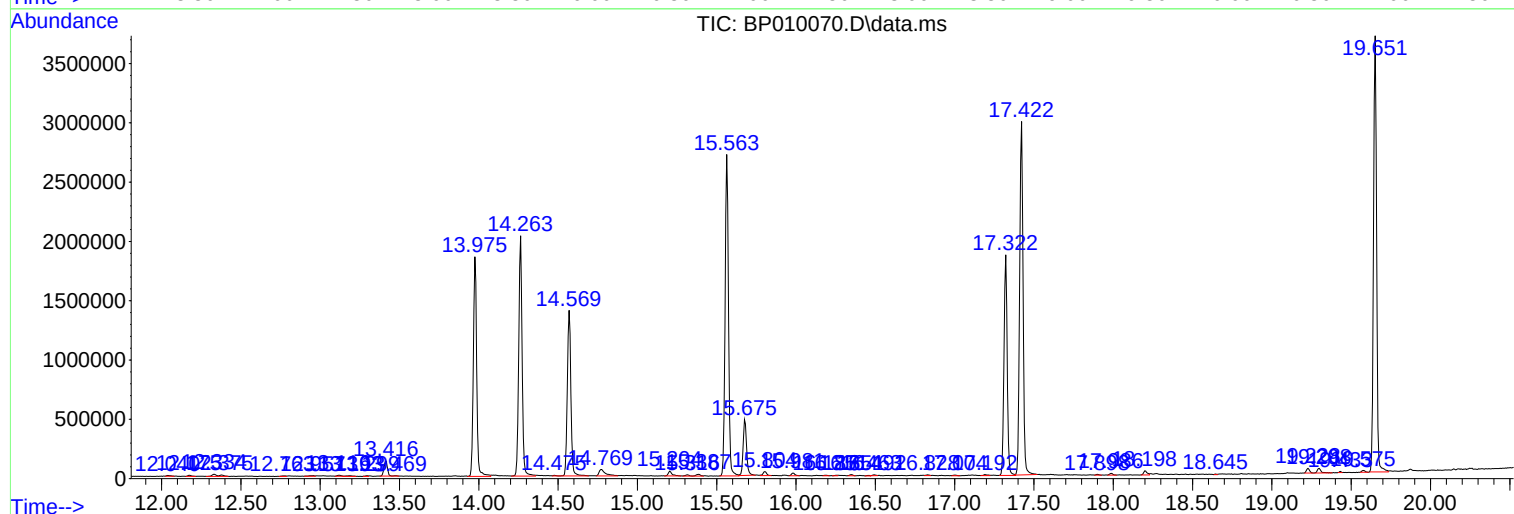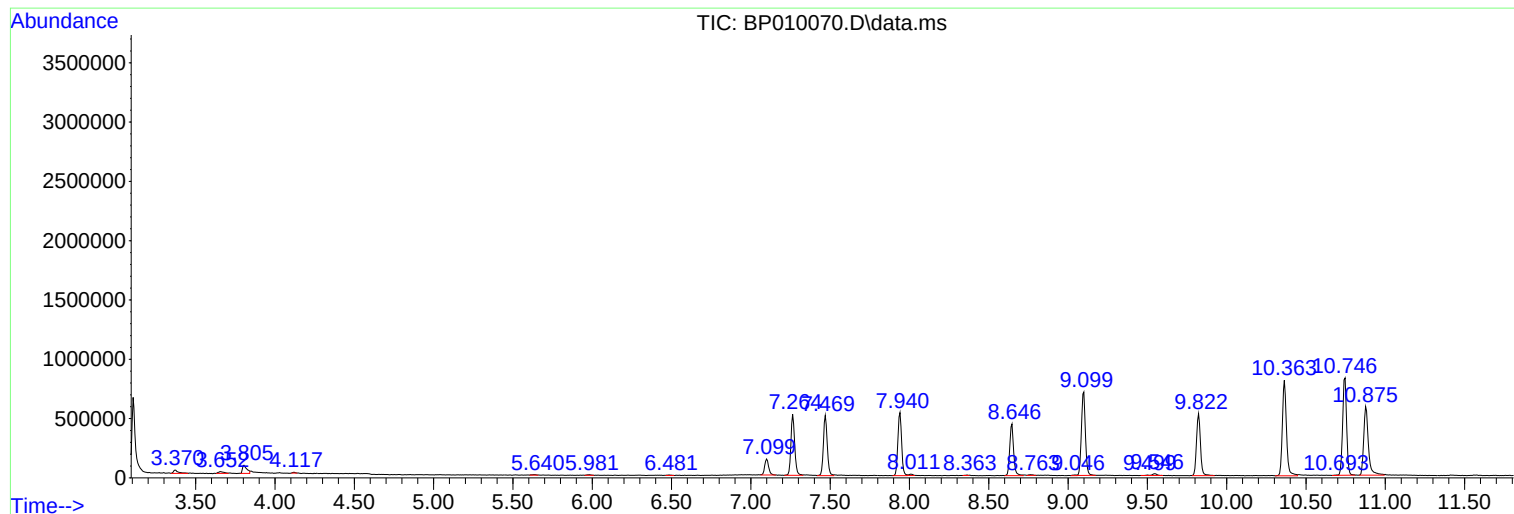

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010070.D
Acq On : 22 Apr 2022 23:55
Operator : CG/JU
Sample : N2475-05
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BN6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010070.D
Acq On : 22 Apr 2022 23:55
Operator : CG/JU
Sample : N2475-05
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BN6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------