

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010072.D
 Acq On : 23 Apr 2022 01:03
 Operator : CG/JU
 Sample : N2475-07
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	52	rBV	23594	36395	0.65%	0.078%
2	3.658	92	97	106	rBV6	11947	29280	0.52%	0.063%
3	3.799	118	121	139	rBV	99011	236191	4.19%	0.505%
4	4.116	171	175	180	rBV3	10925	17141	0.30%	0.037%
5	5.052	332	334	340	rVB7	4235	6035	0.11%	0.013%
6	6.846	633	639	643	rBV8	4293	7880	0.14%	0.017%
7	7.099	675	682	690	rBV	140375	246101	4.36%	0.527%
8	7.263	701	710	722	rBV	547743	903445	16.01%	1.933%
9	7.469	737	745	756	rBV	556592	921750	16.34%	1.972%
10	7.940	818	825	833	rBV	554555	919258	16.29%	1.967%
11	8.004	833	836	844	rVB8	9626	19264	0.34%	0.041%
12	8.645	935	945	956	rBV	462211	803499	14.24%	1.719%
13	9.098	1014	1022	1035	rBV	761896	1314414	23.30%	2.812%
14	9.545	1091	1098	1104	rVB5	14375	30607	0.54%	0.065%
15	9.822	1136	1145	1163	rBV	583329	1013269	17.96%	2.168%
16	10.092	1187	1191	1197	rVB9	2250	5655	0.10%	0.012%
17	10.363	1229	1237	1257	rBV	874149	1557216	27.60%	3.332%
18	10.745	1294	1302	1316	rVB	855295	1489074	26.39%	3.186%
19	10.875	1316	1324	1345	rBV	621650	1266170	22.44%	2.709%
20	12.175	1541	1545	1553	rVB8	6818	13584	0.24%	0.029%
21	12.328	1566	1571	1575	rBV2	18430	33296	0.59%	0.071%
22	12.369	1575	1578	1588	rVB4	14277	36133	0.64%	0.077%
23	13.192	1715	1718	1725	rVB9	2983	7577	0.13%	0.016%
24	13.404	1750	1754	1761	rVB4	16761	26657	0.47%	0.057%
25	13.475	1761	1766	1771	rBV4	12591	20423	0.36%	0.044%
26	13.975	1845	1851	1869	rBV	2060755	2979532	52.81%	6.375%
27	14.263	1890	1900	1918	rBV	2181585	3283631	58.20%	7.026%
28	14.480	1932	1937	1941	rVB8	4562	7378	0.13%	0.016%
29	14.569	1943	1952	1964	rBV	1488338	2231694	39.56%	4.775%
30	14.769	1980	1986	1996	rBV2	59559	151995	2.69%	0.325%
31	14.928	2011	2013	2018	rVB6	3905	6304	0.11%	0.013%
32	15.216	2056	2062	2063	rBV6	4395	7404	0.13%	0.016%
33	15.233	2063	2065	2069	rVB5	5995	7644	0.14%	0.016%
34	15.386	2085	2091	2095	rBV5	8662	14370	0.25%	0.031%
35	15.563	2112	2121	2133	rBV	3064476	4440269	78.70%	9.501%
36	15.675	2134	2140	2154	rVV	589084	909203	16.12%	1.945%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010072.D
 Acq On : 23 Apr 2022 01:03
 Operator : CG/JU
 Sample : N2475-07
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 AOBM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	15.804	2158	2162	2169	rVB	36449	58957	1.05%	0.126%
38	15.927	2181	2183	2190	rVB7	5450	7231	0.13%	0.015%
39	16.286	2242	2244	2249	rVB6	5240	6044	0.11%	0.013%
40	16.345	2249	2254	2258	rBV3	11958	17785	0.32%	0.038%
41	16.810	2327	2333	2335	rBV4	11105	18070	0.32%	0.039%
42	16.998	2359	2365	2374	rVB4	7045	16017	0.28%	0.034%
43	17.322	2413	2420	2429	rBV	1759734	2648171	46.94%	5.666%
44	17.421	2430	2437	2456	rVB	3401426	4913781	87.10%	10.514%
45	17.610	2467	2469	2472	rVB4	6998	6482	0.11%	0.014%
46	18.204	2564	2570	2579	rBV3	42830	73167	1.30%	0.157%
47	18.274	2579	2582	2586	rVB	13104	17022	0.30%	0.036%
48	18.680	2647	2651	2653	rBV5	4849	7429	0.13%	0.016%
49	19.227	2739	2744	2750	rBV2	48467	71782	1.27%	0.154%
50	19.298	2751	2756	2763	rBV	45492	76807	1.36%	0.164%
51	19.433	2777	2779	2781	rBV3	5967	6514	0.12%	0.014%
52	19.574	2800	2803	2808	rVB7	11185	14905	0.26%	0.032%
53	19.651	2810	2816	2837	rVV	4144194	5641741	100.00%	12.072%
54	19.868	2851	2853	2857	rVB4	11805	13179	0.23%	0.028%
55	21.110	3059	3064	3069	rBV2	149682	211388	3.75%	0.452%
56	21.404	3108	3114	3129	rBV	1553806	2240999	39.72%	4.795%
57	23.104	3400	3403	3408	rVB	85369	120224	2.13%	0.257%
58	23.698	3496	3504	3511	rBV2	1705900	3690201	65.41%	7.896%
59	23.856	3524	3531	3545	rVB2	832396	1858086	32.93%	3.976%




Sum of corrected areas: 46735720

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010072.D
Acq On : 23 Apr 2022 01:03
Operator : CG/JU
Sample : N2475-07
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

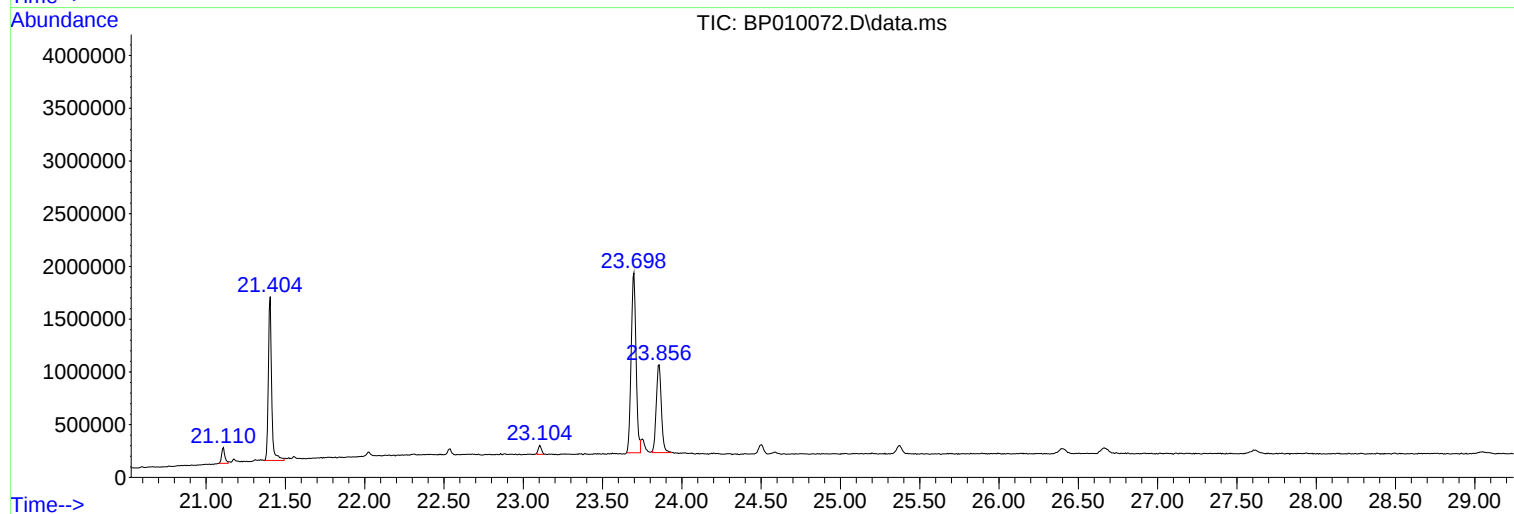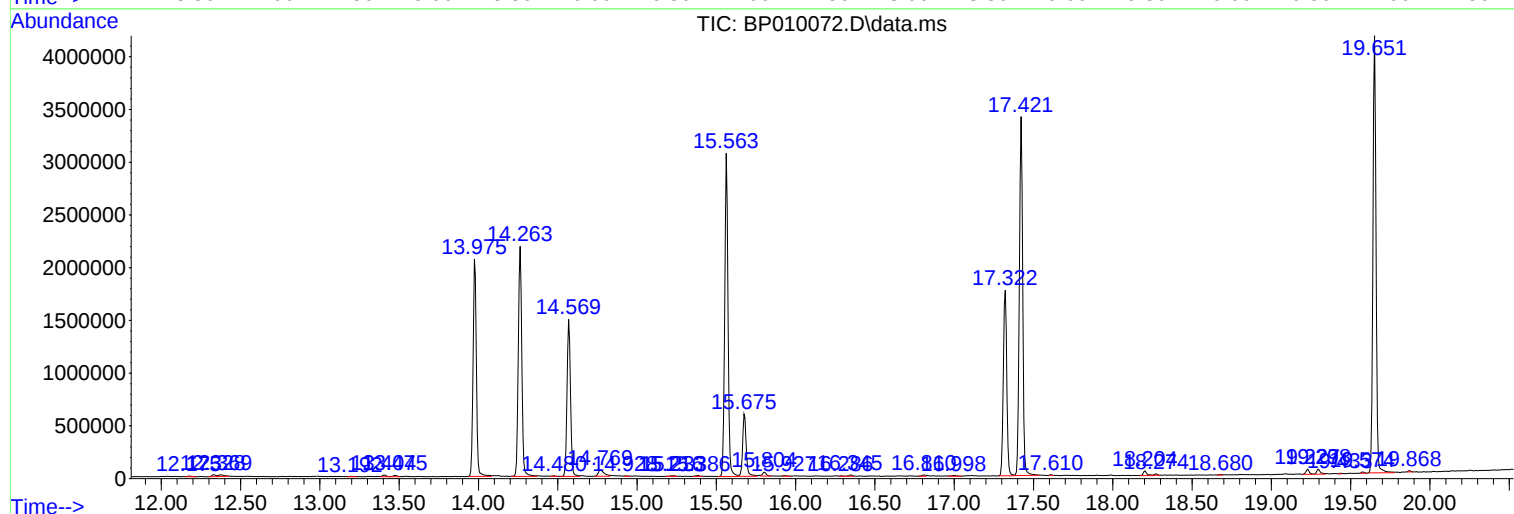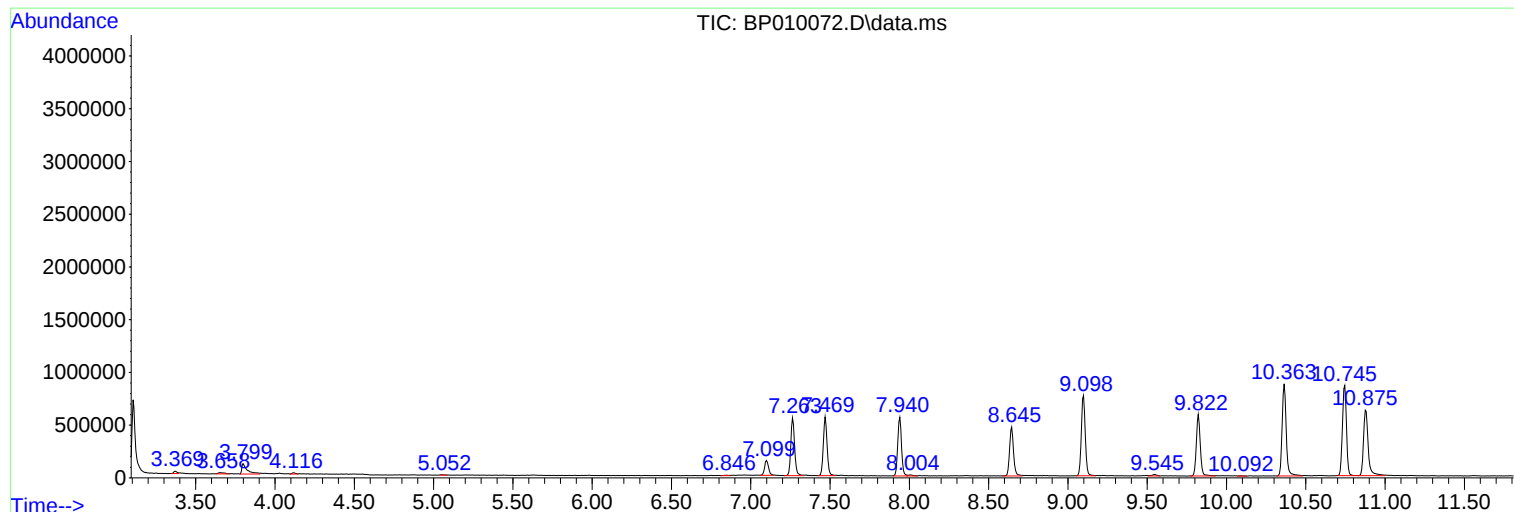

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010072.D
Acq On : 23 Apr 2022 01:03
Operator : CG/JU
Sample : N2475-07
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010072.D
Acq On : 23 Apr 2022 01:03
Operator : CG/JU
Sample : N2475-07
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc