

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010074.D
 Acq On : 23 Apr 2022 02:10
 Operator : CG/JU
 Sample : N2475-06
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	44	48	59	rBV	28421	48466	0.91%	0.111%
2	3.799	117	121	134	rBV	90528	207913	3.89%	0.475%
3	4.117	171	175	181	rVB2	9169	17349	0.32%	0.040%
4	7.099	675	682	691	rVB	140904	232407	4.35%	0.531%
5	7.264	703	710	723	rBV	516249	842112	15.75%	1.925%
6	7.469	738	745	754	rBV	520260	866269	16.20%	1.980%
7	7.575	760	763	768	rVB7	4274	6236	0.12%	0.014%
8	7.940	816	825	835	rBV	489107	831678	15.55%	1.901%
9	8.011	835	837	841	rVB5	5353	5994	0.11%	0.014%
10	8.640	937	944	957	rBV	415883	737366	13.79%	1.686%
11	9.093	1014	1021	1033	rBV	705012	1239478	23.18%	2.834%
12	9.546	1094	1098	1107	rVB4	10396	18849	0.35%	0.043%
13	9.822	1138	1145	1158	rBV	552294	945381	17.68%	2.161%
14	10.363	1230	1237	1254	rBV	803101	1445527	27.03%	3.305%
15	10.740	1289	1301	1316	rBV	770187	1361471	25.46%	3.112%
16	10.875	1316	1324	1349	rBV	621686	1253767	23.45%	2.866%
17	12.181	1542	1546	1552	rVB9	6001	11441	0.21%	0.026%
18	12.328	1565	1571	1577	rBV2	17612	31916	0.60%	0.073%
19	12.904	1664	1669	1672	rBV7	4279	7258	0.14%	0.017%
20	12.963	1673	1679	1690	rVV7	9799	28906	0.54%	0.066%
21	13.193	1713	1718	1724	rVB8	4673	9856	0.18%	0.023%
22	13.404	1750	1754	1761	rVB4	12353	18409	0.34%	0.042%
23	13.634	1788	1793	1800	rVB10	5581	11729	0.22%	0.027%
24	13.975	1844	1851	1871	rBV	1917954	2774030	51.88%	6.342%
25	14.104	1871	1873	1877	rVB5	9331	13065	0.24%	0.030%
26	14.263	1891	1900	1917	rBV	1980743	3074871	57.51%	7.029%
27	14.398	1921	1923	1931	rVV9	6933	16483	0.31%	0.038%
28	14.475	1933	1936	1939	rVB5	6337	8017	0.15%	0.018%
29	14.569	1945	1952	1965	rBV	1343105	2021007	37.80%	4.620%
30	14.769	1980	1986	2002	rBV	62803	177638	3.32%	0.406%
31	15.098	2039	2042	2046	rBV6	7560	9039	0.17%	0.021%
32	15.369	2085	2088	2093	rBV7	7771	10264	0.19%	0.023%
33	15.563	2114	2121	2133	rBV	2829710	4164282	77.88%	9.520%
34	15.675	2135	2140	2155	rVB	608749	892035	16.68%	2.039%
35	15.798	2158	2161	2166	rBV	32214	53121	0.99%	0.121%
36	16.316	2246	2249	2252	rBV2	19736	23891	0.45%	0.055%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
 Data File : BP010074.D
 Acq On : 23 Apr 2022 02:10
 Operator : CG/JU
 Sample : N2475-06
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BP0

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	17.322	2414	2420	2429	rBV	1619942	2396980	44.83%	5.480%
38	17.422	2430	2437	2447	rVV	3161478	4629849	86.59%	10.584%
39	19.651	2810	2816	2833	rBV	3964974	5347077	100.00%	12.224%
40	21.104	3060	3063	3070	rBV4	94875	133569	2.50%	0.305%
41	21.398	3108	3113	3128	rBV	1430146	2080449	38.91%	4.756%
42	22.533	3304	3306	3310	rVB3	69908	79309	1.48%	0.181%
43	23.104	3400	3403	3410	rVB2	80658	119611	2.24%	0.273%
44	23.698	3496	3504	3511	rBV2	1742971	3707385	69.33%	8.475%
45	23.857	3523	3531	3545	rVB2	831895	1831329	34.25%	4.187%




Sum of corrected areas: 43743079

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010074.D
Acq On : 23 Apr 2022 02:10
Operator : CG/JU
Sample : N2475-06
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

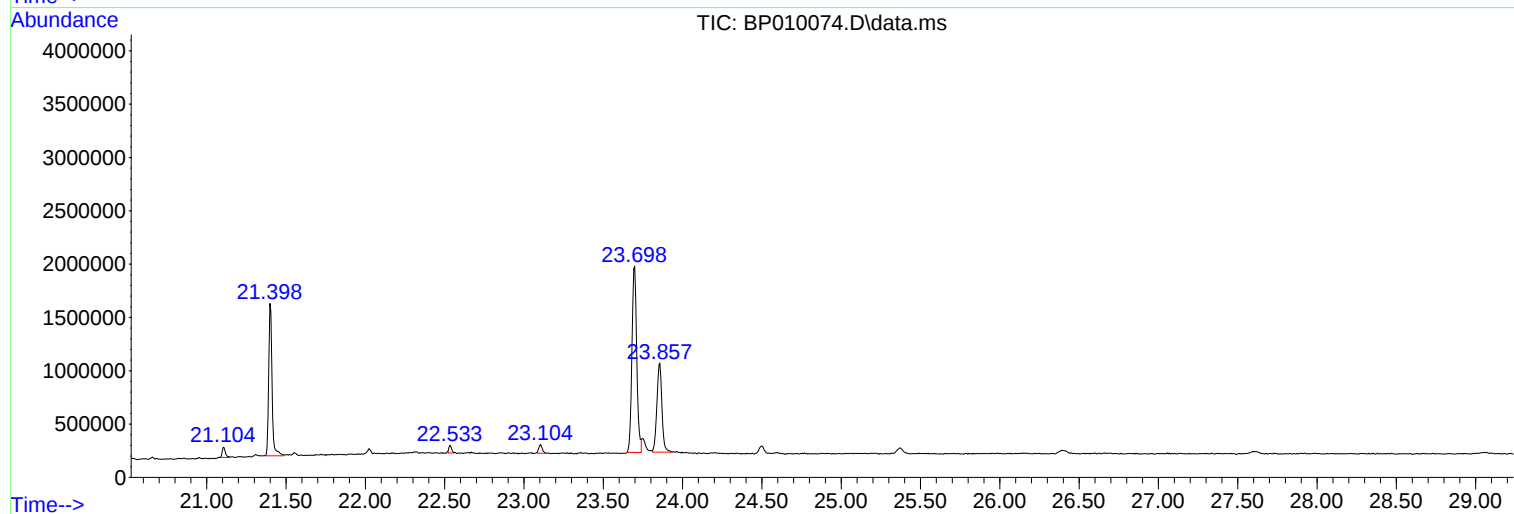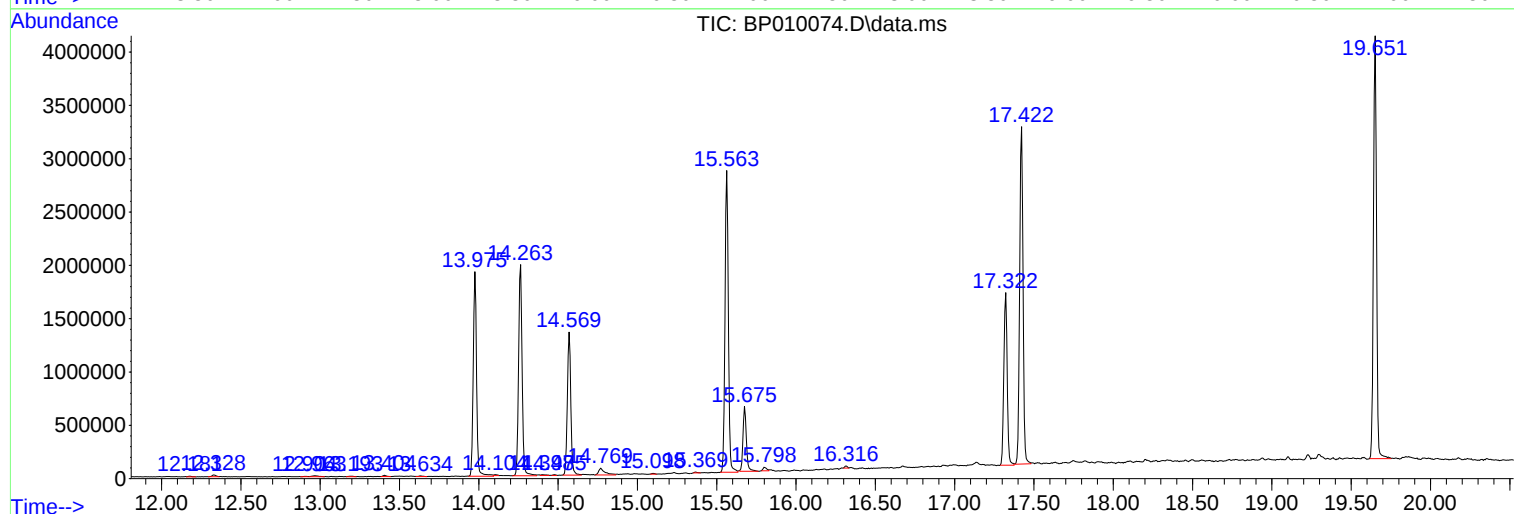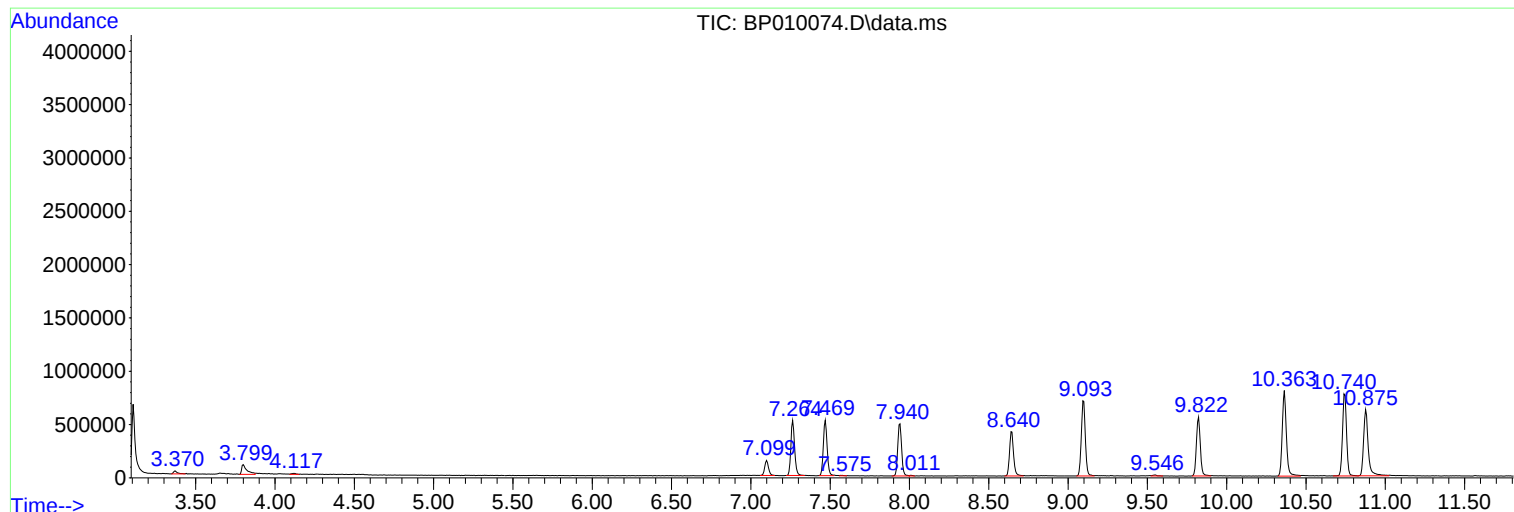

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010074.D
Acq On : 23 Apr 2022 02:10
Operator : CG/JU
Sample : N2475-06
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042122\
Data File : BP010074.D
Acq On : 23 Apr 2022 02:10
Operator : CG/JU
Sample : N2475-06
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------