
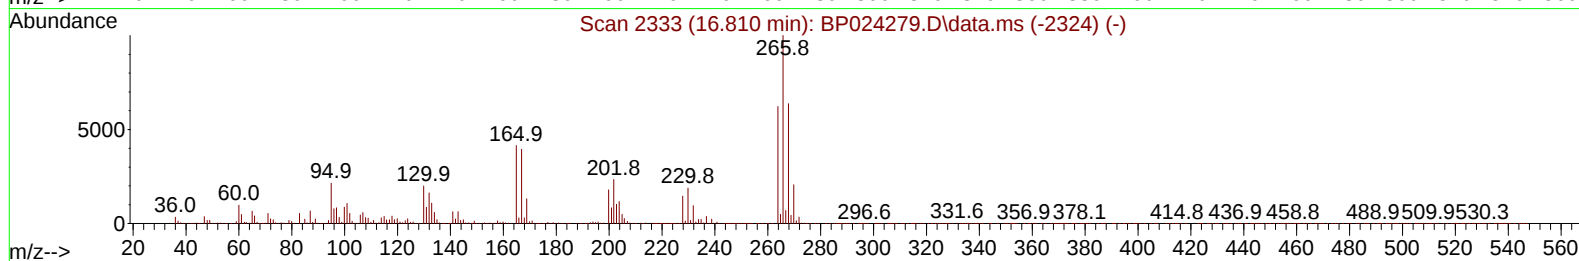
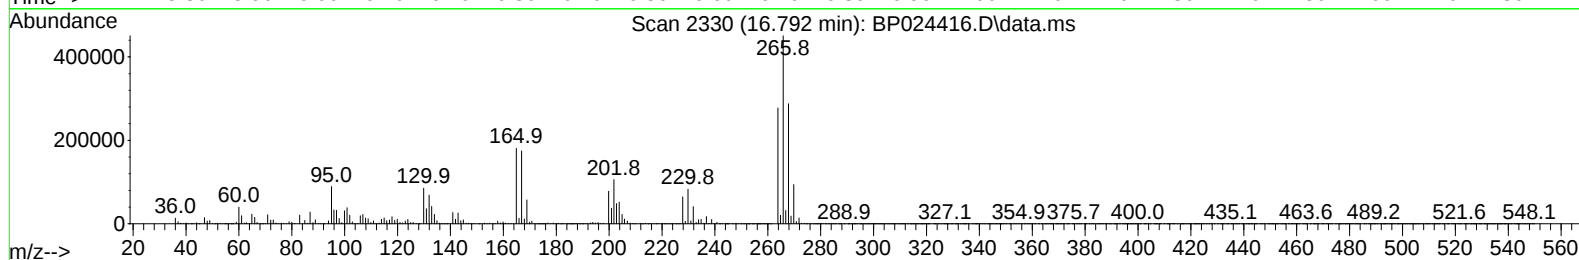


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP042525\  
Data File : BP024416.D  
Acq On : 25 Apr 2025 10:19  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 11:41:31 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP041425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 18 12:04:48 2025  
Response via : Initial Calibration

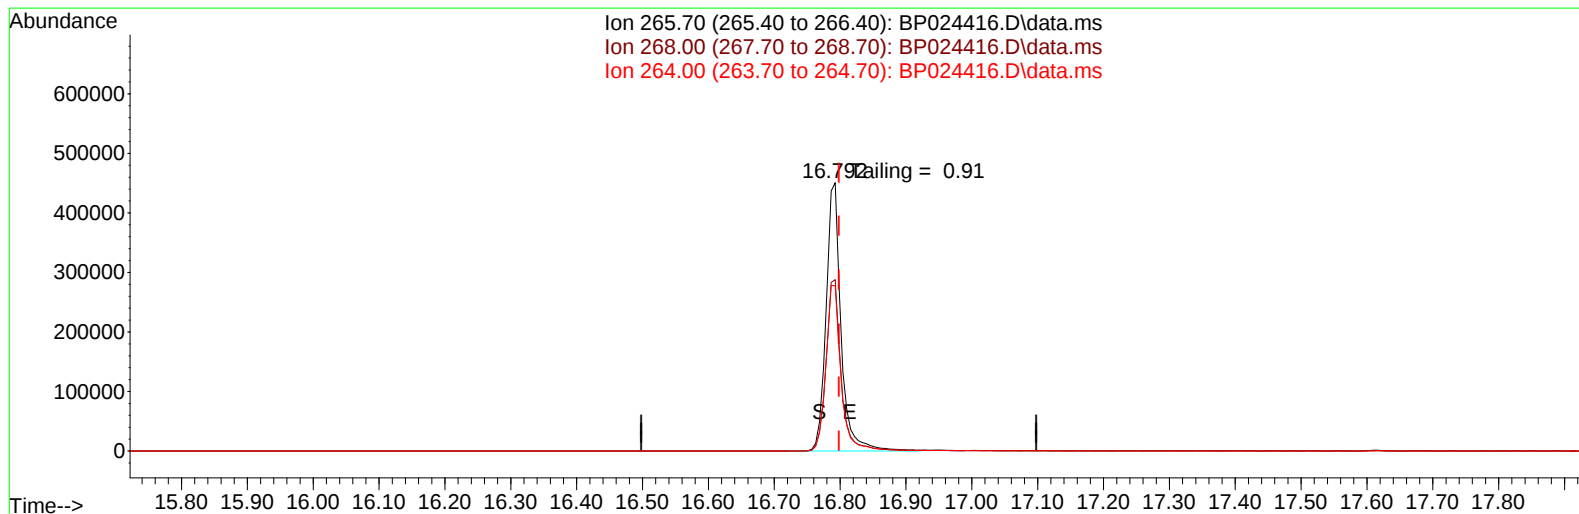

TIC: BP024416.D\data.ms

**(70) Pentachlorophenol (C)**




16.792min (-0.006) 201028.08 ng

response 710809

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 63.84  |
| 264.00 | 62.20  | 61.61  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP042525\  
Data File : BP024416.D  
Acq On : 25 Apr 2025 10:19  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 11:41:31 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP041425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 18 12:04:48 2025  
Response via : Initial Calibration

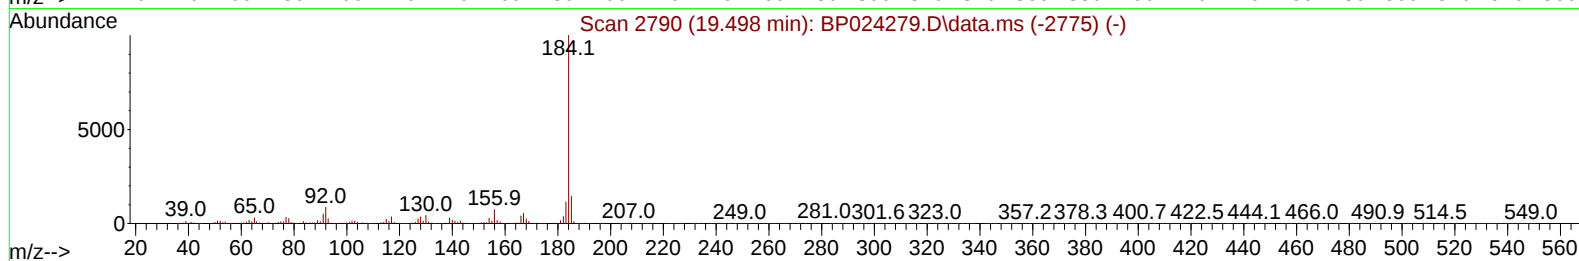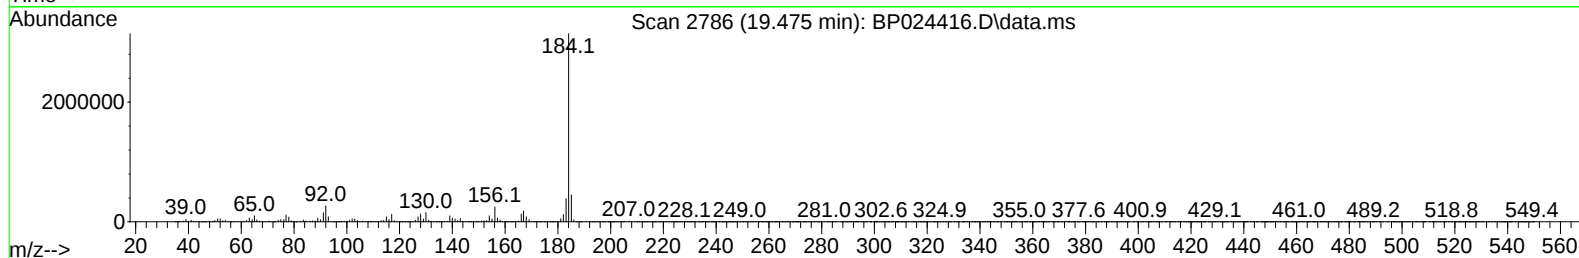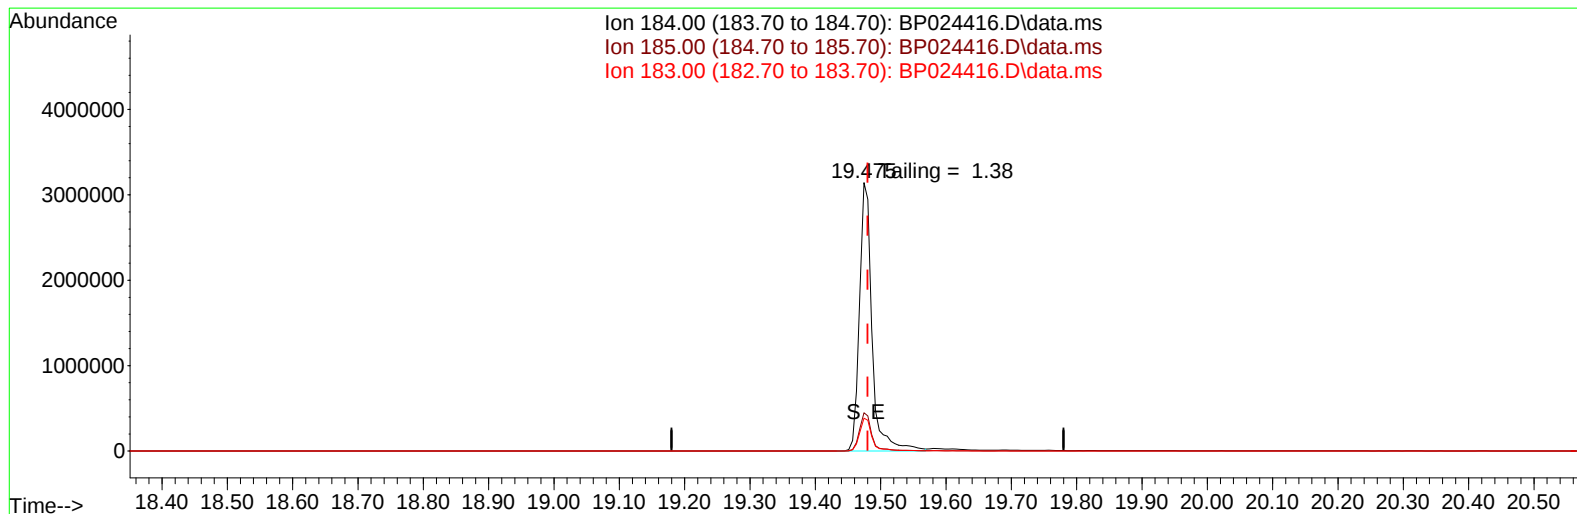

TIC: BP024416.D\data.ms

(77) Benzidine

19.475min (-0.006) 193232.04 ng

response 4225180

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.50  | 14.29  |
| 183.00 | 11.50  | 12.24  |
| 0.00   | 0.00   | 0.00   |