
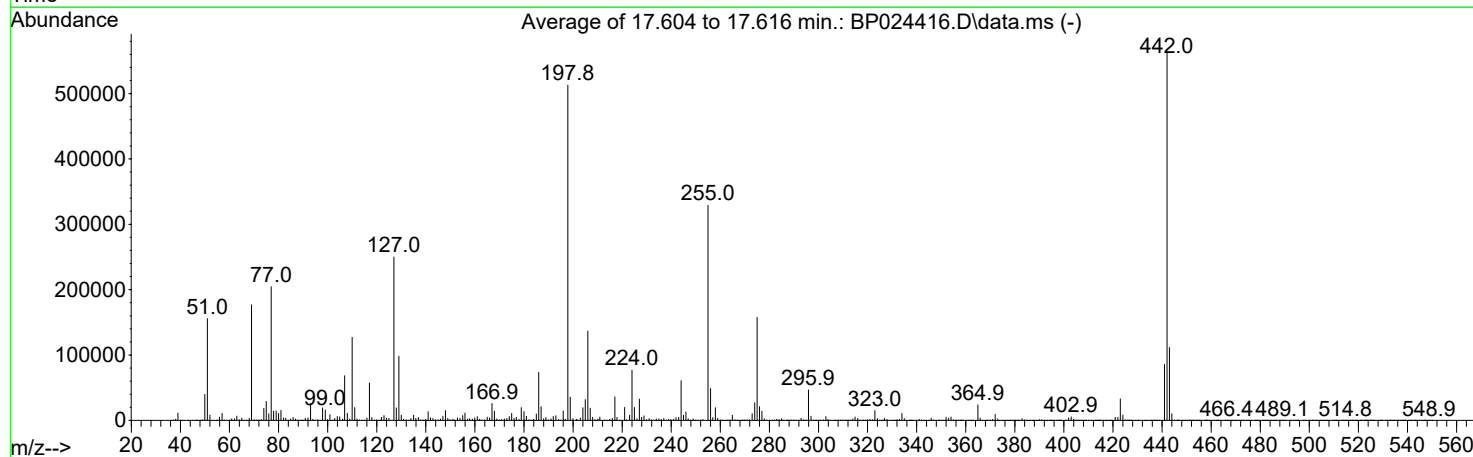


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042525\
Data File : BP024416.D
Acq On : 25 Apr 2025 10:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

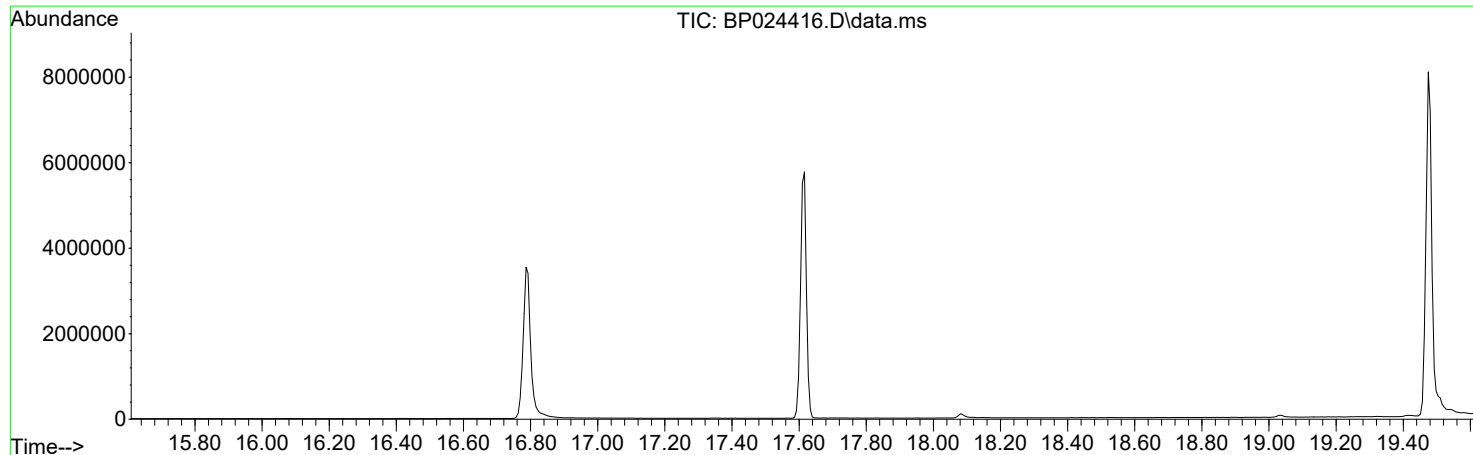

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	155804	PASS
68	69	0.00	2	1.8	3178	PASS
69	198	0.00	100	34.5	176869	PASS
70	69	0.00	2	0.5	952	PASS
127	198	10	80	48.7	249942	PASS
197	198	0.00	2	0.3	1752	PASS
198	198	100	100	100.0	512888	PASS
199	198	5	9	6.9	35434	PASS
275	198	10	60	30.7	157683	PASS
365	198	1	100	4.6	23770	PASS
441	198	0.01	100	16.7	85775	PASS
442	442	100	100	100.0	562923	PASS
443	442	15	24	19.8	111423	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/25/2025	BNA_P	<u>BP024416.D</u>
Compound Name	Response	Retention Time
DDT	1880309	20.757
DDD	37485	20.31
DDE	3427	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
40912	1921221	2.13

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042525\
Data File : BP024416.D
Acq On : 25 Apr 2025 10:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 25 11:41:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

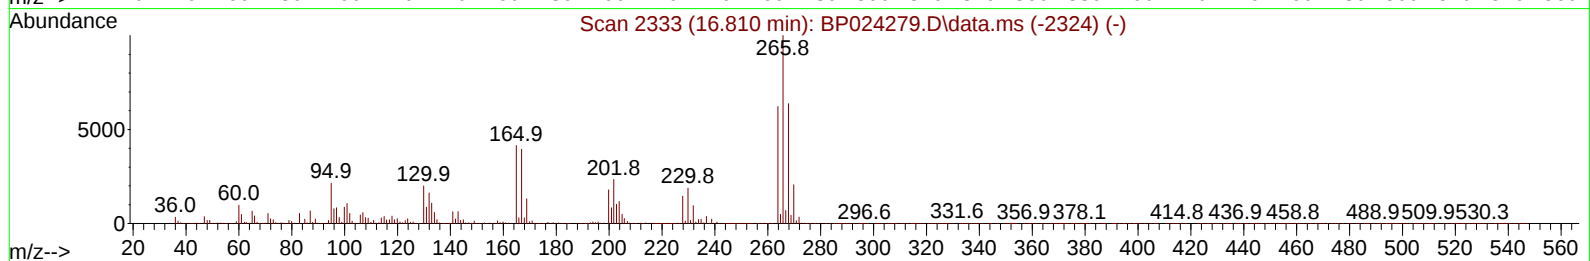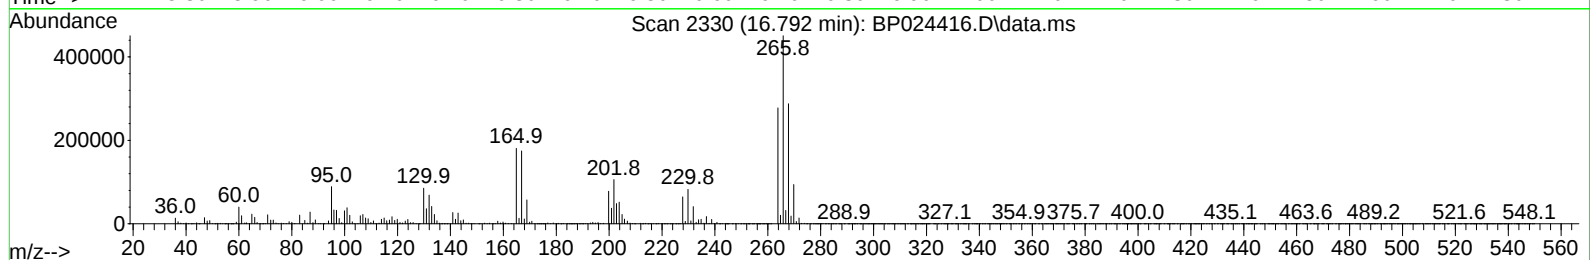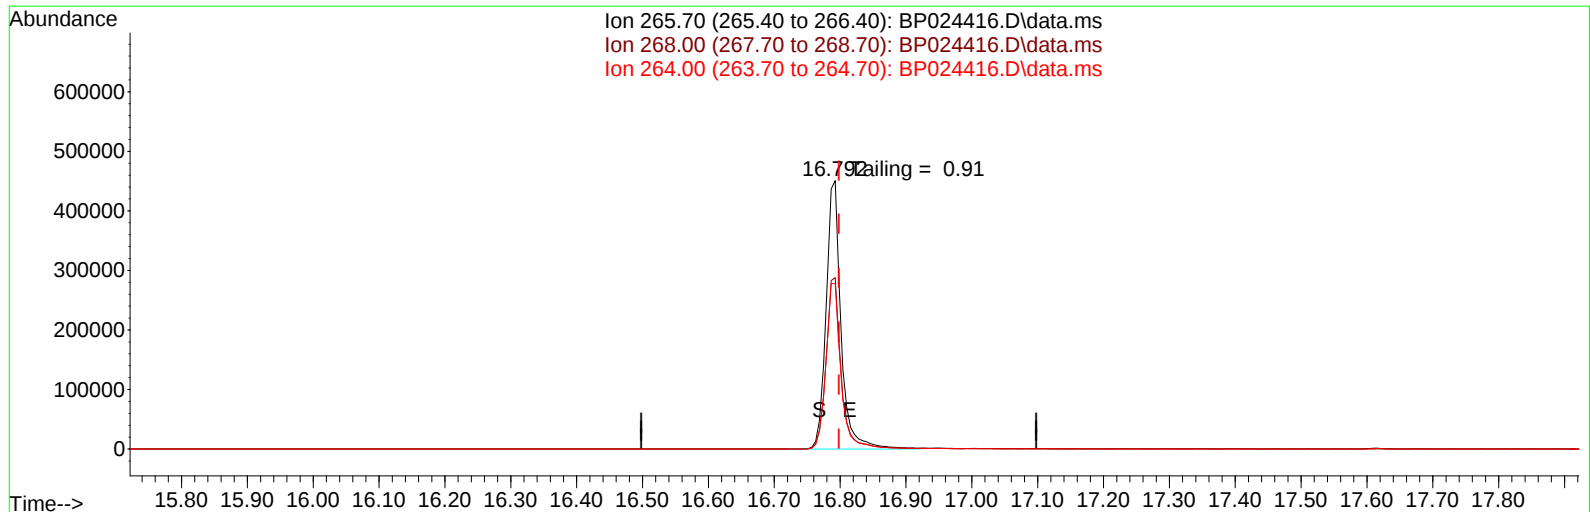

TIC: BP024416.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.006) 201028.08 ng




response 710809

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.84
264.00	62.20	61.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042525\
Data File : BP024416.D
Acq On : 25 Apr 2025 10:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 25 11:41:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

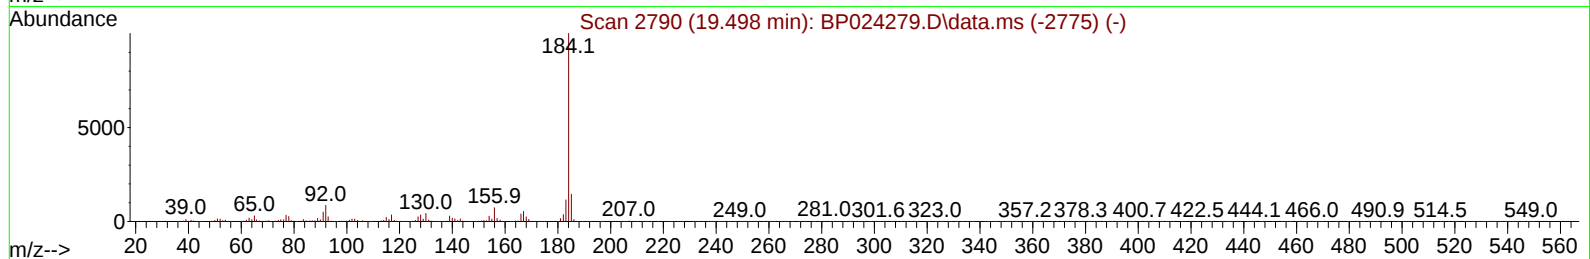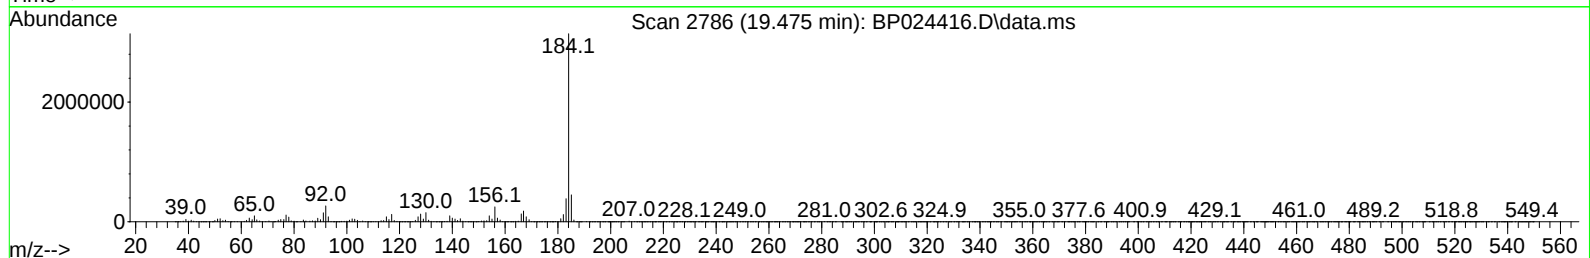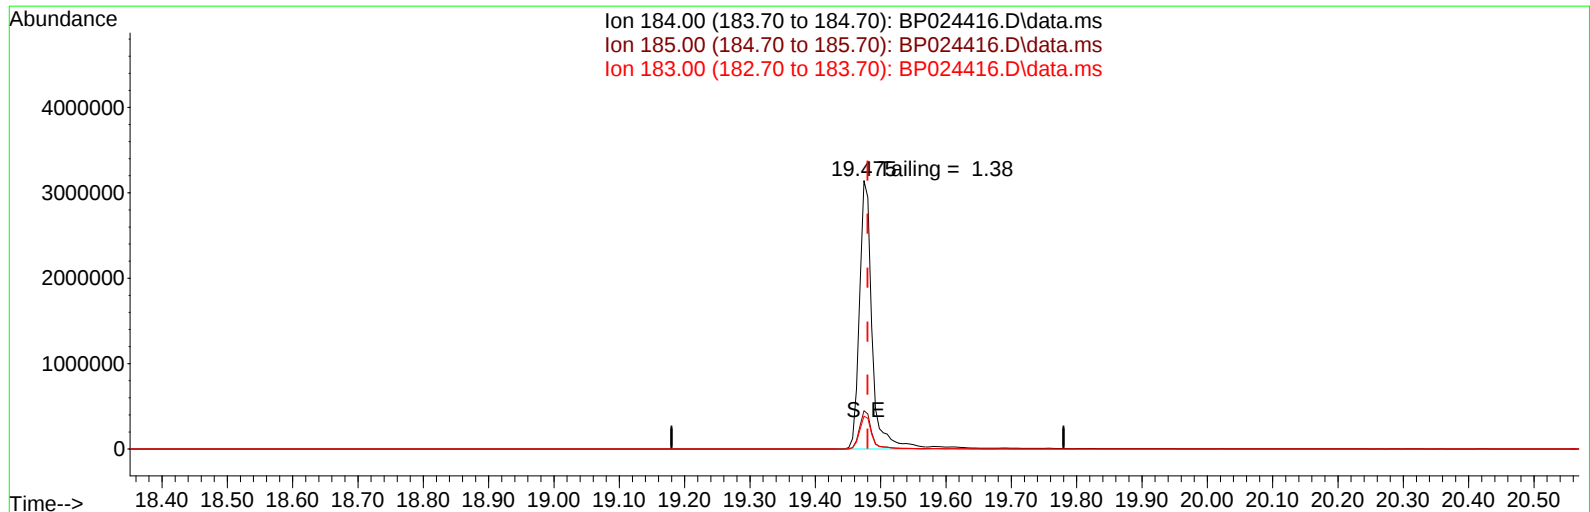

TIC: BP024416.D\data.ms

(77) Benzidine

19.475min (-0.006) 193232.04 ng

response 4225180

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.29
183.00	11.50	12.24
0.00	0.00	0.00