




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010120.D
 Acq On : 27 Apr 2022 13:17
 Operator : CG/JU
 Sample : N2470-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFH0

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:24:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
 Supervised By :Yogesh Patel 05/05/2022

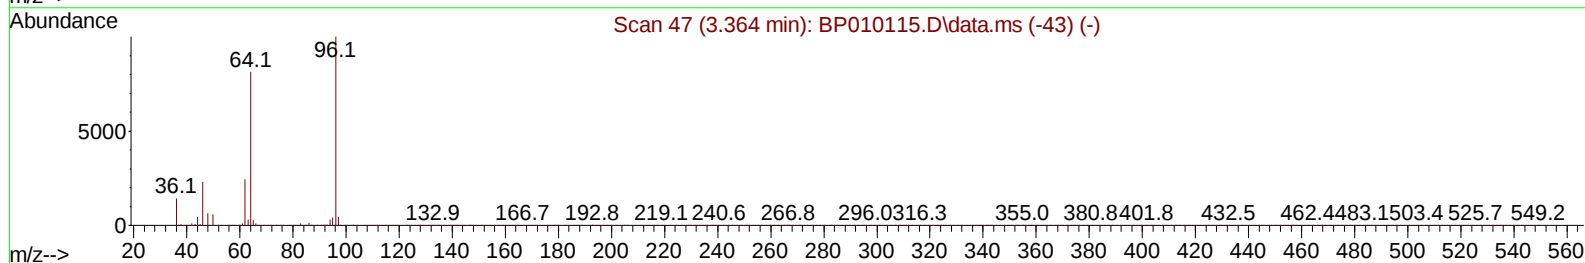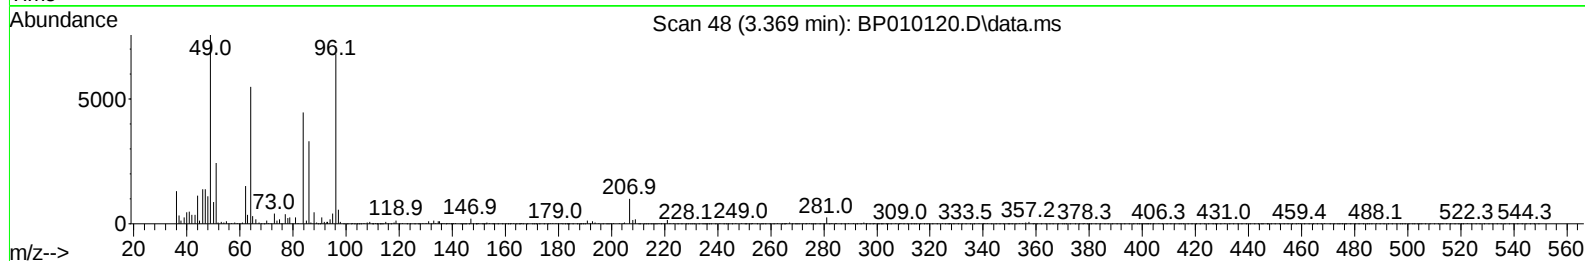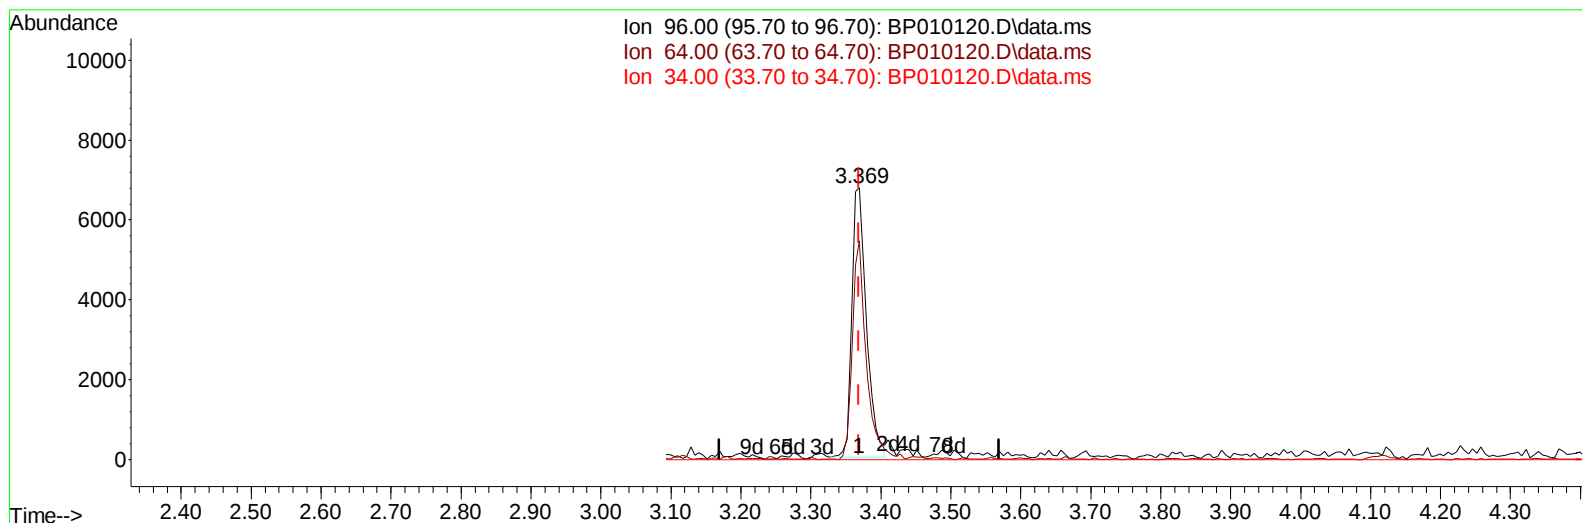

TIC: BP010120.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.369min (+ 0.000) 2.32 ng/uL

response 9723

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	80.64#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010120.D
 Acq On : 27 Apr 2022 13:17
 Operator : CG/JU
 Sample : N2470-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFH0

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:24:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
 Supervised By :Yogesh Patel 05/05/2022

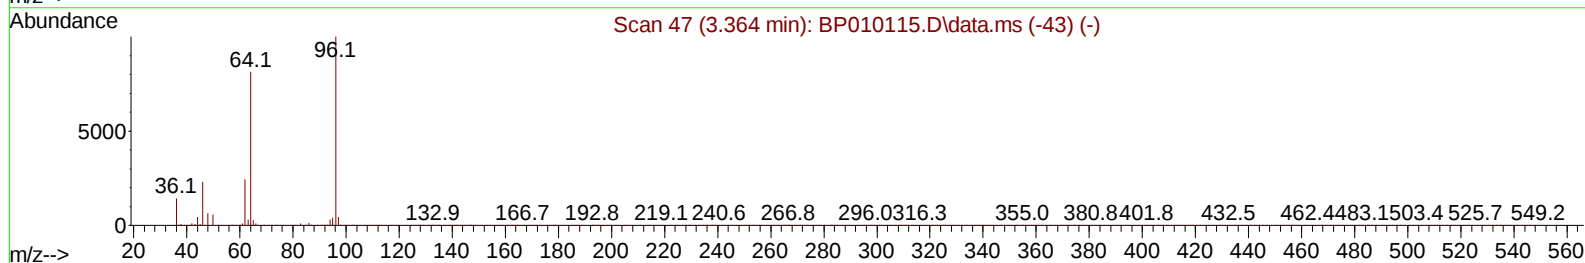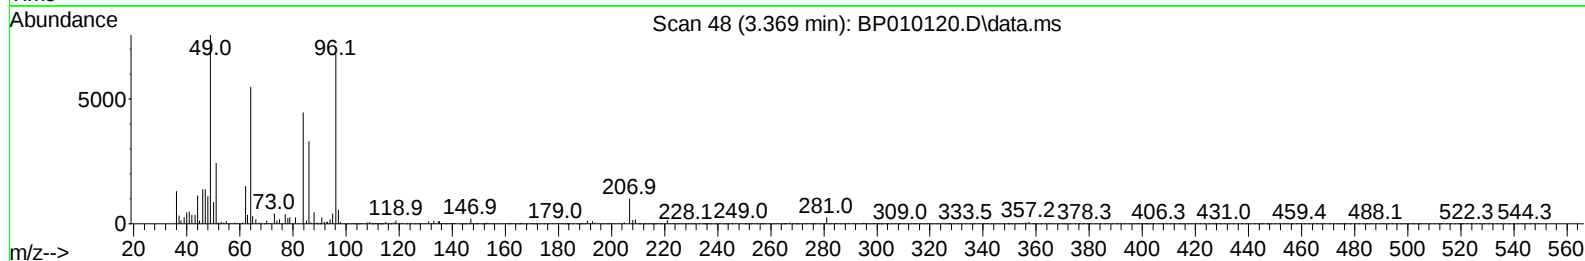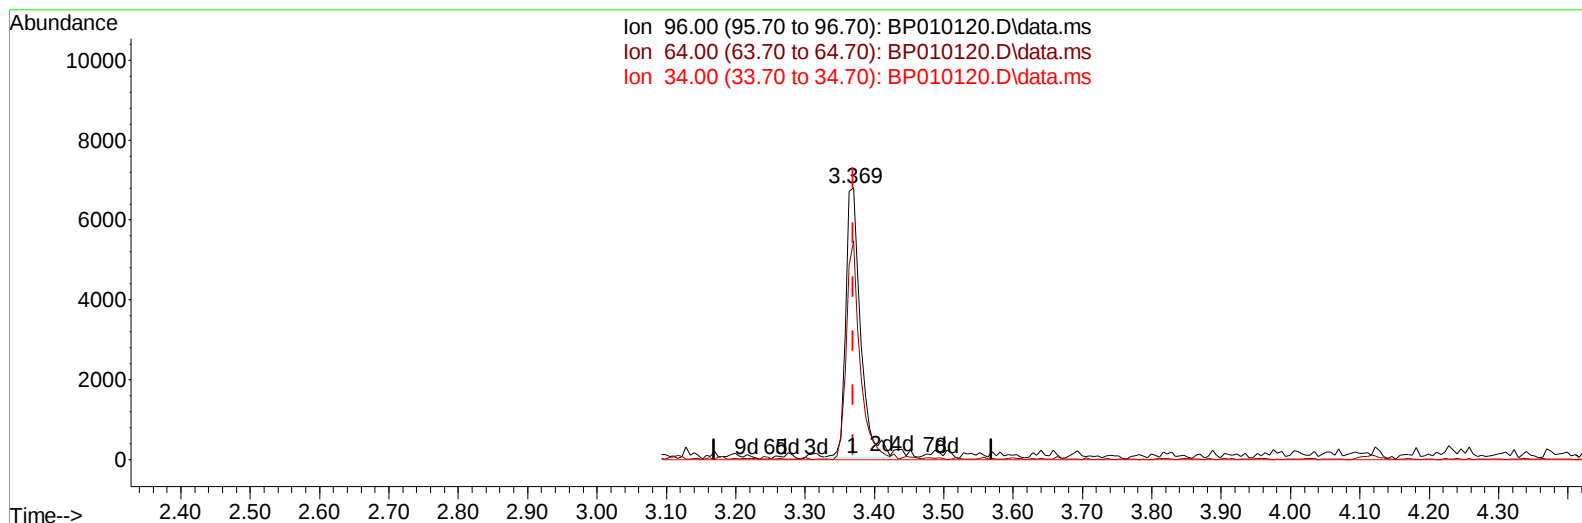

TIC: BP010120.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.369min (+ 0.000) 2.38 ng/uL m

response 10005

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	80.64#
34.00	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010120.D
Acq On : 27 Apr 2022 13:17
Operator : CG/JU
Sample : N2470-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH0

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:24:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

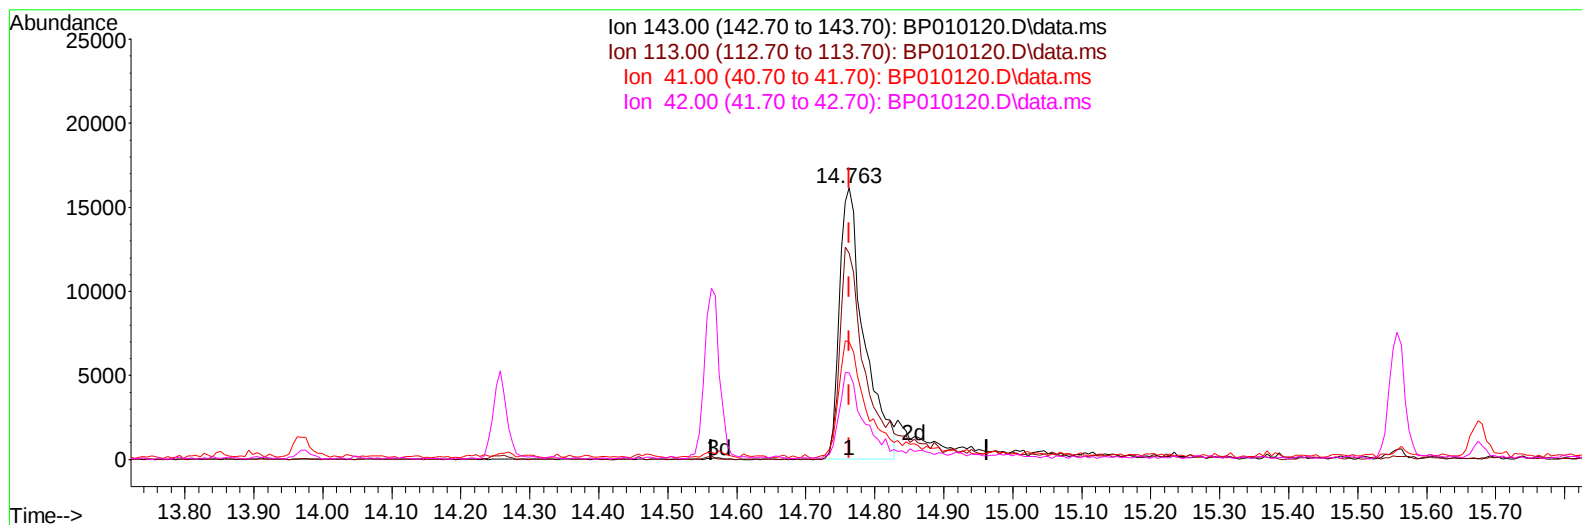

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010120.D
 Acq On : 27 Apr 2022 13:17
 Operator : CG/JU
 Sample : N2470-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFH0

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:24:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
 Supervised By :Yogesh Patel 05/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	182968	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	781268	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.563	164	516112	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.316	188	1075800	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	878600	20.000	ng/ul	# 0.00
88) Perylene-d12	23.857	264	657079	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	10005m	2.384	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.093	99	168599	10.131	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	123367	12.354	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.463	132	145312	11.790	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	148849	10.795	ng/ul	-0.01
21) Nitrobenzene-d5	9.093	128	76825	12.364	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	77900	11.479	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	134919	10.212	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	185290	9.782	ng/ul	-0.01
46) Dimethylphthalate-d6	13.969	166	547972	13.649	ng/ul	-0.01
49) Acenaphthylene-d8	14.257	160	589835	12.139	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	42919m	5.807	ng/ul	0.00
60) Fluorene-d10	15.557	176	467413	13.534	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	40969	6.023	ng/ul	0.00
73) Anthracene-d10	17.416	188	814690	15.653	ng/ul	0.00
81) Pyrene-d10	19.651	212	837880	16.769	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	343320	9.966	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010120.D
Acq On : 27 Apr 2022 13:17
Operator : CG/JU
Sample : N2470-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 28 03:24:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

