




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010121.D
 Acq On : 27 Apr 2022 13:51
 Operator : CG/JU
 Sample : N2470-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFH5

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:25:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
 Supervised By :Yogesh Patel 05/05/2022

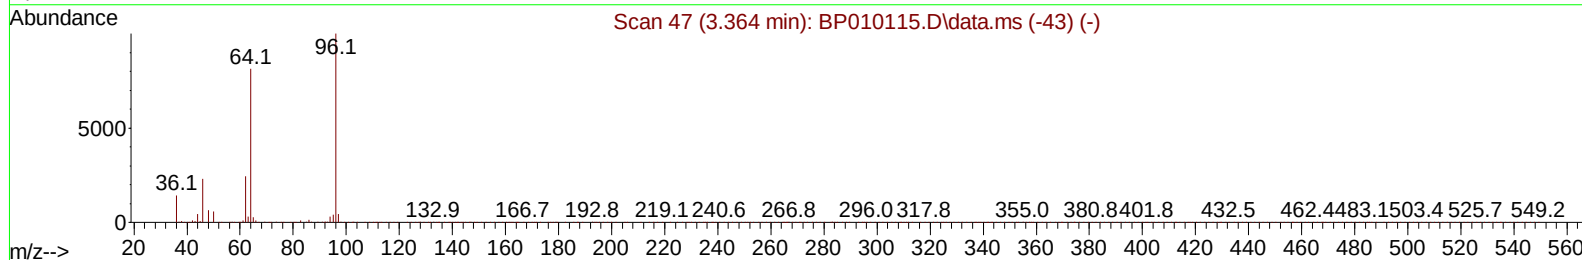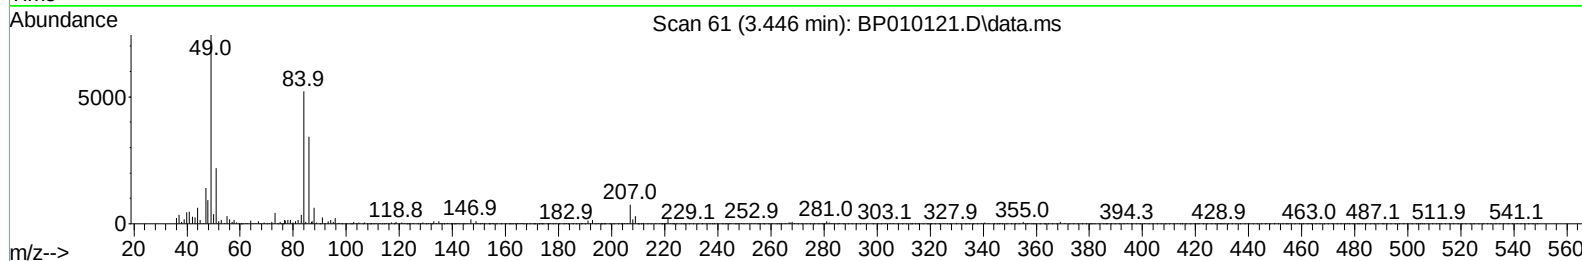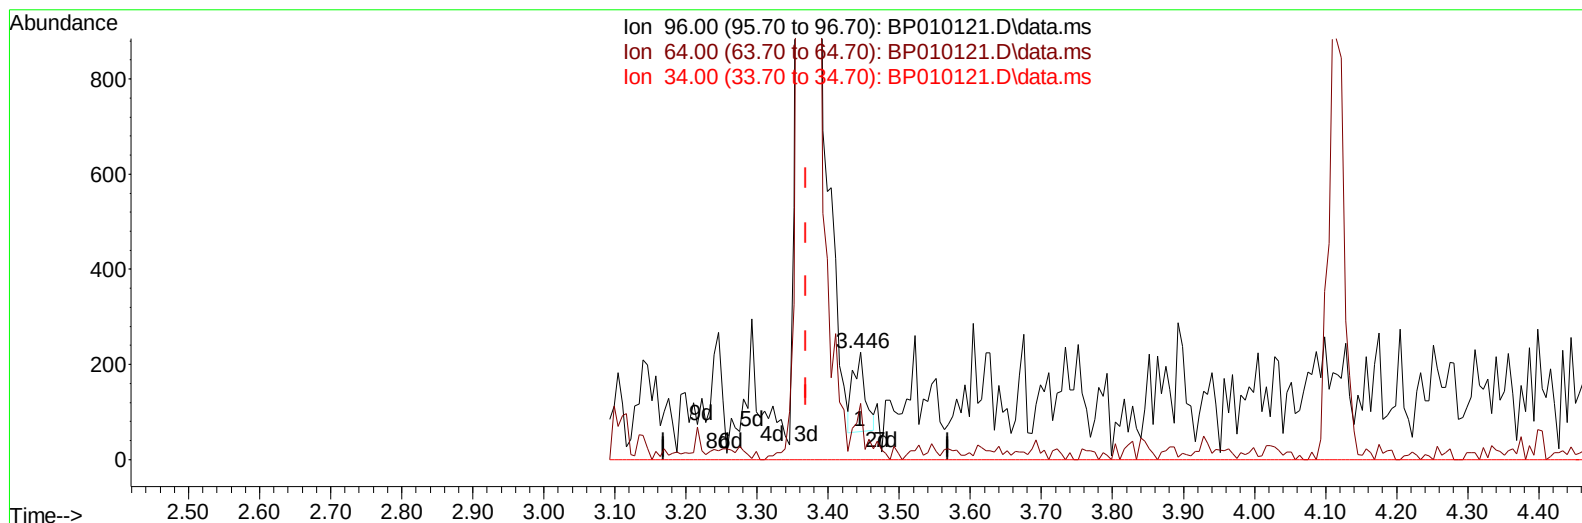

TIC: BP010121.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.446min (+ 0.077) 0.05 ng/uL

response 195

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	52.44
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010121.D
 Acq On : 27 Apr 2022 13:51
 Operator : CG/JU
 Sample : N2470-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFH5

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:25:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
 Supervised By :Yogesh Patel 05/05/2022

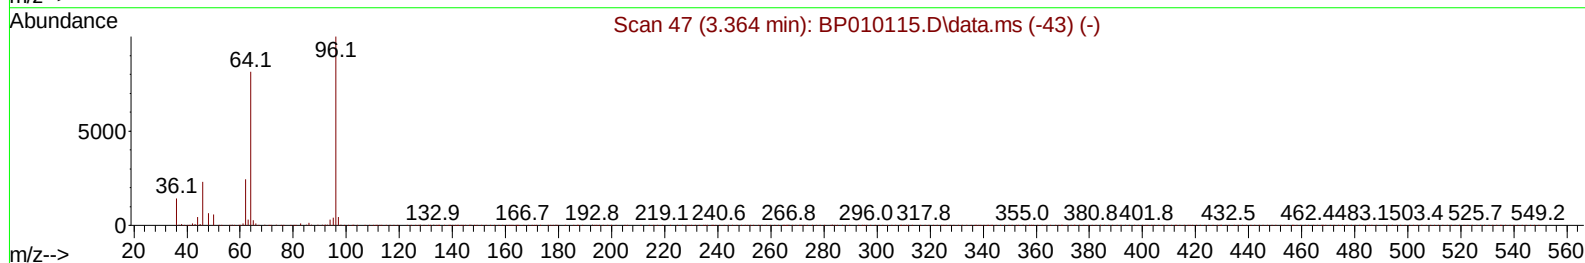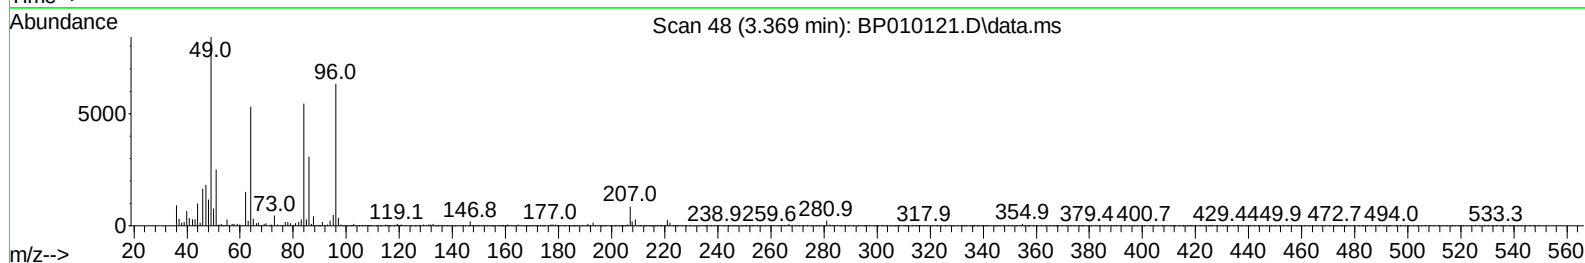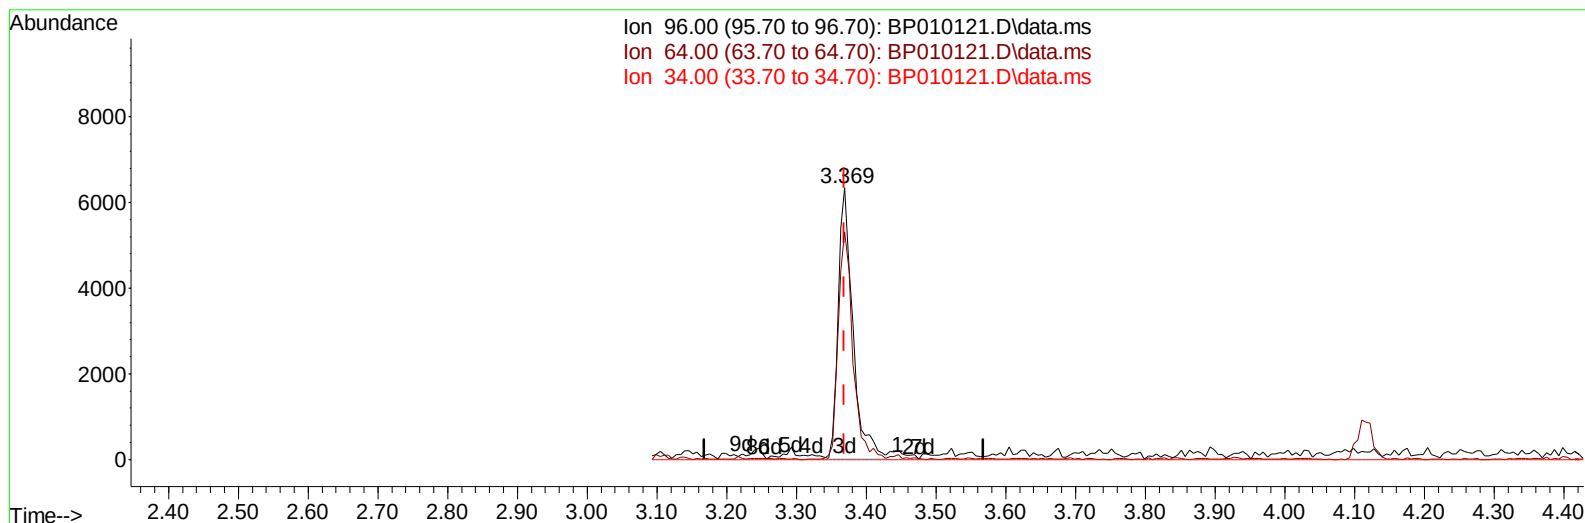

TIC: BP010121.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.369min (+ 0.000) 2.14 ng/uL m

response 9148

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	83.71#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010121.D
Acq On : 27 Apr 2022 13:51
Operator : CG/JU
Sample : N2470-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH5

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:25:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

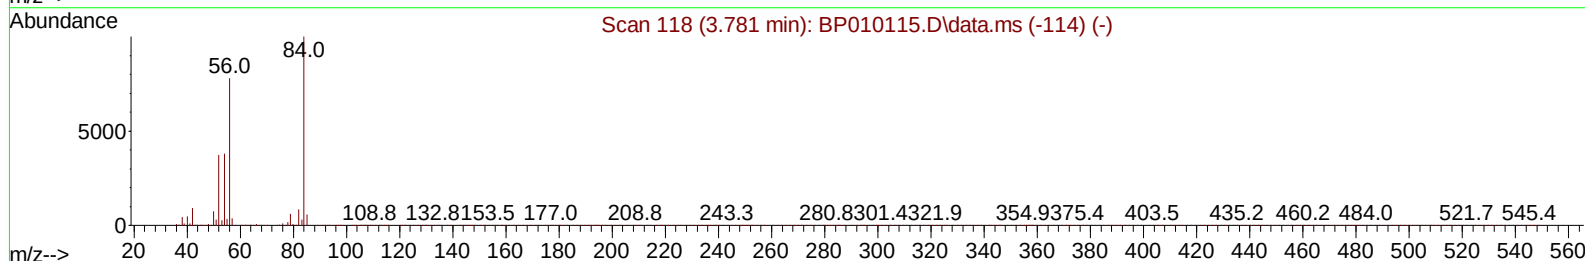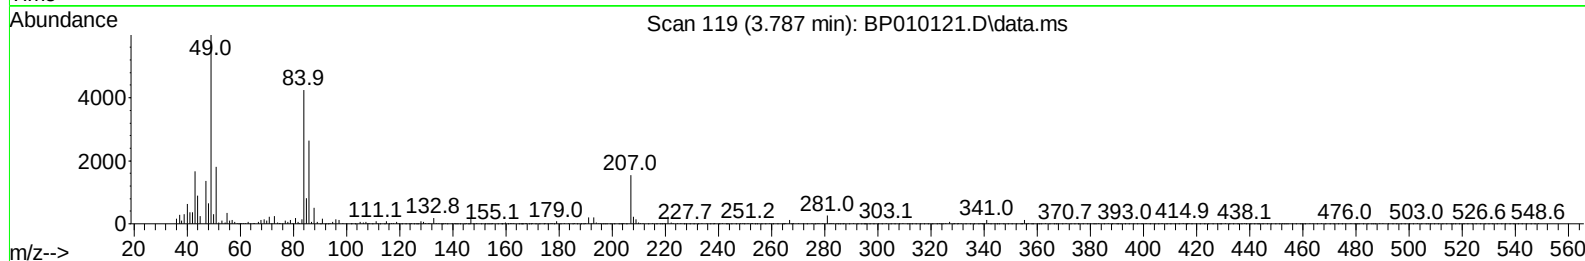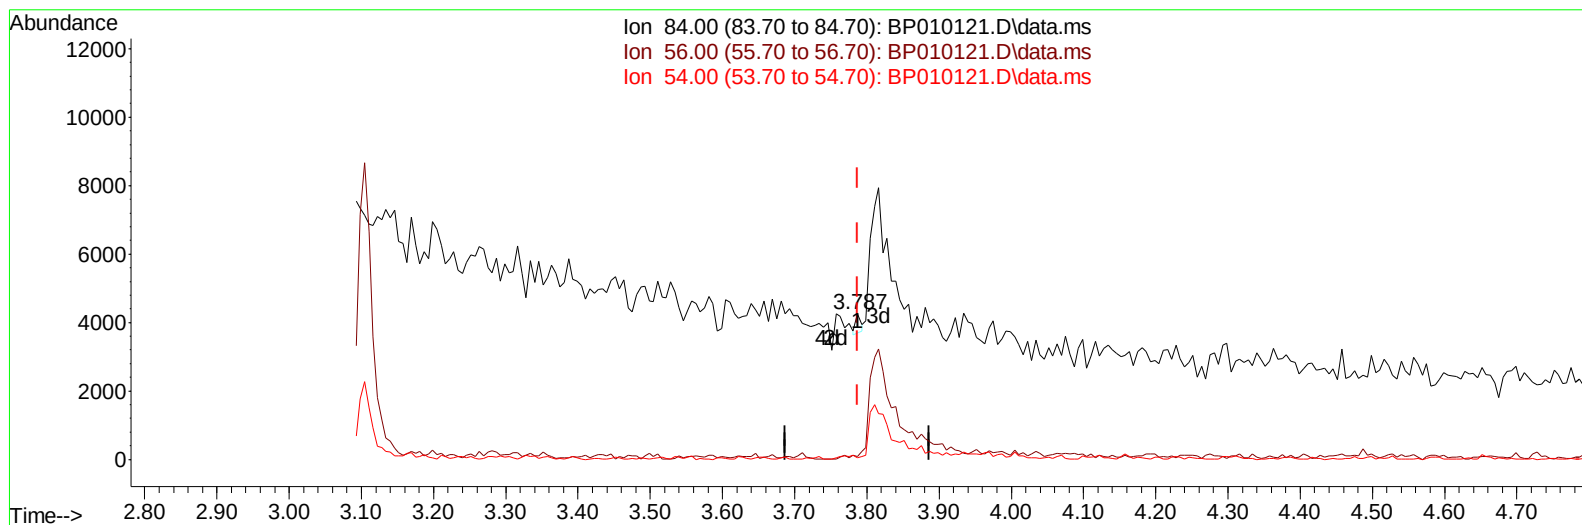

TIC: BP010121.D\data.ms

(4) Pyridine-d5 (S)

3.787min (-0.000) 0.02 ng/u1

response	281	
Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	2.24#
54.00	24.80	1.08#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010121.D
Acq On : 27 Apr 2022 13:51
Operator : CG/JU
Sample : N2470-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH5

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:25:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

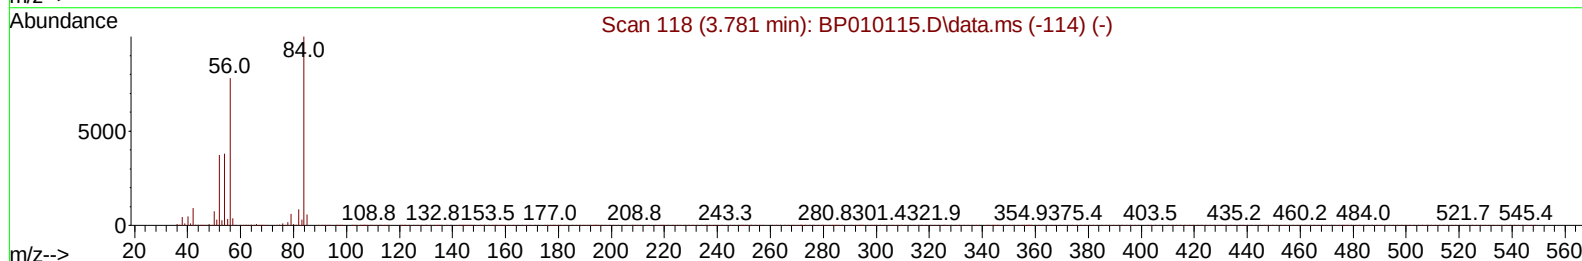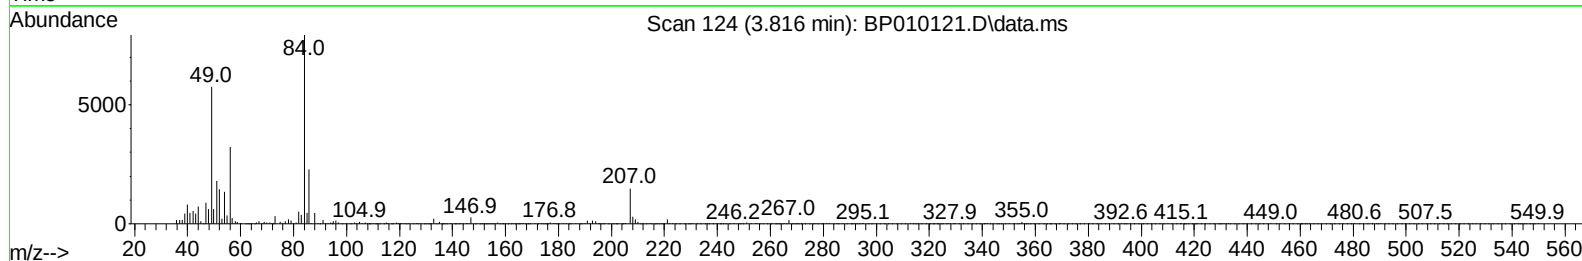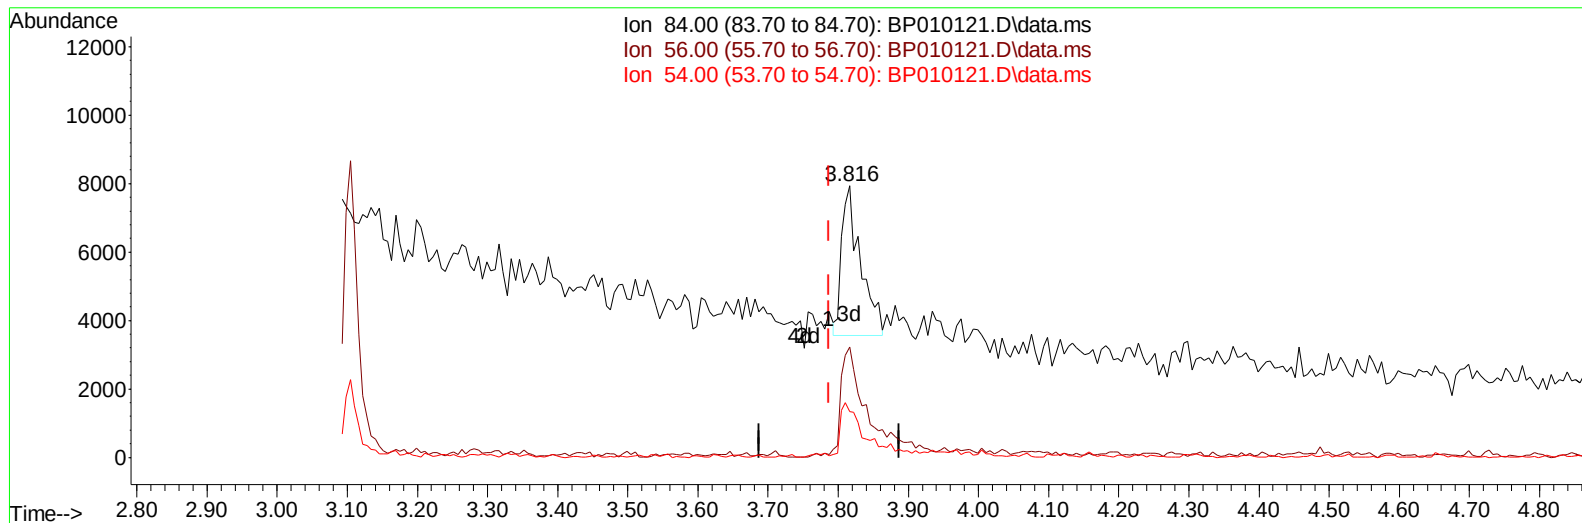

TIC: BP010121.D\data.ms

(4) Pyridine-d5 (S)

3.816min (+ 0.029) 0.68 ng/ul m

response 8189

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	40.68#
54.00	24.80	16.79#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010121.D
Acq On : 27 Apr 2022 13:51
Operator : CG/JU
Sample : N2470-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH5

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:25:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

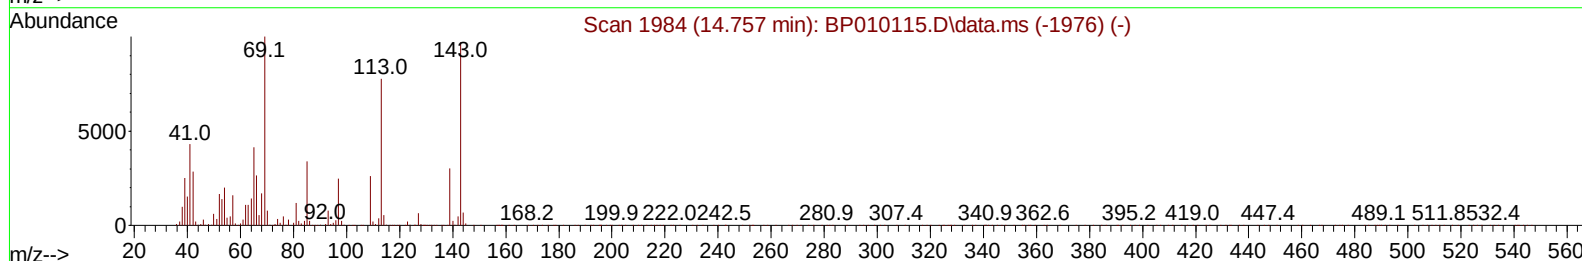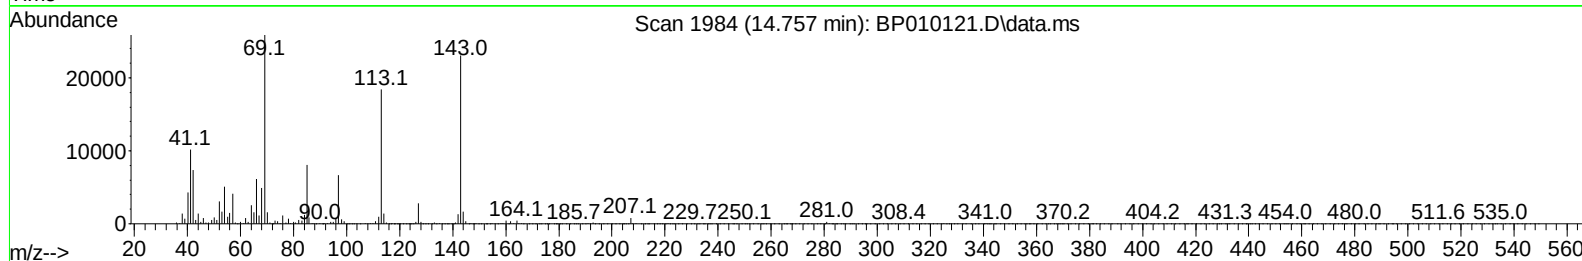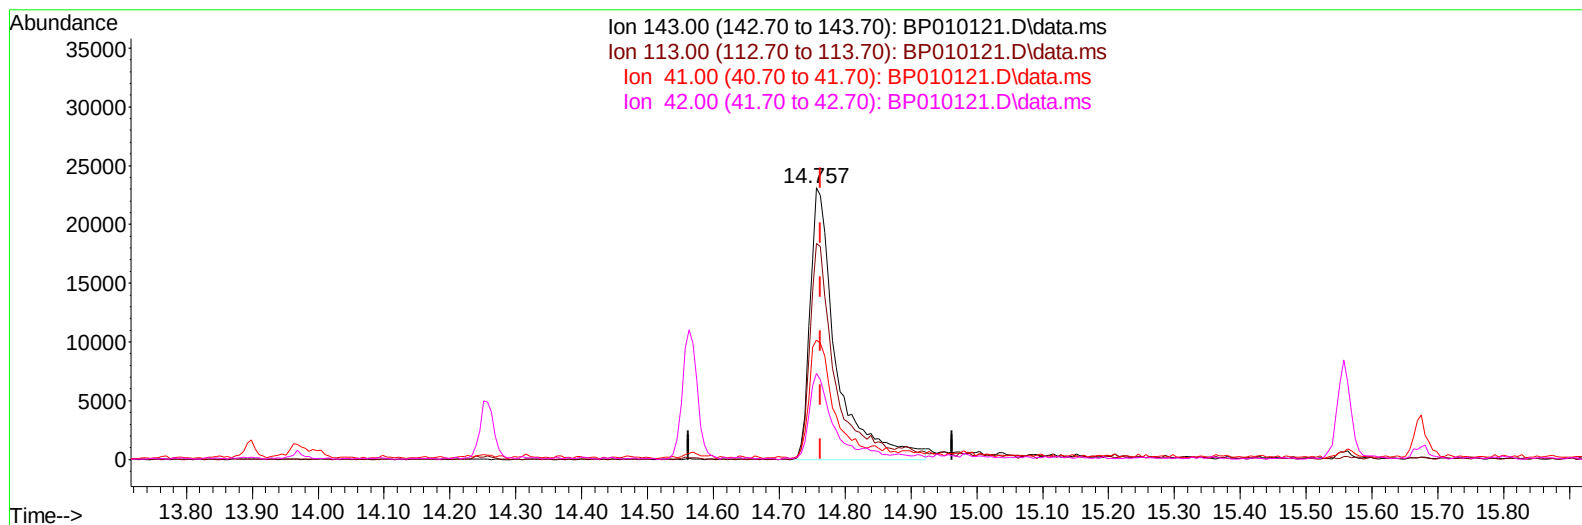

TIC: BP010121.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (-0.006) 8.35 ng/u1

response 63428

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	79.57#
41.00	23.20	43.93#
42.00	18.00	31.79#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010121.D
Acq On : 27 Apr 2022 13:51
Operator : CG/JU
Sample : N2470-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH5

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:25:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

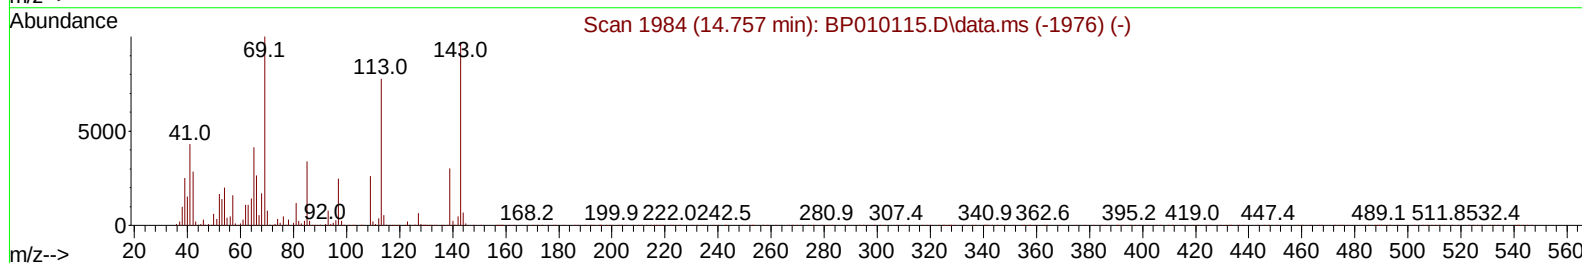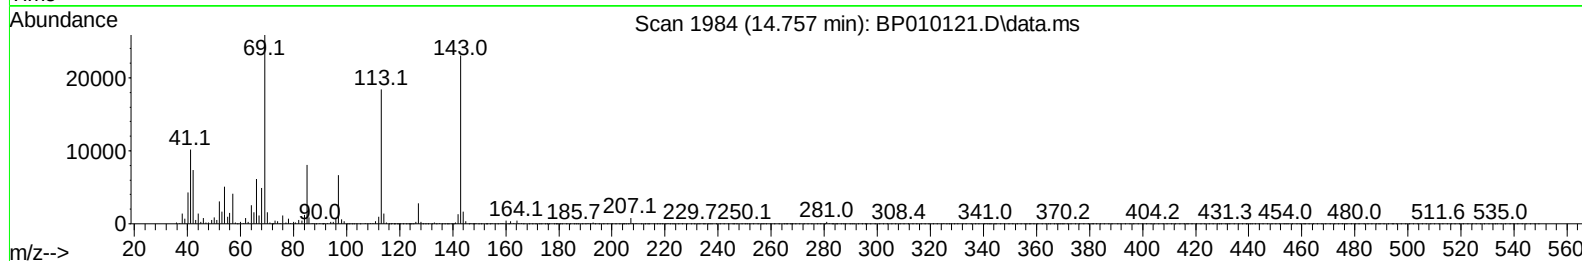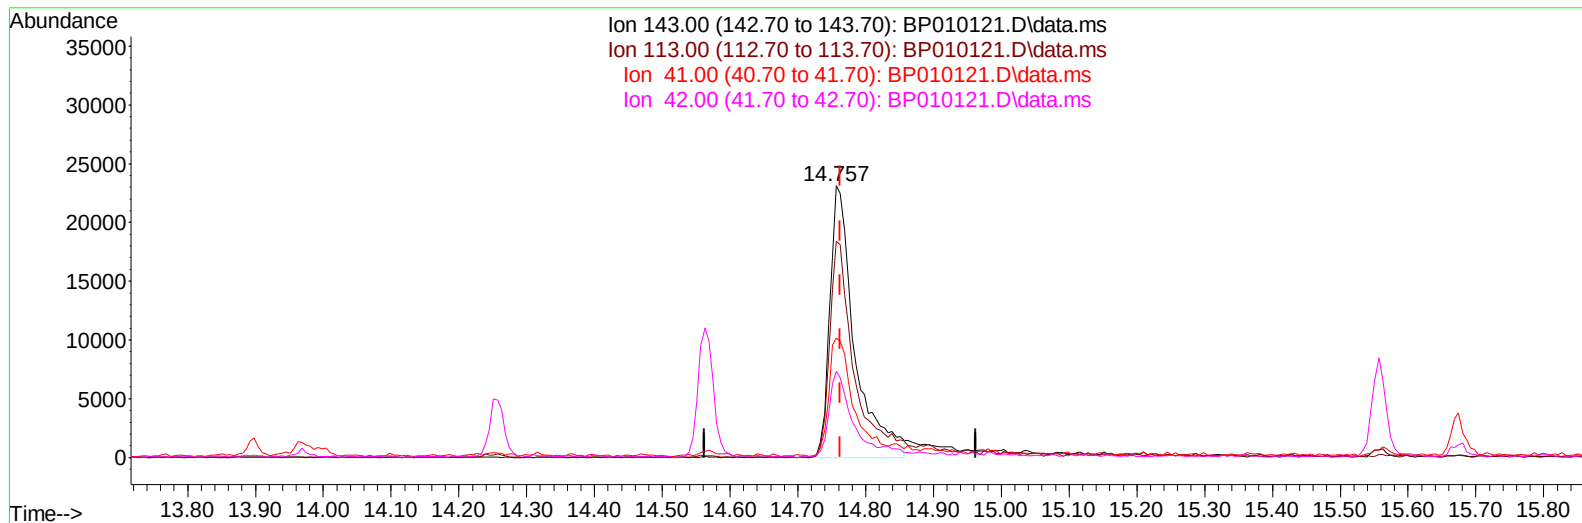

TIC: BP010121.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (-0.006) 7.80 ng/ul m

response 59225

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	79.57#
41.00	23.20	43.93#
42.00	18.00	31.79#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010121.D
 Acq On : 27 Apr 2022 13:51
 Operator : CG/JU
 Sample : N2470-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFH5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/28/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 28 03:25:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	186689	20.000	ng/ul	0.00
20) Naphthalene-d8	10.734	136	808785	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.563	164	530423	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.316	188	1096893	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	795605	20.000	ng/ul	# 0.00
88) Perylene-d12	23.856	264	604971	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	9148m	2.137	ng/uL	0.00
4) Pyridine-d5	3.816	84	8189m	0.680	ng/ul	0.03
7) Phenol-d5	7.093	99	170729	10.054	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.257	67	120661	11.842	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.463	132	143945	11.446	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	142772	10.148	ng/ul	-0.01
21) Nitrobenzene-d5	9.087	128	75011	11.661	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.816	143	78248	11.138	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	137583	10.060	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	179864	9.172	ng/ul	-0.01
46) Dimethylphthalate-d6	13.969	166	546264	13.239	ng/ul	-0.01
49) Acenaphthylene-d8	14.257	160	578713	11.589	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	59225m	7.797	ng/ul	0.00
60) Fluorene-d10	15.557	176	463840	13.069	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.674	200	53697	7.742	ng/ul	0.00
73) Anthracene-d10	17.416	188	754689	14.222	ng/ul	0.00
81) Pyrene-d10	19.645	212	712363	15.744	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.698	264	251315	7.924	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010121.D
Acq On : 27 Apr 2022 13:51
Operator : CG/JU
Sample : N2470-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 28 03:25:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

