




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010126.D
Acq On : 27 Apr 2022 19:08
Operator : CG/JU
Sample : N2542-01 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETNS5

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:26:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

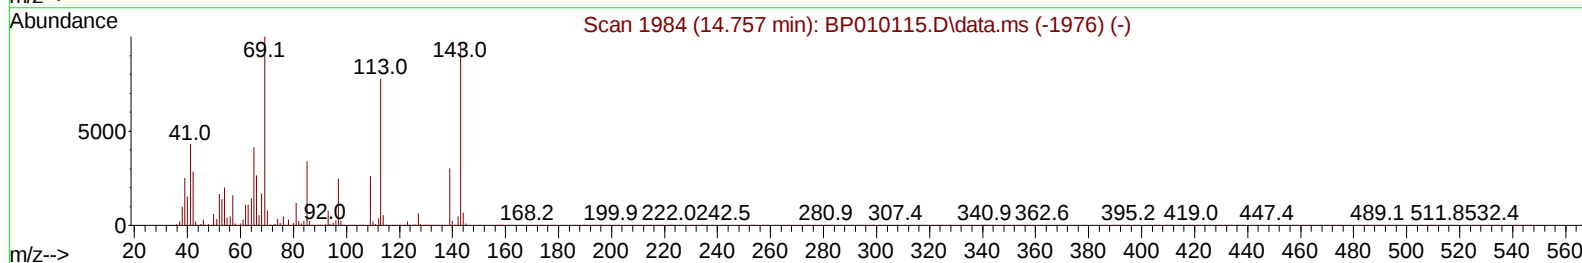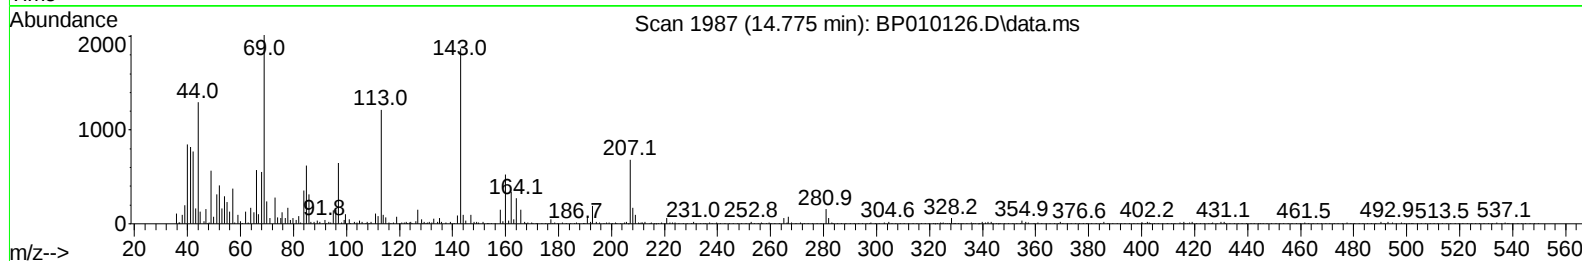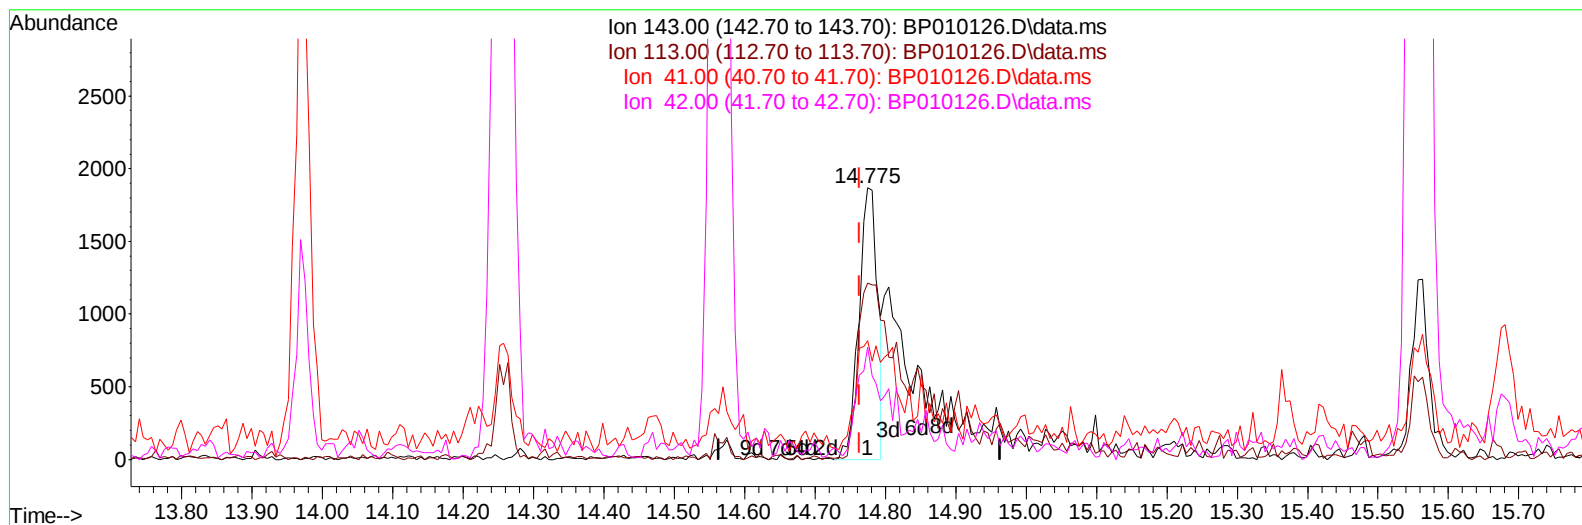

TIC: BP010126.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.775min (+ 0.012) 0.50 ng/u1

response 3424

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	65.04#
41.00	23.20	43.74#
42.00	18.00	41.27#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010126.D
 Acq On : 27 Apr 2022 19:08
 Operator : CG/JU
 Sample : N2542-01 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNS5

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:26:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
 Supervised By :Yogesh Patel 05/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	164823	20.000	ng/ul	0.00
20) Naphthalene-d8	10.734	136	711127	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.563	164	480756	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.316	188	991672	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	809743	20.000	ng/ul	# 0.00
88) Perylene-d12	23.857	264	602308	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	9083	2.403	ng/uL	0.00
4) Pyridine-d5	3.781	84	175969	16.549	ng/ul	0.00
7) Phenol-d5	7.093	99	85033	5.672	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	308718	34.317	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.463	132	268205	24.156	ng/ul	0.00
15) 4-Methylphenol-d8	8.634	113	181525	14.614	ng/ul	-0.02
21) Nitrobenzene-d5	9.093	128	199638	35.297	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	199997	32.378	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	319962	26.608	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	534083	30.975	ng/ul	-0.01
46) Dimethylphthalate-d6	13.975	166	1315555	35.178	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	1504614	33.243	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	7014m	1.019	ng/ul	0.01
60) Fluorene-d10	15.557	176	1148490	35.701	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	16336	2.605	ng/ul	0.00
73) Anthracene-d10	17.422	188	1895542	39.510	ng/ul	0.00
81) Pyrene-d10	19.651	212	2166164	47.039	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1343577	42.550	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010126.D
Acq On : 27 Apr 2022 19:08
Operator : CG/JU
Sample : N2542-01 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETNS5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 28 03:26:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

