




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010127.D
Acq On : 27 Apr 2022 19:41
Operator : CG/JU
Sample : N2542-02 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXER8

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:26:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

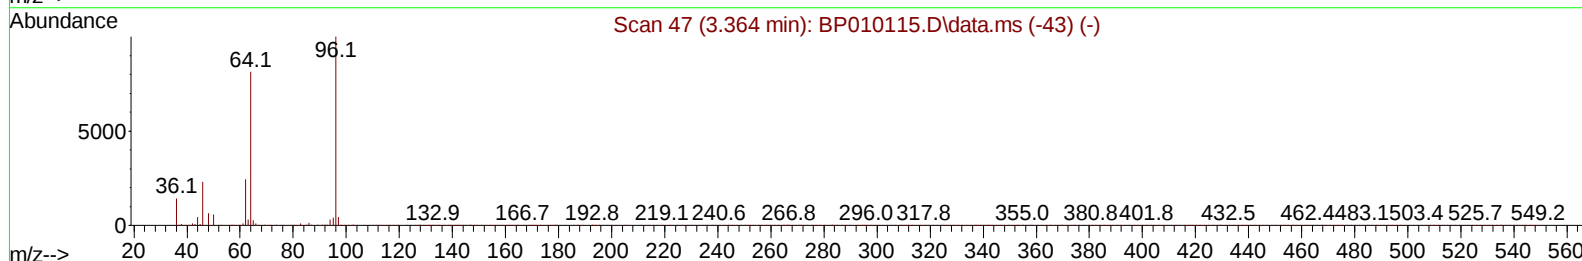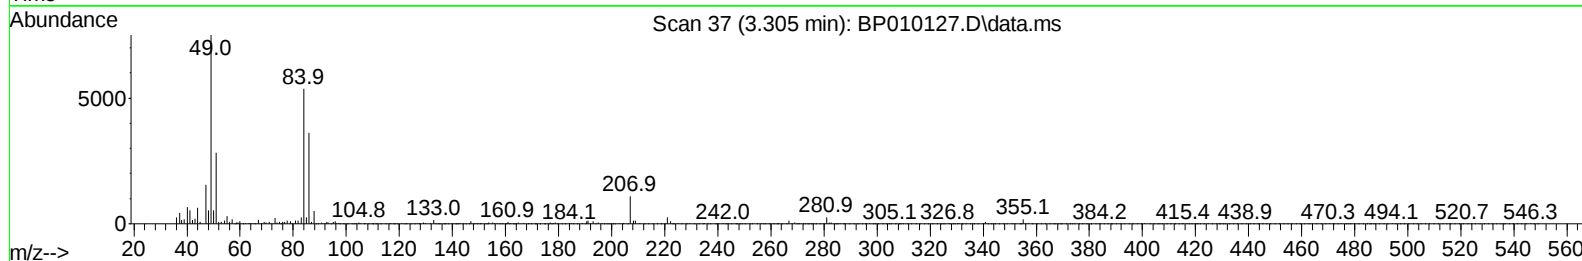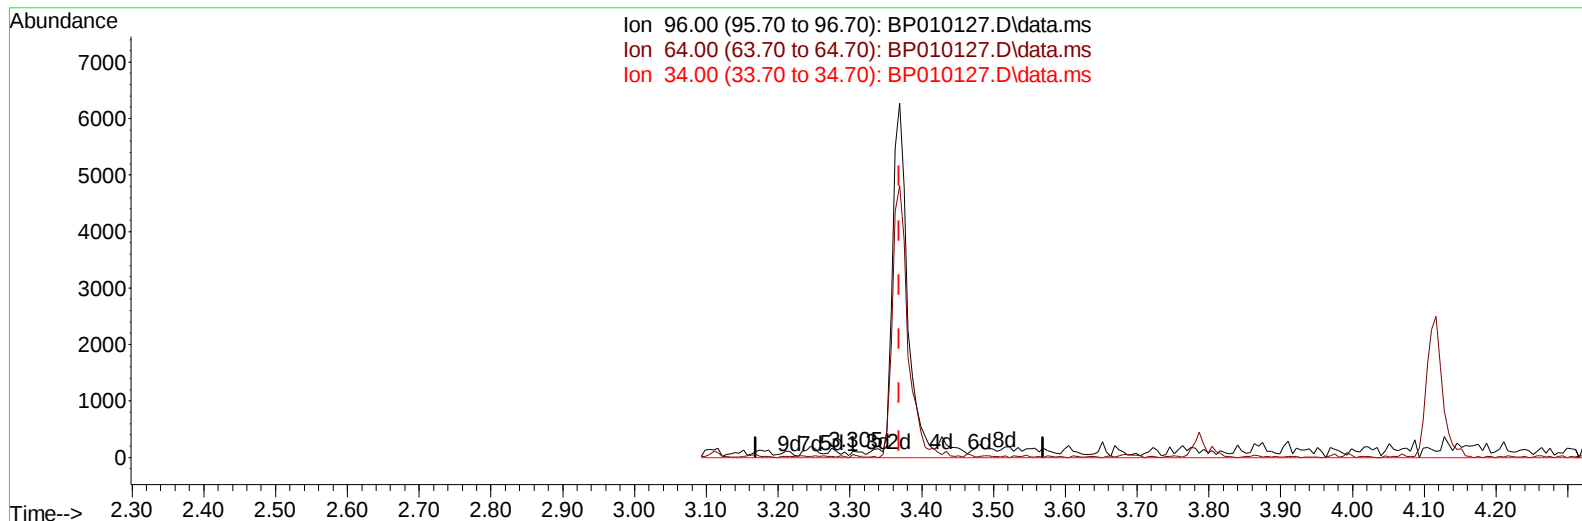

TIC: BP010127.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.305min (-0.065) 0.02 ng/uL

response 79

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	54.81
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010127.D
 Acq On : 27 Apr 2022 19:41
 Operator : CG/JU
 Sample : N2542-02 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXER8

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:26:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
 Supervised By :Yogesh Patel 05/05/2022

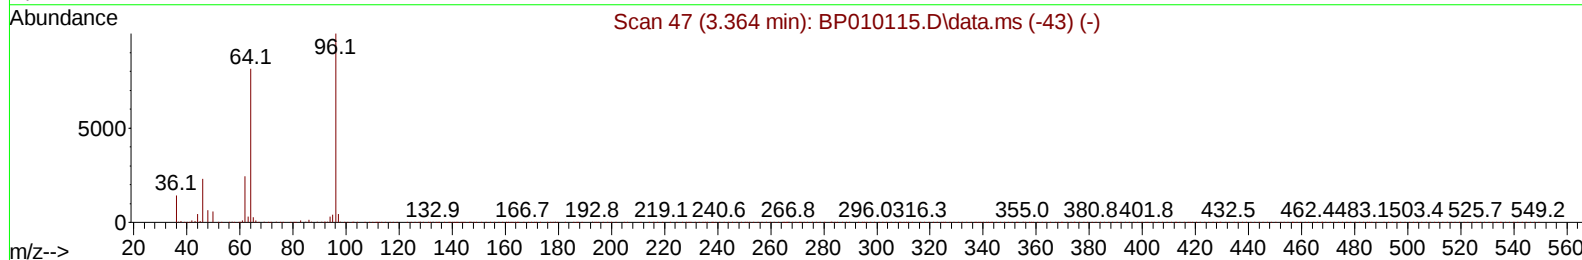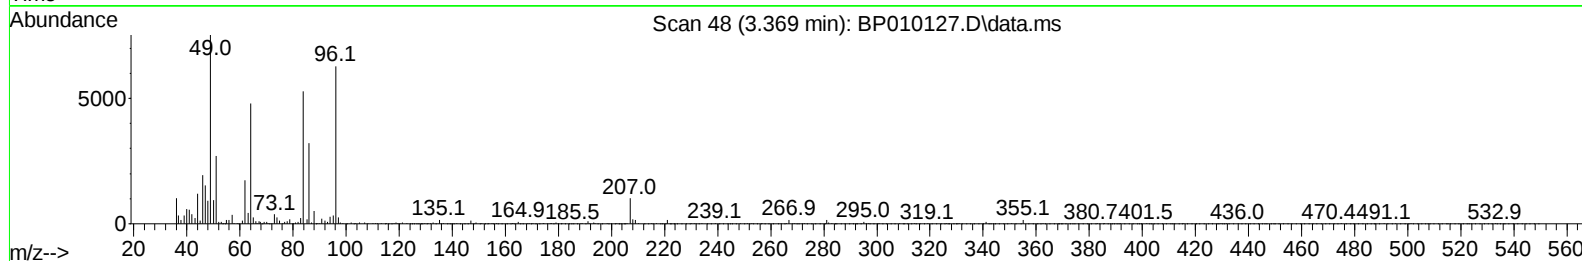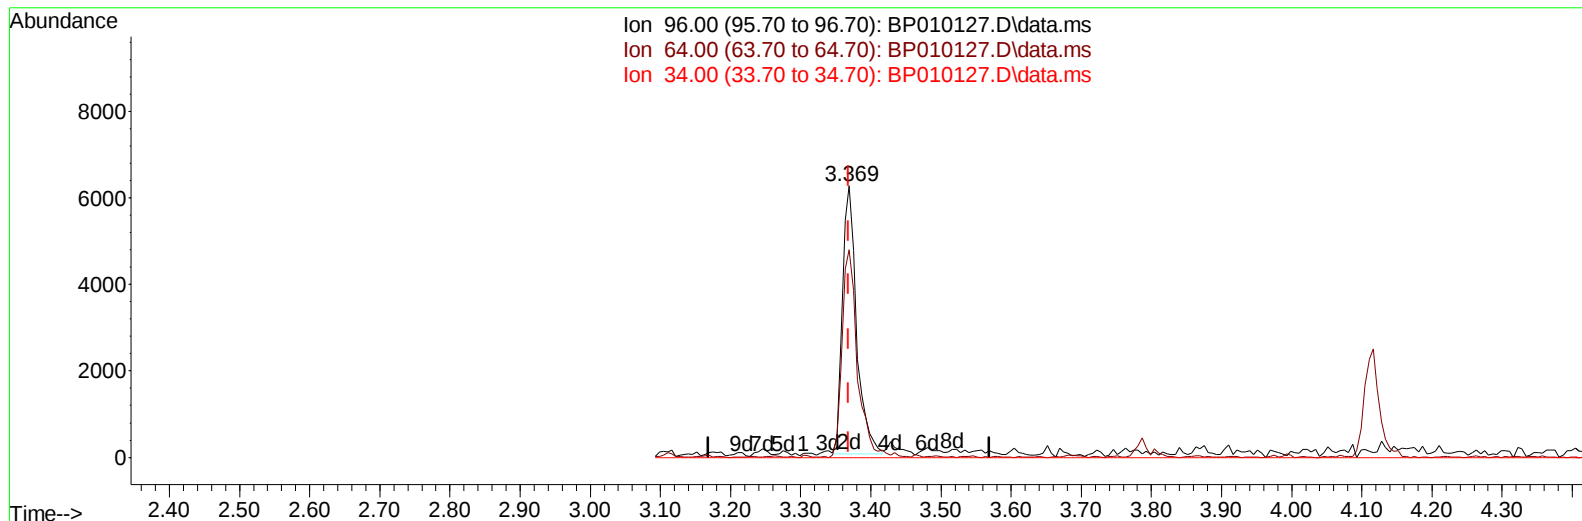

TIC: BP010127.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.369min (+ 0.000) 2.30 ng/uL m

response 8647

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	76.59#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010127.D
Acq On : 27 Apr 2022 19:41
Operator : CG/JU
Sample : N2542-02 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXER8

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:26:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

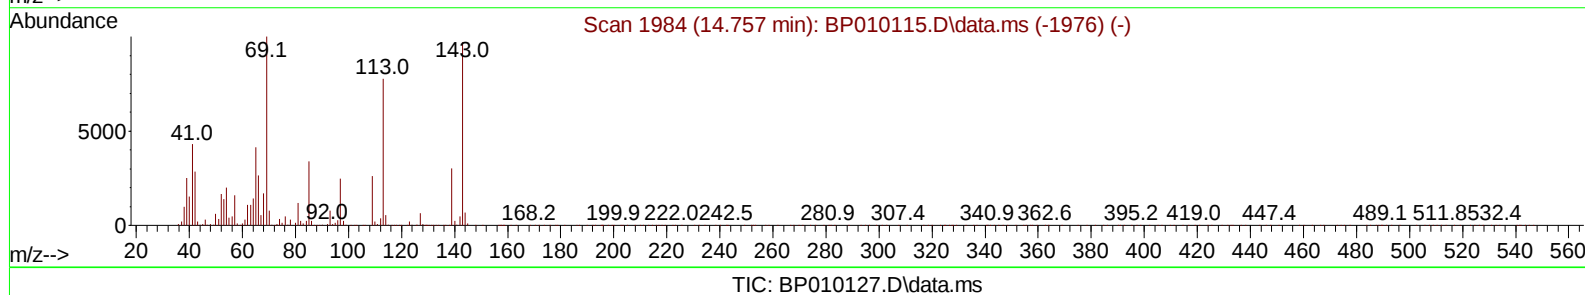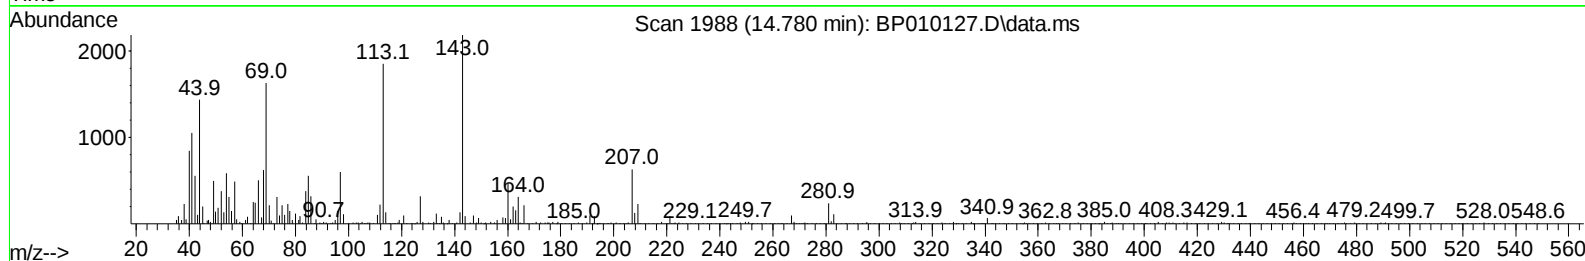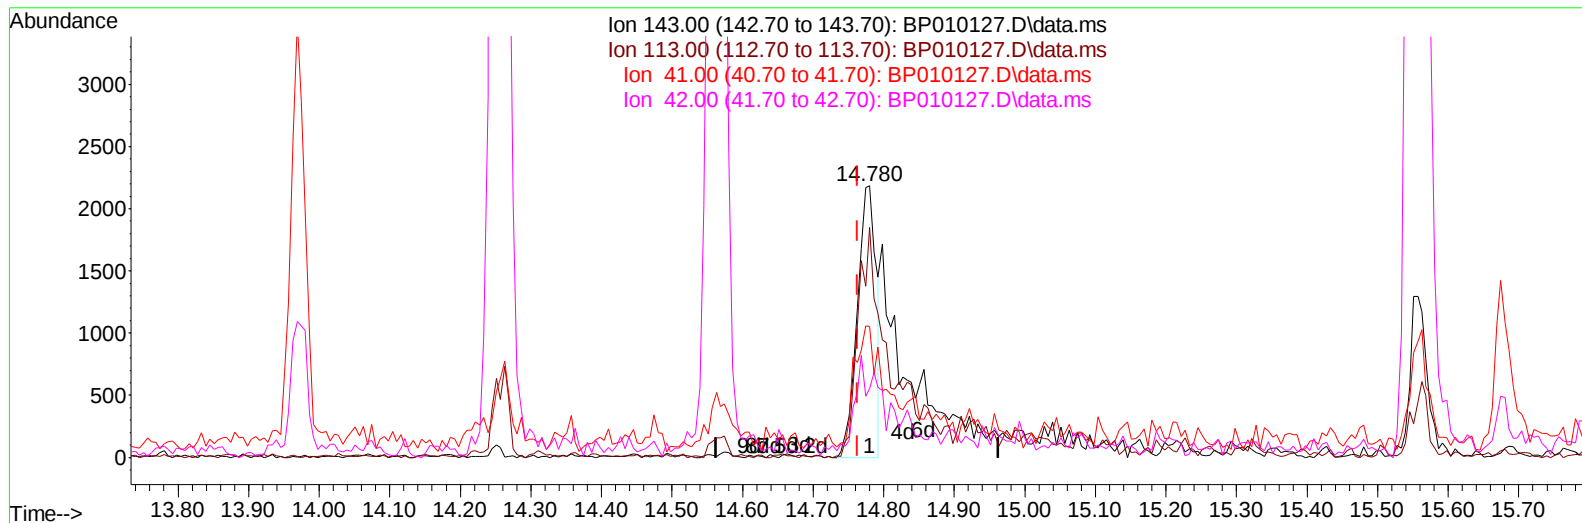

(54) 4-Nitrophenol-d4 (S)

14.780min (+ 0.017) 0.59 ng/u1

response 4077

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	84.88#
41.00	23.20	48.14#
42.00	18.00	25.47#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010127.D
Acq On : 27 Apr 2022 19:41
Operator : CG/JU
Sample : N2542-02 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXER8

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:26:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

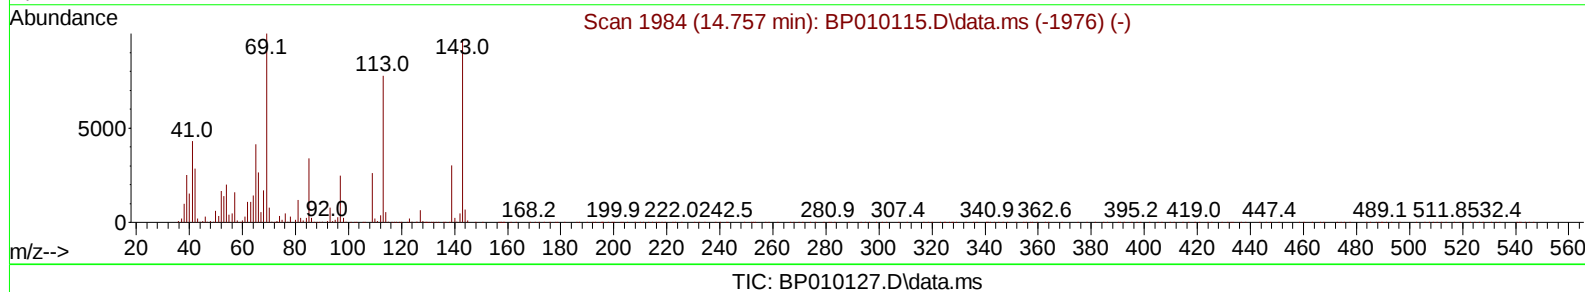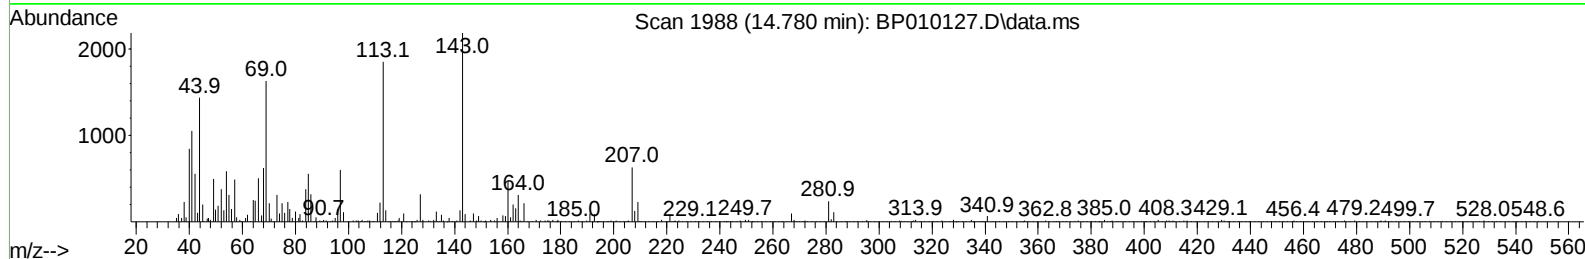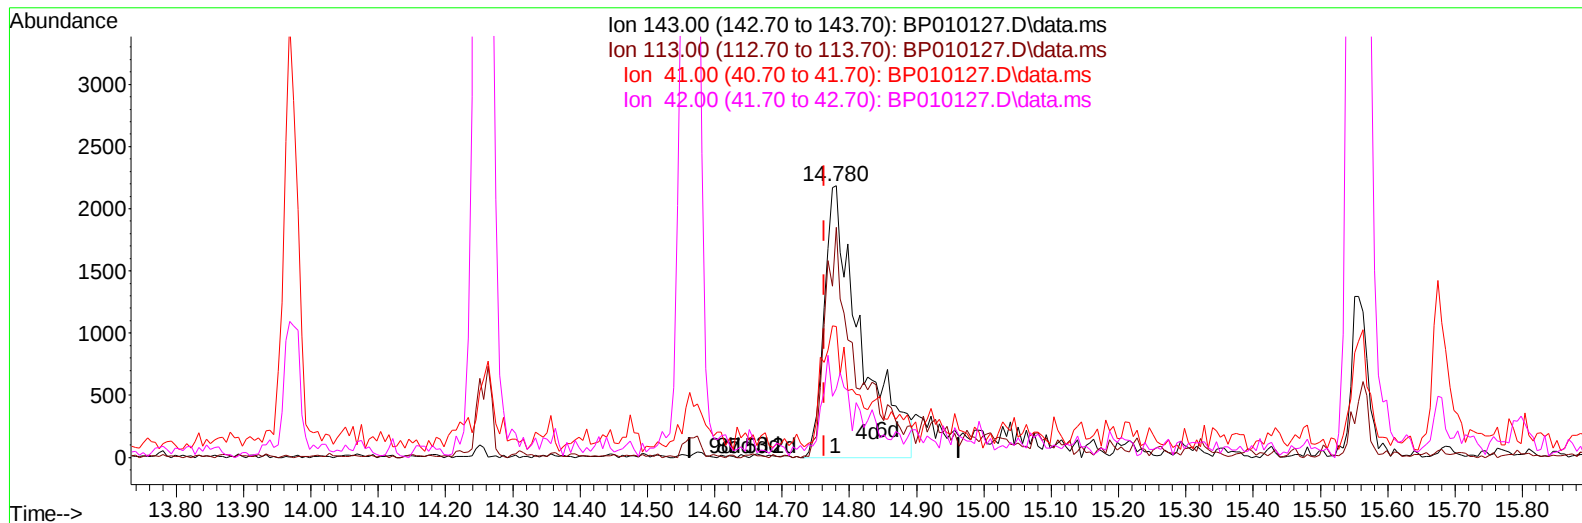

(54) 4-Nitrophenol-d4 (S)

14.780min (+ 0.017) 1.18 ng/ul m

response 8133

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	84.88#
41.00	23.20	48.14#
42.00	18.00	25.47#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010127.D
 Acq On : 27 Apr 2022 19:41
 Operator : CG/JU
 Sample : N2542-02 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXER8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/28/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 28 03:26:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	164184	20.000	ng/ul	0.00
20) Naphthalene-d8	10.734	136	708154	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.563	164	482326	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.316	188	985066	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	812938	20.000	ng/ul	# 0.00
88) Perylene-d12	23.856	264	600395	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	8647m	2.297	ng/uL	0.00
4) Pyridine-d5	3.781	84	179779	16.973	ng/ul	0.00
7) Phenol-d5	7.093	99	86007	5.759	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.257	67	310264	34.624	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.463	132	266803	24.123	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	183639	14.842	ng/ul	-0.01
21) Nitrobenzene-d5	9.092	128	200151	35.536	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	195081	31.714	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	314452	26.259	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	542716	31.608	ng/ul	-0.01
46) Dimethylphthalate-d6	13.969	166	1359243	36.228	ng/ul	-0.01
49) Acenaphthylene-d8	14.257	160	1540651	33.928	ng/ul	0.00
54) 4-Nitrophenol-d4	14.780	143	8133m	1.177	ng/ul	0.02
60) Fluorene-d10	15.557	176	1189844	36.866	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	18252	2.930	ng/ul	0.00
73) Anthracene-d10	17.416	188	1954883	41.020	ng/ul	0.00
81) Pyrene-d10	19.651	212	2222390	48.070	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1373808	43.646	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010127.D
Acq On : 27 Apr 2022 19:41
Operator : CG/JU
Sample : N2542-02 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXER8

Manual IntegrationsAPPROVED

Quant Time: Apr 28 03:26:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/28/2022
Supervised By :Yogesh Patel 05/05/2022

