

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010116.D
 Acq On : 27 Apr 2022 11:03
 Operator : CG/JU
 Sample : PB144346BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK346

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	43	47	55	rBV	40344	58786	1.34%	0.138%
2	3.781	114	118	137	rBV	446891	747871	17.06%	1.758%
3	4.117	170	175	180	rBV2	12373	17047	0.39%	0.040%
4	7.093	674	681	693	rBV	606609	1001673	22.85%	2.355%
5	7.258	703	709	719	rBV	535805	831901	18.98%	1.956%
6	7.464	737	744	756	rBV	657111	1050365	23.96%	2.469%
7	7.934	817	824	836	rVB	573677	948088	21.63%	2.229%
8	8.634	934	943	959	rBV	765036	1340017	30.57%	3.150%
9	9.087	1012	1020	1034	rBV	650053	1108026	25.28%	2.605%
10	9.816	1132	1144	1160	rBV	522812	936111	21.35%	2.201%
11	10.358	1228	1236	1254	rBV	731623	1338022	30.52%	3.146%
12	10.734	1293	1300	1312	rBV	805467	1419607	32.38%	3.337%
13	10.869	1315	1323	1345	rBV	738034	1410705	32.18%	3.317%
14	12.334	1565	1572	1576	rBV4	12003	23660	0.54%	0.056%
15	13.540	1771	1777	1782	rVB8	2877	5411	0.12%	0.013%
16	13.969	1843	1850	1864	rBV	1648828	2382125	54.34%	5.600%
17	14.257	1892	1899	1914	rBV	1722992	2572440	58.68%	6.048%
18	14.563	1944	1951	1967	rBV	1377485	2035863	46.44%	4.786%
19	14.757	1976	1984	2010	rBV	438850	967104	22.06%	2.274%
20	15.557	2113	2120	2133	rBV	2271987	3363478	76.73%	7.907%
21	15.675	2134	2140	2156	rVV	692802	1049368	23.94%	2.467%
22	15.798	2156	2161	2167	rVB	28147	45882	1.05%	0.108%
23	16.345	2248	2254	2259	rVB6	8972	12957	0.30%	0.030%
24	16.998	2359	2365	2370	rVB8	6435	10264	0.23%	0.024%
25	17.110	2375	2384	2387	rBV7	4577	9985	0.23%	0.023%
26	17.316	2412	2419	2430	rBV	1624126	2453153	55.96%	5.767%
27	17.416	2430	2436	2454	rVB	2528090	3776046	86.14%	8.877%
28	19.228	2740	2744	2749	rVV2	34396	46301	1.06%	0.109%
29	19.298	2751	2756	2762	rVV	29811	48697	1.11%	0.114%
30	19.651	2810	2816	2830	rBV	3281677	4383716	100.00%	10.306%
31	21.404	3108	3114	3129	rBV	1582053	2363229	53.91%	5.556%
32	23.698	3496	3504	3521	rBV2	1369071	3036150	69.26%	7.138%
33	23.857	3524	3531	3542	rVB	802685	1741466	39.73%	4.094%




Sum of corrected areas: 42535514

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010116.D
Acq On : 27 Apr 2022 11:03
Operator : CG/JU
Sample : PB144346BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK346

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

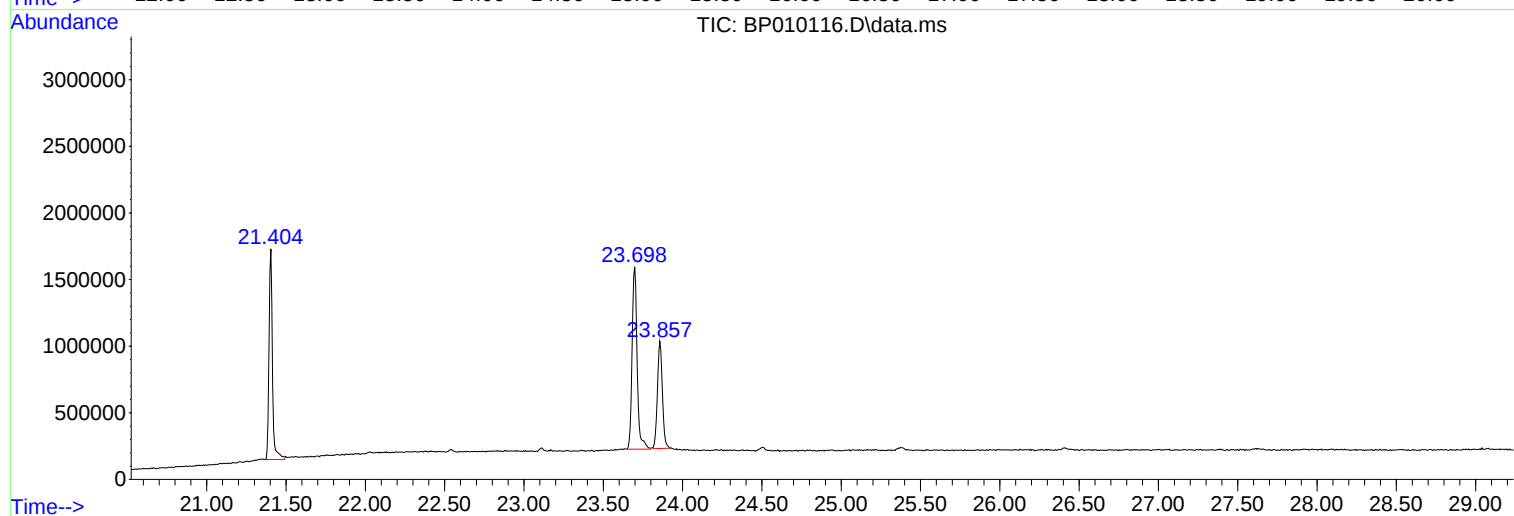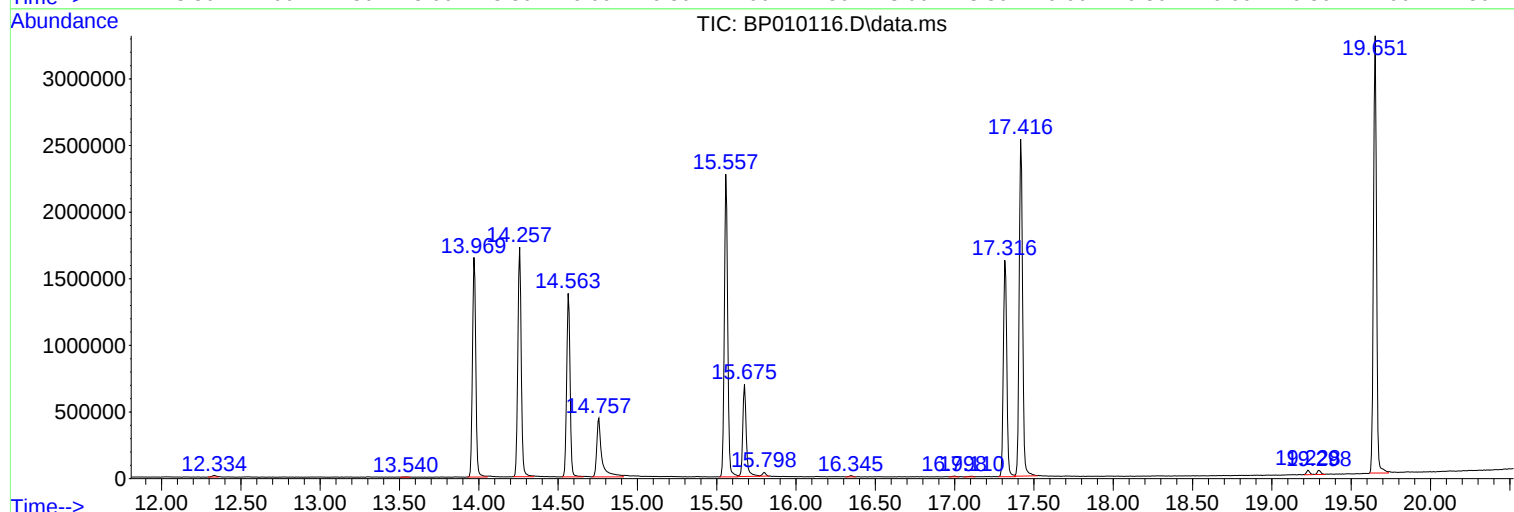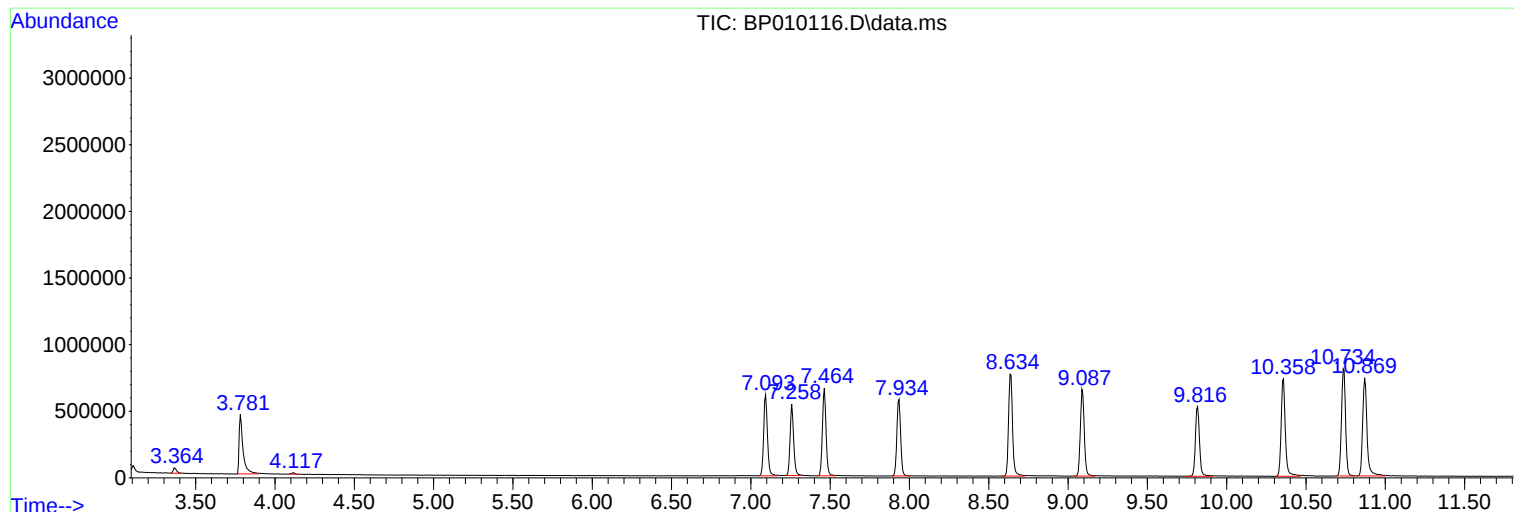

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010116.D
Acq On : 27 Apr 2022 11:03
Operator : CG/JU
Sample : PB144346BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK346

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010116.D
Acq On : 27 Apr 2022 11:03
Operator : CG/JU
Sample : PB144346BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK346

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------