

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010120.D
 Acq On : 27 Apr 2022 13:17
 Operator : CG/JU
 Sample : N2470-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	53	rVB	17812	24740	0.95%	0.091%
2	3.822	122	125	128	rBV5	7538	11458	0.44%	0.042%
3	3.887	134	136	141	rVB5	6604	10404	0.40%	0.038%
4	4.022	155	159	163	rBV4	6548	9907	0.38%	0.036%
5	4.117	170	175	181	rVB2	14204	22469	0.86%	0.083%
6	5.034	328	331	338	rBV5	5973	10944	0.42%	0.040%
7	6.211	527	531	533	rBV5	1948	2828	0.11%	0.010%
8	6.622	597	601	607	rVB6	7469	11868	0.45%	0.044%
9	6.940	650	655	658	rBV6	2516	4280	0.16%	0.016%
10	7.093	673	681	698	rBV	298535	520485	19.93%	1.916%
11	7.258	703	709	721	rVV	269259	430810	16.50%	1.586%
12	7.463	736	744	753	rBV	330849	536089	20.53%	1.974%
13	7.563	757	761	766	rVB7	4666	7643	0.29%	0.028%
14	7.934	816	824	834	rBV	659777	1106638	42.37%	4.074%
15	8.181	861	866	870	rBV7	1770	3995	0.15%	0.015%
16	8.246	872	877	879	rBV5	2116	2982	0.11%	0.011%
17	8.528	921	925	928	rVB6	1531	2669	0.10%	0.010%
18	8.634	935	943	956	rBV	380598	672924	25.77%	2.477%
19	8.757	959	964	972	rVB	24112	42657	1.63%	0.157%
20	9.093	1013	1021	1036	rBV	321548	572829	21.93%	2.109%
21	9.263	1047	1050	1054	rBV5	2568	3837	0.15%	0.014%
22	9.540	1092	1097	1102	rVB2	20979	32624	1.25%	0.120%
23	9.816	1136	1144	1160	rBV	247290	447761	17.15%	1.648%
24	10.163	1200	1203	1206	rBV5	2457	3730	0.14%	0.014%
25	10.357	1228	1236	1250	rBV	351704	658852	25.23%	2.426%
26	10.734	1289	1300	1309	rBV	929727	1641288	62.85%	6.043%
27	10.869	1315	1323	1336	rBV	331112	639324	24.48%	2.354%
28	11.775	1473	1477	1480	rBV6	2101	2983	0.11%	0.011%
29	12.169	1541	1544	1550	rVB8	3279	5487	0.21%	0.020%
30	12.328	1564	1571	1580	rBV5	7007	15767	0.60%	0.058%
31	13.175	1712	1715	1720	rVB7	1820	3172	0.12%	0.012%
32	13.304	1735	1737	1742	rVB6	2427	2695	0.10%	0.010%
33	13.404	1750	1754	1761	rVB3	7083	9602	0.37%	0.035%
34	13.540	1773	1777	1781	rBV6	2189	3817	0.15%	0.014%
35	13.851	1825	1830	1834	rBV7	3019	5124	0.20%	0.019%
36	13.898	1834	1838	1842	rVB5	8298	13764	0.53%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010120.D
 Acq On : 27 Apr 2022 13:17
 Operator : CG/JU
 Sample : N2470-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	13.969	1842	1850	1862	rBV	804440	1201037	45.99%	4.422%
38	14.257	1891	1899	1917	rBV	864332	1310108	50.16%	4.823%
39	14.469	1932	1935	1939	rVB5	2167	3381	0.13%	0.012%
40	14.563	1943	1951	1962	rBV	1478705	2227830	85.31%	8.202%
41	14.763	1978	1985	2003	rBV	115261	316331	12.11%	1.165%
42	14.981	2018	2022	2029	rVB9	7867	15082	0.58%	0.056%
43	15.369	2084	2088	2089	rBV4	4306	4687	0.18%	0.017%
44	15.557	2112	2120	2133	rBV	1161224	1745365	66.83%	6.426%
45	15.675	2134	2140	2155	rVV	194753	320823	12.28%	1.181%
46	15.798	2157	2161	2168	rVB2	14875	24765	0.95%	0.091%
47	16.051	2203	2204	2209	rVB5	3873	3305	0.13%	0.012%
48	16.134	2214	2218	2222	rVV7	3812	6374	0.24%	0.023%
49	16.210	2226	2231	2234	rVB7	2418	3527	0.14%	0.013%
50	16.251	2234	2238	2239	rBV4	3281	3699	0.14%	0.014%
51	16.286	2241	2244	2248	rVV5	3727	6768	0.26%	0.025%
52	16.345	2251	2254	2260	rVB8	5606	7887	0.30%	0.029%
53	16.398	2260	2263	2265	rBV4	2728	2943	0.11%	0.011%
54	16.457	2270	2273	2277	rVV5	2520	4192	0.16%	0.015%
55	16.522	2280	2284	2286	rVV5	2260	2963	0.11%	0.011%
56	16.722	2315	2318	2320	rBV4	3342	3569	0.14%	0.013%
57	16.792	2325	2330	2333	rBV7	2908	4621	0.18%	0.017%
58	16.998	2361	2365	2370	rVB8	2365	4351	0.17%	0.016%
59	17.081	2376	2379	2381	rBV4	3180	3950	0.15%	0.015%
60	17.104	2381	2383	2387	rVB3	4423	4964	0.19%	0.018%
61	17.245	2404	2407	2410	rBV4	2982	3500	0.13%	0.013%
62	17.316	2412	2419	2430	rBV	1701158	2611601	100.00%	9.615%
63	17.416	2430	2436	2449	rVV	1359079	2096522	80.28%	7.719%
64	17.510	2449	2452	2460	rVB8	18949	35989	1.38%	0.132%
65	17.710	2482	2486	2493	rVB9	7817	13138	0.50%	0.048%
66	17.810	2499	2503	2507	rBV6	8403	11177	0.43%	0.041%
67	17.992	2530	2534	2540	rVB6	9835	15050	0.58%	0.055%
68	18.198	2565	2569	2574	rBV7	17806	29316	1.12%	0.108%
69	18.275	2578	2582	2585	rVB4	5941	9504	0.36%	0.035%
70	18.616	2636	2640	2644	rBV	62808	72735	2.79%	0.268%
71	18.651	2644	2646	2652	rVB6	6163	10256	0.39%	0.038%
72	18.851	2678	2680	2682	rBV3	5941	5983	0.23%	0.022%
73	18.975	2699	2701	2704	rBV4	4252	4704	0.18%	0.017%
74	19.027	2706	2710	2713	rBV5	8314	11595	0.44%	0.043%
75	19.227	2741	2744	2751	rVB4	24697	36140	1.38%	0.133%
76	19.298	2752	2756	2758	rBV	19755	23583	0.90%	0.087%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010120.D
Acq On : 27 Apr 2022 13:17
Operator : CG/JU
Sample : N2470-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

77	19.651	2810	2816	2832	rBV	1497506	2190038	83.86%	8.063%
78	20.504	2957	2961	2964	rBV3	45347	57737	2.21%	0.213%
79	21.110	3060	3064	3071	rBV	251027	338839	12.97%	1.247%
80	21.404	3108	3114	3128	rBV	1654663	2375266	90.95%	8.745%
81	23.698	3498	3504	3511	rBV2	377450	786980	30.13%	2.897%
82	23.857	3524	3531	3545	rVB2	776689	1691664	64.77%	6.228%


Sum of corrected areas: 27162285

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010120.D
Acq On : 27 Apr 2022 13:17
Operator : CG/JU
Sample : N2470-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

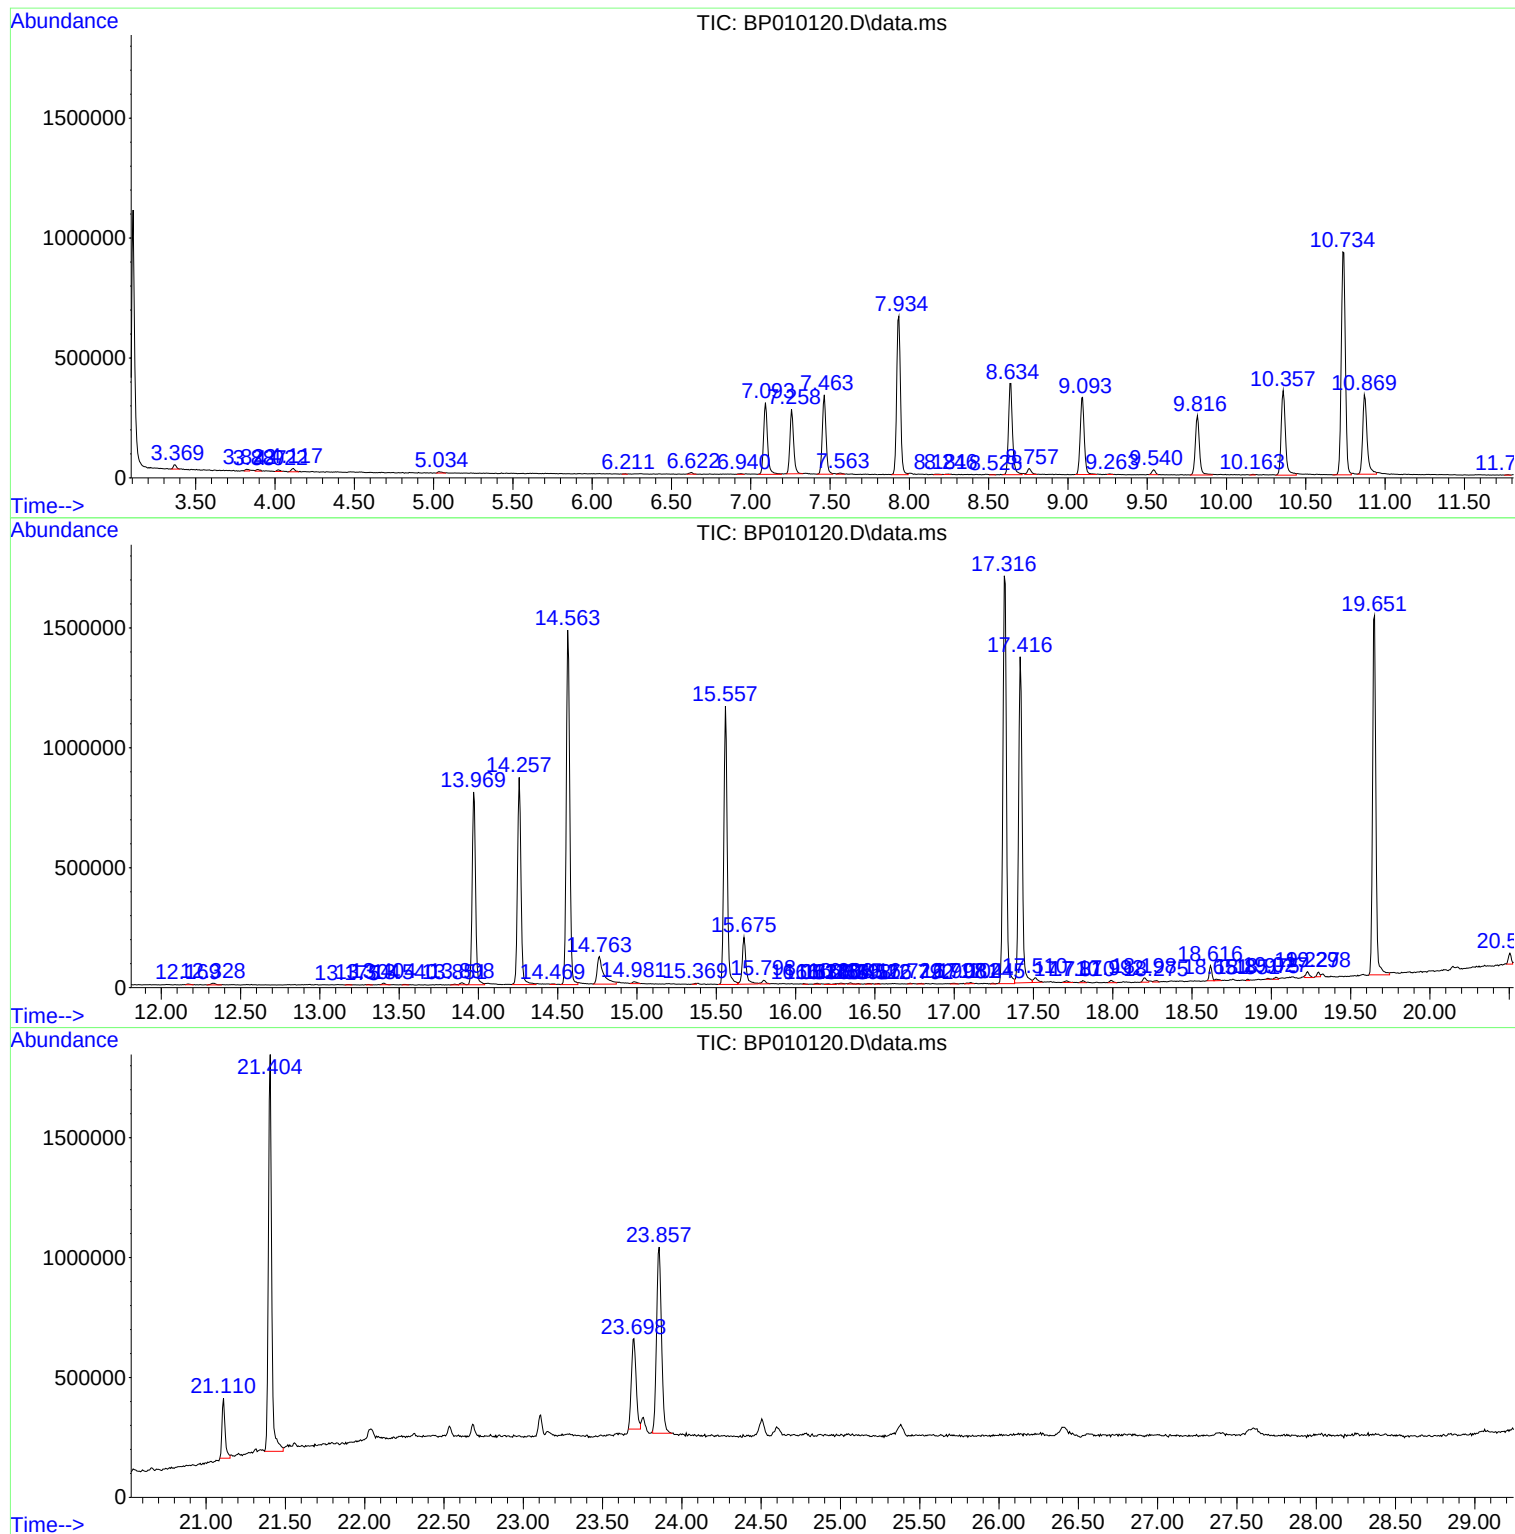

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010120.D
Acq On : 27 Apr 2022 13:17
Operator : CG/JU
Sample : N2470-07
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
BFFH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.110	2.85 ng/ul	338839	Chrysene-d12		21.404	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Nonadecene		266	C19H38	018435-45-5	98
2	1-Hexacosene		364	C26H52	018835-33-1	94
3	Trichloroacetic acid, hexadecyl ...		386	C18H33Cl3O2	074339-54-1	94
4	Heptadecyl heptafluorobutyrate		452	C21H35F7O2	959085-66-6	94
5	Octacosanol		410	C28H58O	000557-61-9	91

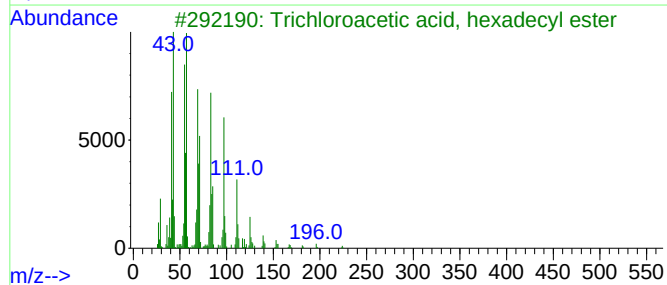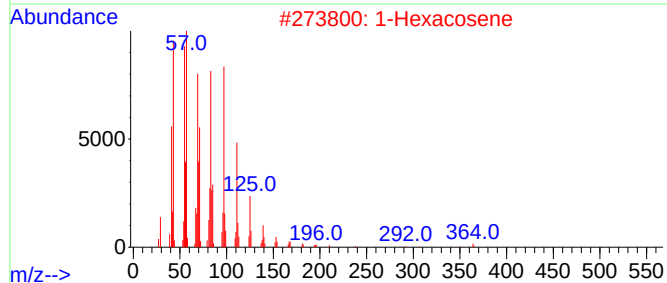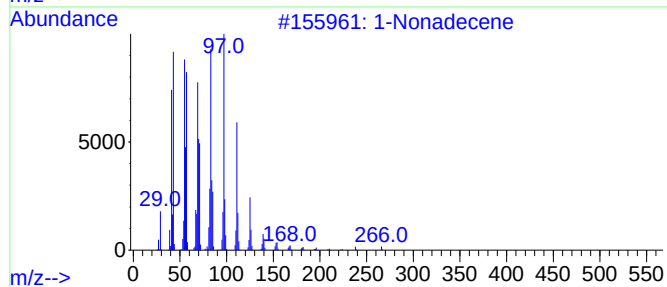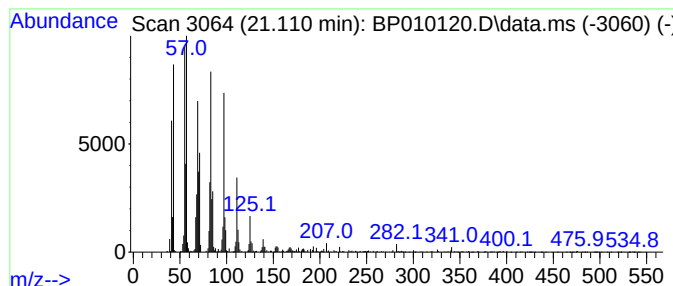

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010120.D
Acq On : 27 Apr 2022 13:17
Operator : CG/JU
Sample : N2470-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.110	2.9	ng/u1	338839	5	21.404	2375270	20.0